

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
 Data File : BF108555.D
 Acq On : 28 Aug 2018 15:12
 Operator : JU/SJ
 Sample : J4538-03RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VSS3RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.366	3	5	14	rVB	311429	350764	11.16%	1.234%
2	5.254	492	496	505	rBV	68459	103637	3.30%	0.364%
3	5.648	559	563	599	rBV	1534379	2688303	85.56%	9.454%
4	6.636	727	731	750	rBV	1978238	2824065	89.89%	9.932%
5	6.778	750	755	777	rVB	2559440	2815141	89.60%	9.900%
6	7.001	789	793	806	rBV	744721	746465	23.76%	2.625%
7	7.154	815	819	832	rBV	2202095	2195234	69.87%	7.720%
8	7.566	884	889	897	rBV	1697537	1861870	59.26%	6.548%
9	8.283	1007	1011	1025	rBV	971518	945354	30.09%	3.325%
10	9.354	1186	1193	1197	rBV	3337205	3141842	100.00%	11.049%
11	9.748	1256	1260	1264	rBV	208565	174638	5.56%	0.614%
12	9.936	1289	1292	1295	rBV	60502	47334	1.51%	0.166%
13	10.042	1306	1310	1319	rVB	1153077	1085164	34.54%	3.816%
14	10.842	1441	1446	1457	rBV	2123281	1954186	62.20%	6.872%
15	11.542	1561	1565	1568	rBV	1224758	1068677	34.01%	3.758%
16	12.048	1647	1651	1656	rBV	98637	103068	3.28%	0.362%
17	13.124	1830	1834	1838	rBV	2699773	2323387	73.95%	8.171%
18	13.330	1864	1869	1874	rVB2	31757	41761	1.33%	0.147%
19	13.671	1924	1927	1930	rBV2	41066	38277	1.22%	0.135%
20	14.006	1980	1984	1994	rVB	149311	204346	6.50%	0.719%
21	14.195	2012	2016	2022	rBV	794794	713171	22.70%	2.508%
22	14.318	2034	2037	2040	rBV	63039	54293	1.73%	0.191%
23	14.624	2086	2089	2091	rBV	92077	81567	2.60%	0.287%
24	14.953	2141	2145	2156	rVB	144601	227684	7.25%	0.801%
25	15.112	2169	2172	2178	rVB	83697	90324	2.87%	0.318%
26	15.312	2202	2206	2210	rBV	213213	246958	7.86%	0.869%
27	15.359	2210	2214	2221	rVV2	65637	108479	3.45%	0.381%
28	15.724	2271	2276	2278	rBV	172178	247195	7.87%	0.869%
29	15.753	2278	2281	2288	rVB	548712	715101	22.76%	2.515%
30	15.948	2311	2314	2320	rVB5	43331	59823	1.90%	0.210%
31	16.200	2351	2357	2362	rVB	263062	432114	13.75%	1.520%
32	16.277	2367	2370	2378	rVV4	36268	73401	2.34%	0.258%
33	16.747	2446	2450	2456	rVB2	74310	127827	4.07%	0.450%
34	17.536	2579	2584	2592	rBV5	59498	157209	5.00%	0.553%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108555.D
Acq On : 28 Aug 2018 15:12
Operator : JU/SJ
Sample : J4538-03RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS3RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	17.706	2608	2613	2622	rvB7	45667	95682	3.05%	0.336%
36	17.994	2656	2662	2675	rvB9	91863	290641	9.25%	1.022%


Sum of corrected areas: 28434982

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108555.D
Acq On : 28 Aug 2018 15:12
Operator : JU/SJ
Sample : J4538-03RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS3RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

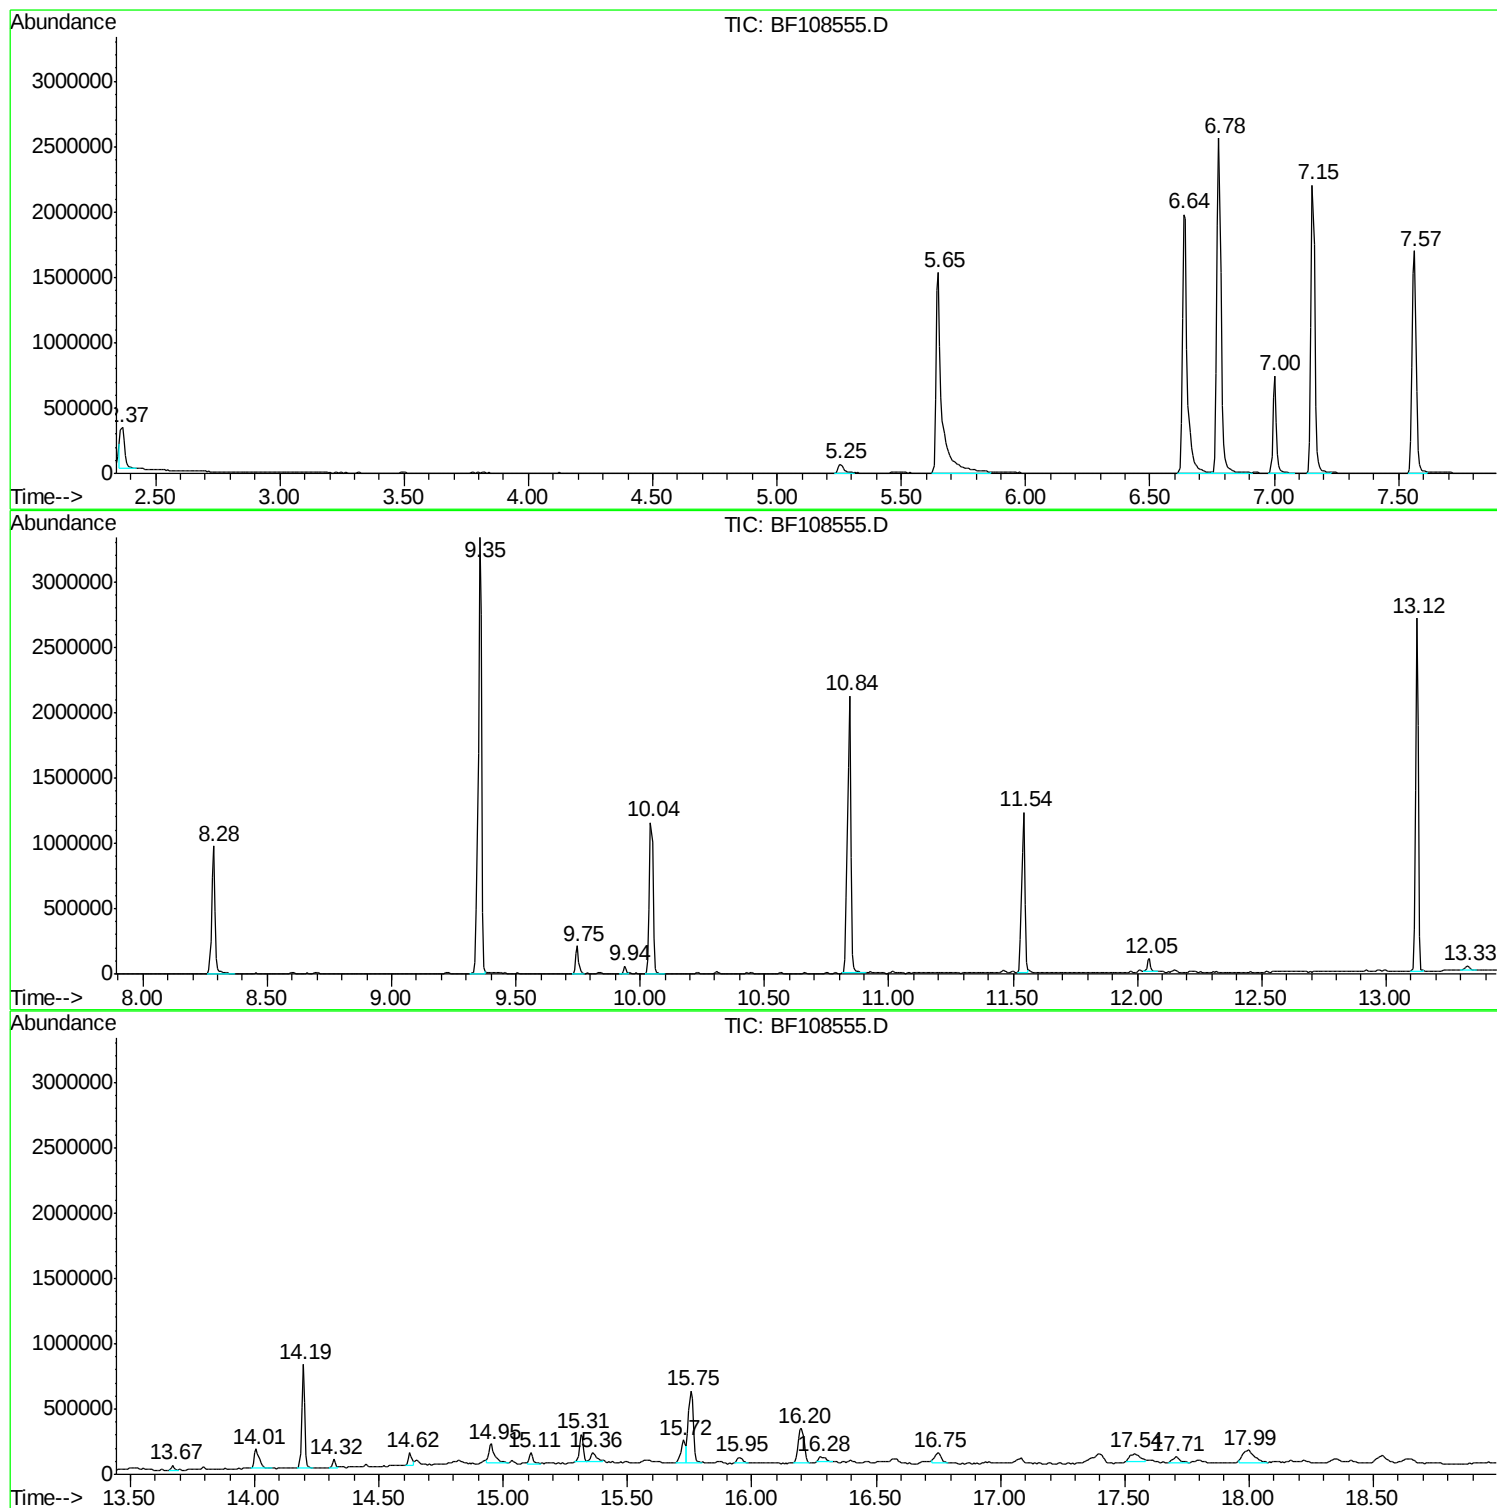

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data_File : BF108555.D
Acq_On : 28_Aug_2018_ 15:122
Operator : JU/SJJ
Sample : J4538-03REE
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
VSS3RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
