

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
 Data File : BF108556.D
 Acq On : 28 Aug 2018 15:38
 Operator : JU/SJ
 Sample : J4538-04RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 VSS4RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.243	491	494	507	rBV	51393	77231	3.05%	0.261%
2	5.643	558	562	609	rBV	1109527	2055939	81.25%	6.957%
3	6.637	727	731	750	rBV	1620997	2178711	86.10%	7.372%
4	6.778	750	755	772	rVB	1902074	2165065	85.56%	7.326%
5	7.001	789	793	806	rVB	686486	699932	27.66%	2.368%
6	7.154	815	819	831	rBV	1729526	1685752	66.62%	5.704%
7	7.560	884	888	897	rBV	1345511	1386693	54.80%	4.692%
8	8.284	1007	1011	1023	rBV	955450	911682	36.03%	3.085%
9	9.354	1189	1193	1197	rBV	2909112	2530450	100.00%	8.563%
10	9.748	1256	1260	1264	rVB	162900	135943	5.37%	0.460%
11	10.042	1306	1310	1319	rVB	1106345	1035625	40.93%	3.504%
12	10.842	1441	1446	1452	rBV	1595385	1535351	60.68%	5.195%
13	11.013	1470	1475	1479	rBV3	27105	33598	1.33%	0.114%
14	11.466	1548	1552	1556	rBV	72625	76569	3.03%	0.259%
15	11.542	1561	1565	1568	rVV	1205674	1058965	41.85%	3.583%
16	11.566	1568	1569	1572	rVB	50850	31157	1.23%	0.105%
17	11.977	1634	1639	1642	rBV3	23293	34058	1.35%	0.115%
18	12.048	1647	1651	1655	rBV	211209	185109	7.32%	0.626%
19	12.219	1676	1680	1686	rVB4	22183	38351	1.52%	0.130%
20	12.924	1796	1800	1804	rBV3	30491	30735	1.21%	0.104%
21	13.124	1830	1834	1838	rBV	2305572	1941742	76.74%	6.571%
22	13.324	1864	1868	1874	rVB2	47900	63868	2.52%	0.216%
23	13.554	1905	1907	1912	rVB	43928	37576	1.48%	0.127%
24	13.795	1945	1948	1955	rBV	54305	50636	2.00%	0.171%
25	14.007	1981	1984	1991	rBV	154962	209520	8.28%	0.709%
26	14.130	2002	2005	2009	rBV4	24695	31488	1.24%	0.107%
27	14.195	2012	2016	2020	rBV	807755	729819	28.84%	2.470%
28	14.318	2034	2037	2040	rBV	30496	33441	1.32%	0.113%
29	14.624	2086	2089	2091	rBV	96262	94393	3.73%	0.319%
30	14.648	2091	2093	2103	rVB4	70754	101042	3.99%	0.342%
31	14.954	2141	2145	2148	rBV	89246	96594	3.82%	0.327%
32	15.036	2156	2159	2165	rVB	71400	75146	2.97%	0.254%
33	15.112	2168	2172	2176	rVB	302440	313325	12.38%	1.060%
34	15.318	2202	2207	2210	rBV	345546	392883	15.53%	1.329%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108556.D
Acq On : 28 Aug 2018 15:38
Operator : JU/SJ
Sample : J4538-04RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS4RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.354	2210	2213	2228	rVB	326183	602051	23.79%	2.037%
36	15.724	2272	2276	2278	rBV	146887	199021	7.87%	0.673%
37	15.754	2278	2281	2288	rVB	542207	738098	29.17%	2.498%
38	15.948	2310	2314	2321	rBV	126474	189234	7.48%	0.640%
39	16.201	2351	2357	2364	rVB	583565	961747	38.01%	3.254%
40	16.277	2365	2370	2378	rBV2	100097	244432	9.66%	0.827%
41	16.407	2388	2392	2395	rVB5	35950	51631	2.04%	0.175%
42	16.483	2399	2405	2409	rBV	129613	275549	10.89%	0.932%
43	16.754	2447	2451	2456	rVB3	77504	127936	5.06%	0.433%
44	17.083	2501	2507	2515	rVB	131385	268008	10.59%	0.907%
45	17.536	2576	2584	2595	rBV3	285272	903875	35.72%	3.059%
46	17.995	2653	2662	2679	rBV2	462362	1529506	60.44%	5.176%
47	18.230	2698	2702	2709	rVB2	106113	219898	8.69%	0.744%
48	18.353	2718	2723	2729	rBV7	58531	128022	5.06%	0.433%
49	18.542	2744	2755	2763	rBV10	184433	722137	28.54%	2.444%
50	18.648	2769	2773	2782	rVB5	138918	332843	13.15%	1.126%


Sum of corrected areas: 29552377

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108556.D
Acq On : 28 Aug 2018 15:38
Operator : JU/SJ
Sample : J4538-04RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
VSS4RE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

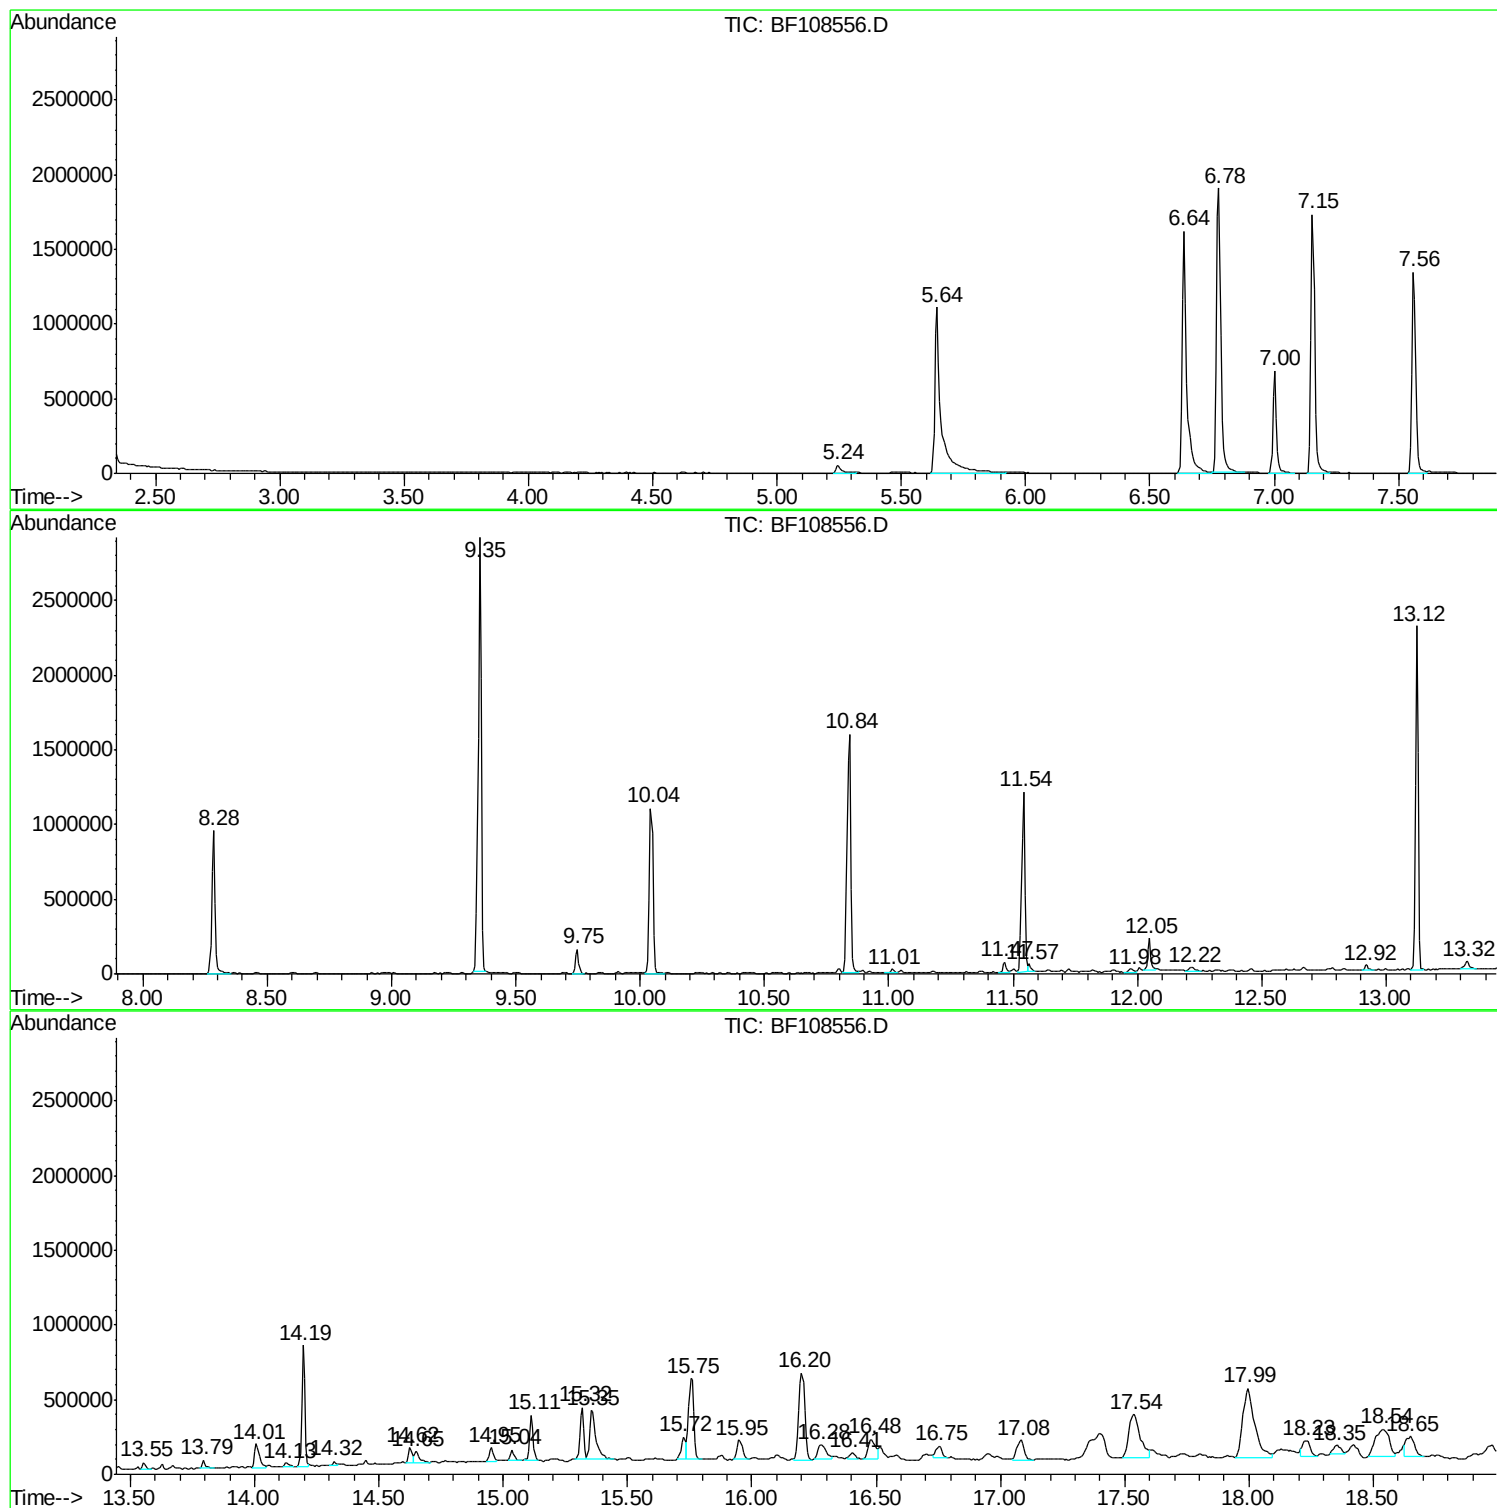

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data_File : BF108556.D
Acq_On : 28_Aug_2018_ 15:388
Operator : JU/SJJ
Sample : J4538-04REE
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
VSS4RE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
