

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
 Data File : BF108563.D
 Acq On : 28 Aug 2018 18:45
 Operator : JU/SJ
 Sample : J4277-11 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-01-082718-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.643	558	562	586	rBV	91217	281616	29.54%	3.064%
2	6.637	727	731	751	rBV	159139	364226	38.20%	3.963%
3	6.778	751	755	770	rVB	256787	366275	38.42%	3.985%
4	7.001	789	793	808	rBV	593141	660399	69.26%	7.185%
5	7.154	815	819	835	rBV	254444	294232	30.86%	3.201%
6	7.560	884	888	901	rBV	175995	230441	24.17%	2.507%
7	8.284	1007	1011	1031	rBV	886143	872063	91.46%	9.488%
8	9.354	1189	1193	1202	rVB	508155	437125	45.85%	4.756%
9	9.748	1255	1260	1267	rVB	43307	46971	4.93%	0.511%
10	9.907	1282	1287	1290	rBV	21898	20536	2.15%	0.223%
11	10.042	1306	1310	1315	rBV2	991760	901916	94.59%	9.813%
12	10.472	1381	1383	1386	rBV	13100	11726	1.23%	0.128%
13	10.554	1393	1397	1401	rBV2	8545	12994	1.36%	0.141%
14	10.595	1401	1404	1409	rVB	12739	14074	1.48%	0.153%
15	10.836	1441	1445	1452	rBV	205707	210323	22.06%	2.288%
16	10.925	1457	1460	1464	rBV2	7665	11959	1.25%	0.130%
17	11.542	1561	1565	1567	rBV	889753	806772	84.61%	8.778%
18	11.566	1567	1569	1575	rVV	124225	104022	10.91%	1.132%
19	11.619	1575	1578	1582	rVV	29941	25185	2.64%	0.274%
20	12.042	1646	1650	1653	rBV	30641	35535	3.73%	0.387%
21	12.072	1653	1655	1659	rVB	34405	26724	2.80%	0.291%
22	12.119	1660	1663	1666	rBV	12549	11443	1.20%	0.125%
23	12.154	1666	1669	1672	rBV2	40086	50155	5.26%	0.546%
24	12.336	1698	1700	1702	rBV	14363	11036	1.16%	0.120%
25	12.372	1703	1706	1710	rVB3	19434	19975	2.09%	0.217%
26	12.519	1728	1731	1733	rBV2	12993	9898	1.04%	0.108%
27	12.595	1739	1744	1747	rBV2	46860	52031	5.46%	0.566%
28	12.630	1747	1750	1752	rVV2	15655	20426	2.14%	0.222%
29	12.683	1756	1759	1763	rBV4	21867	30178	3.17%	0.328%
30	12.760	1768	1772	1775	rBV	254577	216806	22.74%	2.359%
31	12.913	1796	1798	1800	rBV	12450	10207	1.07%	0.111%
32	12.995	1805	1812	1817	rBV	264038	291001	30.52%	3.166%
33	13.042	1817	1820	1823	rVB	23017	21080	2.21%	0.229%
34	13.119	1830	1833	1837	rBV	414966	384188	40.29%	4.180%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108563.D
Acq On : 28 Aug 2018 18:45
Operator : JU/SJ
Sample : J4277-11 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-01-082718-B

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.148	1837	1838	1844	rVB4	14130	14920	1.56%	0.162%
36	13.213	1844	1849	1853	rBV6	27184	50662	5.31%	0.551%
37	13.319	1865	1867	1872	rVB2	43290	44124	4.63%	0.480%
38	13.383	1876	1878	1881	rBV	28139	25077	2.63%	0.273%
39	13.424	1882	1885	1887	rVV2	39350	33342	3.50%	0.363%
40	13.489	1893	1896	1898	rBV3	8459	10723	1.12%	0.117%
41	13.519	1898	1901	1904	rVV	35190	34146	3.58%	0.372%
42	13.548	1904	1906	1909	rVV	31810	28430	2.98%	0.309%
43	13.801	1946	1949	1952	rBV5	13194	21215	2.23%	0.231%
44	13.830	1952	1954	1958	rVB	25058	24349	2.55%	0.265%
45	13.889	1962	1964	1967	rVB3	14542	11492	1.21%	0.125%
46	13.942	1971	1973	1976	rVB	26223	20415	2.14%	0.222%
47	13.971	1976	1978	1980	rVB	19882	13740	1.44%	0.149%
48	14.001	1980	1983	1985	rBV3	32726	44661	4.68%	0.486%
49	14.195	2011	2016	2019	rBV	932035	953463	100.00%	10.374%
50	14.219	2019	2020	2026	rVB	115191	93178	9.77%	1.014%
51	14.301	2032	2034	2036	rBV	31121	29584	3.10%	0.322%
52	15.283	2198	2201	2204	rBV	76305	106469	11.17%	1.158%
53	15.618	2255	2258	2265	rVB	52479	73129	7.67%	0.796%
54	15.683	2265	2269	2273	rBV	83179	120299	12.62%	1.309%
55	15.754	2277	2281	2286	rVB	430765	573986	60.20%	6.245%


Sum of corrected areas: 9190942

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108563.D
Acq On : 28 Aug 2018 18:45
Operator : JU/SJ
Sample : J4277-11 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-01-082718-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

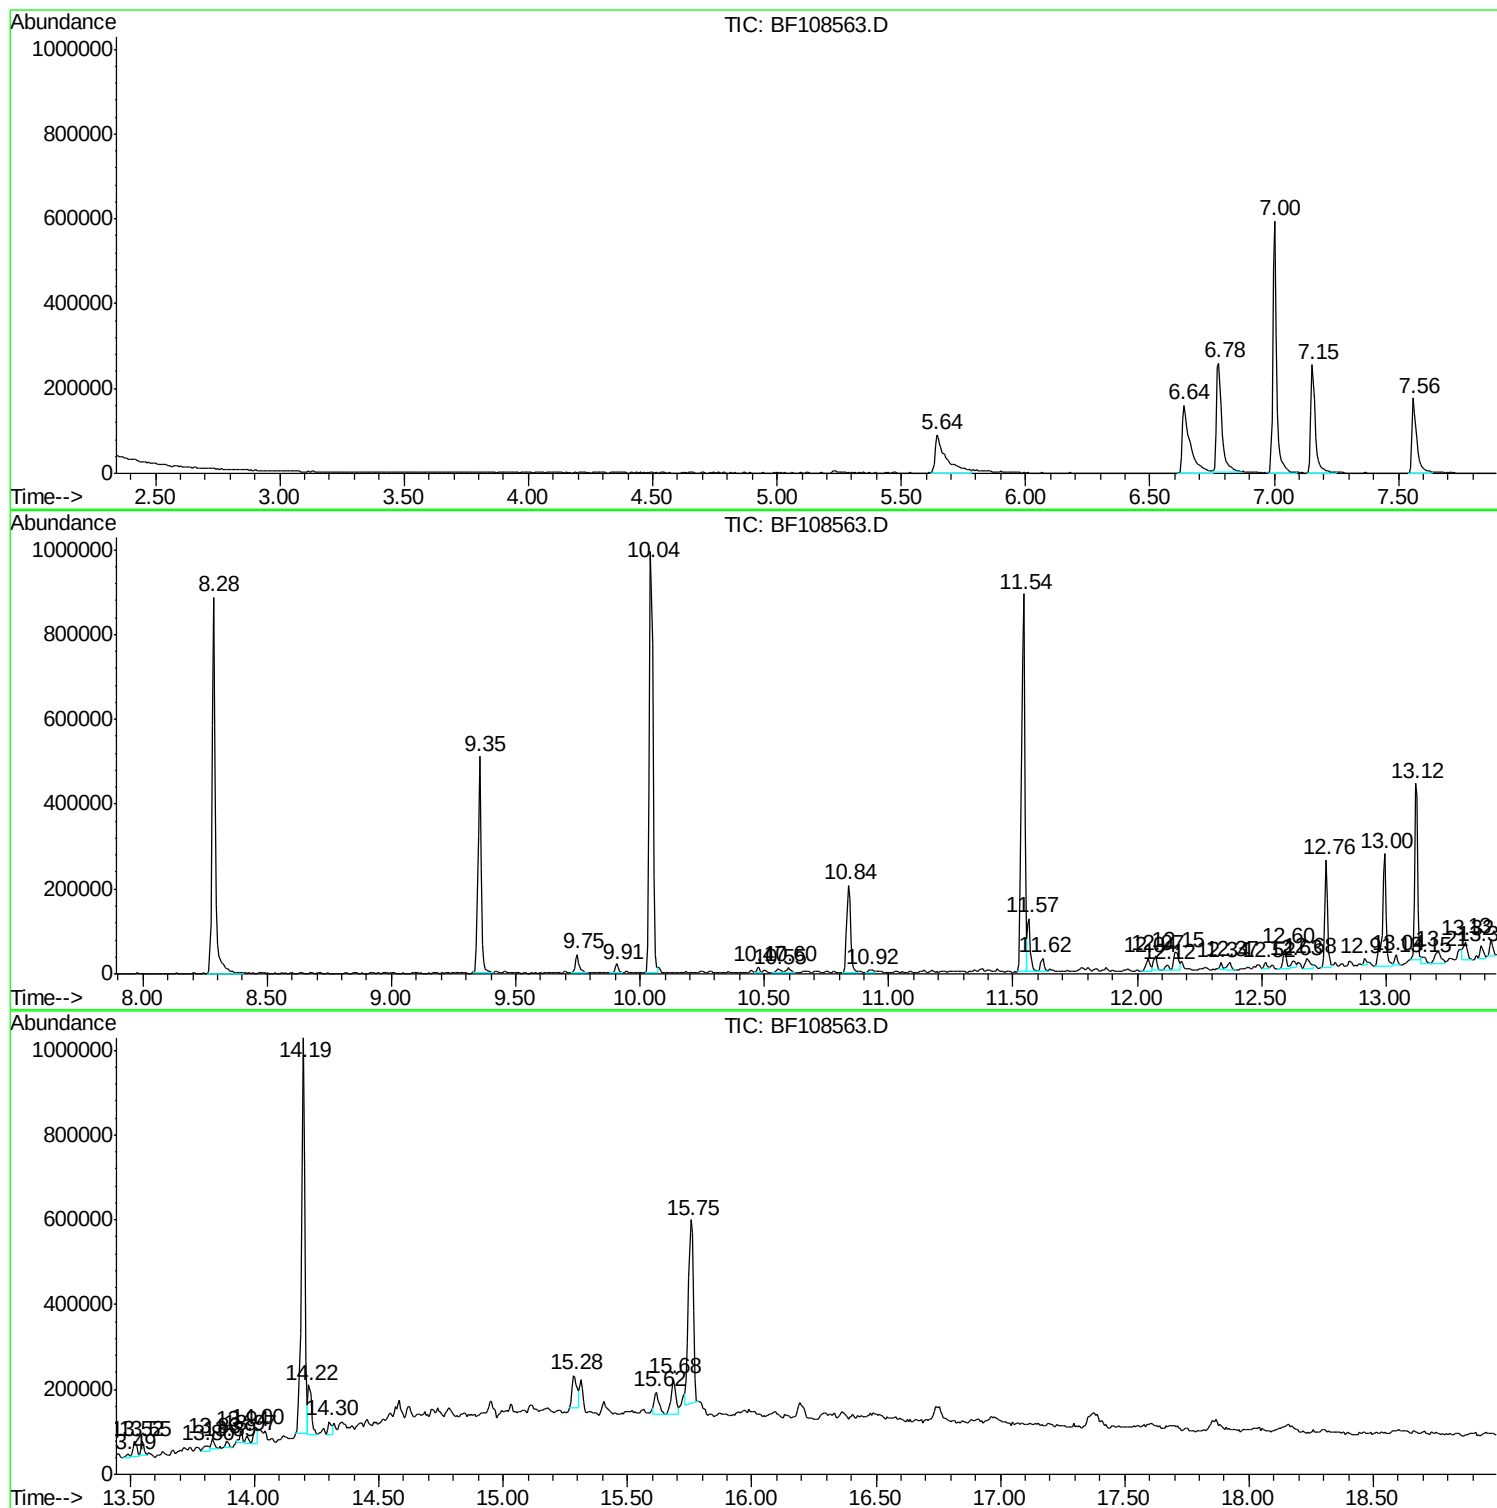

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data_File : BF108563.D
Acq_On : 28_Aug_2018_ 18:455
Operator : JU/SJJ
Sample : J4277-11_5XX
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
OR-01-082718-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
