

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
 Data File : BF108579.D
 Acq On : 29 Aug 2018 2:28
 Operator : JU/SJ
 Sample : J4656-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082418-SIDI-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.237	490	493	504	rBV	34193	54213	1.79%	0.315%
2	5.643	558	562	584	rBV	214517	588437	19.38%	3.417%
3	6.631	727	730	750	rBV	159302	424498	13.98%	2.465%
4	6.772	750	754	778	rVV	1065112	1429229	47.07%	8.299%
5	7.001	789	793	808	rVB	453381	562363	18.52%	3.266%
6	7.154	815	819	841	rBV	2108929	2212721	72.88%	12.849%
7	7.560	884	888	909	rBV	1429310	1789470	58.94%	10.391%
8	8.284	1007	1011	1027	rBV	541553	664527	21.89%	3.859%
9	9.354	1189	1193	1208	rBV	3326177	3036303	100.00%	17.632%
10	9.742	1256	1259	1269	rBV	113988	134943	4.44%	0.784%
11	10.042	1307	1310	1318	rVB	687812	646016	21.28%	3.751%
12	10.701	1419	1422	1428	rVB	53028	49583	1.63%	0.288%
13	10.836	1441	1445	1458	rBV	986282	1002246	33.01%	5.820%
14	11.536	1561	1564	1572	rBV	628484	611230	20.13%	3.549%
15	13.124	1829	1834	1837	rBV	2989173	2593585	85.42%	15.061%
16	14.195	2012	2016	2022	rBV	734930	721599	23.77%	4.190%
17	15.307	2202	2205	2210	rVB2	26607	31719	1.04%	0.184%
18	15.748	2271	2280	2286	rBV	410418	593746	19.55%	3.448%
19	16.189	2351	2355	2360	rVB3	22914	36933	1.22%	0.214%
20	16.736	2443	2448	2454	rBV5	17774	37514	1.24%	0.218%


Sum of corrected areas: 17220875

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108579.D
Acq On : 29 Aug 2018 2:28
Operator : JU/SJ
Sample : J4656-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

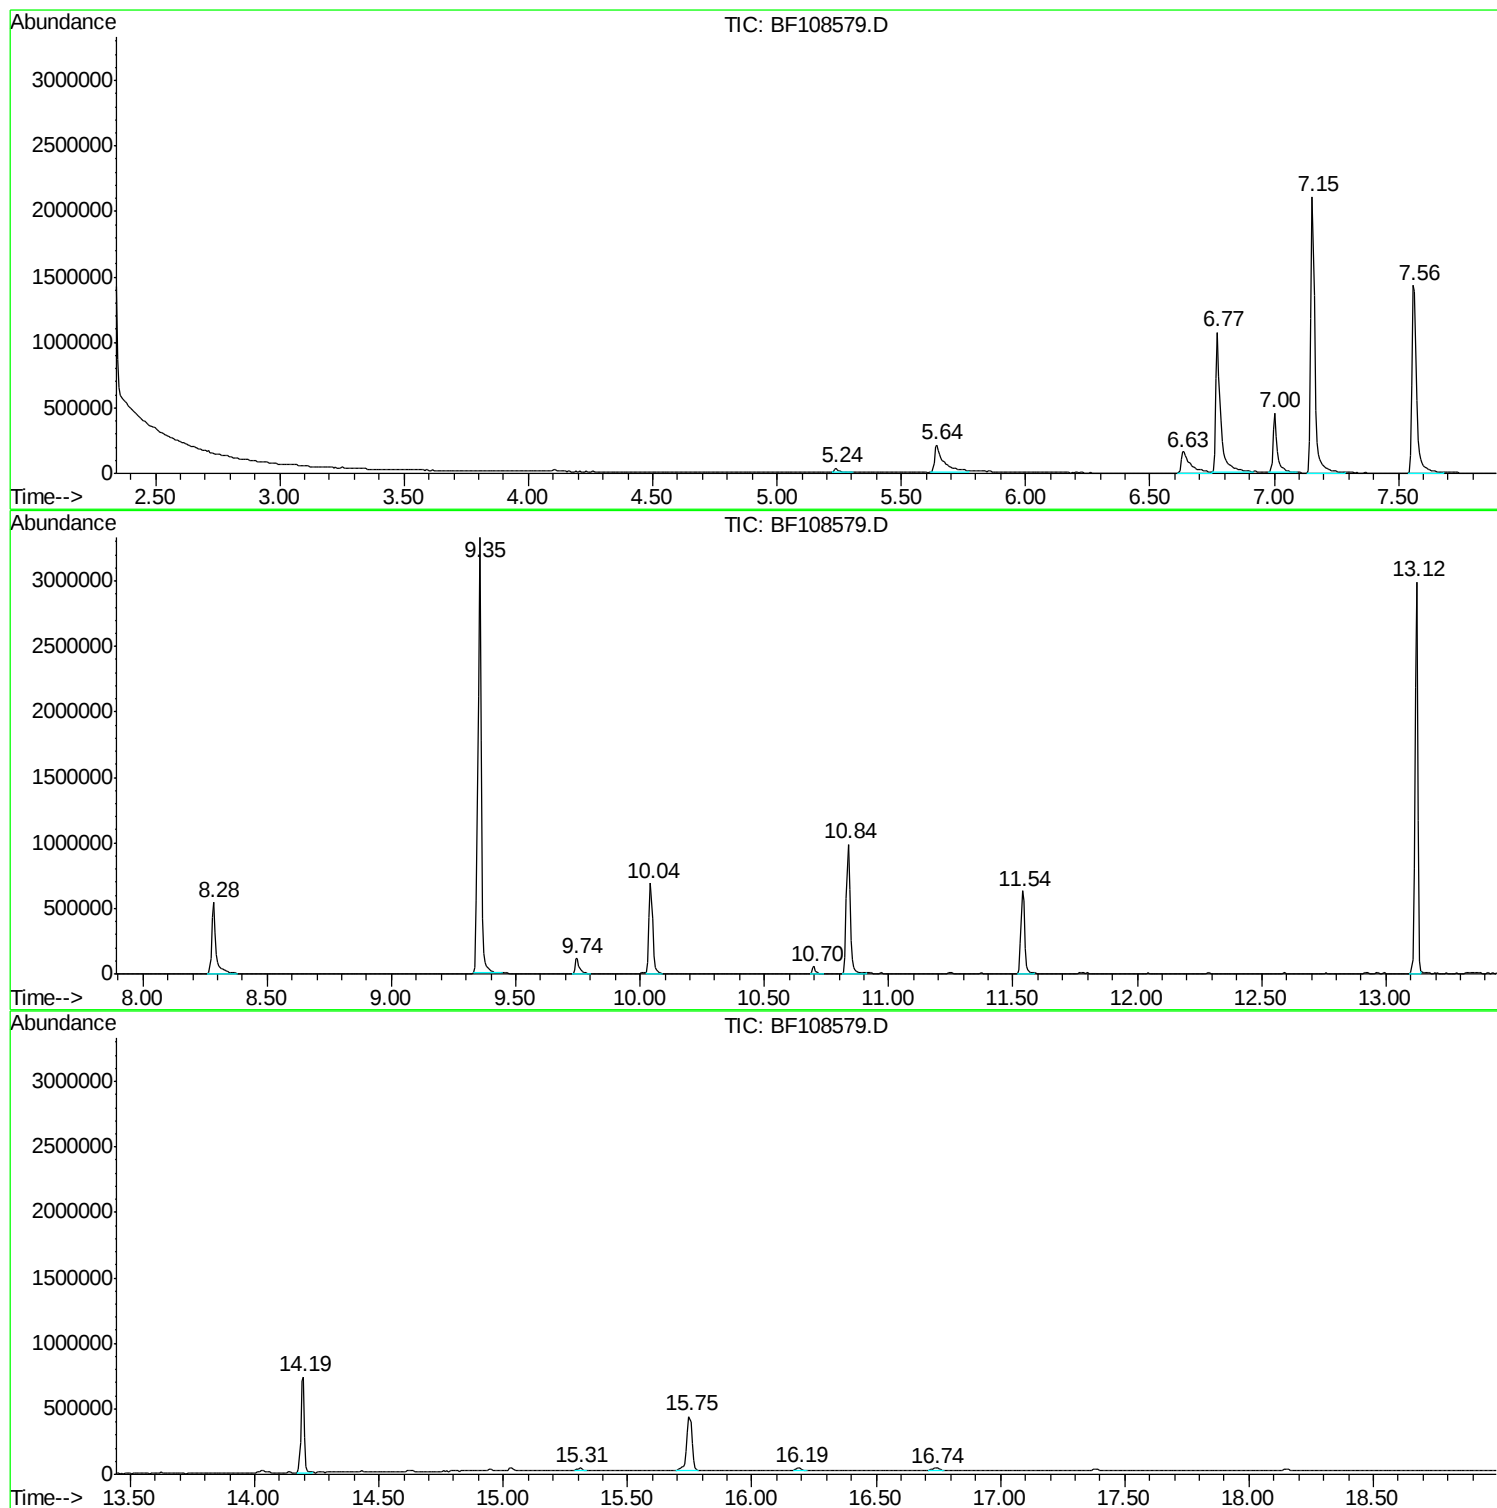

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108579.D
Acq On : 29 Aug 2018 2:28
Operator : JU/SJ
Sample : J4656-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-D-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	50.83 ng	1429230	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

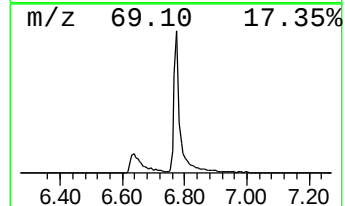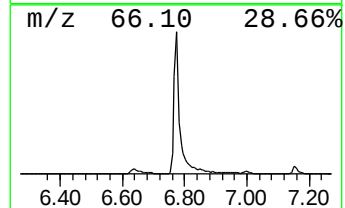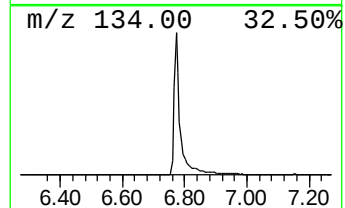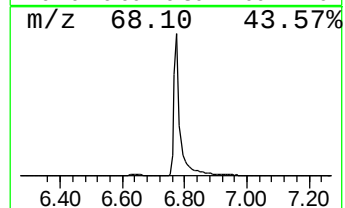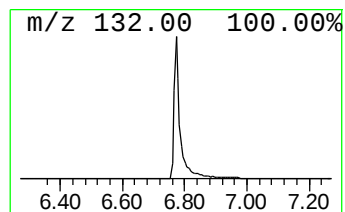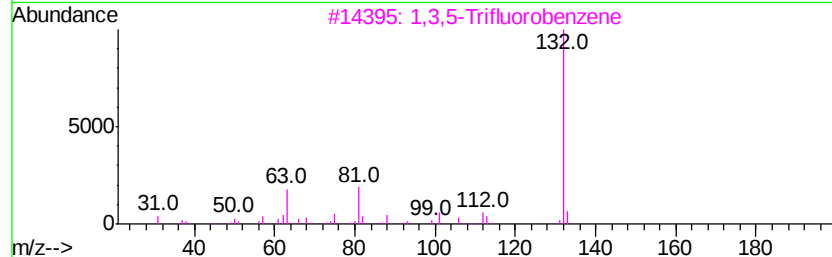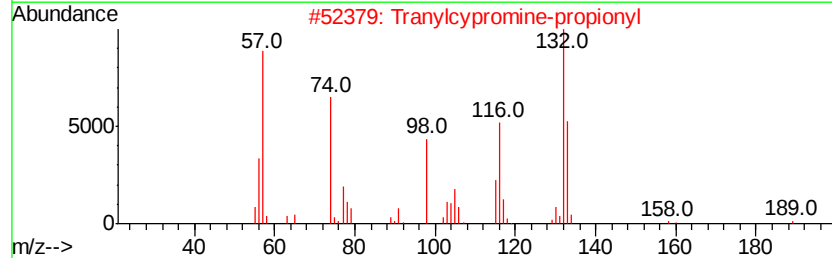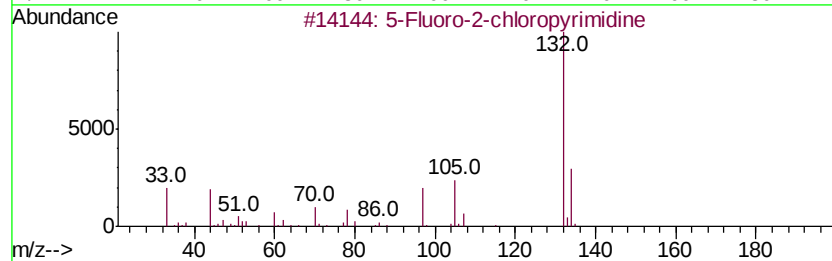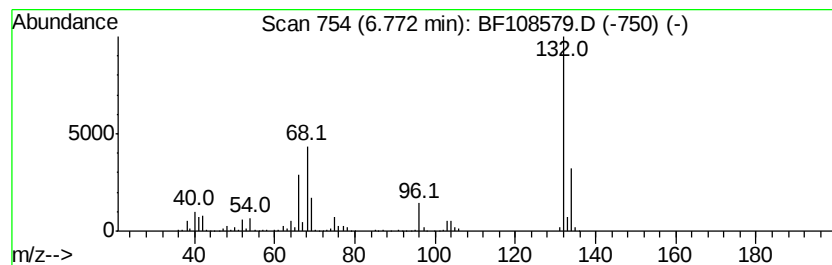

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108579.D
Acq On : 29 Aug 2018 2:28
Operator : JU/SJ
Sample : J4656-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.77	6.77	50.8	ng	1429230	1	7.00	562363	20.0