

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
 Data File : BF108582.D
 Acq On : 29 Aug 2018 3:49
 Operator : JU/SJ
 Sample : J4656-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082418-SIDI-F-U-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.636	557	561	589	rBV	323634	816048	20.28%	3.871%
2	6.630	726	730	750	rBV	251075	590808	14.68%	2.802%
3	6.772	750	754	778	rVB	1508270	1877578	46.66%	8.906%
4	7.001	789	793	810	rVB	520083	672461	16.71%	3.190%
5	7.154	815	819	846	rBV	2546580	2752949	68.41%	13.058%
6	7.566	884	889	913	rBV	1993935	2283875	56.76%	10.833%
7	8.283	1007	1011	1033	rBV	699853	838042	20.83%	3.975%
8	9.354	1189	1193	1208	rVB	4100901	4024036	100.00%	19.087%
9	9.748	1256	1260	1267	rBV	122316	144992	3.60%	0.688%
10	10.042	1307	1310	1322	rVB	894745	853374	21.21%	4.048%
11	10.701	1418	1422	1428	rBV	71103	65218	1.62%	0.309%
12	10.836	1441	1445	1458	rBV	1299268	1324681	32.92%	6.283%
13	11.536	1561	1564	1572	rBV	709400	716976	17.82%	3.401%
14	13.124	1829	1834	1837	rBV	3172494	2801256	69.61%	13.287%
15	14.195	2012	2016	2024	rBV	807234	744341	18.50%	3.531%
16	15.747	2272	2280	2289	rBV	417133	576247	14.32%	2.733%


Sum of corrected areas: 21082882

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108582.D
Acq On : 29 Aug 2018 3:49
Operator : JU/SJ
Sample : J4656-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

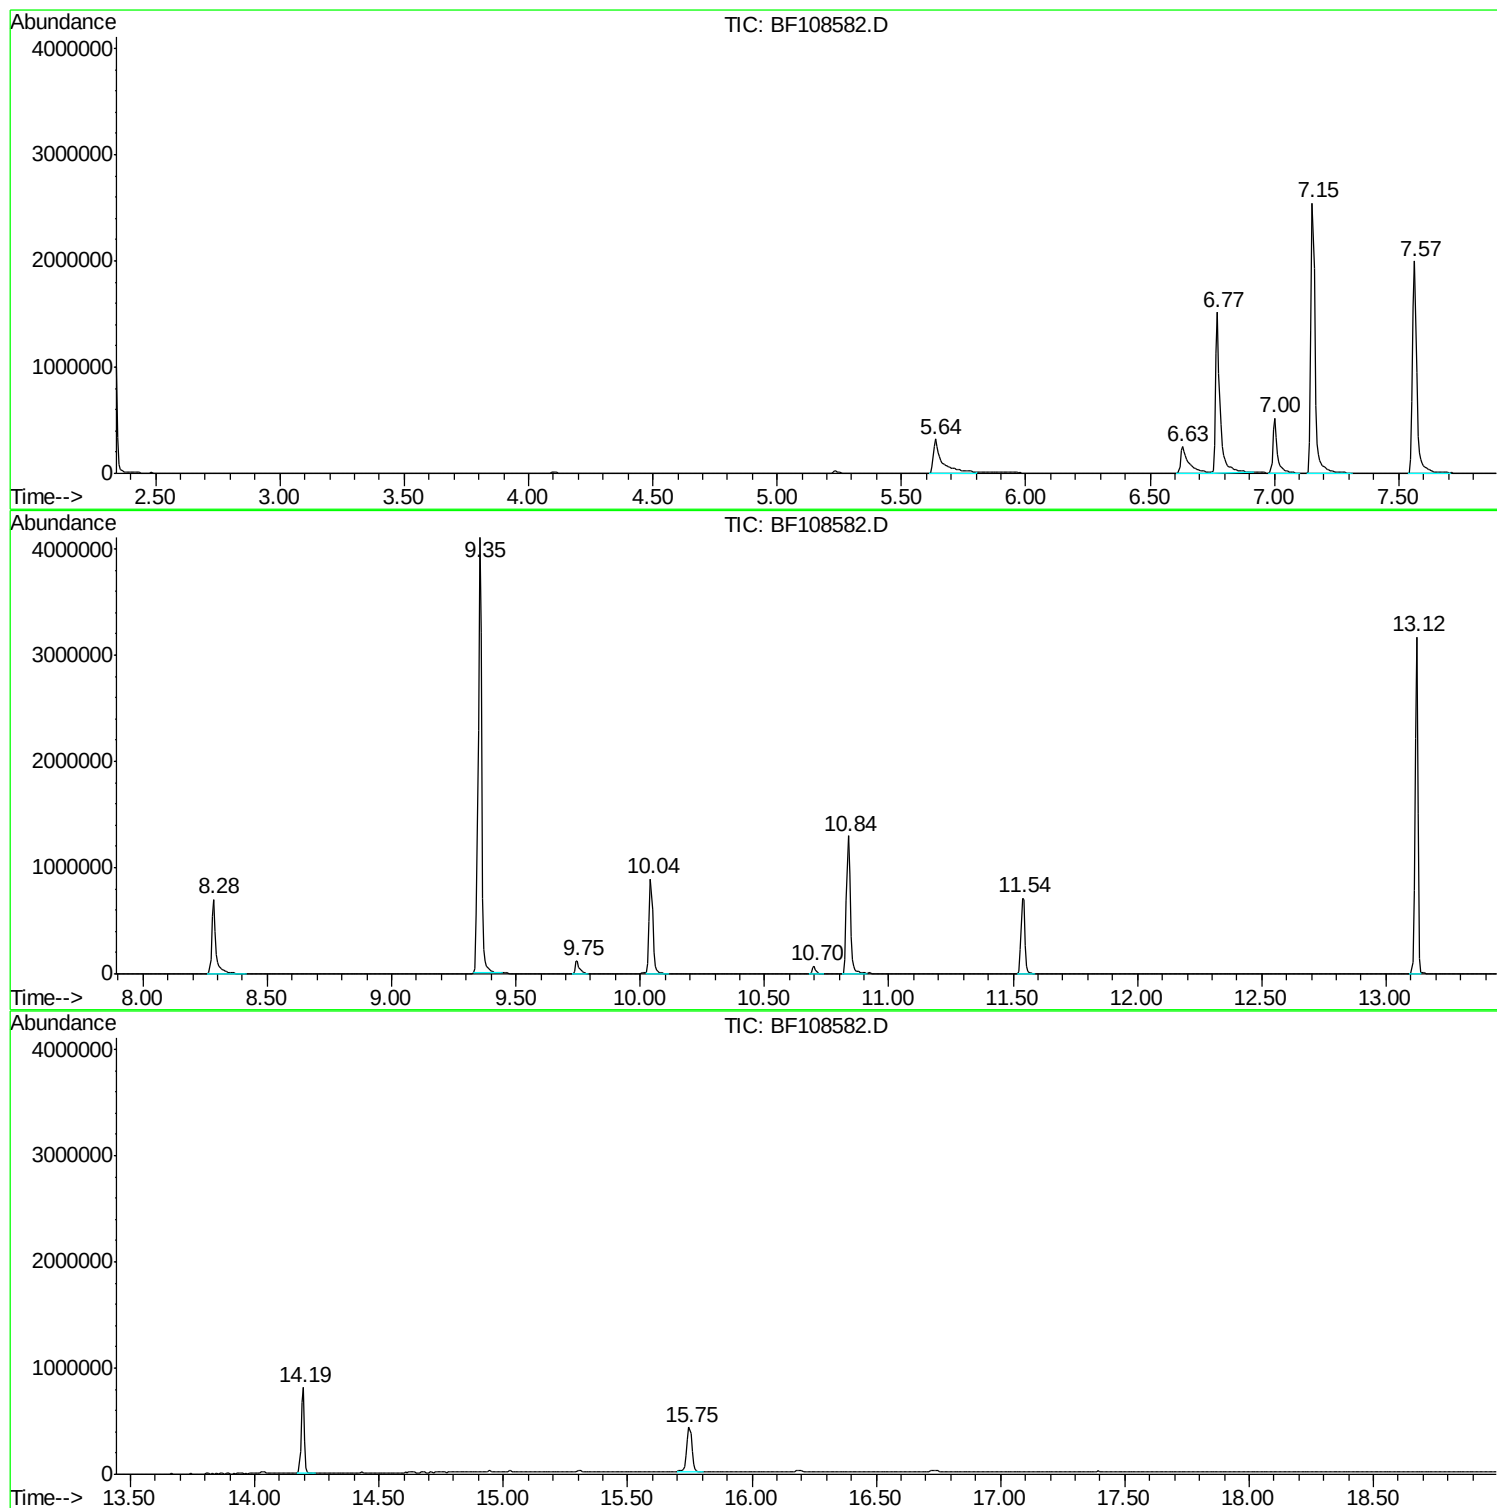

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108582.D
Acq On : 29 Aug 2018 3:49
Operator : JU/SJ
Sample : J4656-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-U-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	55.84 ng	1877580	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
4		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9
5		Xenon	132	Xe	007440-63-3	9

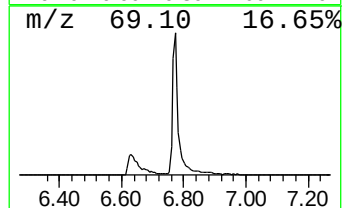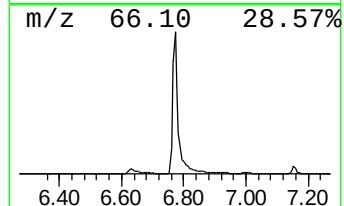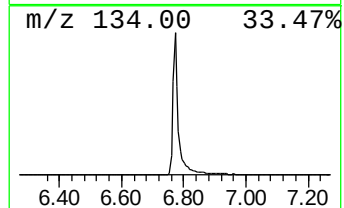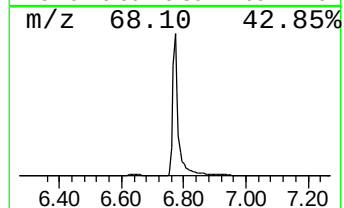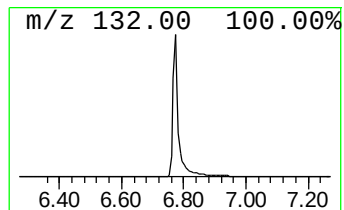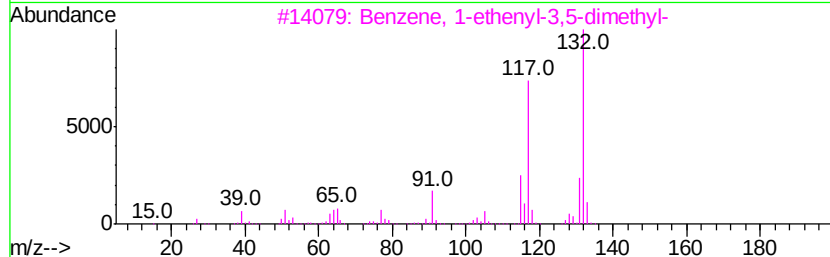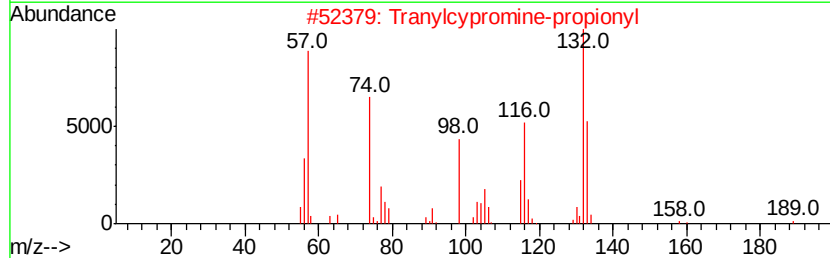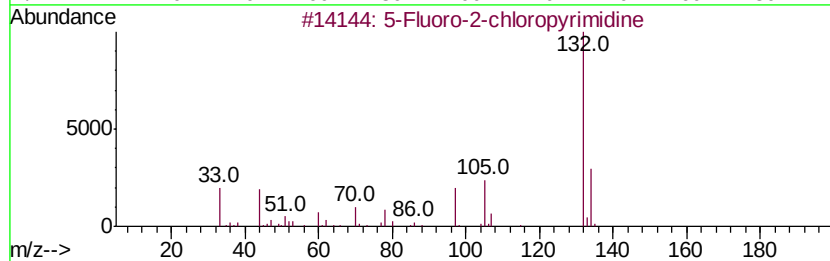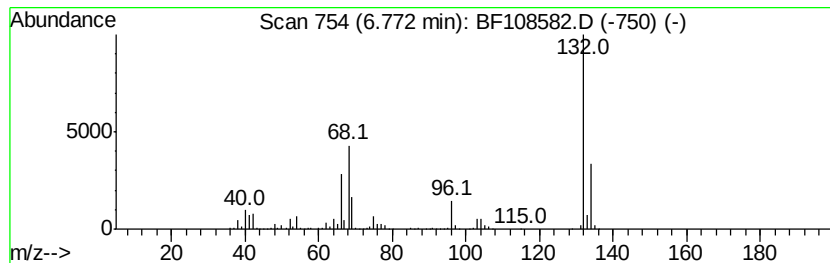

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108582.D
Acq On : 29 Aug 2018 3:49
Operator : JU/SJ
Sample : J4656-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-U-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.77	6.77	55.8	ng	1877580	1	7.00	672461	20.0