

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
 Data File : BF108583.D
 Acq On : 29 Aug 2018 4:16
 Operator : JU/SJ
 Sample : J4656-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082418-SIDI-F-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.237	489	493	504	rBV	21118	36834	1.01%	0.189%
2	5.637	558	561	590	rBV	270183	716537	19.63%	3.667%
3	6.631	726	730	750	rBV	210897	518899	14.22%	2.656%
4	6.772	750	754	778	rVB	1271459	1659285	45.46%	8.492%
5	7.001	789	793	810	rVB	503927	635501	17.41%	3.252%
6	7.154	815	819	847	rBV	2344874	2474705	67.80%	12.665%
7	7.566	884	889	909	rBV	1674181	2074833	56.85%	10.618%
8	8.284	1007	1011	1028	rBV	660927	796455	21.82%	4.076%
9	9.354	1189	1193	1207	rVB	3785189	3649770	100.00%	18.678%
10	9.742	1256	1259	1273	rBV	116518	142202	3.90%	0.728%
11	10.042	1307	1310	1323	rVB	858204	835380	22.89%	4.275%
12	10.701	1418	1422	1429	rBV	49680	48279	1.32%	0.247%
13	10.836	1441	1445	1466	rBV	1160494	1218068	33.37%	6.234%
14	11.536	1561	1564	1574	rBV	702754	724491	19.85%	3.708%
15	13.124	1829	1834	1837	rBV	2982916	2694131	73.82%	13.788%
16	14.189	2012	2015	2026	rBV	752681	738487	20.23%	3.779%
17	15.748	2275	2280	2290	rVB	416350	576351	15.79%	2.950%


Sum of corrected areas: 19540208

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108583.D
Acq On : 29 Aug 2018 4:16
Operator : JU/SJ
Sample : J4656-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

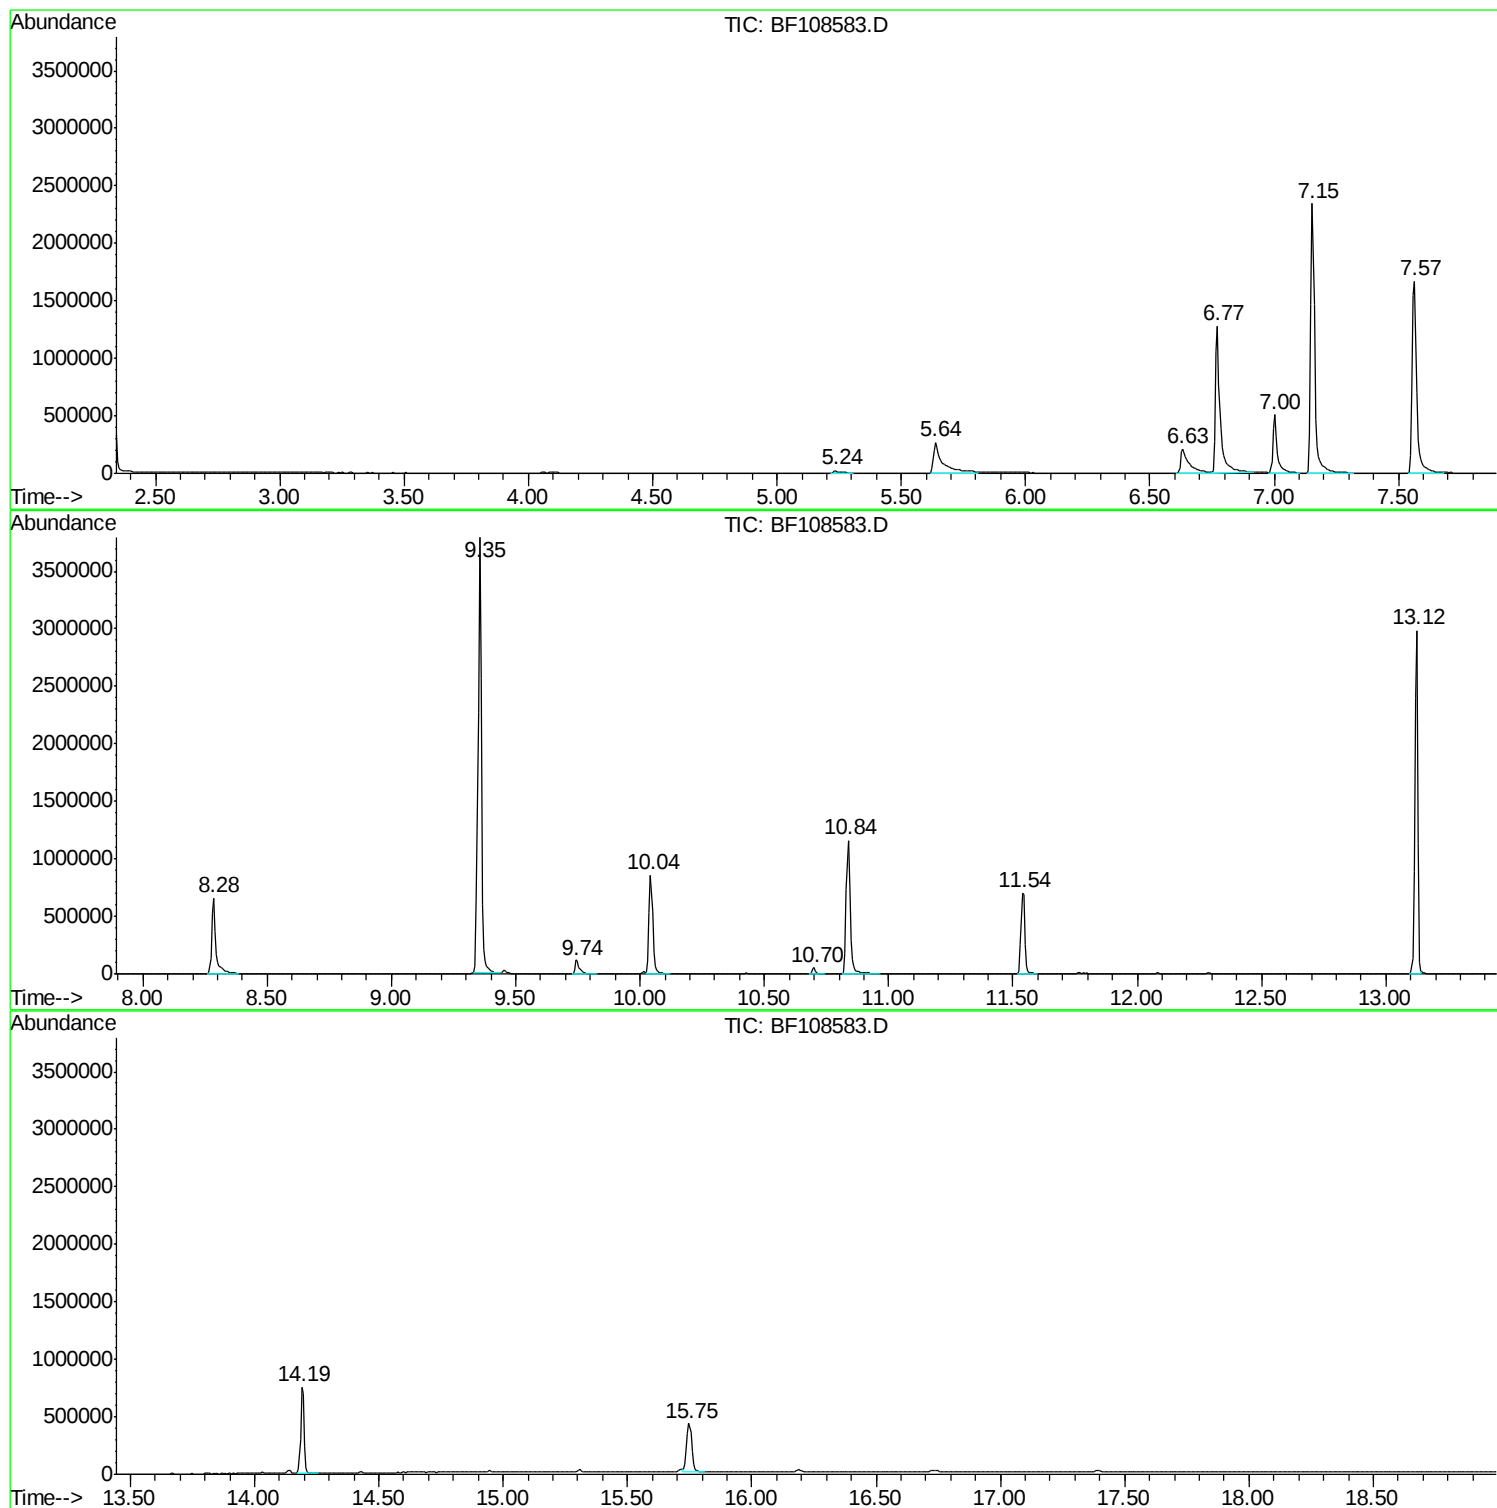

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082818\
Data File : BF108583.D
Acq On : 29 Aug 2018 4:16
Operator : JU/SJ
Sample : J4656-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-U-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	52.22 ng	1659290	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranvlcypramine-propionyl	189	C12H15NO	1000123-86-3	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

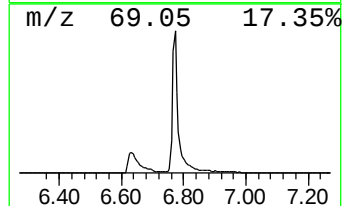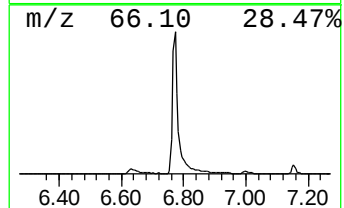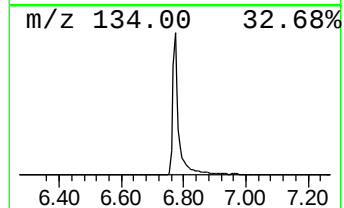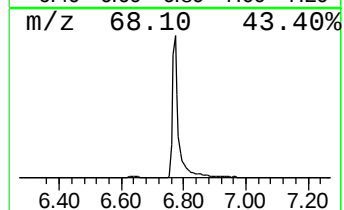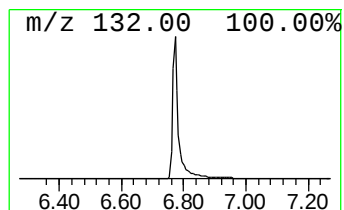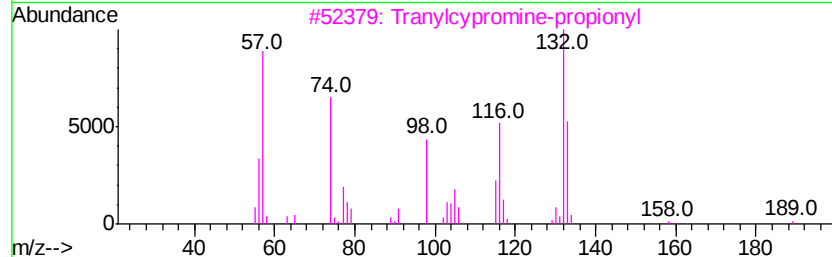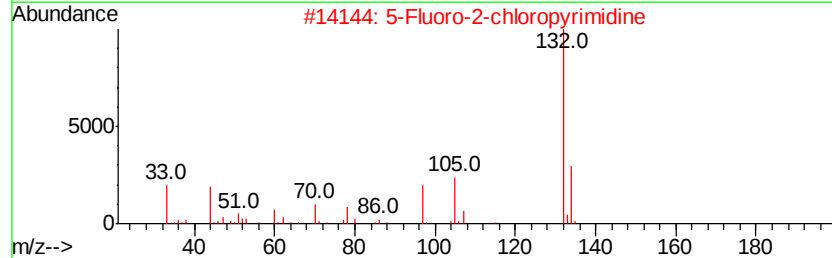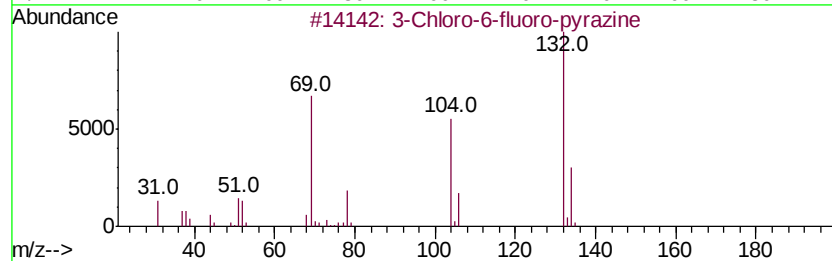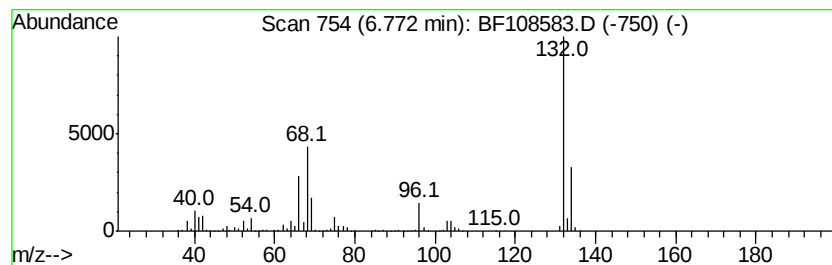

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082818\
Data File : BF108583.D
Acq On : 29 Aug 2018 4:16
Operator : JU/SJ
Sample : J4656-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082418-SIDI-F-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	52.2	ng	1659290	1	7.00	635501	20.0