


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082818\
 Data File : BF108551.D
 Acq On : 28 Aug 2018 12:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

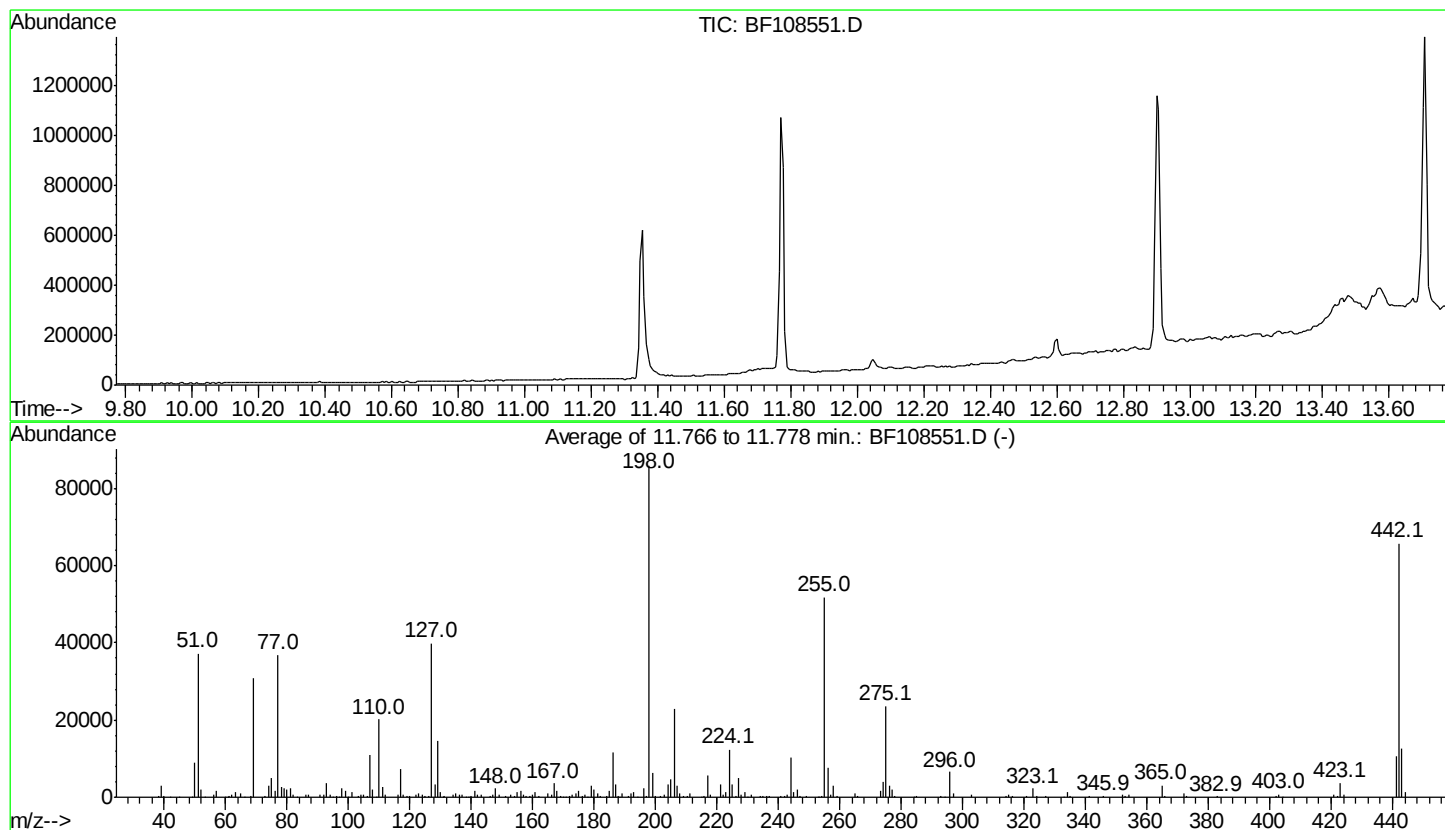

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	37306	PASS
68	69	0.00	2	1.6	504	PASS
69	198	0.00	100	35.8	30726	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	39931	PASS
197	198	0.00	2	0.5	460	PASS
198	198	100	100	100.0	85922	PASS
199	198	5	9	7.2	6204	PASS
275	198	10	60	27.4	23584	PASS
365	198	1	100	3.5	2996	PASS
441	198	0.01	100	12.5	10711	PASS
442	198	50	100	76.6	65792	PASS
443	442	15	24	19.1	12543	PASS