
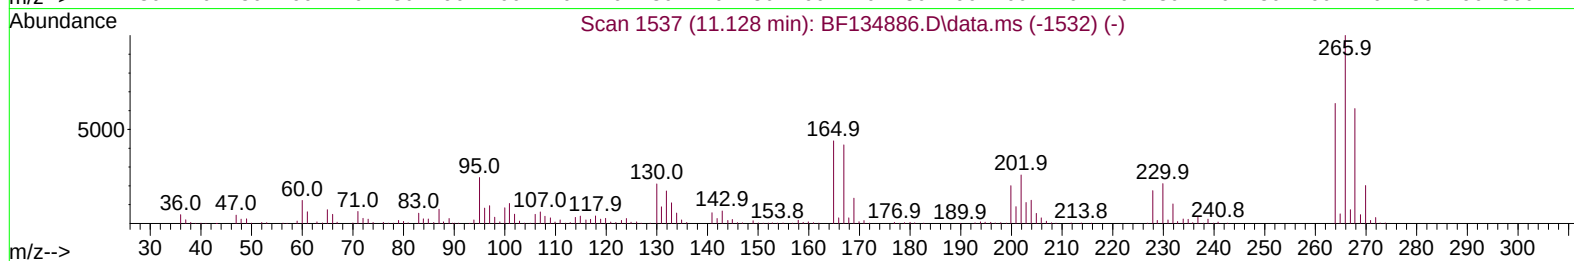
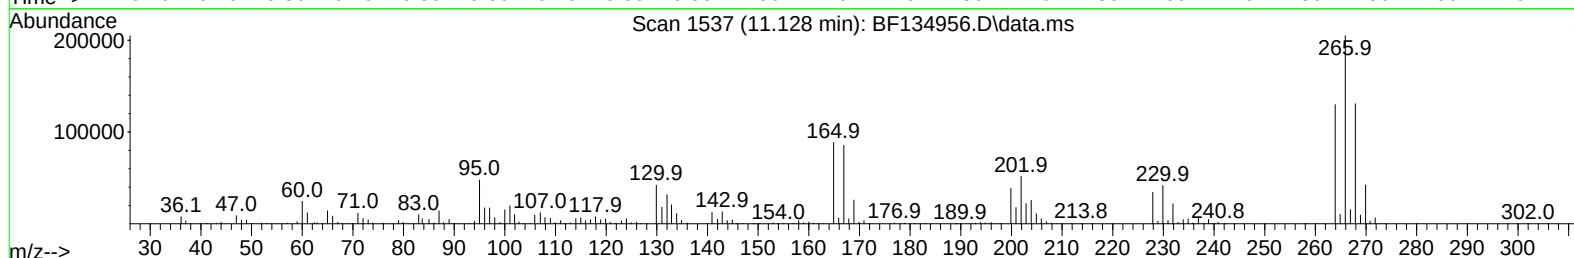


Quant Time: Aug 29 06:07:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 02:45:19 2023
Response via : Initial Calibration

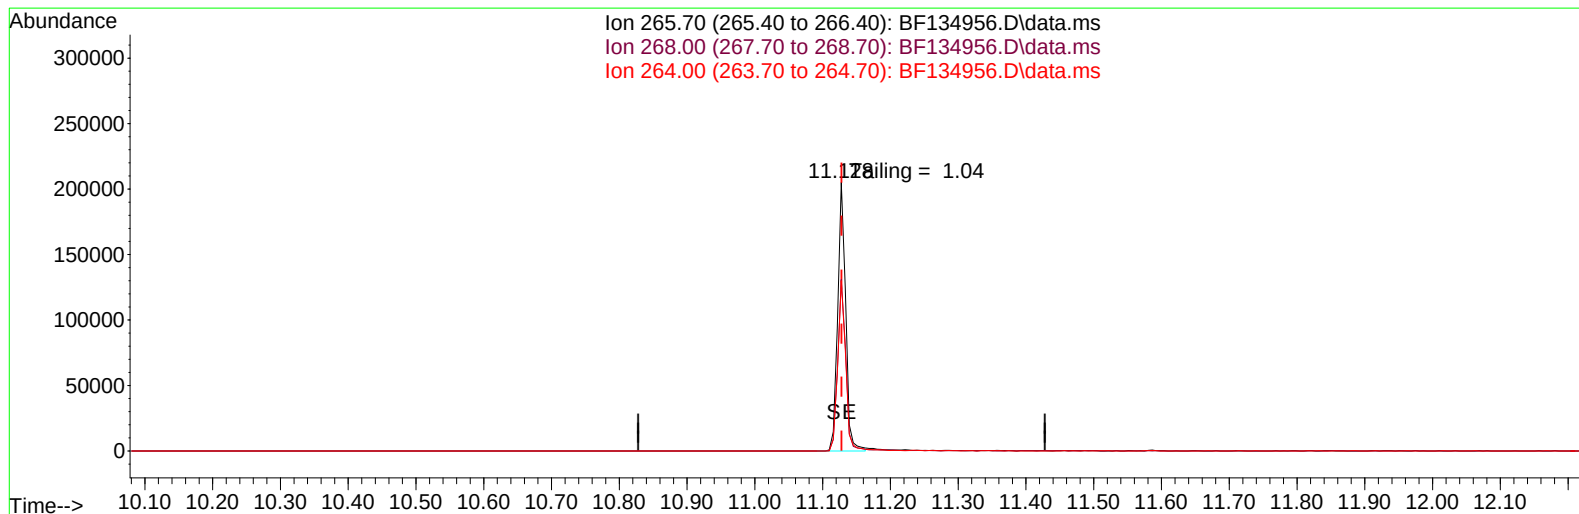

TIC: BF134956.D\data.ms

(70) Pentachlorophenol (C)




11.128min (-0.000) 412887.58 ng

response **170735**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.81
264.00	63.80	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082823\
Data File : BF134956.D
Acq On : 28 Aug 2023 08:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 06:07:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 02:45:19 2023
Response via : Initial Calibration

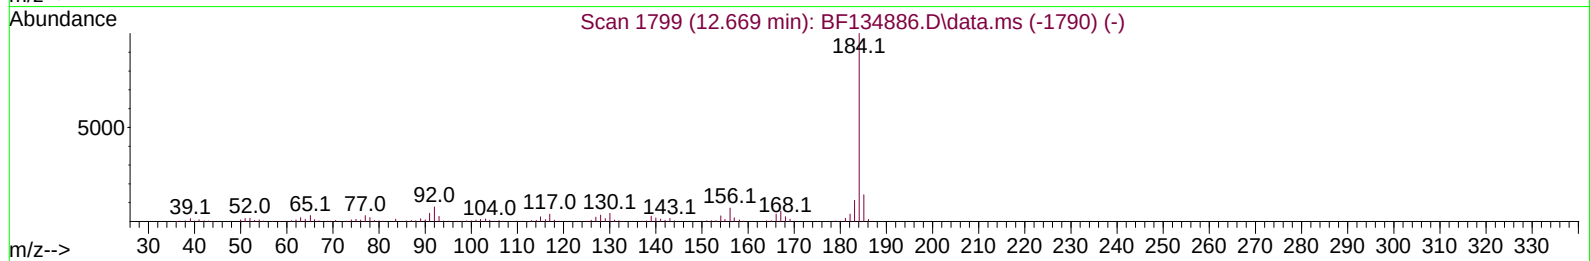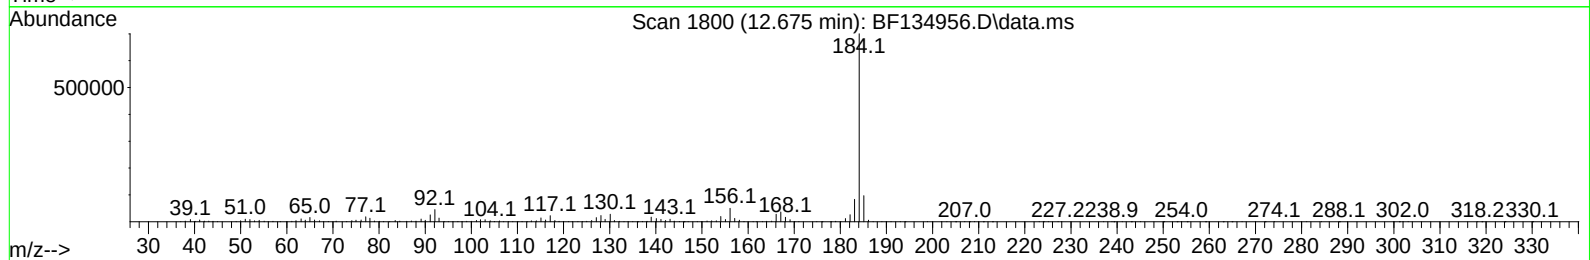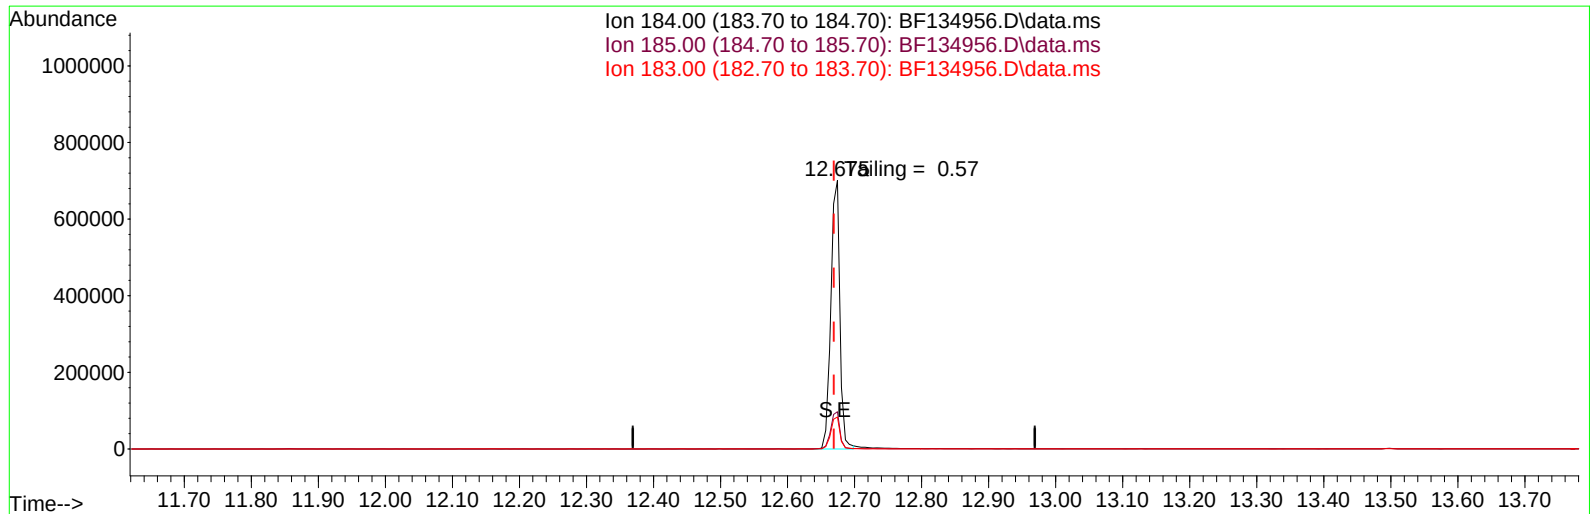

TIC: BF134956.D\data.ms

(77) Benzidine

12.675min (+ 0.005) 45574.52 ng

response 667714

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.86
183.00	11.20	11.92
0.00	0.00	0.00