

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082823\
 Data File : BF134958.D
 Acq On : 28 Aug 2023 09:28
 Operator : CG\JU
 Sample : PB155019BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155019BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.110	3	4	9	rVB	52202	46242	1.03%	0.167%
2	5.434	564	569	572	rBV	3630316	3751498	83.29%	13.589%
3	6.434	733	739	742	rBV	3157929	3833656	85.11%	13.886%
4	6.792	796	800	803	rBV	976943	758766	16.85%	2.748%
5	7.357	890	896	899	rBV	2468331	2485835	55.19%	9.004%
6	8.069	1013	1017	1021	rBV	1091335	1028044	22.82%	3.724%
7	9.151	1195	1201	1204	rBV	4586342	4504364	100.00%	16.316%
8	9.828	1311	1316	1320	rBV	1401520	1179107	26.18%	4.271%
9	10.627	1445	1452	1455	rBV	3173417	2975079	66.05%	10.776%
10	11.322	1566	1570	1574	rBV	1438343	1210866	26.88%	4.386%
11	12.921	1837	1842	1846	rBV	4224255	4350676	96.59%	15.759%
12	13.980	2018	2022	2025	rBV	751310	720170	15.99%	2.609%
13	15.457	2267	2273	2284	rVB	585455	763351	16.95%	2.765%




Sum of corrected areas: 27607654

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082823\
Data File : BF134958.D
Acq On : 28 Aug 2023 09:28
Operator : CG\JU
Sample : PB155019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155019BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

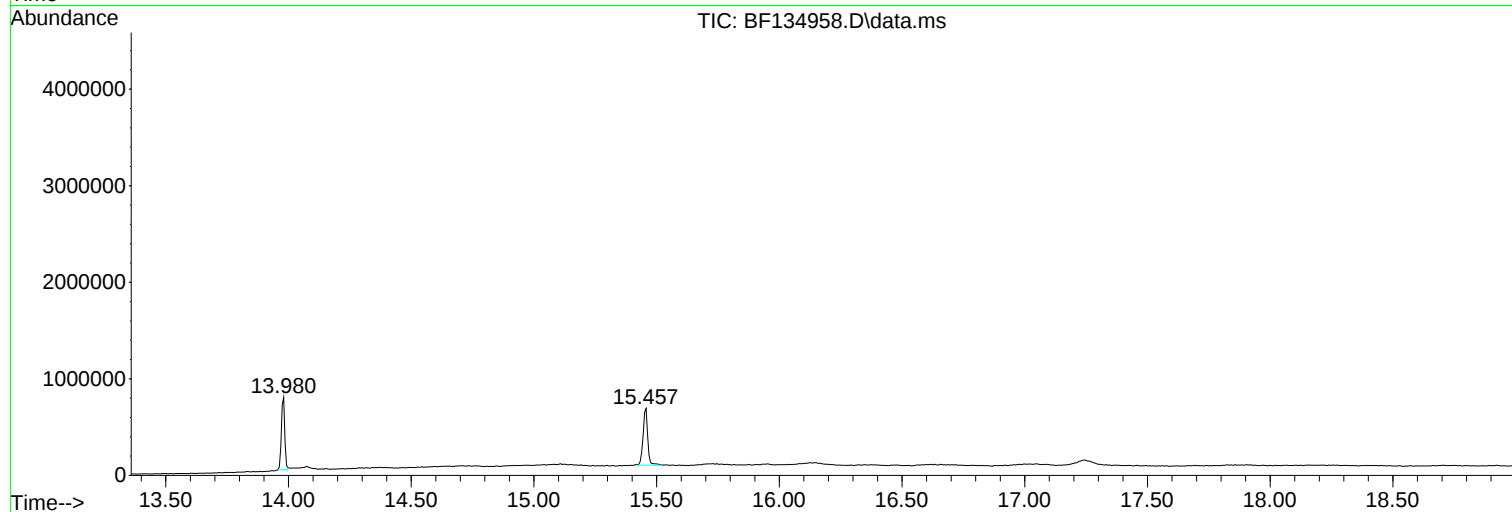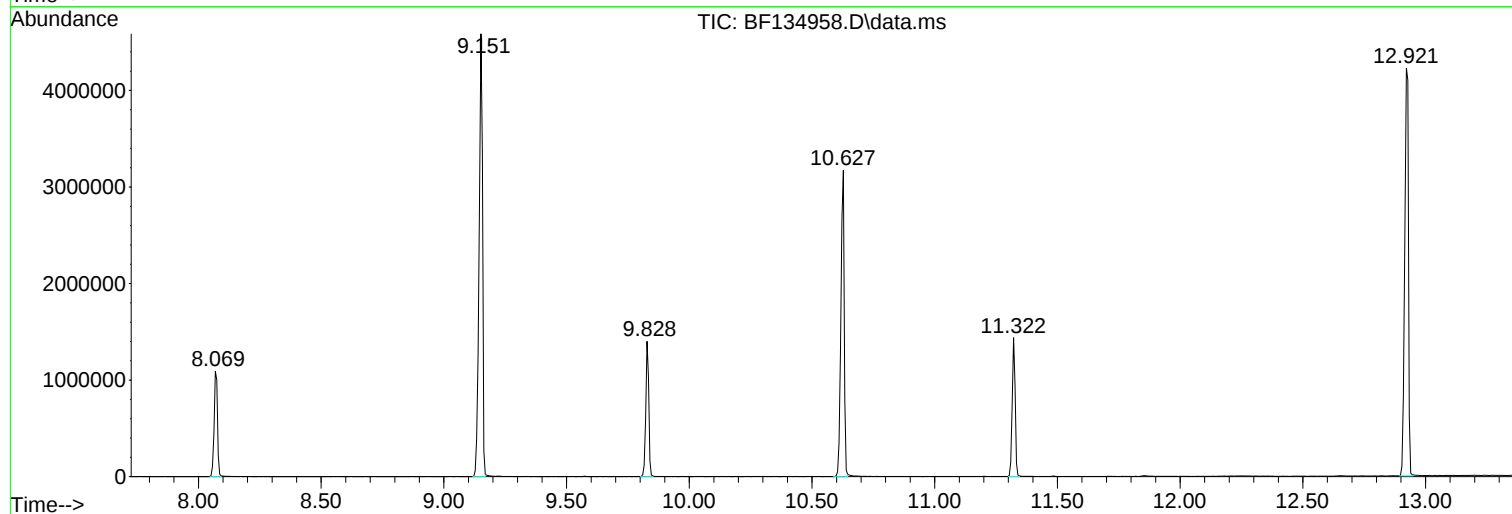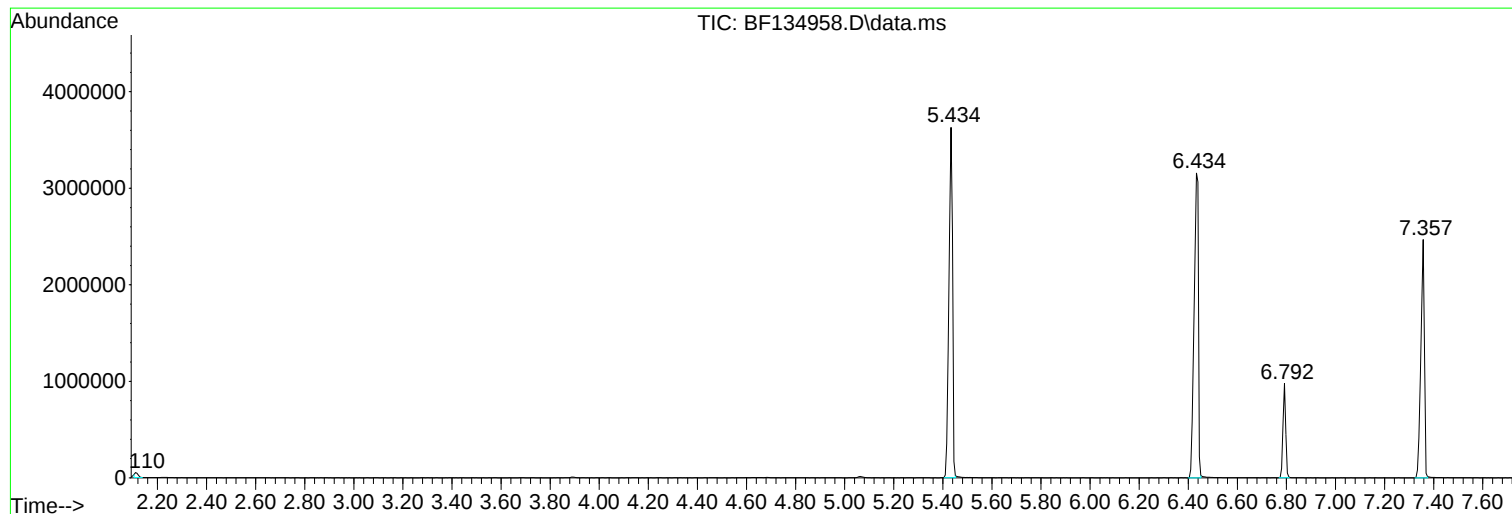

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082823\
Data File : BF134958.D
Acq On : 28 Aug 2023 09:28
Operator : CG\JU
Sample : PB155019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155019BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082823\
Data File : BF134958.D
Acq On : 28 Aug 2023 09:28
Operator : CG\JU
Sample : PB155019BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155019BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------