


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082823\
Data File : BF134956.D
Acq On : 28 Aug 2023 08:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 28 02:45:19 2023

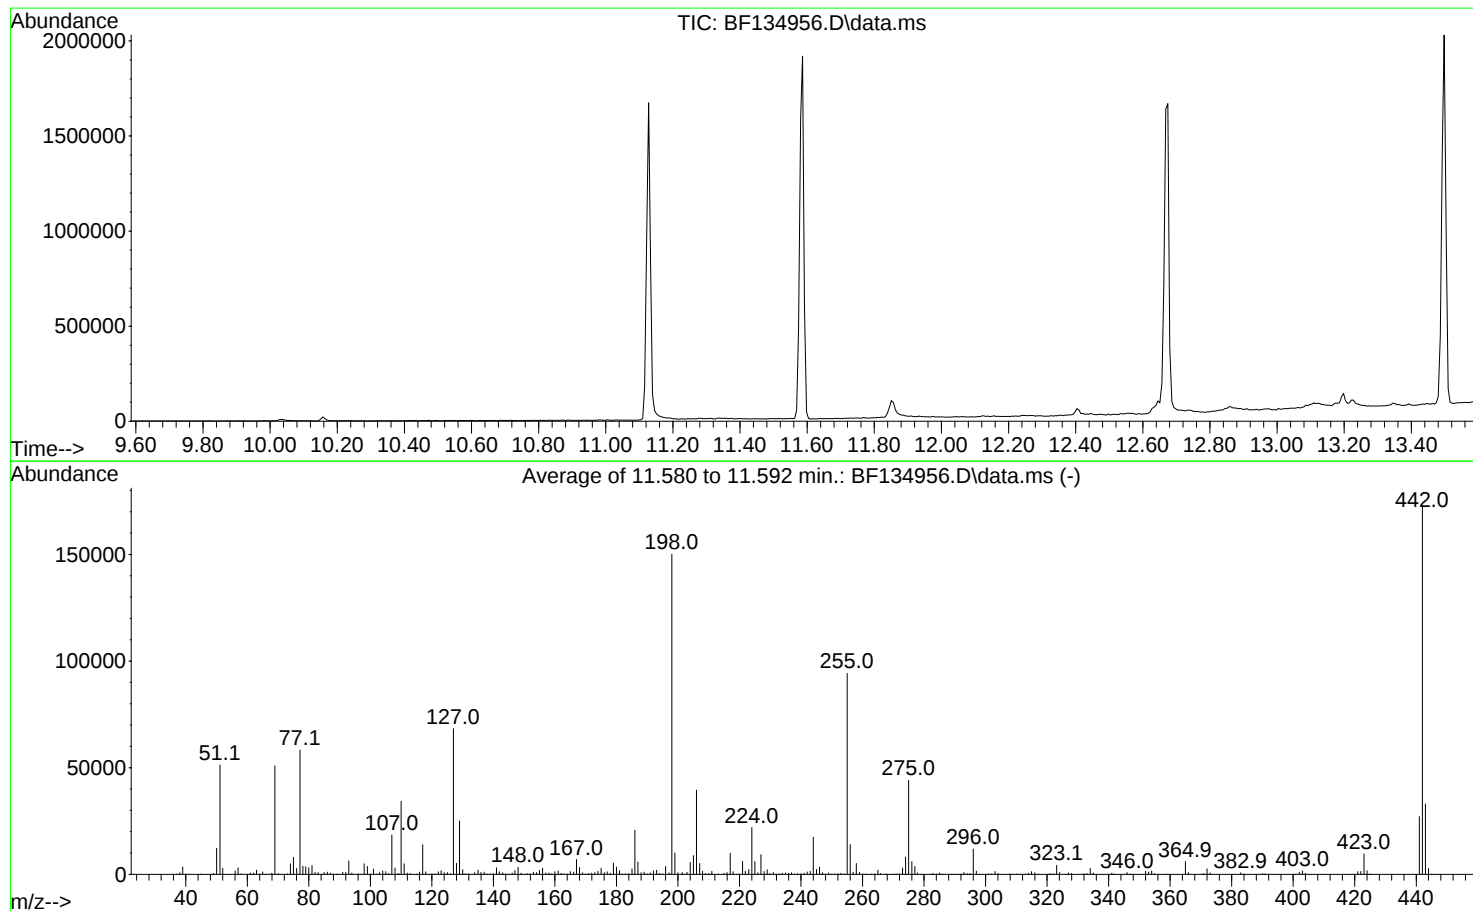




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	51335	PASS
68	69	0.00	2	0.9	476	PASS
69	198	0.00	100	33.9	50861	PASS
70	69	0.00	2	0.7	361	PASS
127	198	10	80	45.5	68341	PASS
197	198	0.00	2	0.4	670	PASS
198	198	100	100	100.0	150088	PASS
199	198	5	9	6.7	9984	PASS
275	198	10	60	29.4	44077	PASS
365	198	1	100	4.0	5976	PASS
441	198	0.01	100	18.1	27091	PASS
442	442	50	100	100.0	172483	PASS
443	442	15	24	19.1	32989	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082823\
Data File : BF134956.D
Acq On : 28 Aug 2023 08:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 29 06:07:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 02:45:19 2023
Response via : Initial Calibration

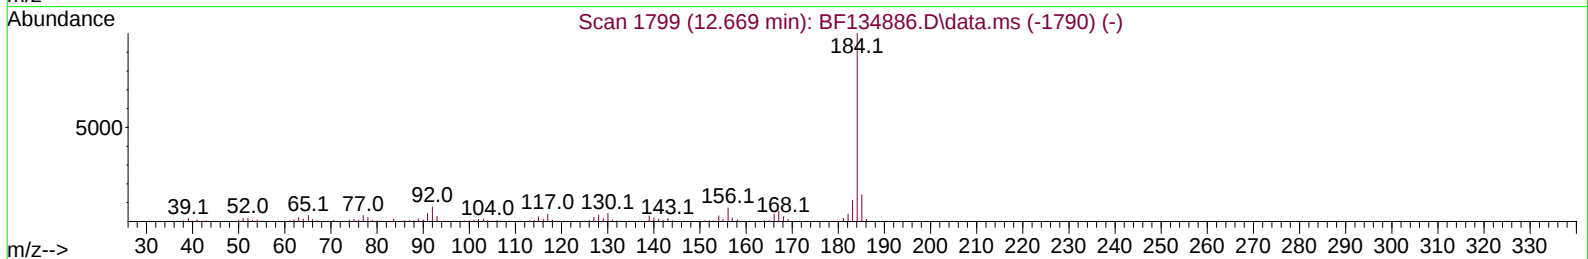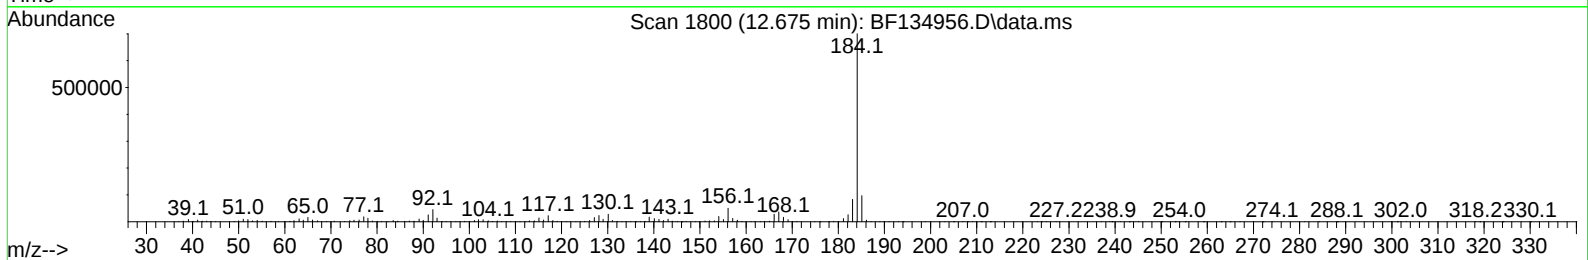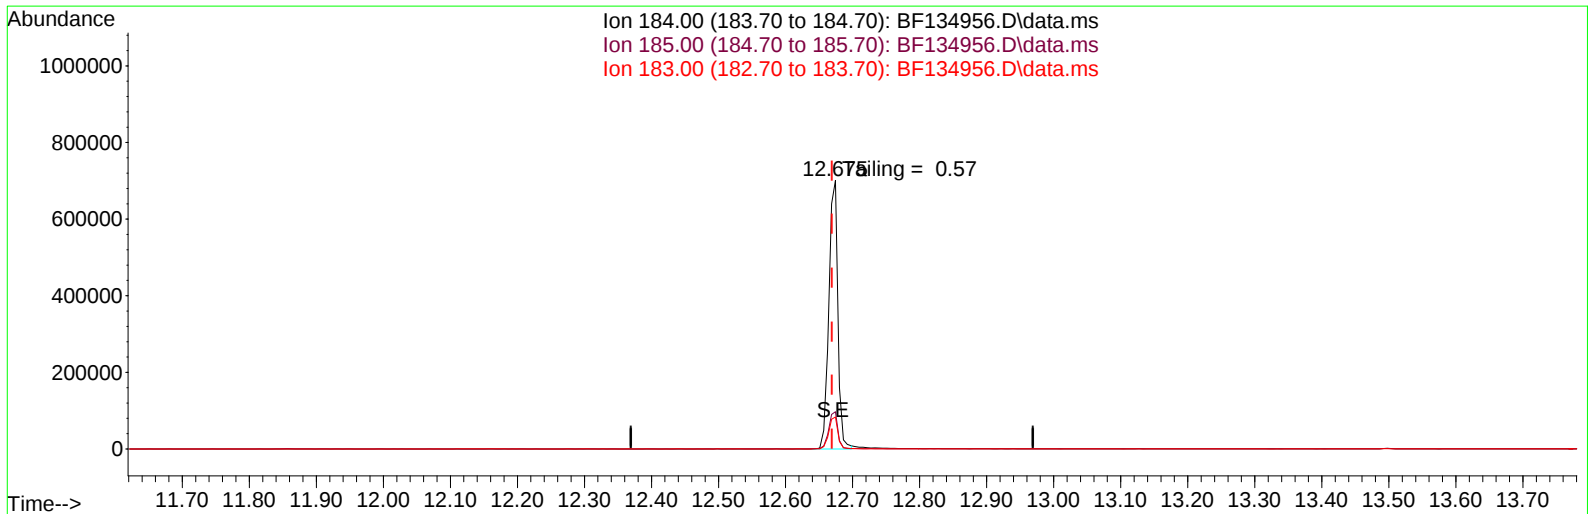

TIC: BF134956.D\data.ms

(77) Benzidine

12.675min (+ 0.005) 45574.52 ng

response 667714

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.86
183.00	11.20	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/28/2023	BNA_F	<u>BF134956.D</u>
Compound Name	Response	Retention Time
DDT	335487	13.498
DDD	16398	13.198
DDE	4201	11.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20599	356086	5.78

Instrument :
BNA_F
ClientSampleId :
DFTPP