


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082824\
Data File : BF139198.D
Acq On : 28 Aug 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 27 02:51:47 2024

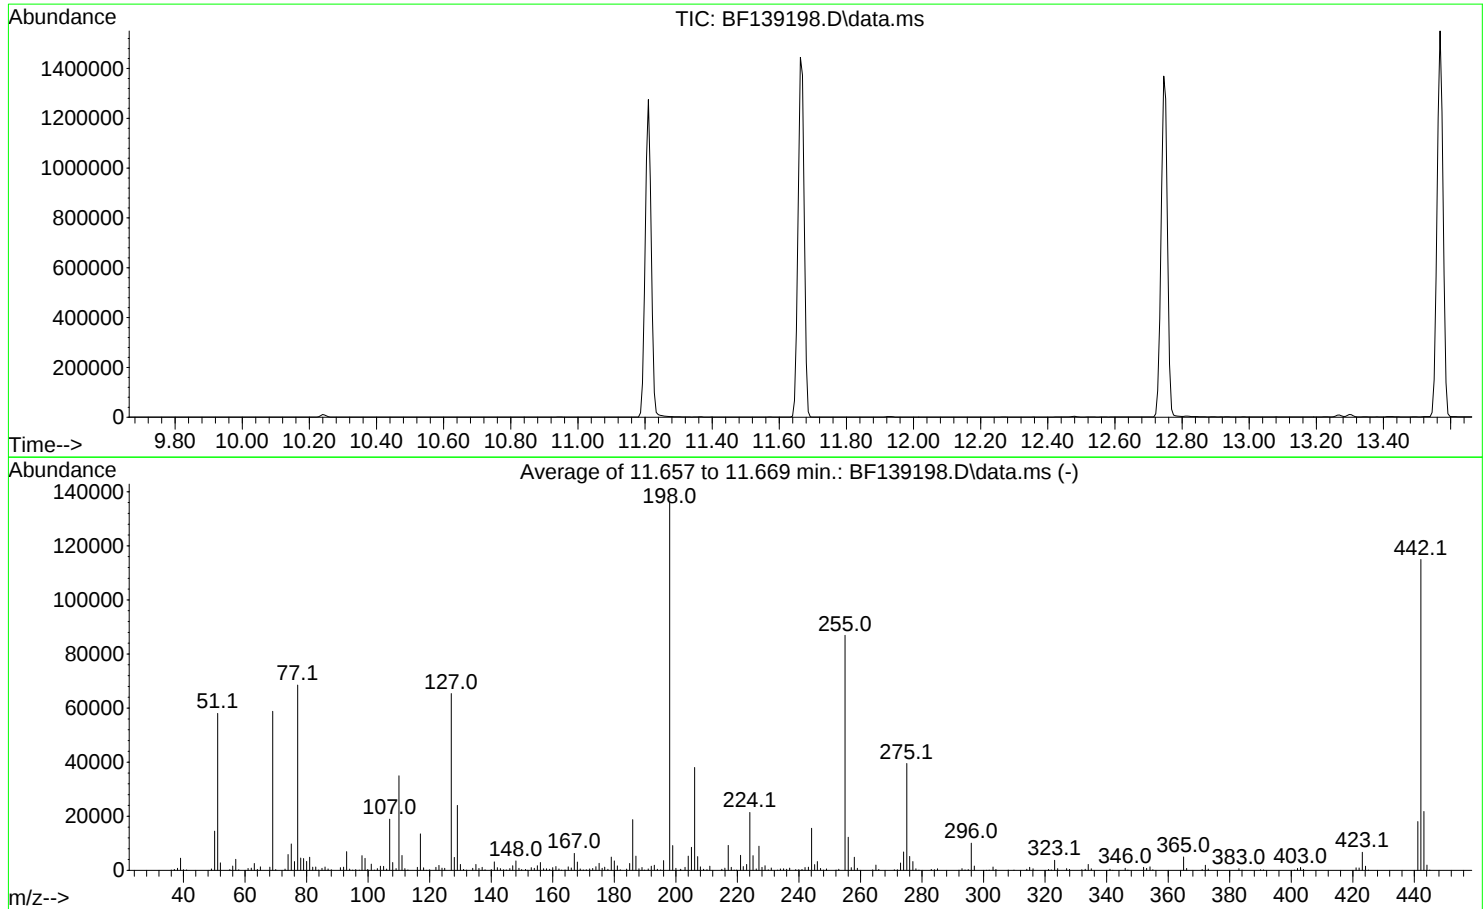

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	58067	PASS
68	69	0.00	2	2.0	1160	PASS
69	198	0.00	100	43.3	58837	PASS
70	69	0.00	2	0.5	283	PASS
127	198	10	80	48.1	65403	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	136027	PASS
199	198	5	9	6.8	9190	PASS
275	198	10	60	29.0	39504	PASS
365	198	1	100	3.7	4975	PASS
441	198	0.01	100	13.3	18032	PASS
442	442	50	100	100.0	114965	PASS
443	442	15	24	18.9	21781	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/28/2024	BNA_F	<u>BF139198.D</u>
Compound Name	Response	Retention Time
DDT	372075	13.569
DDD	5779	13.298
DDE	272	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6051	378126	1.60

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082824\
Data File : BF139198.D
Acq On : 28 Aug 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 28 11:23:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 02:51:47 2024
Response via : Initial Calibration

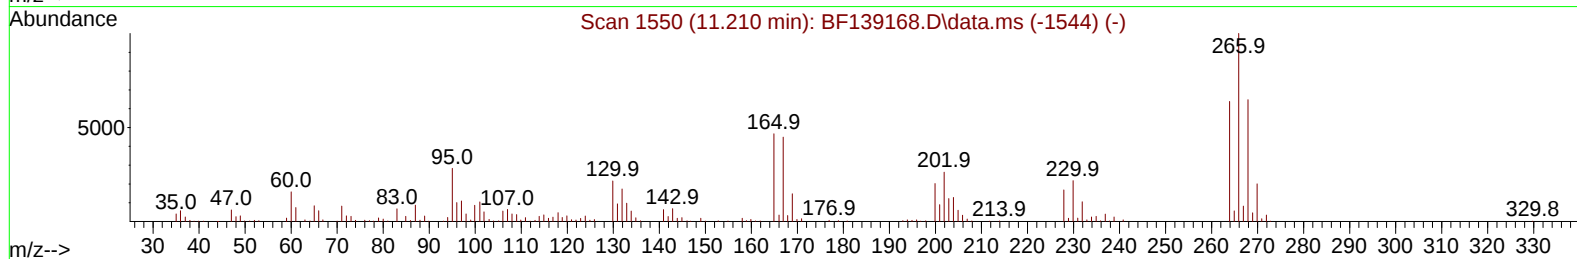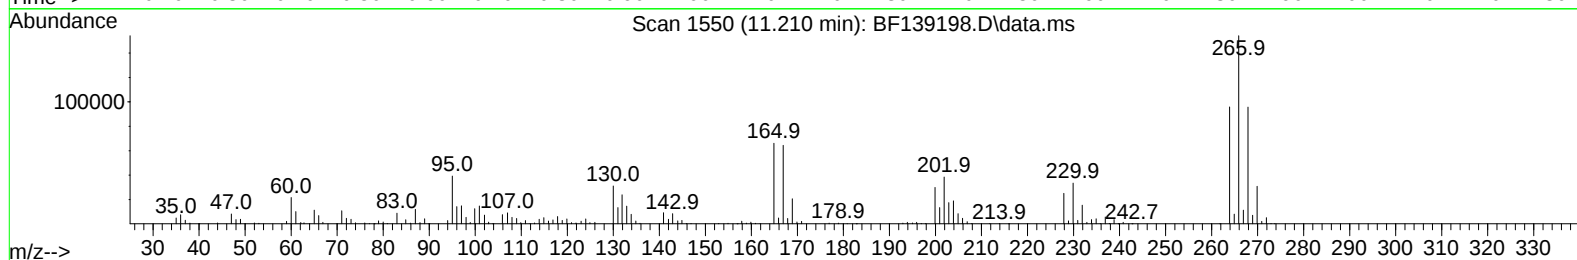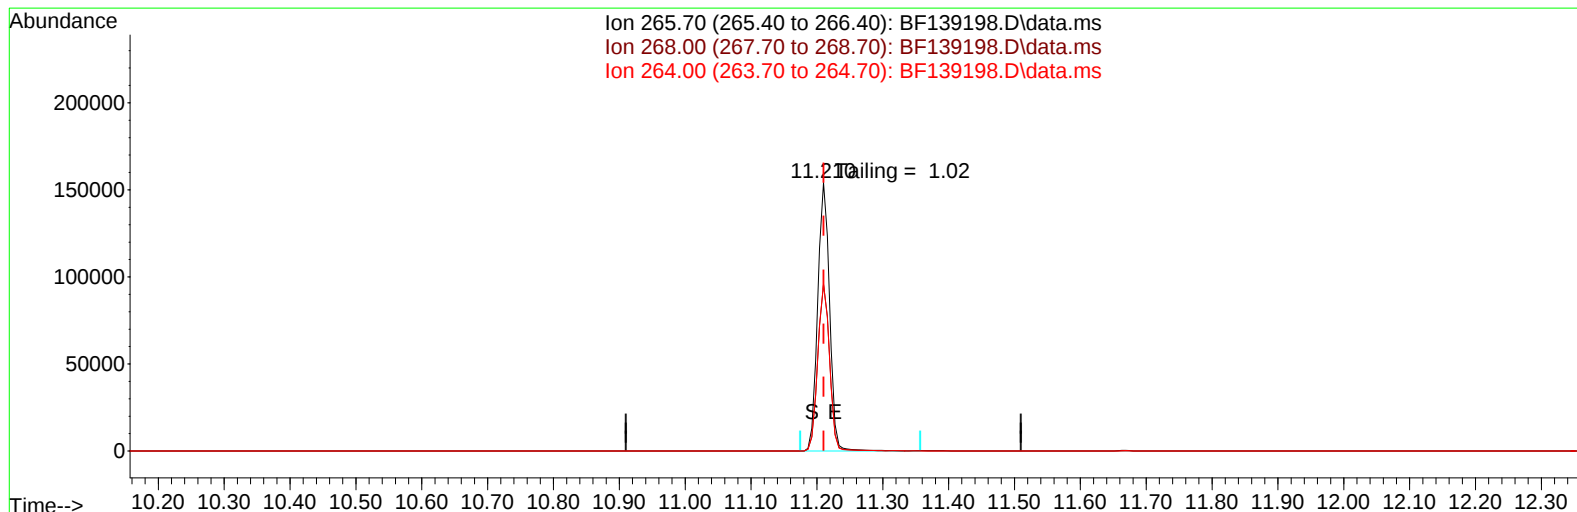

TIC: BF139198.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 34072.93 ng




response 193453

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	62.04
264.00	63.80	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082824\
Data File : BF139198.D
Acq On : 28 Aug 2024 09:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 28 11:23:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 27 02:51:47 2024
Response via : Initial Calibration

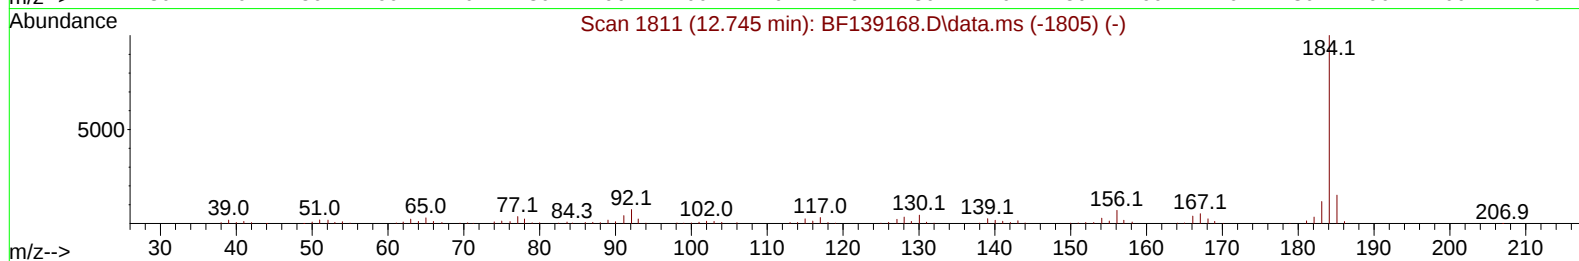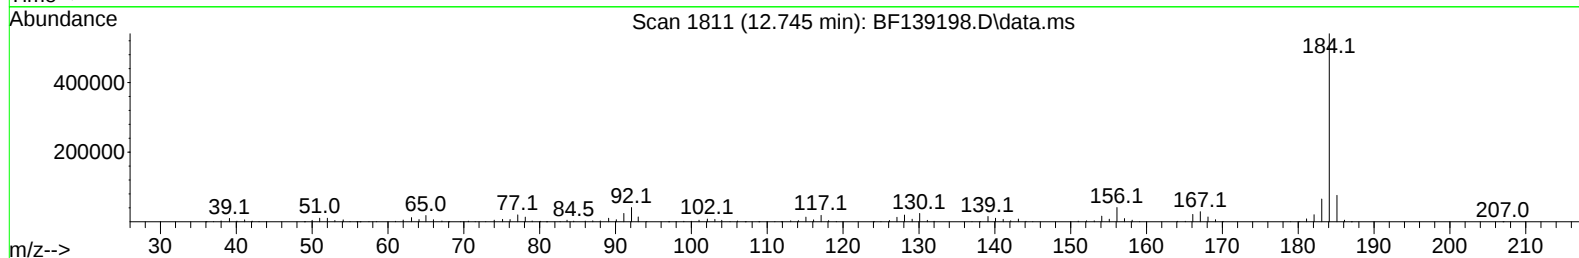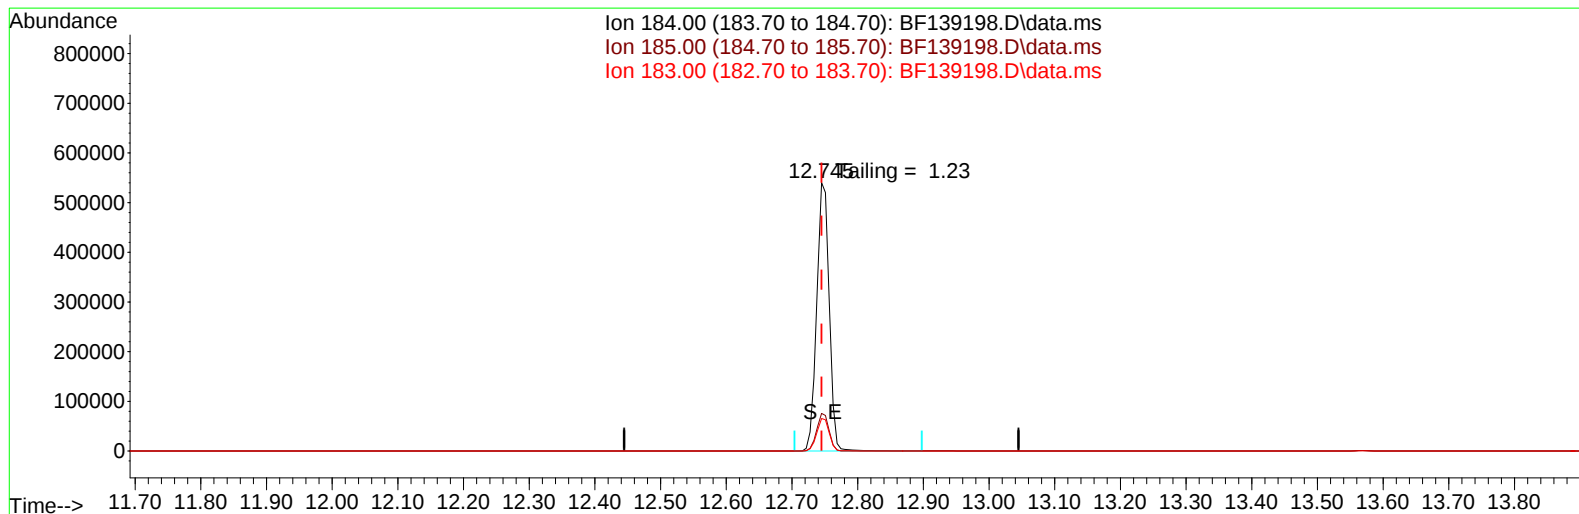

TIC: BF139198.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 0.00 ng

response 719154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.03
183.00	11.70	12.13
0.00	0.00	0.00