
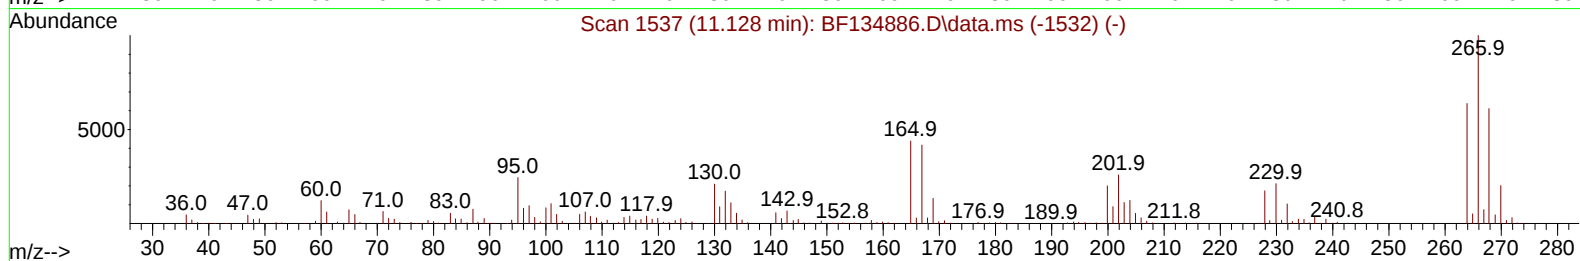
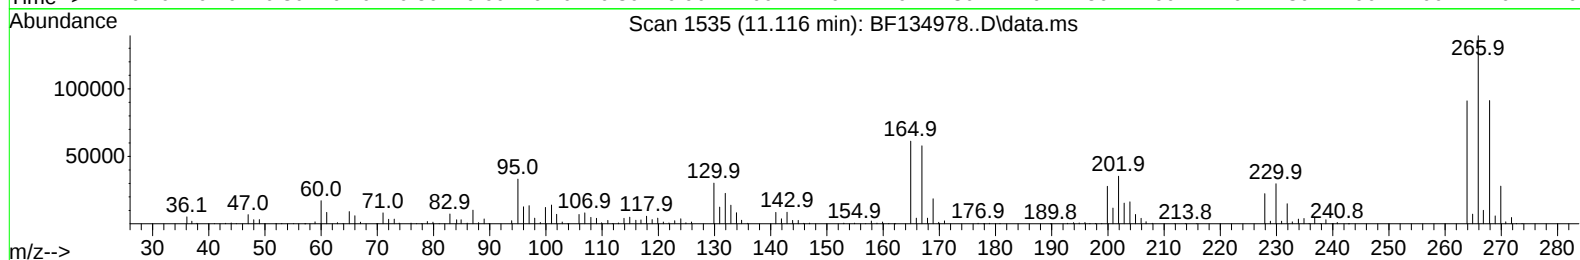


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082923\
Data File : BF134978..D
Acq On : 29 Aug 2023 12:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 13:36:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 02:45:19 2023
Response via : Initial Calibration

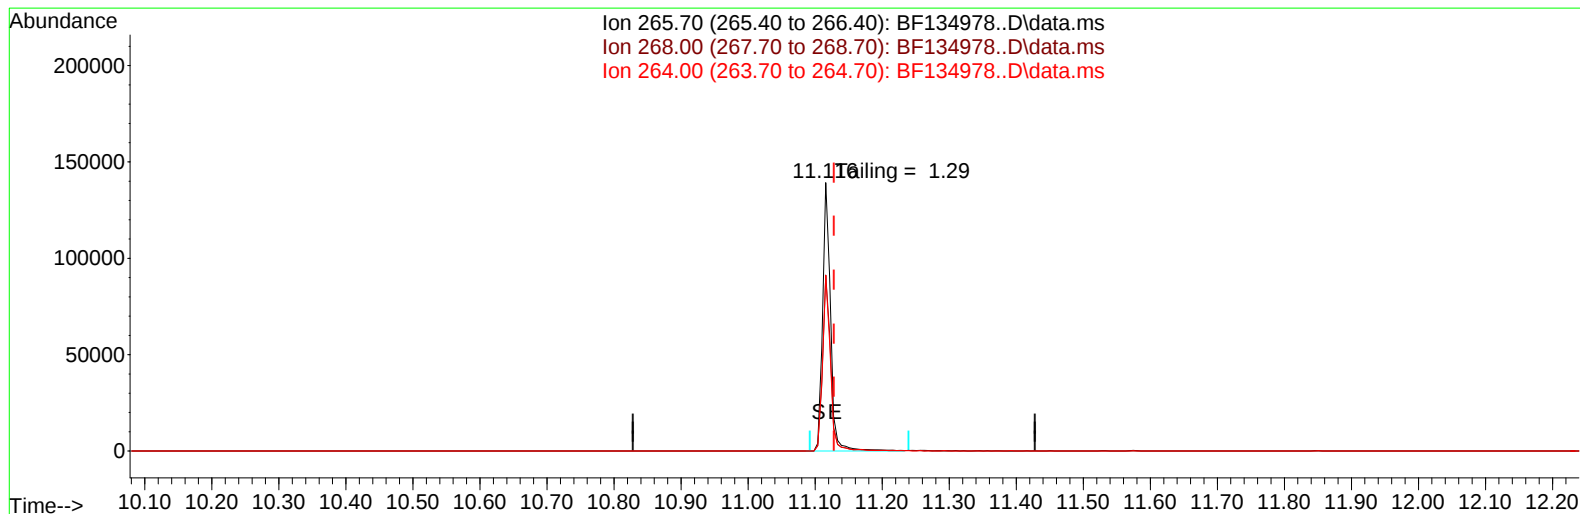

TIC: BF134978..D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.012) 25044.41 ng

response 115213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.58
264.00	63.80	65.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082923\
Data File : BF134978..D
Acq On : 29 Aug 2023 12:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 29 13:36:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 02:45:19 2023
Response via : Initial Calibration

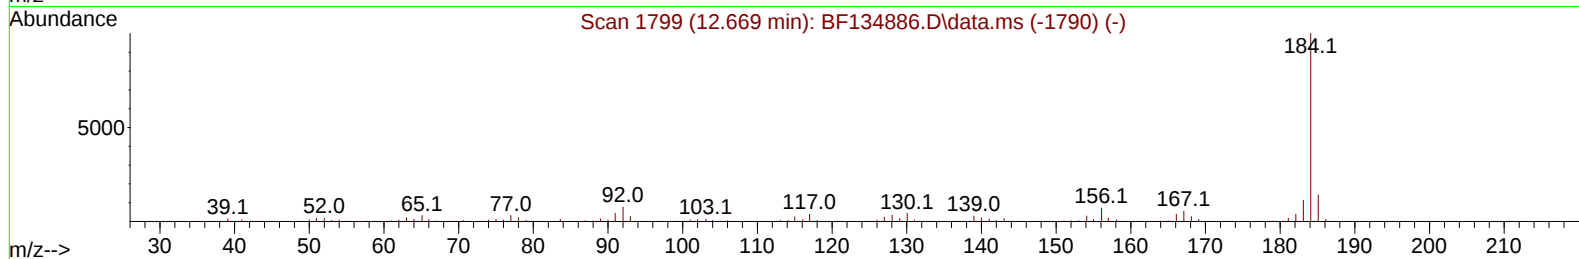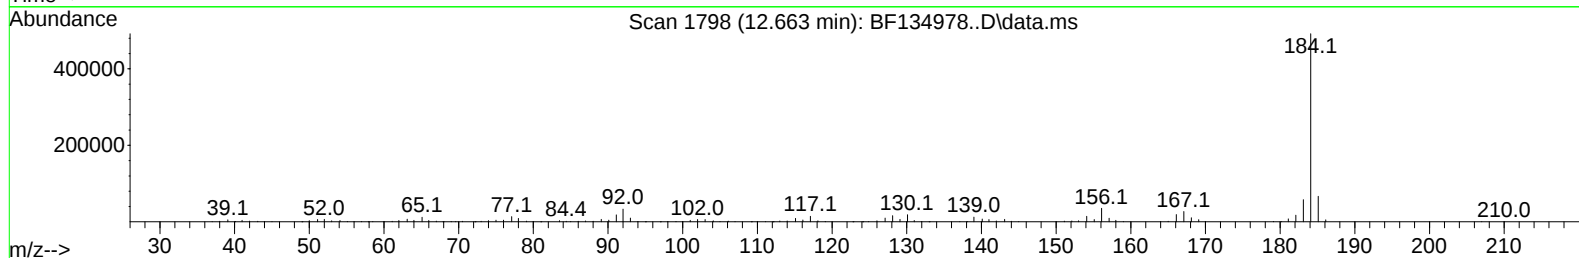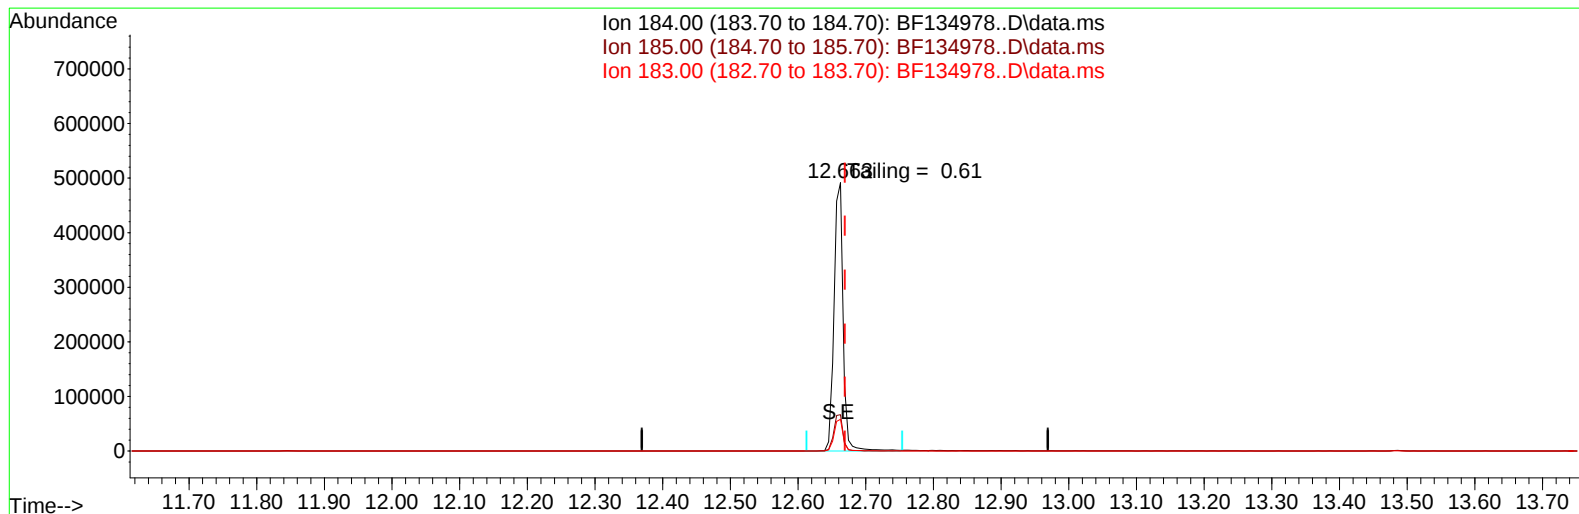

TIC: BF134978..D\data.ms

(77) Benzidine

12.663min (-0.006) 0.00 ng m

response 462723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.56
183.00	11.20	11.81
0.00	0.00	0.00