


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082923\
Data File : BF134978.D
Acq On : 29 Aug 2023 12:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 28 02:45:19 2023

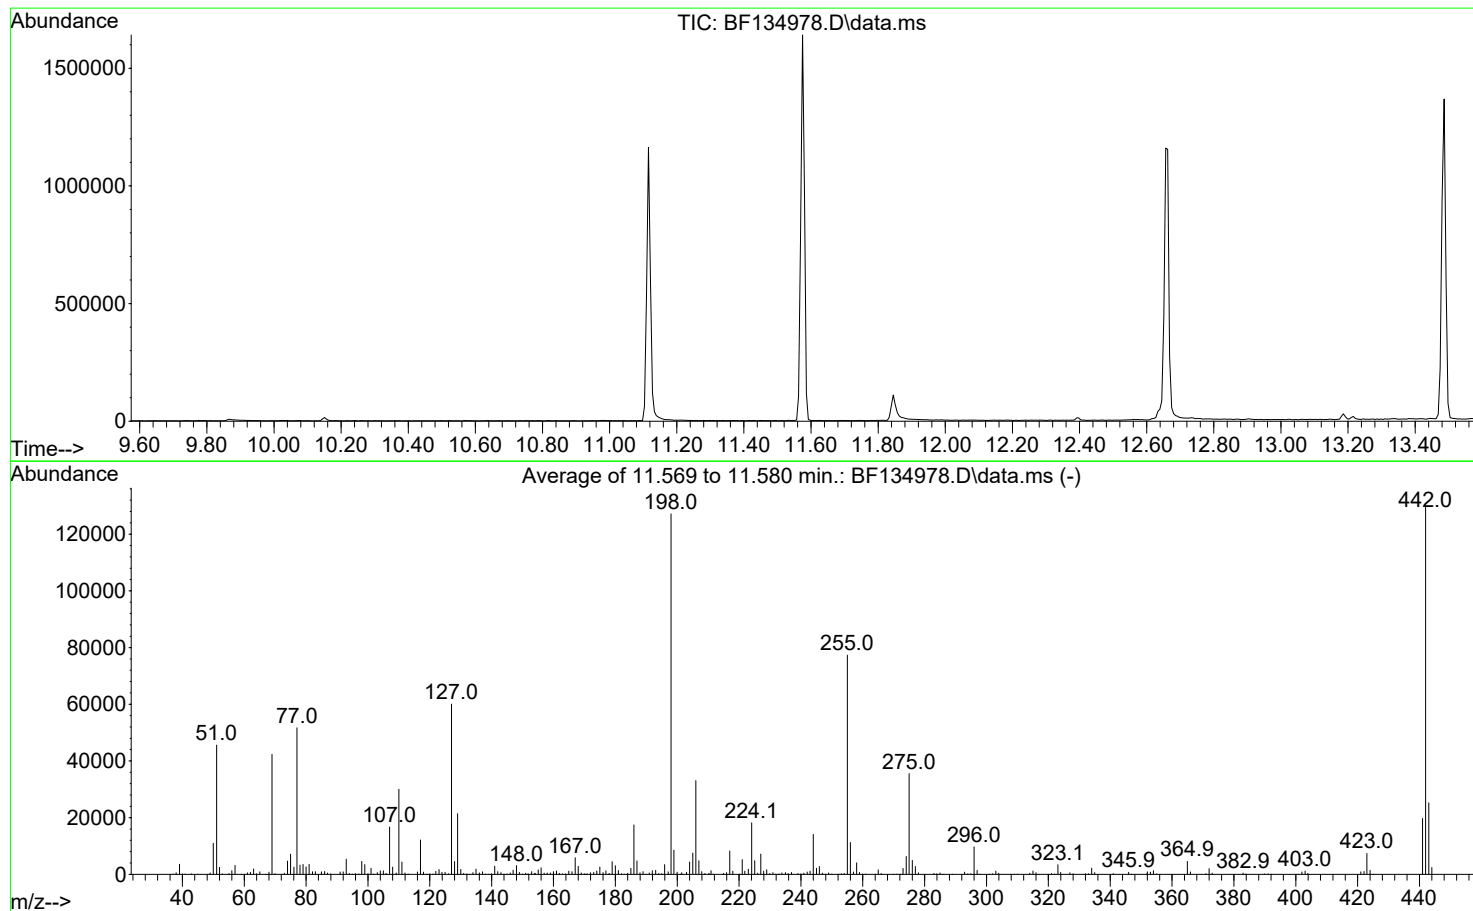




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	45592	PASS
68	69	0.00	2	1.9	807	PASS
69	198	0.00	100	33.3	42364	PASS
70	69	0.00	2	0.5	224	PASS
127	198	10	80	47.2	60045	PASS
197	198	0.00	2	0.7	912	PASS
198	198	100	100	100.0	127157	PASS
199	198	5	9	6.7	8552	PASS
275	198	10	60	28.0	35587	PASS
365	198	1	100	3.6	4605	PASS
441	198	0.01	100	15.5	19728	PASS
442	442	50	100	100.0	129773	PASS
443	442	15	24	19.5	25254	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082923\
Data File : BF134978..D
Acq On : 29 Aug 2023 12:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 29 13:36:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 28 02:45:19 2023
Response via : Initial Calibration

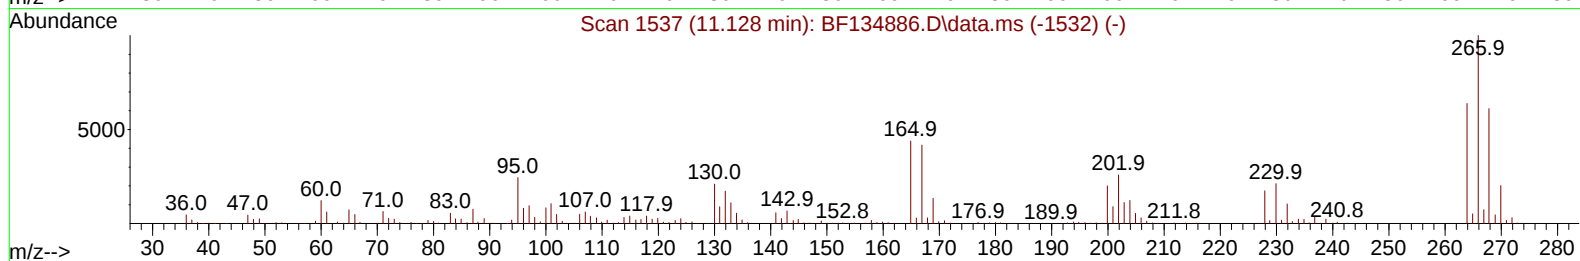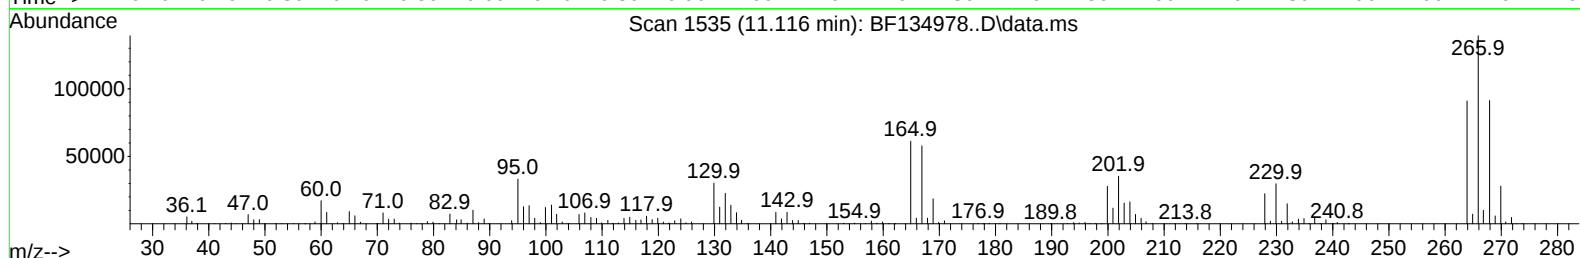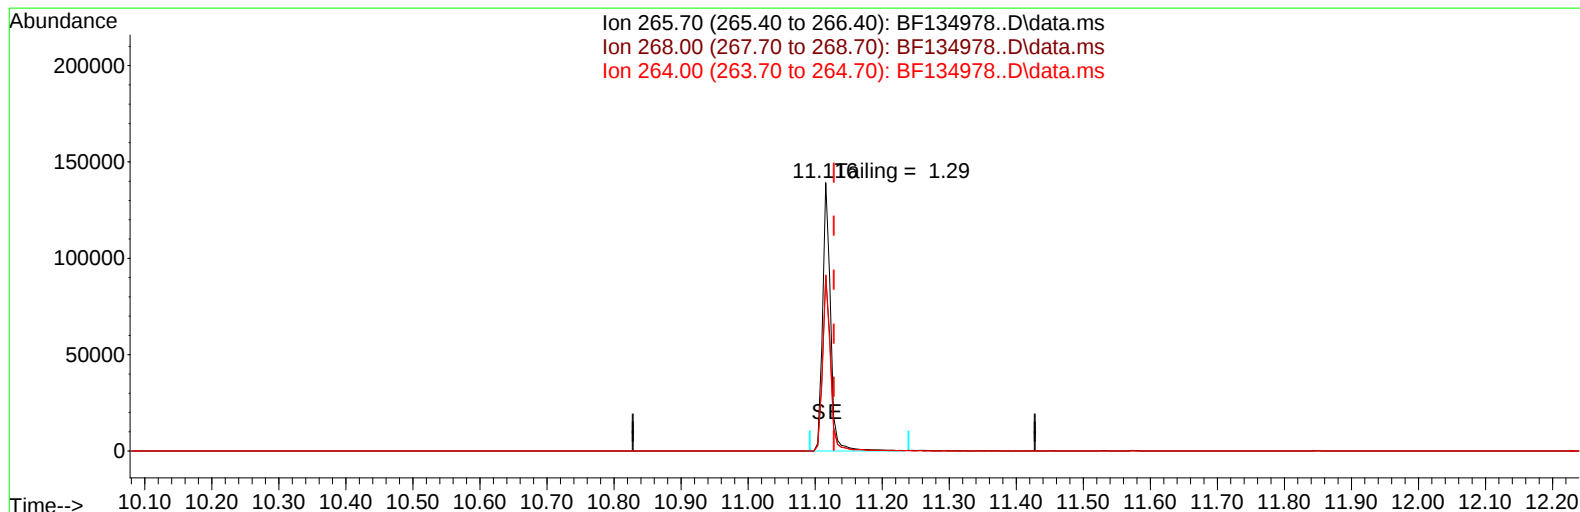

TIC: BF134978..D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.012) 25044.41 ng




response 115213

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.58
264.00	63.80	65.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082923\
 Data File : BF134978..D
 Acq On : 29 Aug 2023 12:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 29 13:36:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 28 02:45:19 2023
 Response via : Initial Calibration

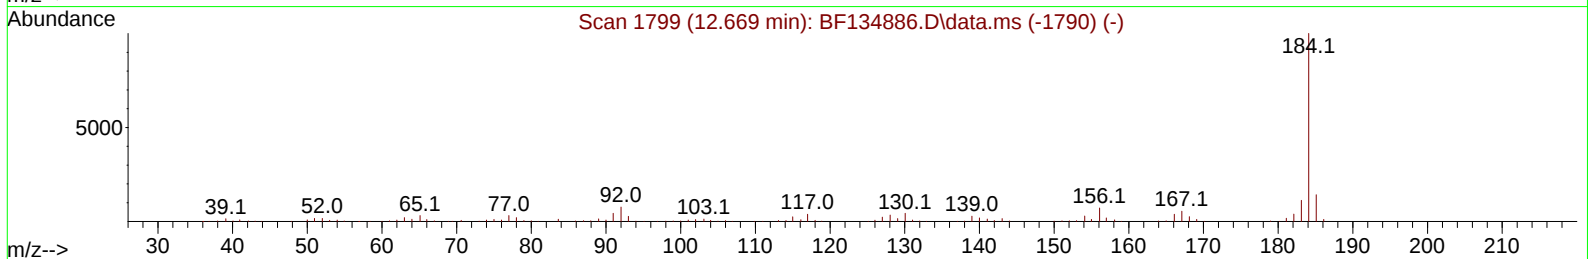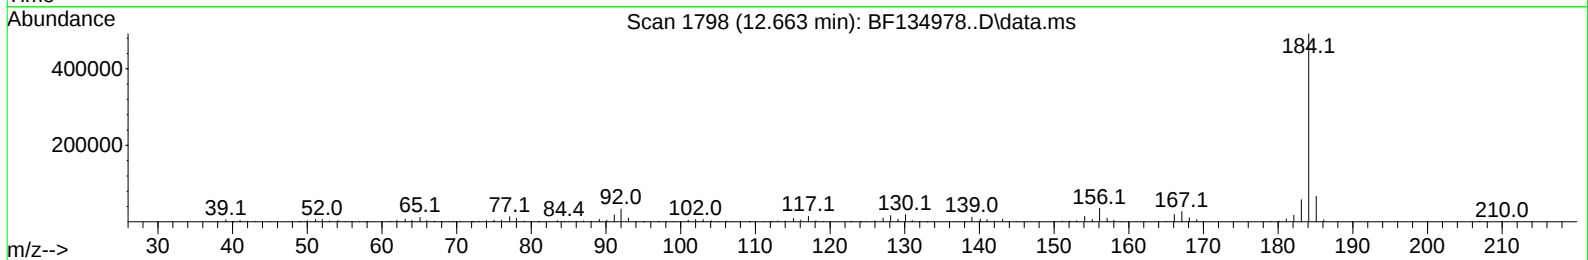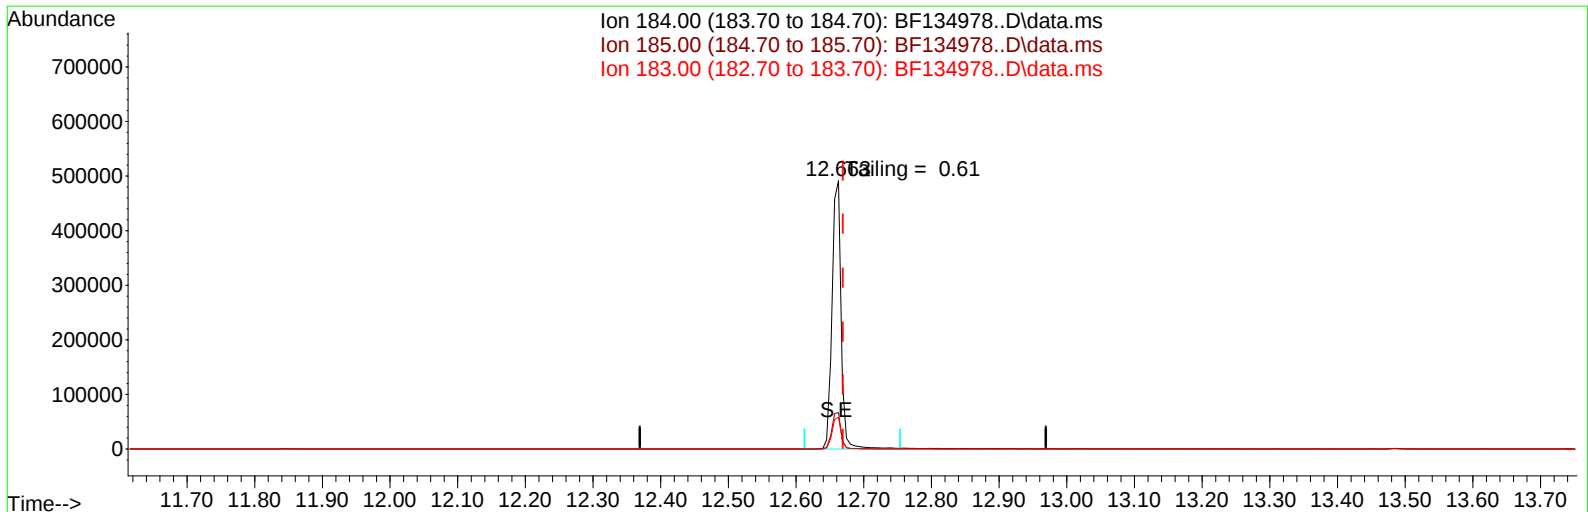

TIC: BF134978..D\data.ms

(77) Benzidine

12.663min (-0.006) 0.00 ng m

response 462723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.56
183.00	11.20	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/29/2023	BNA_F	<u>BF134978.D</u>
Compound Name	Response	Retention Time
DDT	225831	13.486
DDD	7010	13.186
DDE	3116	11.575
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10126	235957	4.29

Instrument :
BNA_F
ClientSampleId :
DFTPP