
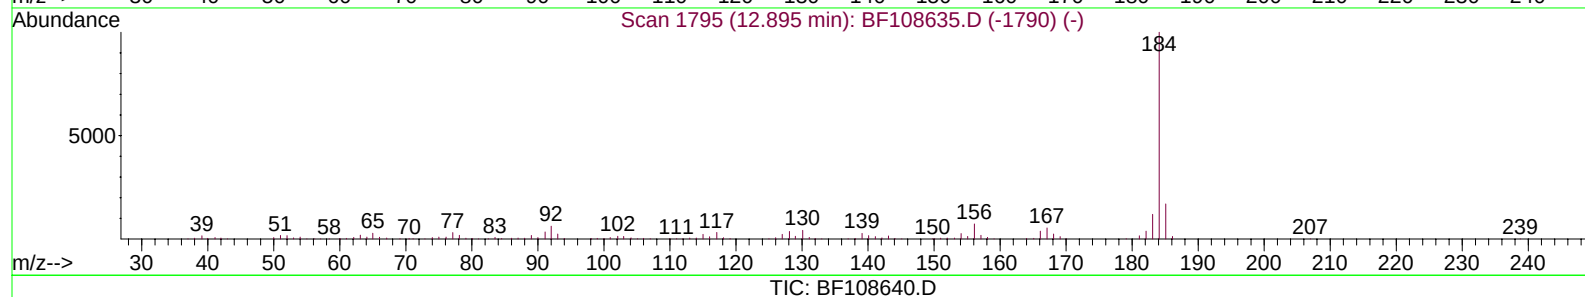
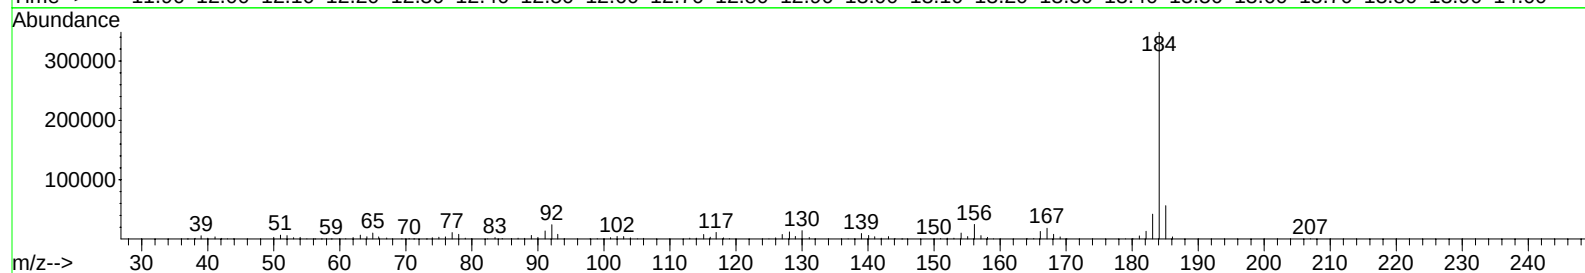


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF083018\
Data File : BF108640.D
Acq On : 30 Aug 2018 15:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 15:50:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

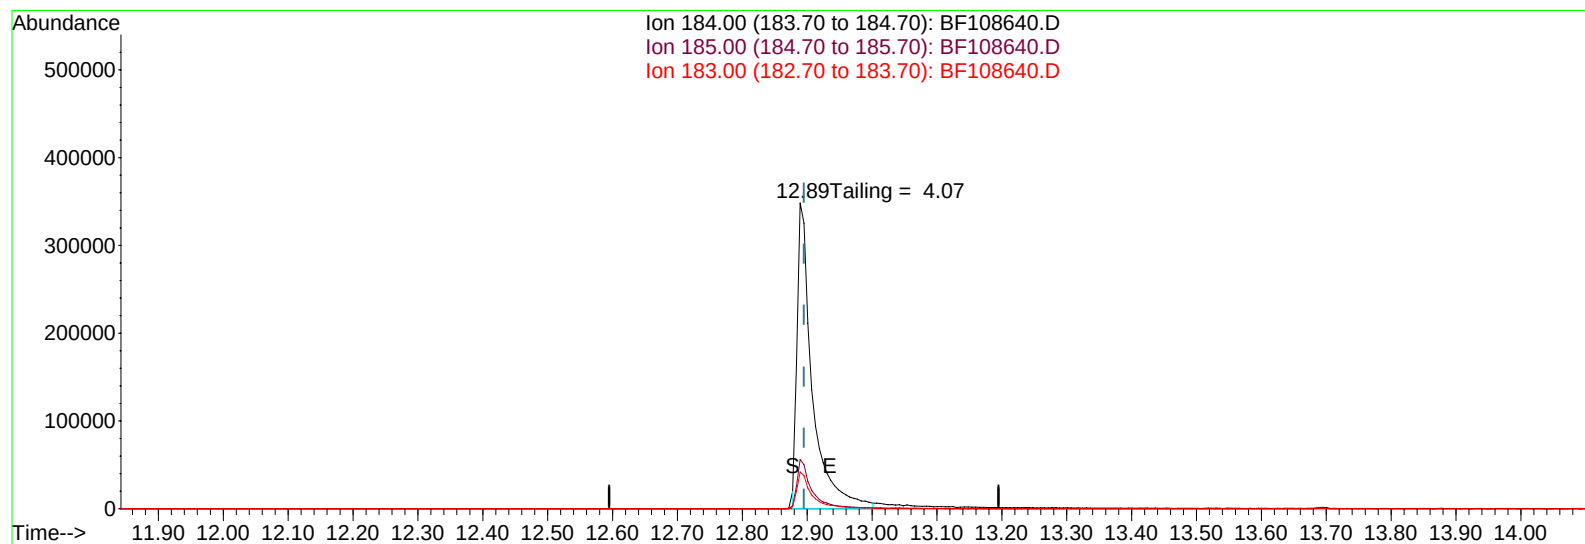

(76) Benzidine




12.889min (-0.006) 0.00ng

response 603665

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.15
183.00	11.60	12.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF083018\
Data File : BF108640.D
Acq On : 30 Aug 2018 15:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 15:50:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

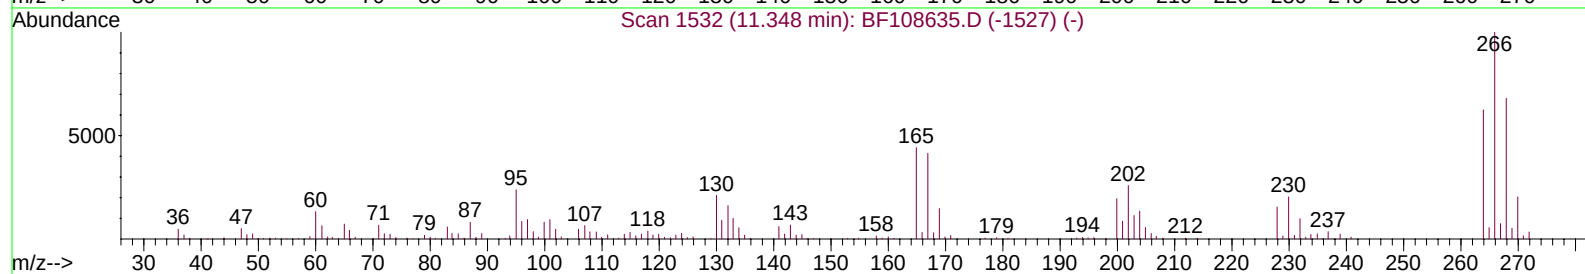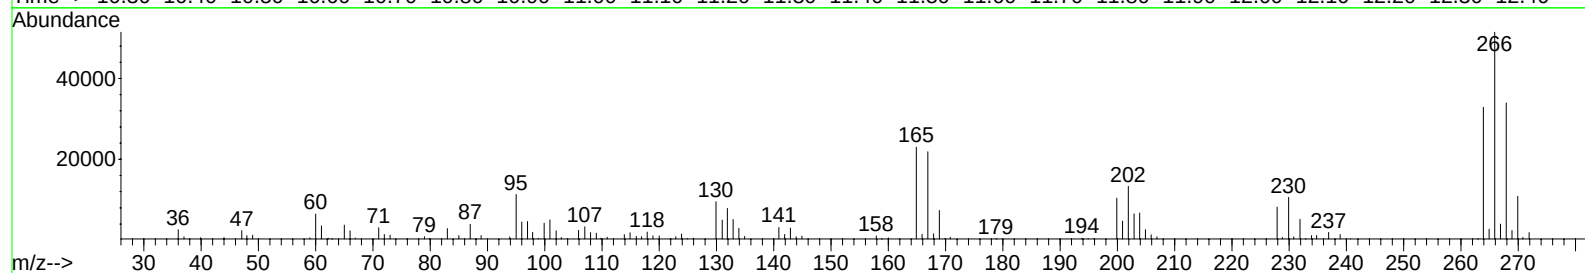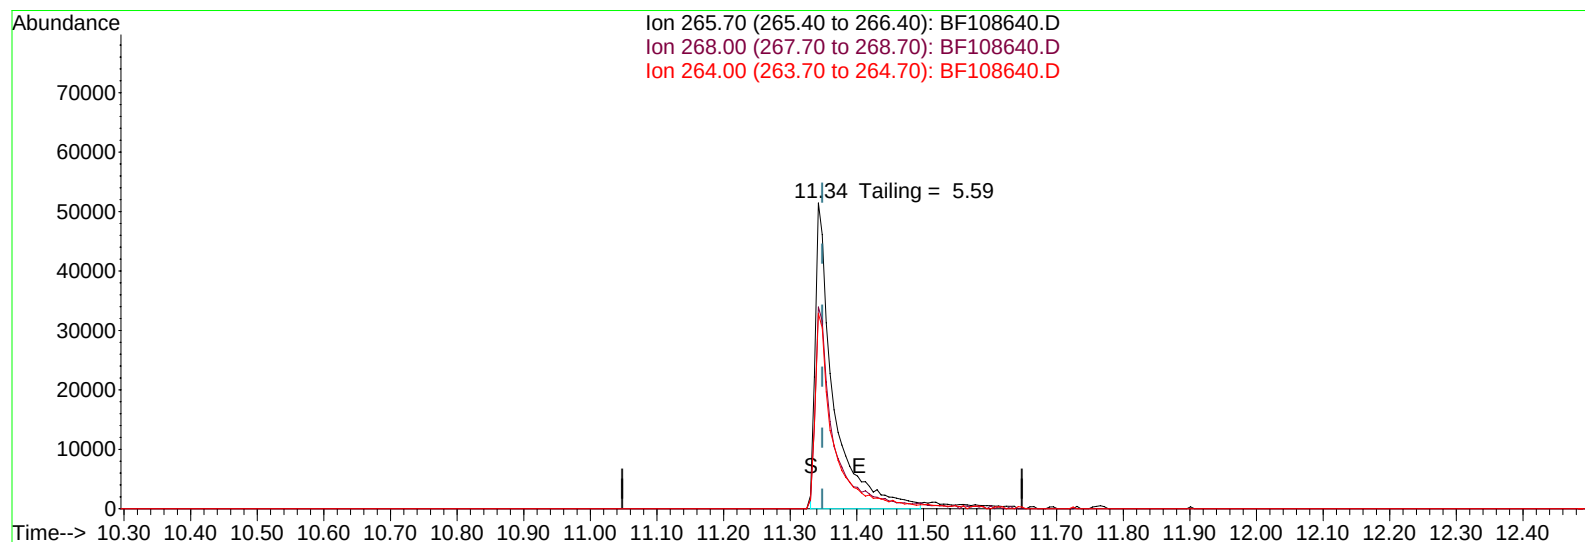

TIC: BF108640.D

(69) Pentachlorophenol (C)

11.342min (-0.006) 30793.37ng

response 99013

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.97
264.00	61.90	63.92
0.00	0.00	0.00