
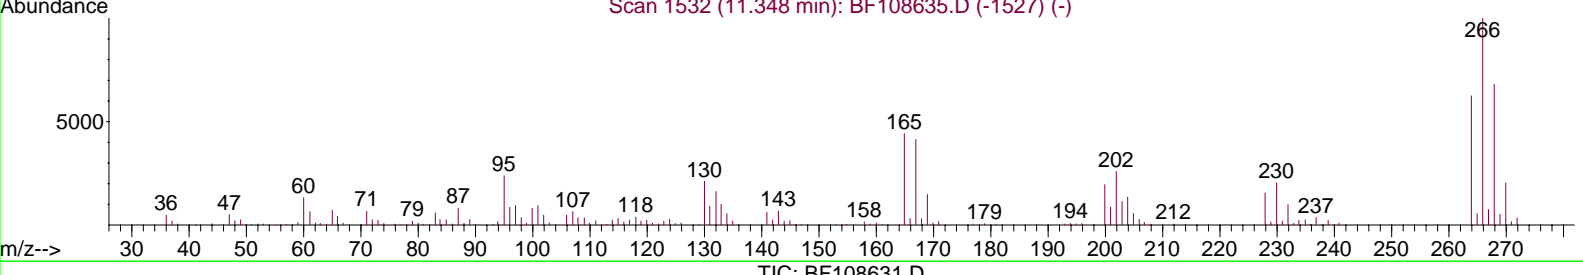
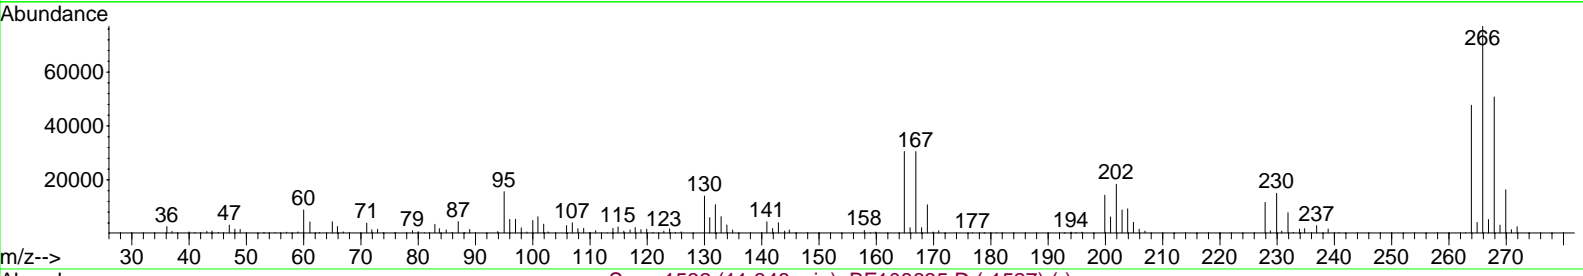


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF083018\
 Data File : BF108631.D
 Acq On : 30 Aug 2018 10:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 15:50:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 30 15:06:55 2018
 Response via : Initial Calibration

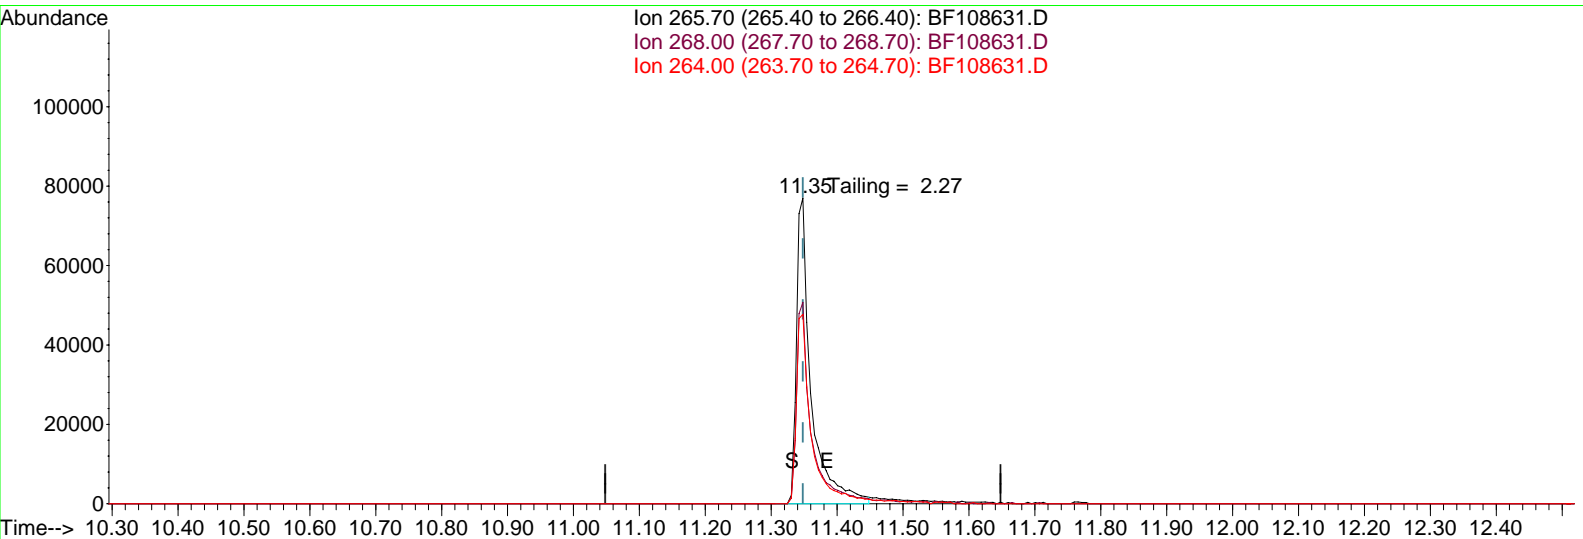

(69) Pentachlorophenol (C)




11.348min (+0.000) 33668.75ng

response 124367

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.89
264.00	61.90	61.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF083018\
 Data File : BF108631.D
 Acq On : 30 Aug 2018 10:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 30 15:50:25 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 30 15:06:55 2018
 Response via : Initial Calibration

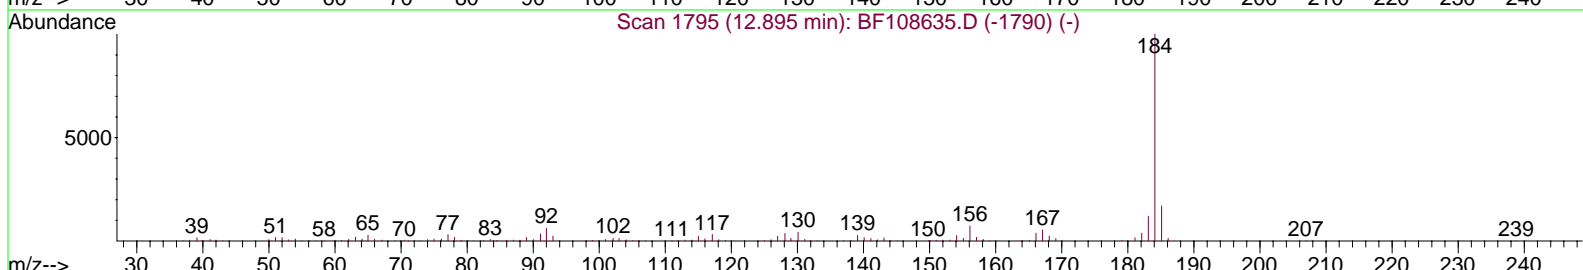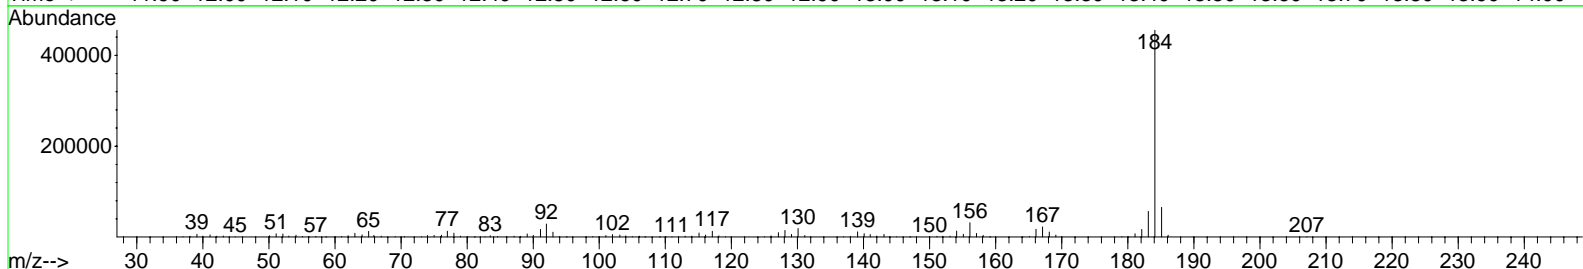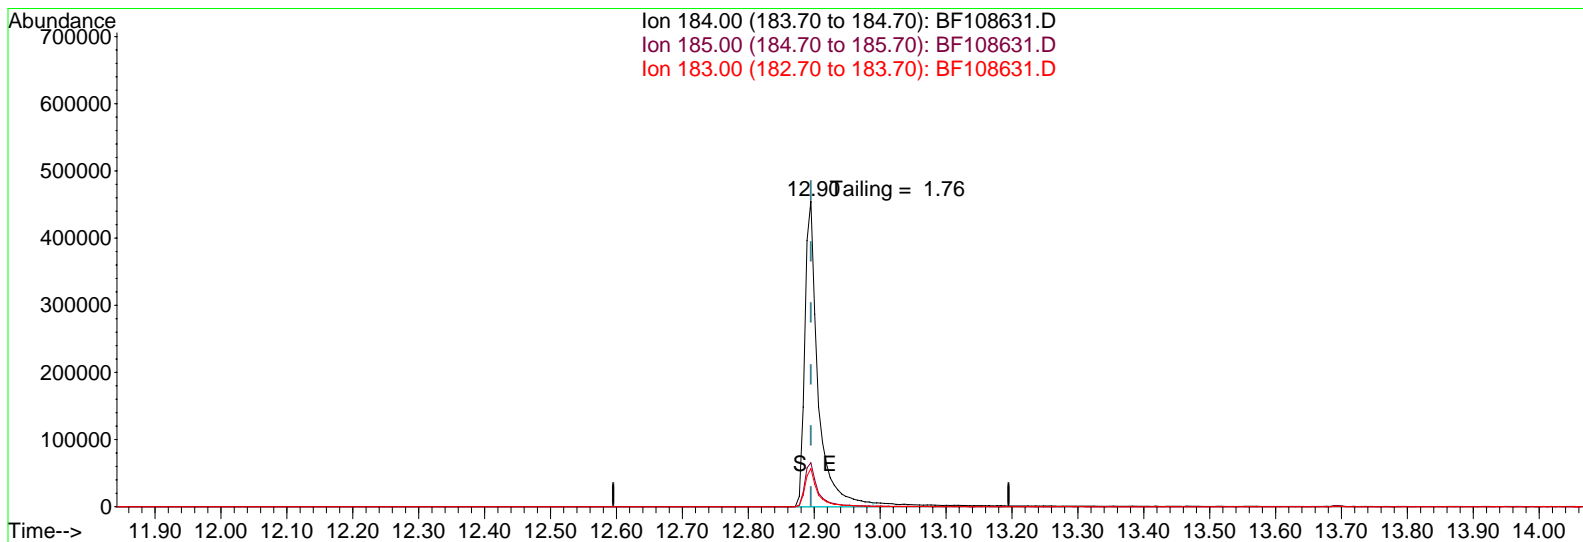

TIC: BF108631.D

(76) Benzidine

12.895min (0.000) 160870.96ng

response 656606

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.37
183.00	11.60	12.46
0.00	0.00	0.00