

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
 Data File : BF108648.D
 Acq On : 30 Aug 2018 18:56
 Operator : JU/SJ
 Sample : J4702-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-039

Quant Time: Aug 31 02:13:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 30 15:06:55 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	81176	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	345435	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	180579	20.00	ng	0.00
63) Phenanthrene-d10	11.54	188	381087	20.00	ng	-0.01
75) Chrysene-d12	14.19	240	285258	20.00	ng	-0.01
86) Perylene-d12	15.75	264	273621	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	292785	62.66	ng	0.00
7) Phenol-d6	6.64	99	486059	72.63	ng	0.00
23) Nitrobenzene-d5	7.57	82	327412	48.11	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	162179	68.03	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	654046	48.70	ng	0.00
78) Terphenyl-d14	13.12	244	738028	50.27	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.75	163	74298	5.225	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
Data File : BF108648.D
Acq On : 30 Aug 2018 18:56
Operator : JU/SJ
Sample : J4702-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-039

Quant Time: Aug 31 02:13:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

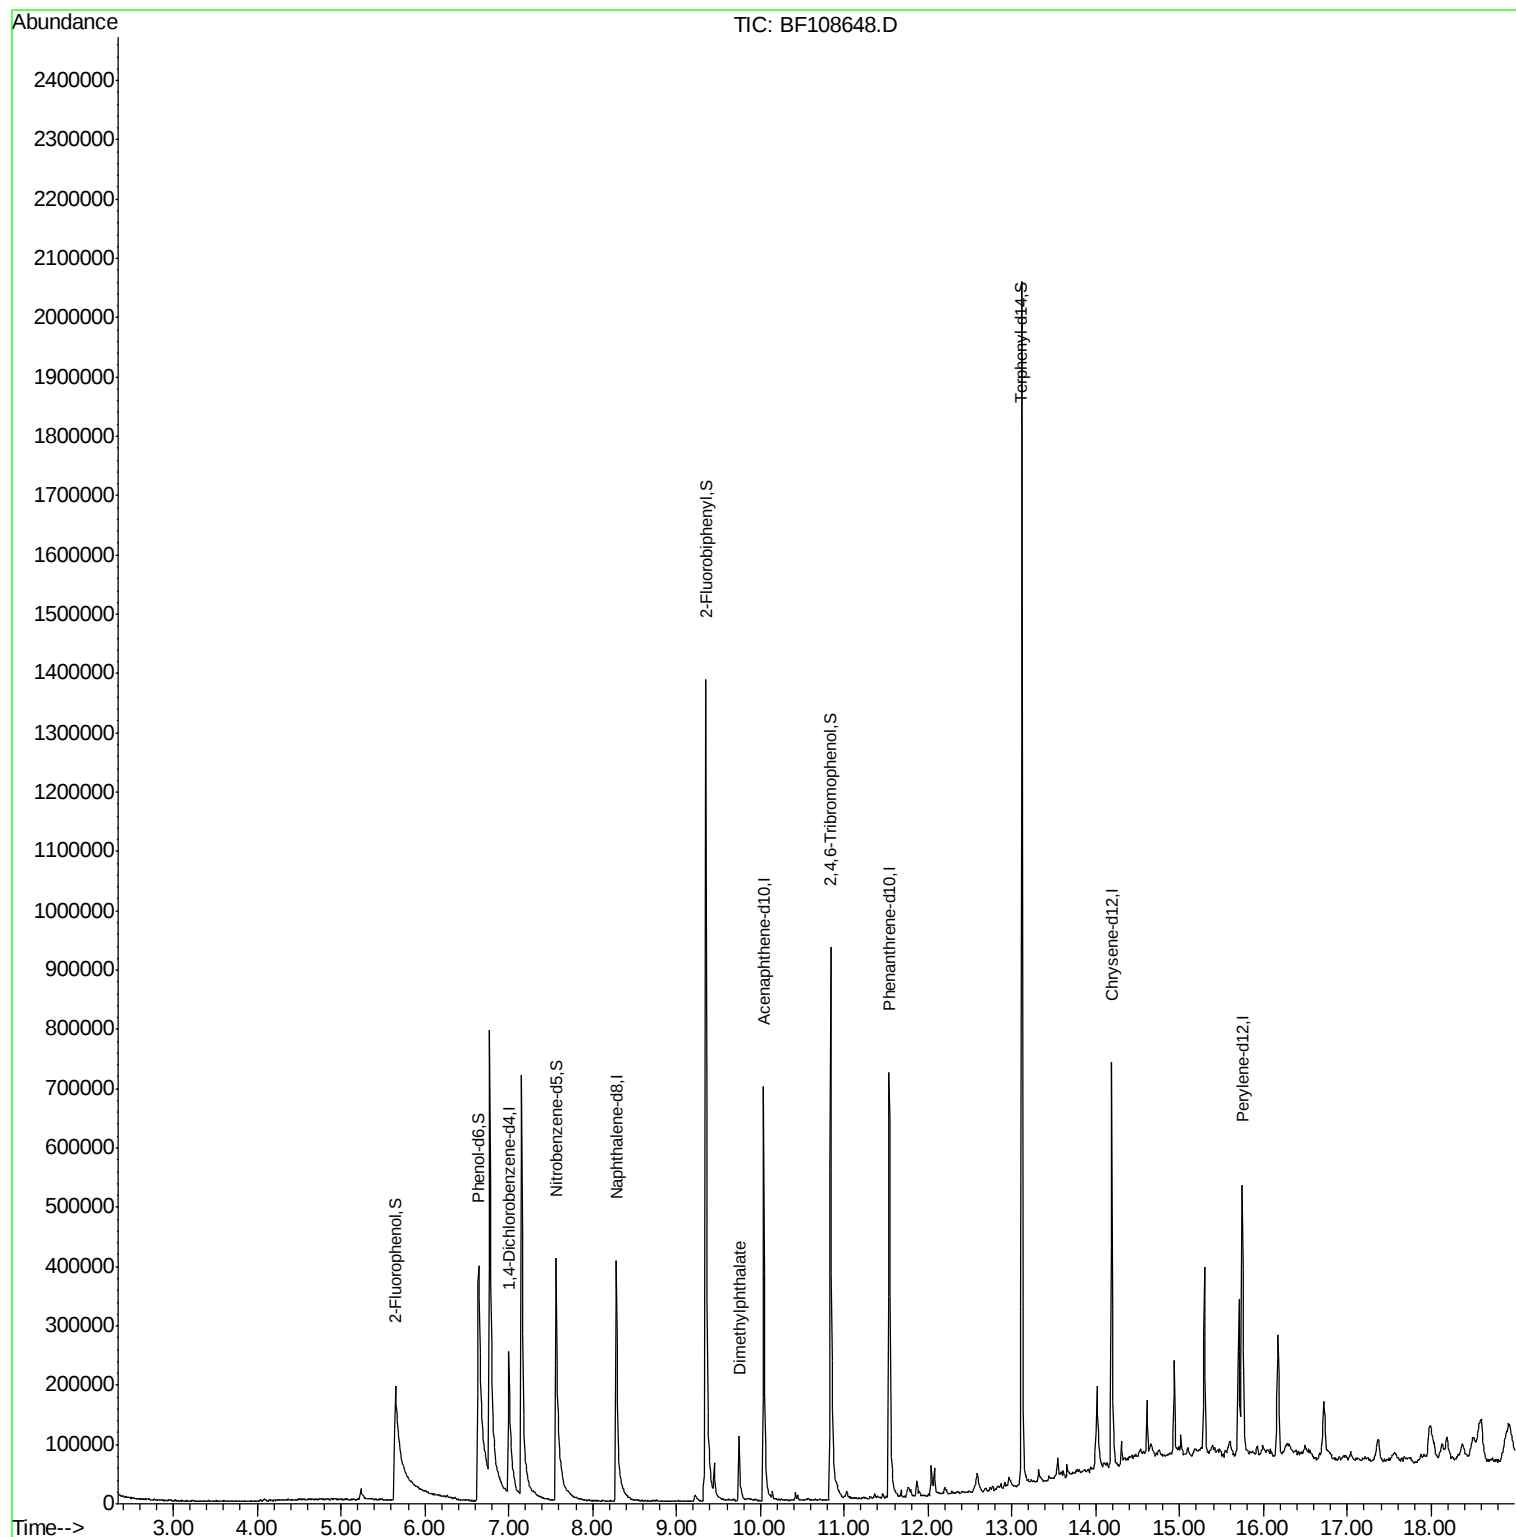

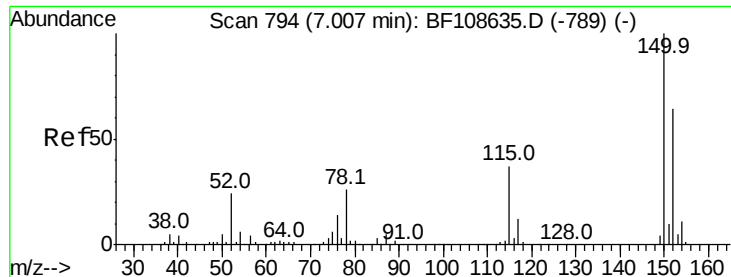


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF108648.D
Acq: 30 Aug 2018 18:56

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-039

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.3	124.6	186.8
115	62.5	50.1	75.1



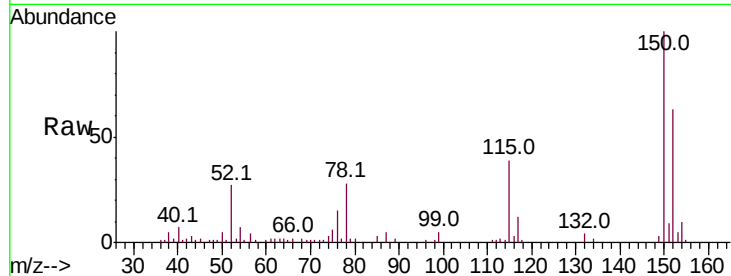


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

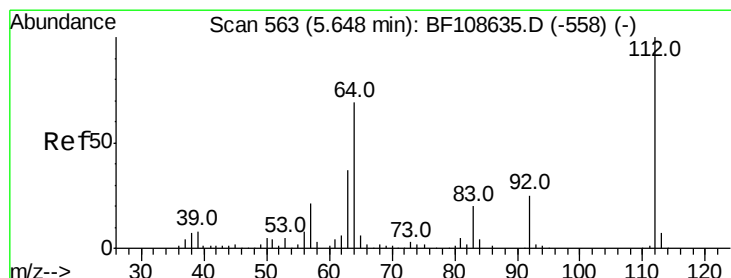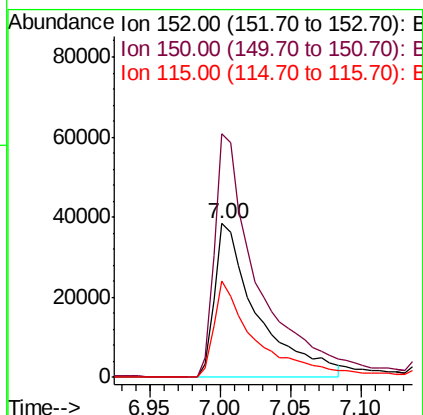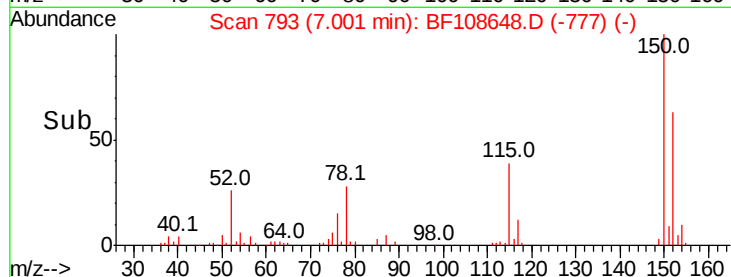

#5

2-Fluorophenol
Concen: 62.657 ng
RT: 5.65 min Scan# 563
Delta R.T. 0.00 min
Lab File: BF108648.D
Acq: 30 Aug 2018 18:56

Tgt Ion	Ratio	Lower	Upper
112	100		
64	66.4	47.9	71.9
63	34.2	23.7	35.5


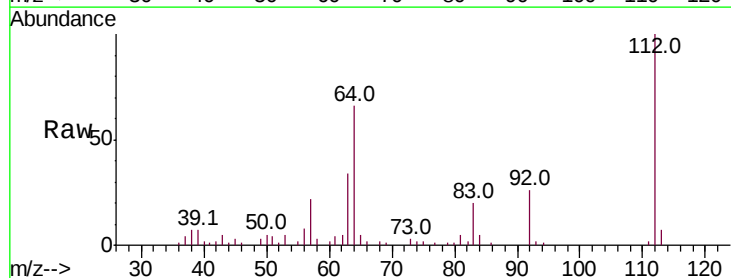



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

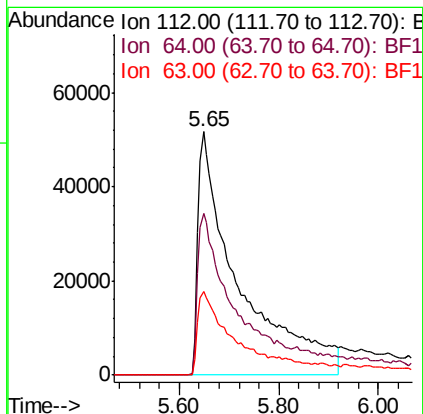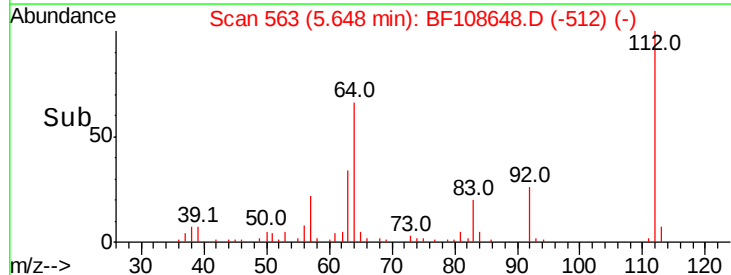

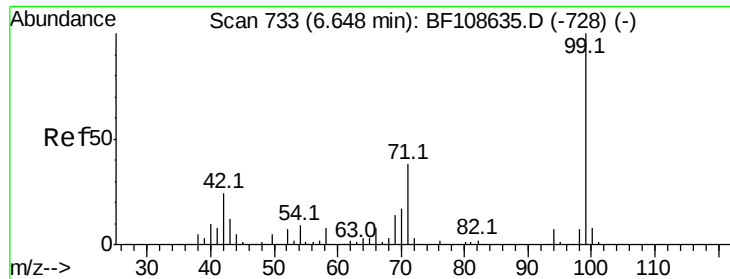

#7

Phenol-d6

Concen: 72.626 ng

RT: 6.64 min Scan# 732

Delta R.T. -0.01 min

Lab File: BF108648.D

Acq: 30 Aug 2018 18:56

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-039


Tot Ion: 99 Resp: 486059

Ion Ratio Lower Upper




99 100

42 21.3 14.5 21.7

71 34.9 25.4 38.0

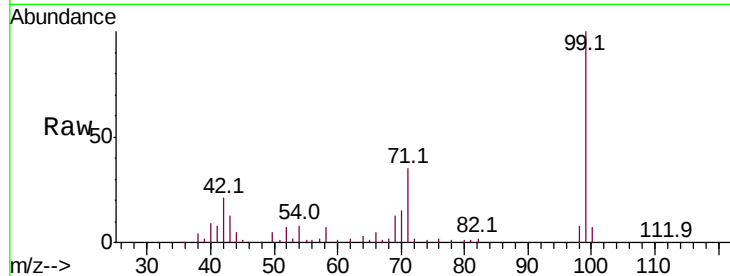

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

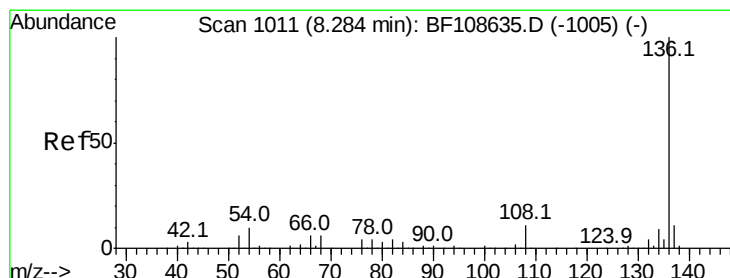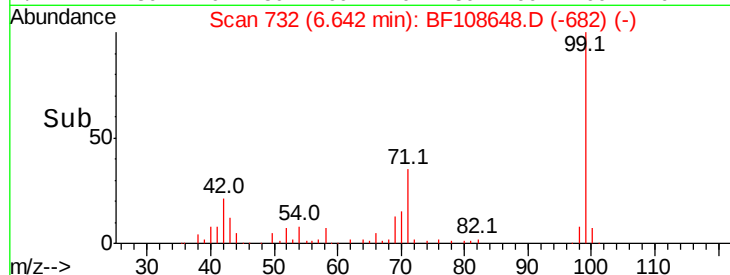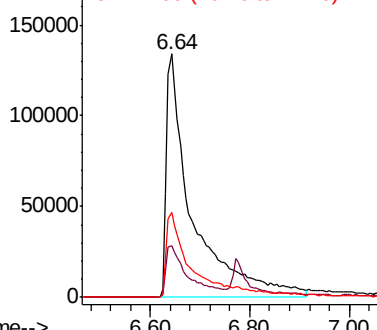

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011

Delta R.T. -0.00 min

Lab File: BF108648.D

Acq: 30 Aug 2018 18:56

Tgt Ion:136 Resp: 345435


Ion Ratio Lower Upper

136 100



137 10.7 8.9 13.3

54 9.6 6.6 9.8

68 5.3 5.0 7.4

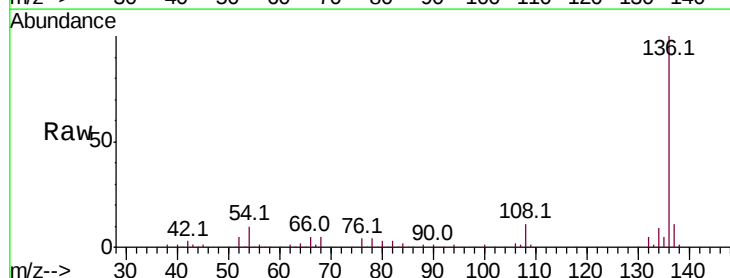

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



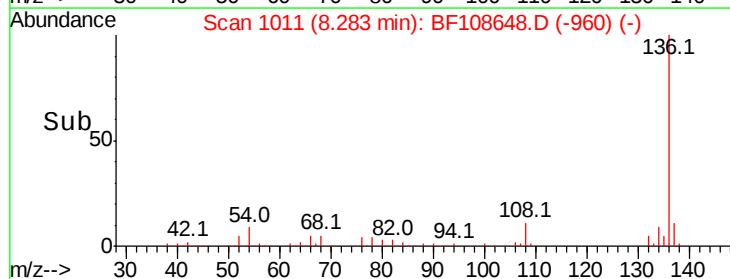
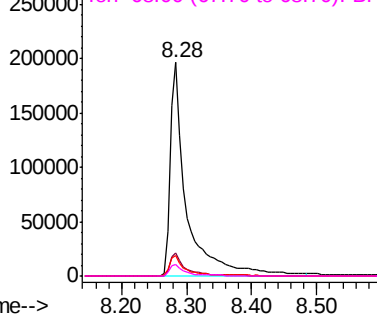




#23
 Nitrobenzene-d5
 Concen: 48.110 ng
 RT: 7.57 min Scan# 889
 Delta R.T. -0.01 min
 Lab File: BF108648.D
 Acq: 30 Aug 2018 18:56




Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-039


Tot Ion: 82 Resp: 327412
 Ion Ratio Lower Upper
 82 100
 128 42.5 36.1 54.1
 54 59.0 41.4 62.2

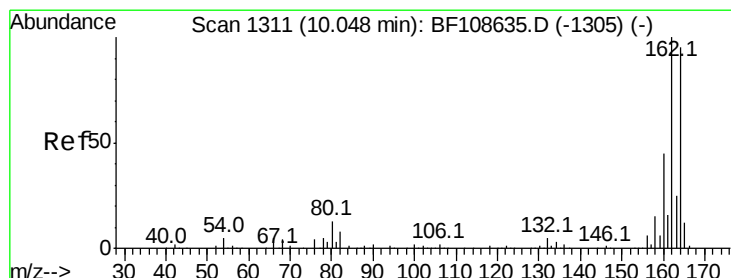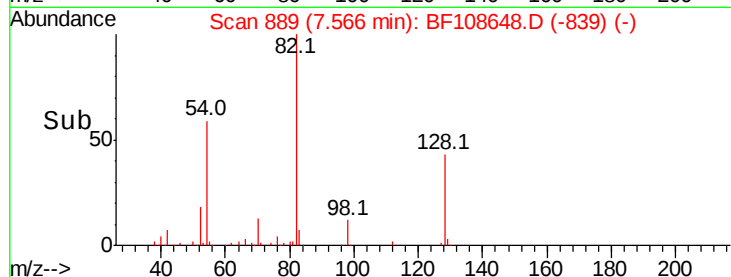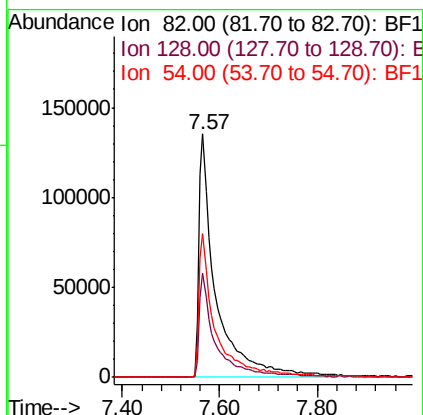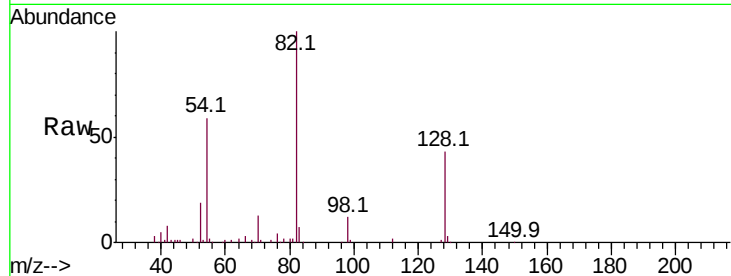

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.04 min Scan# 1310
 Delta R.T. -0.01 min
 Lab File: BF108648.D
 Acq: 30 Aug 2018 18:56

Tgt Ion:164 Resp: 180579
 Ion Ratio Lower Upper
 164 100
 162 103.8 86.1 129.1
 160 45.8 38.3 57.5

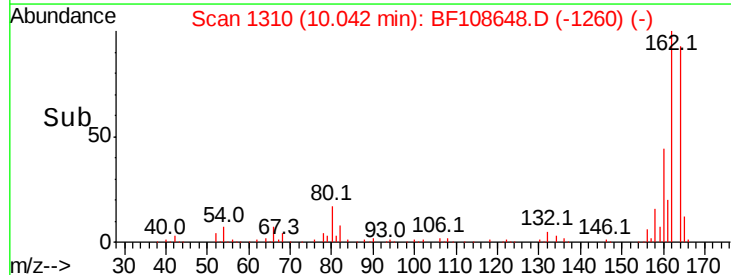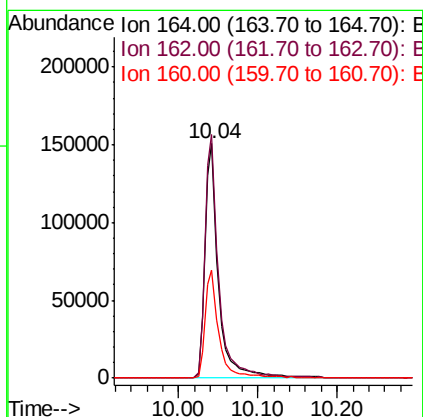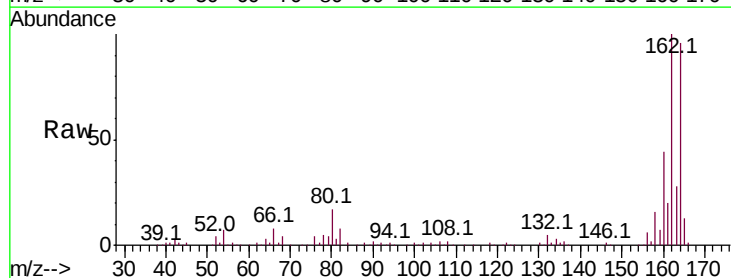


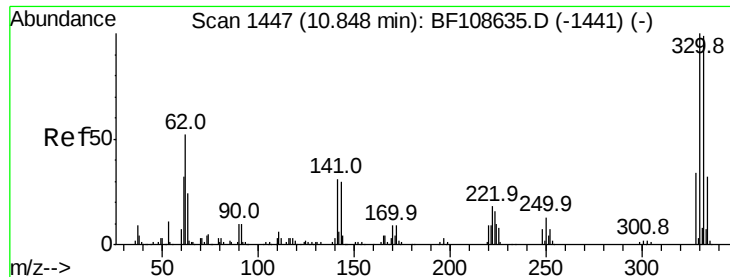




#41
 2,4,6-Tribromophenol
 Concen: 68.032 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108648.D
 Acq: 30 Aug 2018 18:56

Instrument :
 BNA_F
 ClientSampleId :
 FK-PS-01-039

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.7	77.0	115.6
141	33.2	29.9	44.9

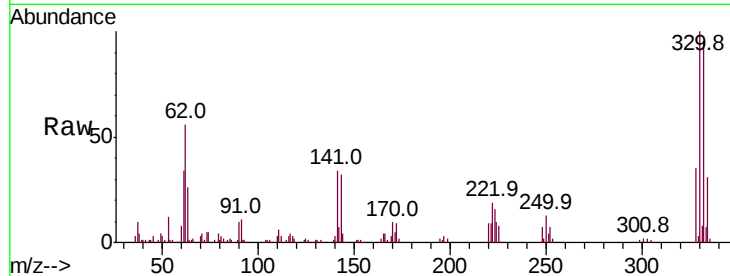


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

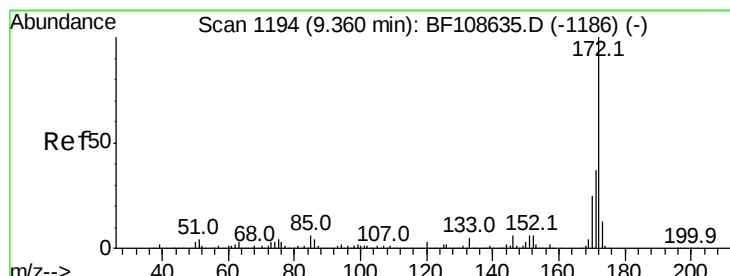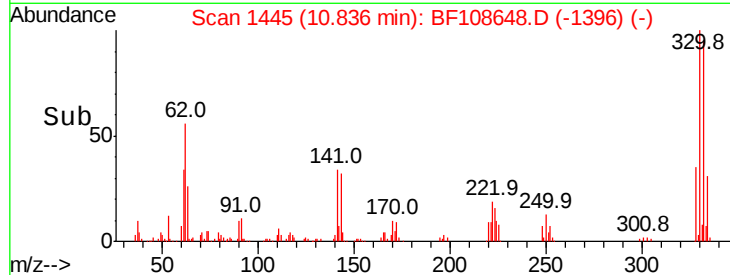
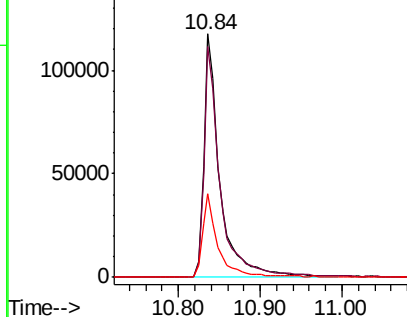


#44
 2-Fluorobiphenyl
 Concen: 48.700 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108648.D
 Acq: 30 Aug 2018 18:56

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.2	29.7	44.5
170	23.1	19.6	29.4

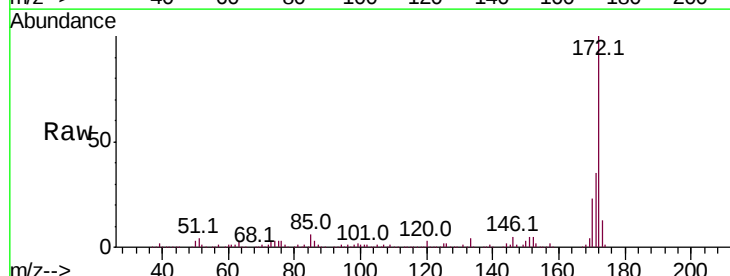

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

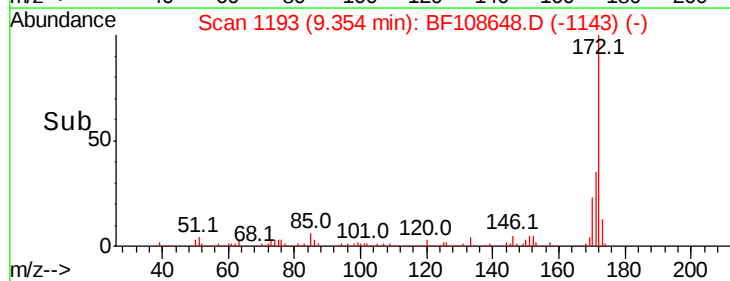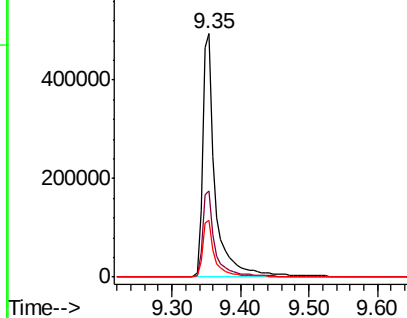







#49
Dimethylphthalate
Concen: 5.225 ng
RT: 9.75 min Scan# 1260
Delta R.T. -0.02 min
Lab File: BF108648.D
Acq: 30 Aug 2018 18:56

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-039

Tot Ion:163 Resp: 74298
Ion Ratio Lower Upper
163 100
194 4.0 2.7 4.1
164 9.5 8.2 12.2

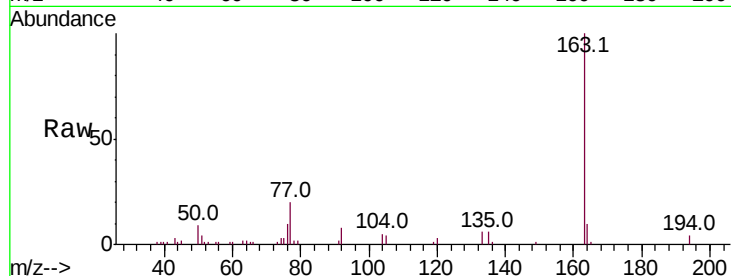


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

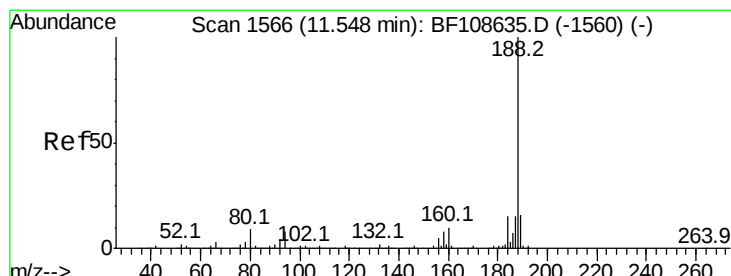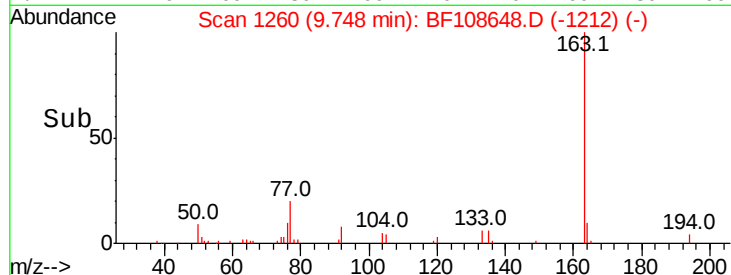
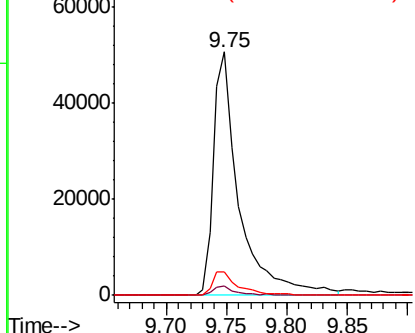



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1564
Delta R.T. -0.01 min
Lab File: BF108648.D
Acq: 30 Aug 2018 18:56

Tgt Ion:188 Resp: 381087
Ion Ratio Lower Upper
188 100
94 8.7 8.5 12.7
80 9.6 9.2 13.8

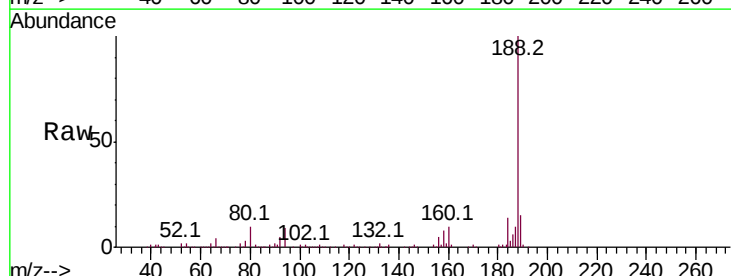

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

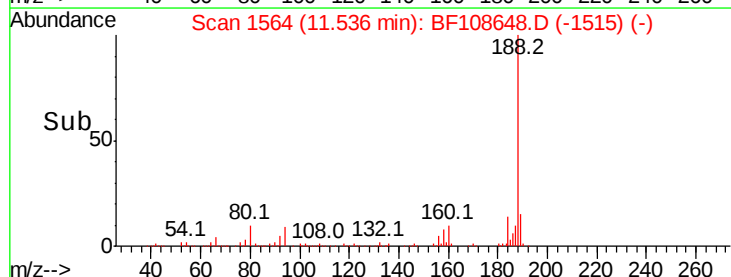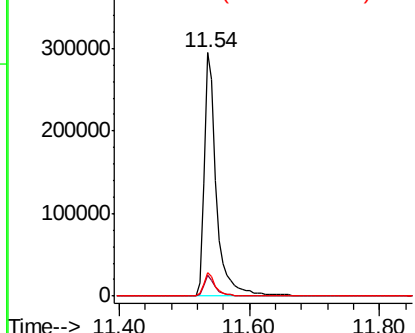

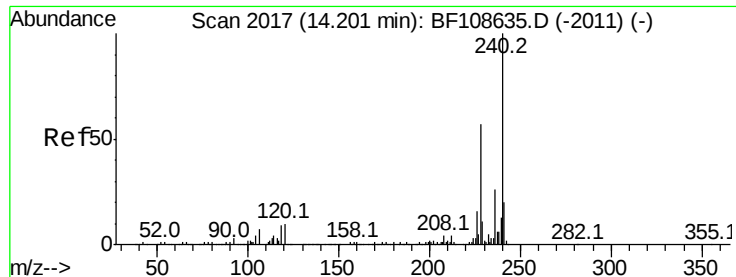

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 2015

Delta R.T. -0.01 min

Lab File: BF108648.D

Acq: 30 Aug 2018 18:56

Instrument :

BNA_F

ClientSampleId :

FK-PS-01-039


Tot Ion:240 Resp: 285258

Ion Ratio Lower Upper

240 100

120 9.2 9.5 14.3#




236 25.8 20.7 31.1

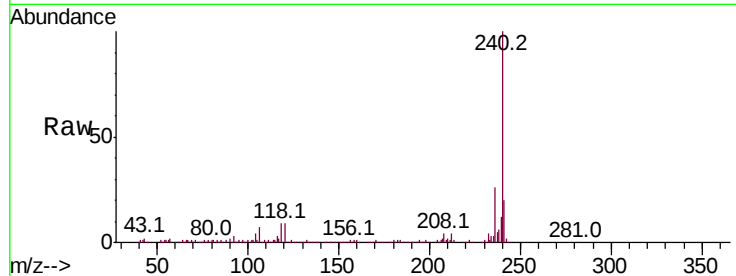

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

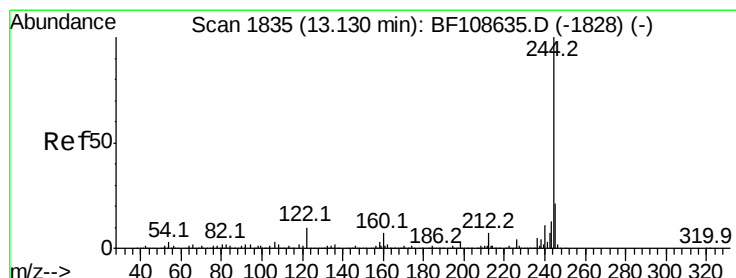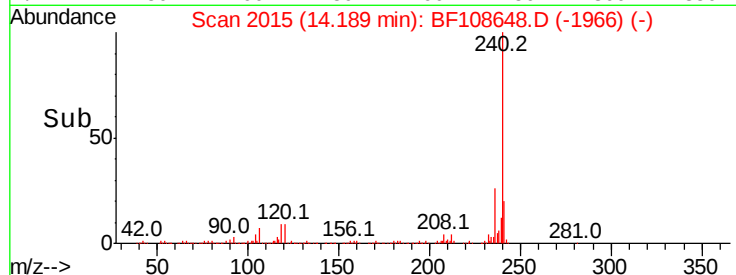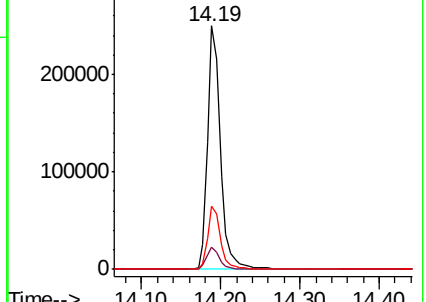

#78

Terphenyl-d14

Concen: 50.269 ng

RT: 13.12 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BF108648.D

Acq: 30 Aug 2018 18:56


Tgt Ion:244 Resp: 738028

Ion Ratio Lower Upper

244 100

212 7.4 5.4 8.0



122 9.4 11.0 16.4#

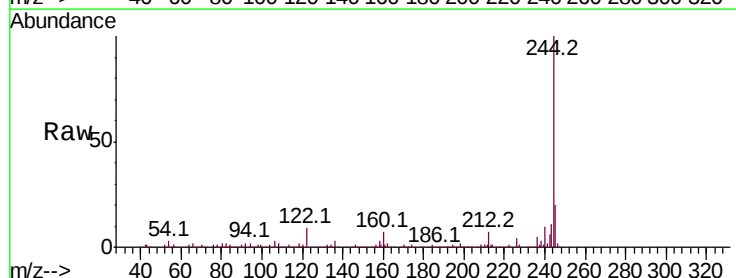


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

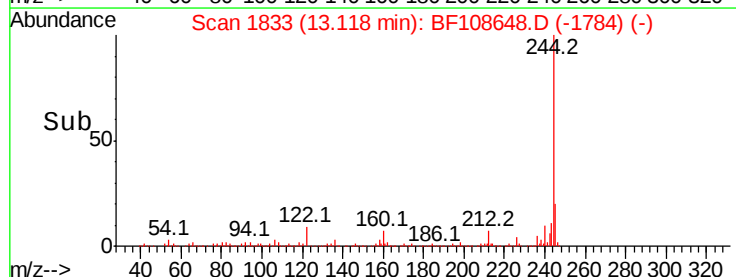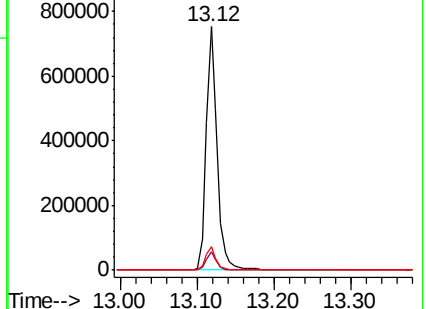

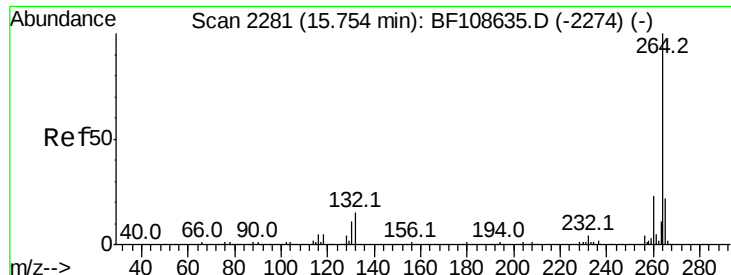

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.75 min Scan# 2280
Delta R.T. -0.01 min
Lab File: BF108648.D
Acq: 30 Aug 2018 18:56

Instrument :
BNA_F
ClientSampleId :
FK-PS-01-039

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.2	28.8
265	21.5	17.5	26.3

