

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
 Data File : BF108662.D
 Acq On : 31 Aug 2018 1:16
 Operator : JU/SJ
 Sample : J4700-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082818-SIDI-F-D-S

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:18:34 PM

Quant Time: Aug 31 11:09:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 30 15:06:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	81648	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	337623	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	157906	20.00	ng	0.00
63) Phenanthrene-d10	11.54	188	291604	20.00	ng	0.00
75) Chrysene-d12	14.19	240	302357	20.00	ng	-0.01
86) Perylene-d12	15.75	264	246457	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.67	112	136484m	29.04	ng	0.02
7) Phenol-d6	6.66	99	143105	21.26	ng	0.01
23) Nitrobenzene-d5	7.57	82	657908	98.91	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	169236	81.19	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	1276602	108.70	ng	0.00
78) Terphenyl-d14	13.12	244	1129106	72.56	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.75	163	114365	9.197	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
Data File : BF108662.D
Acq On : 31 Aug 2018 1:16
Operator : JU/SJ
Sample : J4700-02
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-D-S

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:34 PM

Quant Time: Aug 31 11:09:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

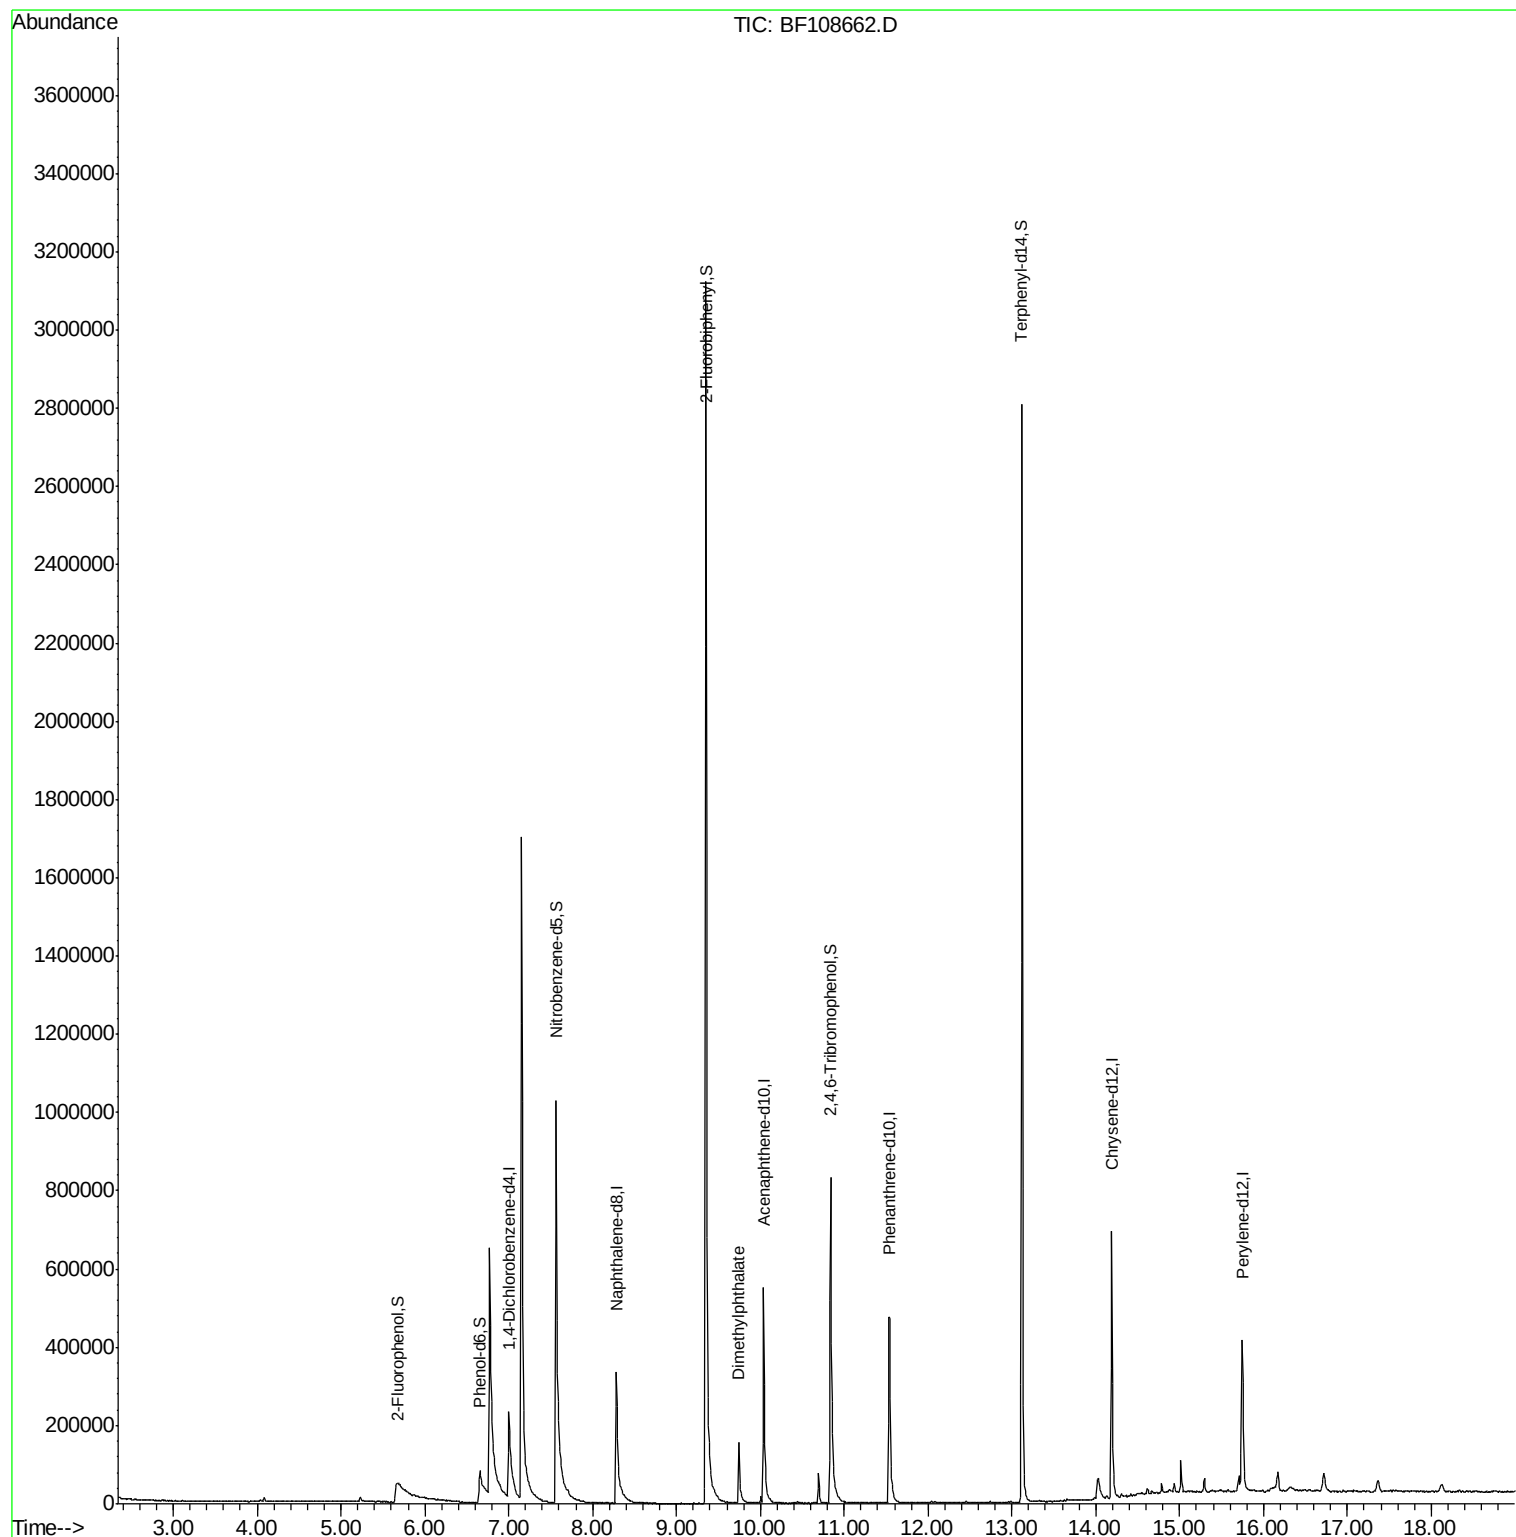

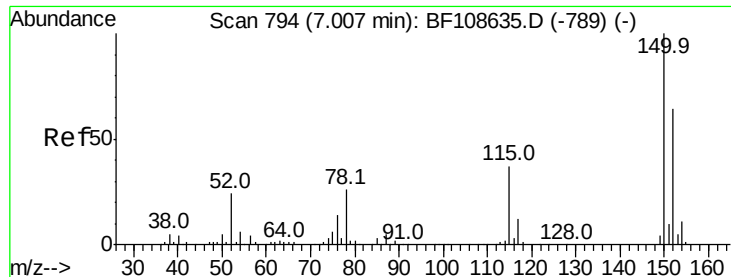

#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.01 min Scan# 794
Delta R.T. 0.00 min
Lab File: BF108662.D
Acq: 31 Aug 2018 1:16

Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-D-S

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.8	124.6	186.8
115	59.1	50.1	75.1

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:34 PM



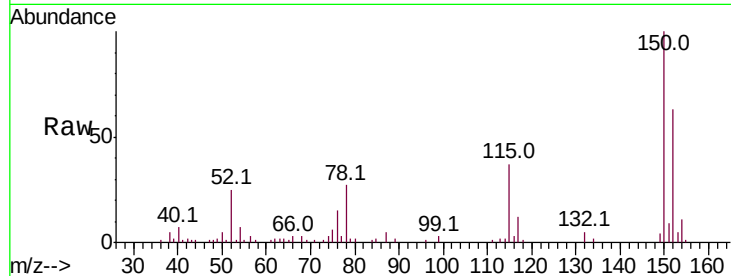


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

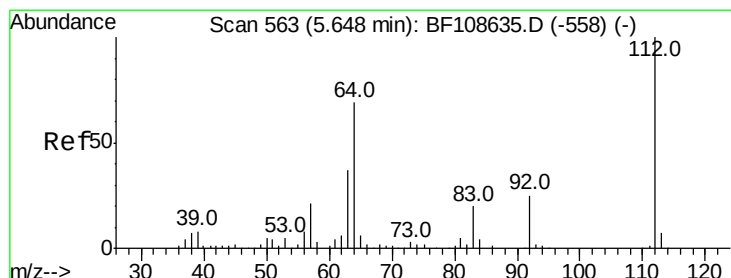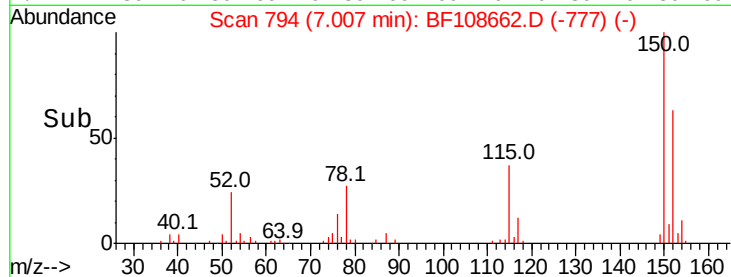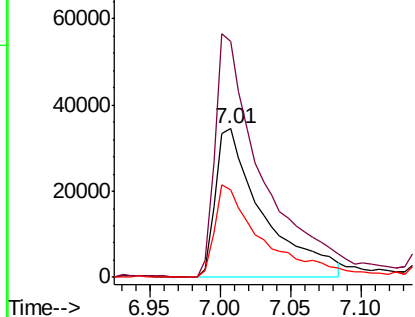

#5

2-Fluorophenol
Concen: 29.039 ng m
RT: 5.67 min Scan# 567
Delta R.T. 0.02 min
Lab File: BF108662.D
Acq: 31 Aug 2018 1:16

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.1	47.9	71.9
63	32.9	23.7	35.5


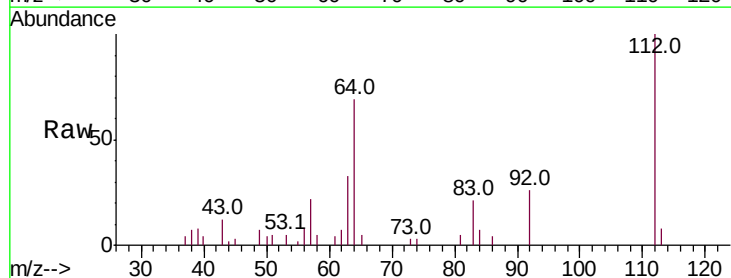



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

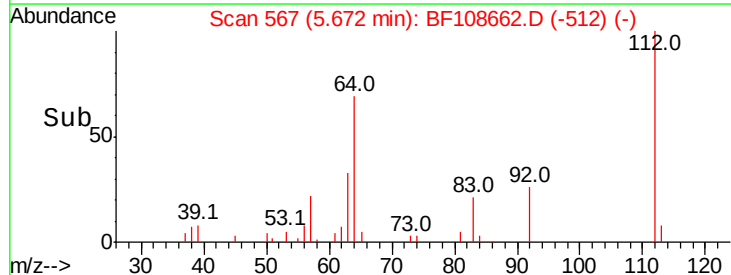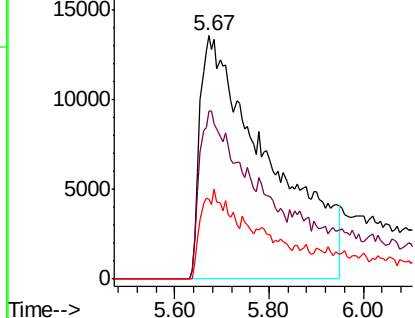

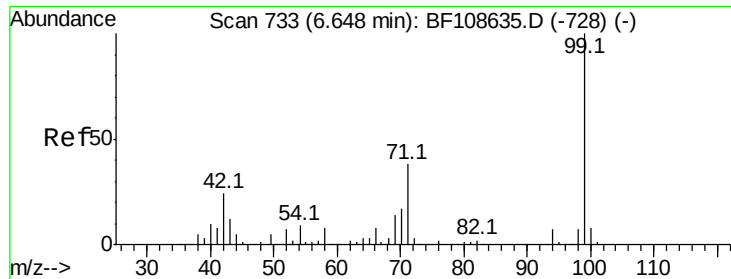

#7

Phenol-d6

Concen: 21.259 ng

RT: 6.66 min Scan# 735

Delta R.T. 0.01 min

Lab File: BF108662.D

Acq: 31 Aug 2018 1:16

Instrument :

BNA_F

ClientSampleId :

082818-SIDI-F-D-S

Tot Ion: 99 Resp: 143105

Ion Ratio Lower Upper

99 100





42 22.6 14.5 21.7#

71 38.0 25.4 38.0

Manual Integrations
APPROVED

Sohil

8/31/2018 12:18:34 PM

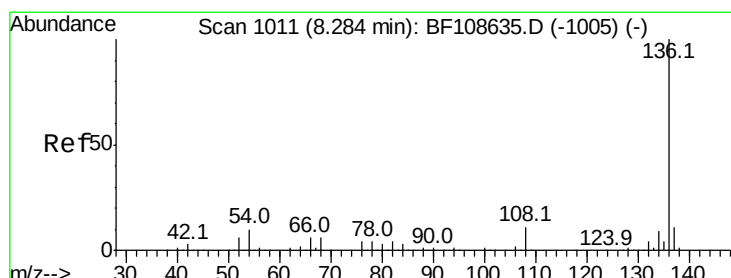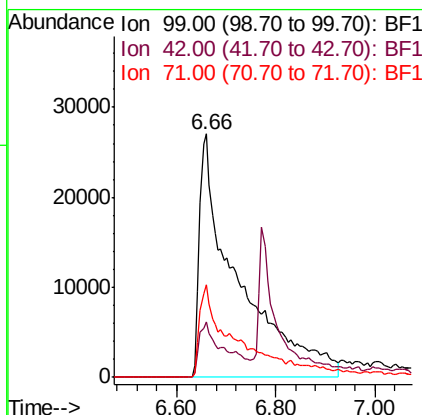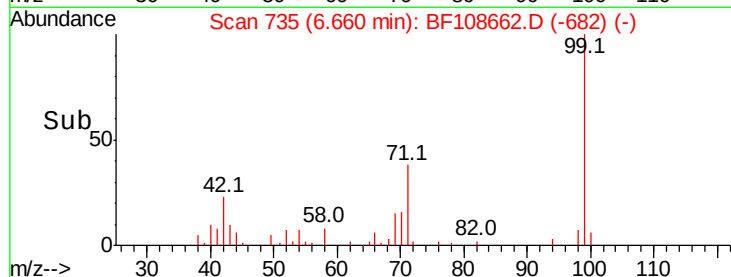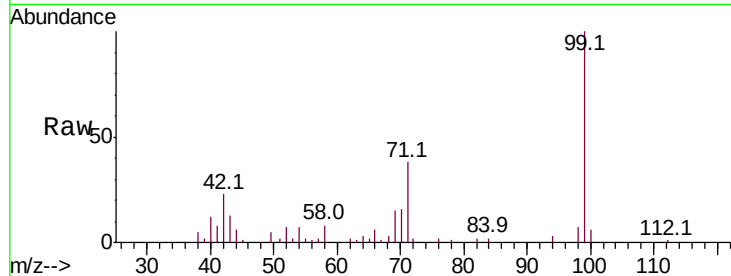

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011

Delta R.T. 0.00 min

Lab File: BF108662.D

Acq: 31 Aug 2018 1:16

Tgt Ion: 136 Resp: 337623




Ion Ratio Lower Upper


136 100

137 10.2 8.9 13.3

54 9.3 6.6 9.8

68 5.6 5.0 7.4

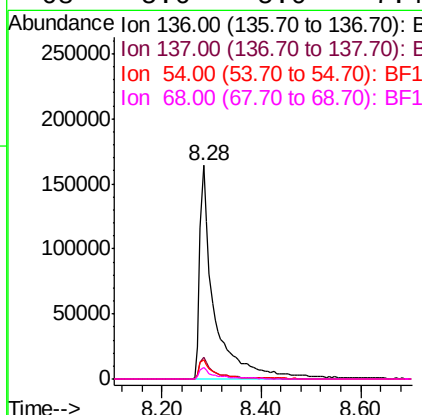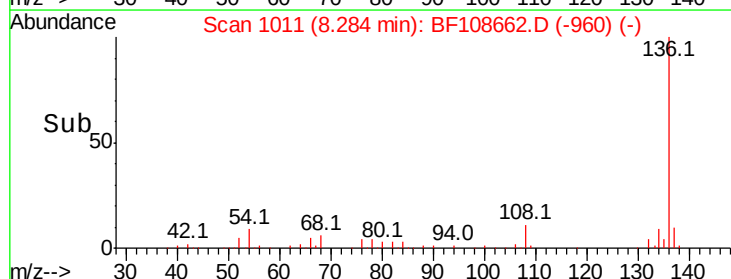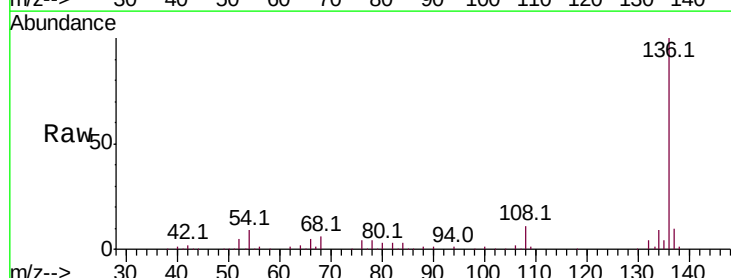

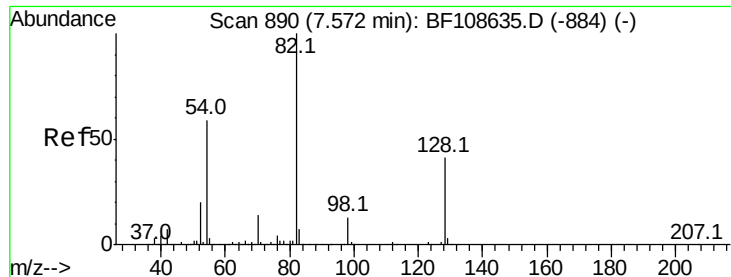





#23
Nitrobenzene-d5
Concen: 98.911 ng
RT: 7.57 min Scan# 889
Delta R.T. -0.01 min
Lab File: BF108662.D
Acq: 31 Aug 2018 1:16

Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-D-S

Tot Ion	Ratio	Lower	Upper
82	100		
128	42.2	36.1	54.1
54	57.5	41.4	62.2




Manual Integrations
APPROVED


Sohil
8/31/2018 12:18:34 PM

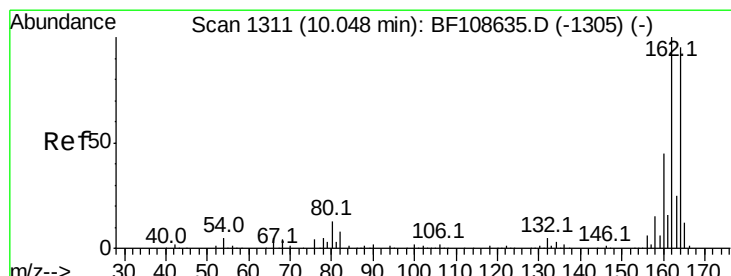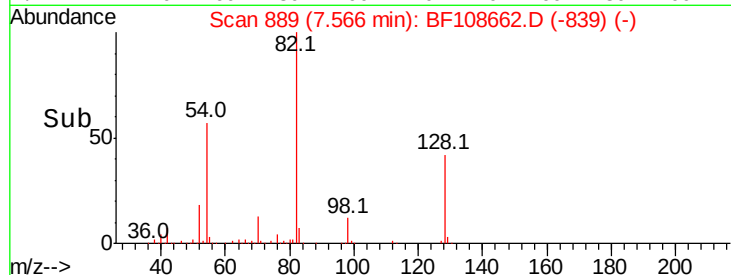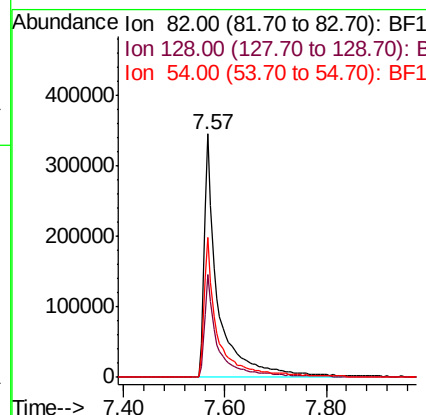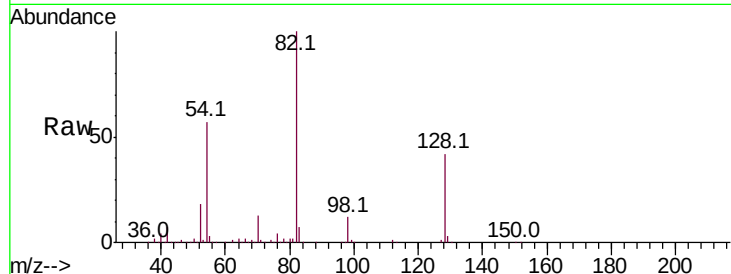

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.04 min Scan# 1310
Delta R.T. -0.01 min
Lab File: BF108662.D
Acq: 31 Aug 2018 1:16

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.1	86.1	129.1
160	47.5	38.3	57.5

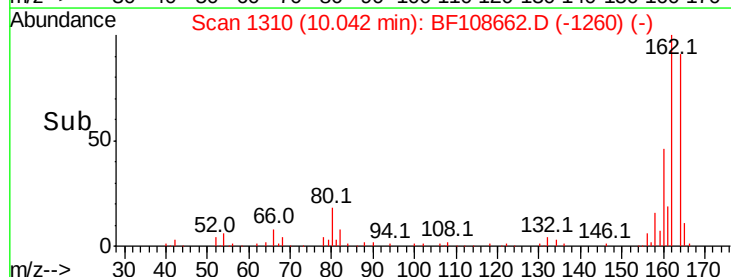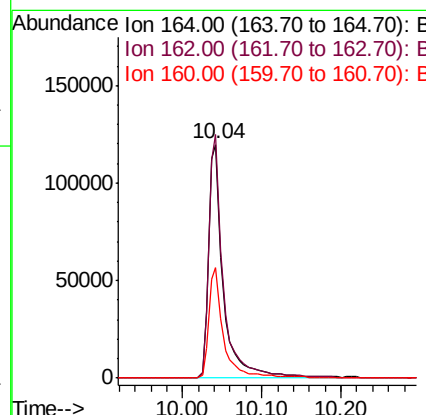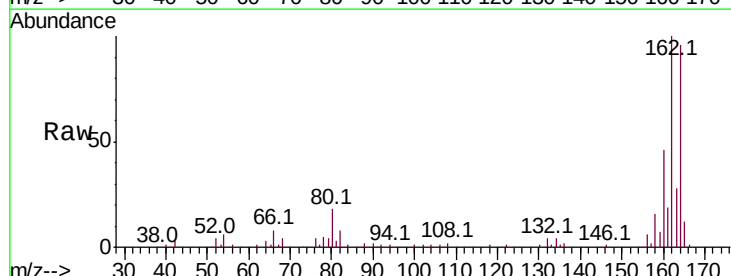

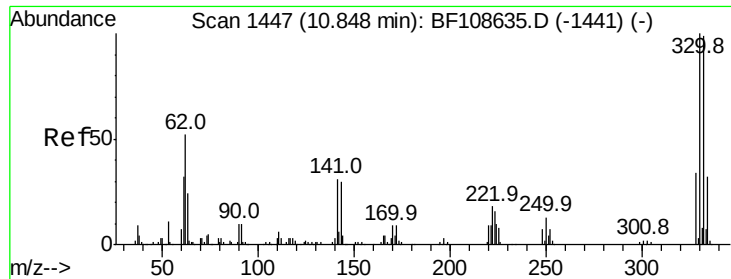


#41
 2,4,6-Tribromophenol
 Concen: 81.186 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108662.D
 Acq: 31 Aug 2018 1:16

Instrument :
 BNA_F
 ClientSampleId :
 082818-SIDI-F-D-S

Tot Ion	Ratio	Resp	Lower	Upper
330	100	169236		
332	92.6	77.0	115.6	
141	32.6	29.9	44.9	

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:18:34 PM



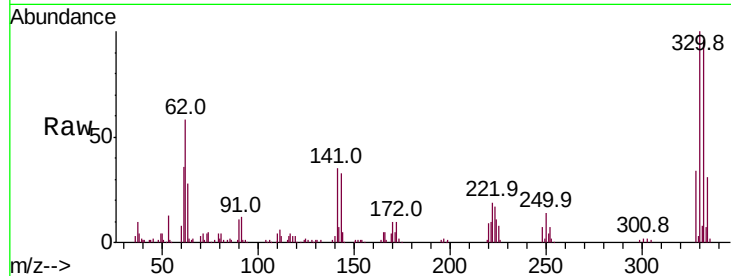


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

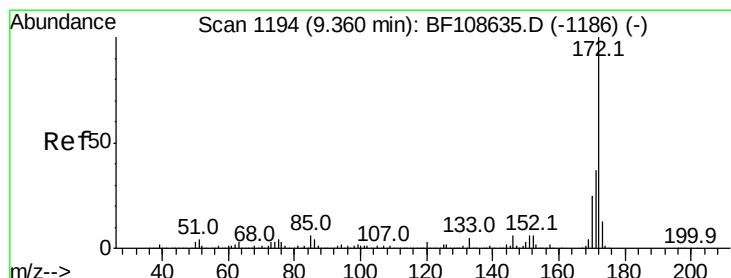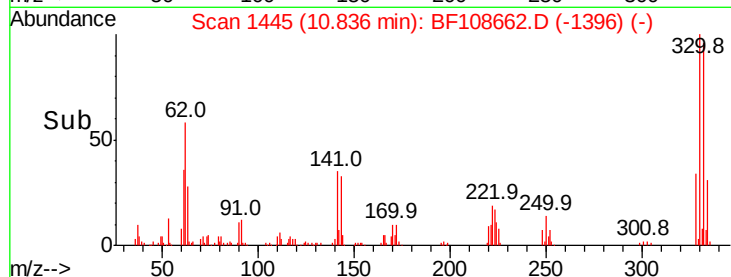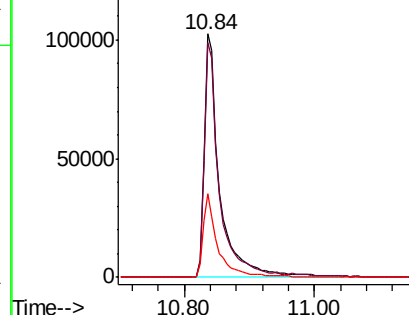

#44
 2-Fluorobiphenyl
 Concen: 108.703 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108662.D
 Acq: 31 Aug 2018 1:16

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	1276602		
171	35.9	29.7	44.5	
170	24.3	19.6	29.4	


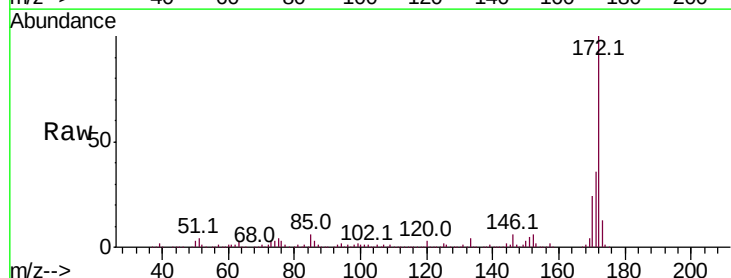



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

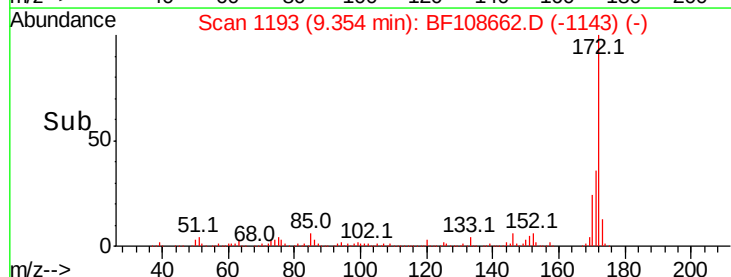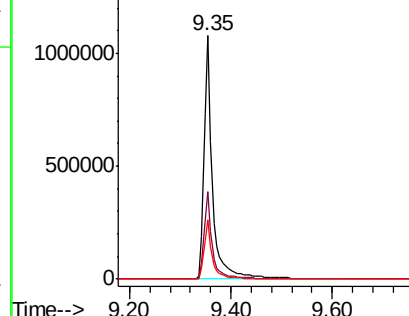

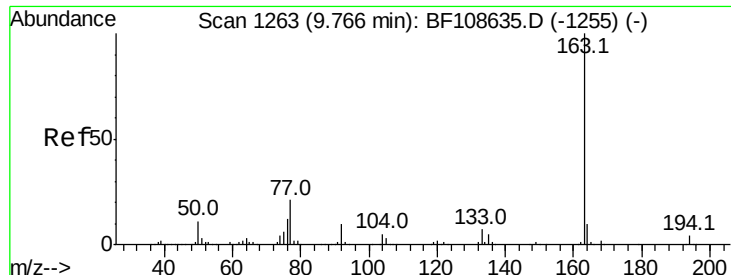


#49
Dimethylphthalate
Concen: 9.197 ng
RT: 9.75 min Scan# 1260
Delta R.T. -0.02 min
Lab File: BF108662.D
Acq: 31 Aug 2018 1:16

Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-D-S




Tot Ion	Ratio	Resp	Lower	Upper
163	100			
194	4.0	2.7	4.1	
164	9.6	8.2	12.2	

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:34 PM

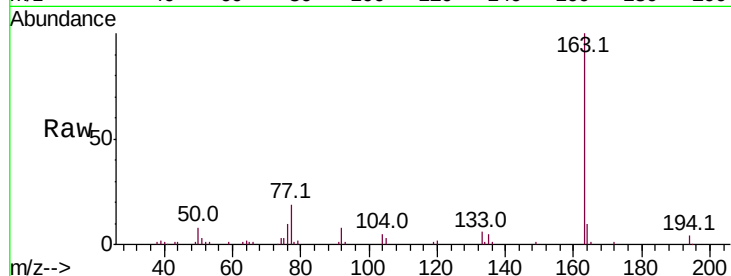


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

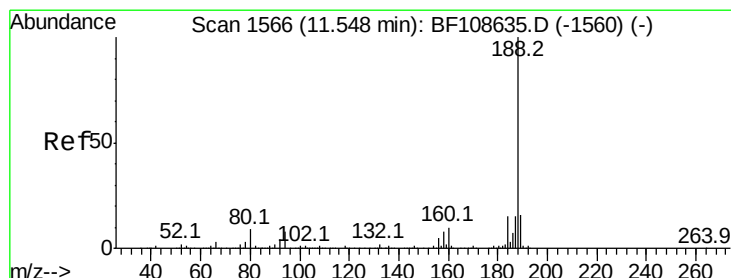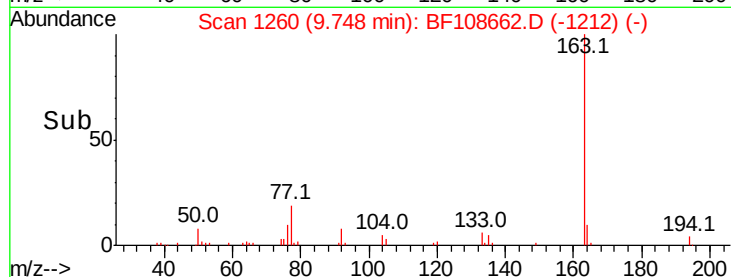
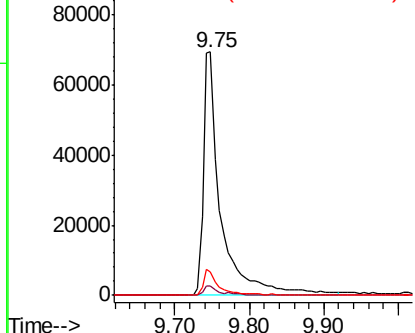



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1565
Delta R.T. -0.01 min
Lab File: BF108662.D
Acq: 31 Aug 2018 1:16

Tgt Ion	Ratio	Resp	Lower	Upper
188	100			
94	7.2	8.5	12.7#	
80	8.8	9.2	13.8#	

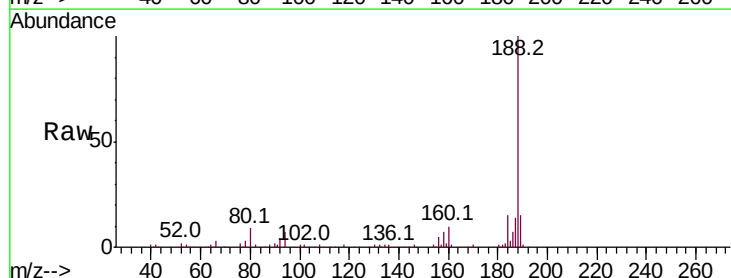

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

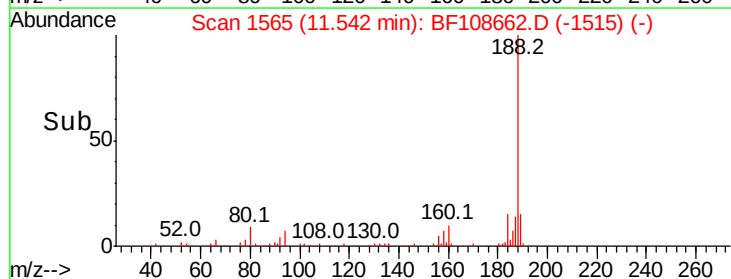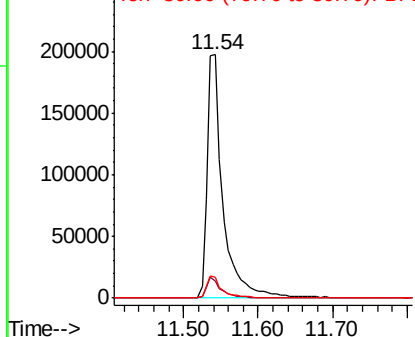

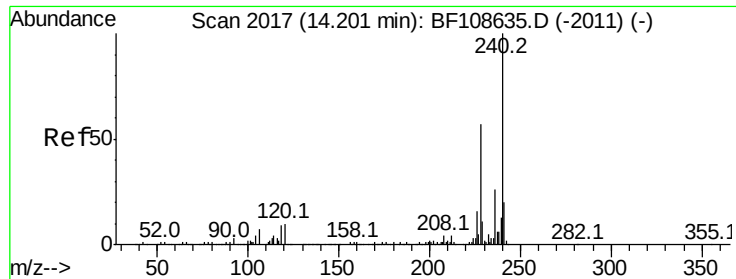

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 2015

Delta R.T. -0.01 min

Lab File: BF108662.D

Acq: 31 Aug 2018 1:16

Instrument :

BNA_F





ClientSampleId :

082818-SIDI-F-D-S

Tot Ion	Ratio	Lower	Upper
240	100		
120	9.7	9.5	14.3
236	25.6	20.7	31.1

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:34 PM

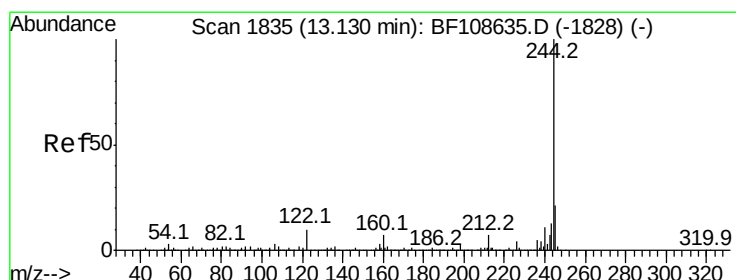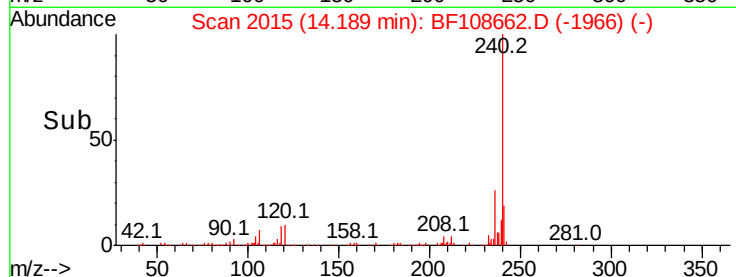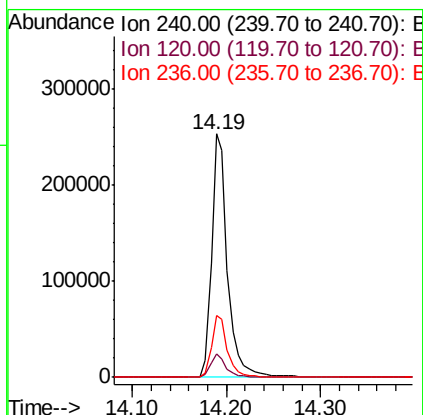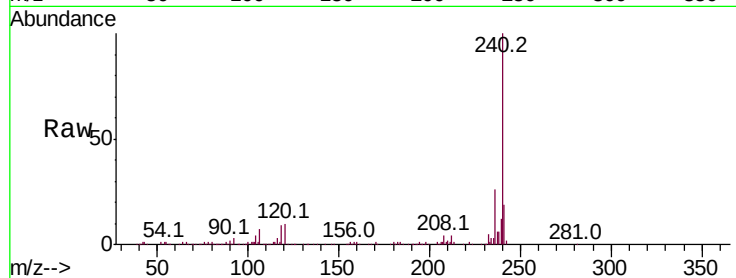

#78

Terphenyl-d14

Concen: 72.557 ng




RT: 13.12 min Scan# 1833


Delta R.T. -0.01 min

Lab File: BF108662.D

Acq: 31 Aug 2018 1:16

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.2	5.4	8.0
122	10.5	11.0	16.4#

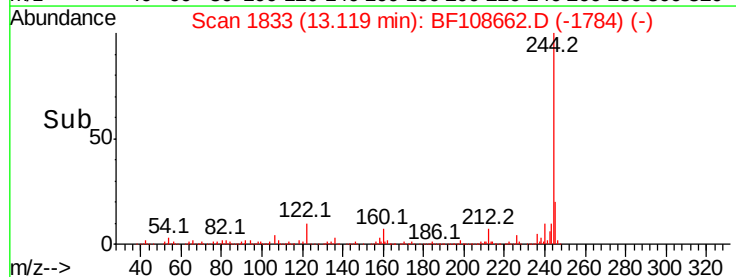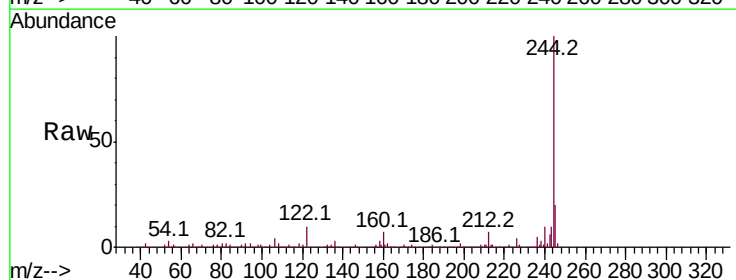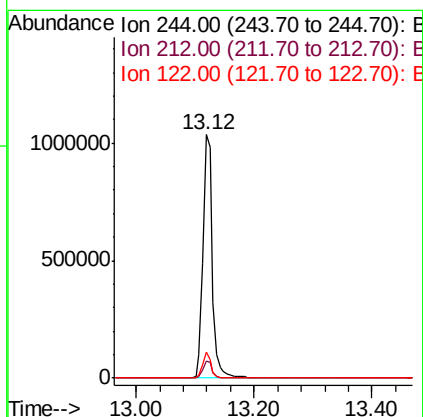

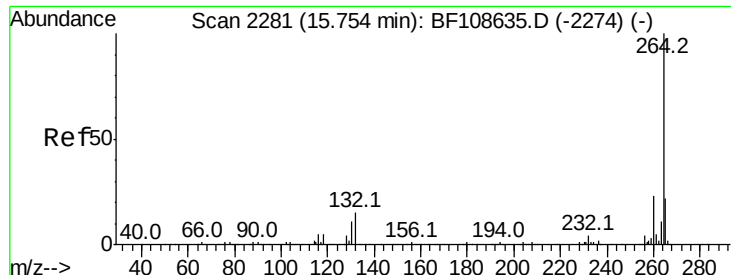

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.75 min Scan# 2280
 Delta R.T. -0.01 min
 Lab File: BF108662.D
 Acq: 31 Aug 2018 1:16

Instrument :
 BNA_F
 ClientSampleId :
 082818-SIDI-F-D-S

Tot Ion:	264	Resp:	246457
Ion Ratio	Lower	Upper	
264	100		
260	23.5	19.2	28.8
265	21.1	17.5	26.3

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:18:34 PM

