

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
 Data File : BF108663.D
 Acq On : 31 Aug 2018 1:43
 Operator : JU/SJ
 Sample : J4700-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082818-SIDI-F-U-B

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:18:37 PM

Quant Time: Aug 31 11:10:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 30 15:06:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	80919	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	345520	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	175173	20.00	ng	0.00
63) Phenanthrene-d10	11.54	188	345373	20.00	ng	-0.01
75) Chrysene-d12	14.19	240	322205	20.00	ng	0.00
86) Perylene-d12	15.75	264	267471	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.68	112	126508m	27.16	ng	0.03
7) Phenol-d6	6.66	99	133695	20.04	ng	0.01
23) Nitrobenzene-d5	7.57	82	621376	91.28	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	177114	76.59	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	1252064	96.10	ng	0.00
78) Terphenyl-d14	13.12	244	1228334	74.07	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.74	163	130678	9.473	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
Data File : BF108663.D
Acq On : 31 Aug 2018 1:43
Operator : JU/SJ
Sample : J4700-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-U-B

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:37 PM

Quant Time: Aug 31 11:10:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

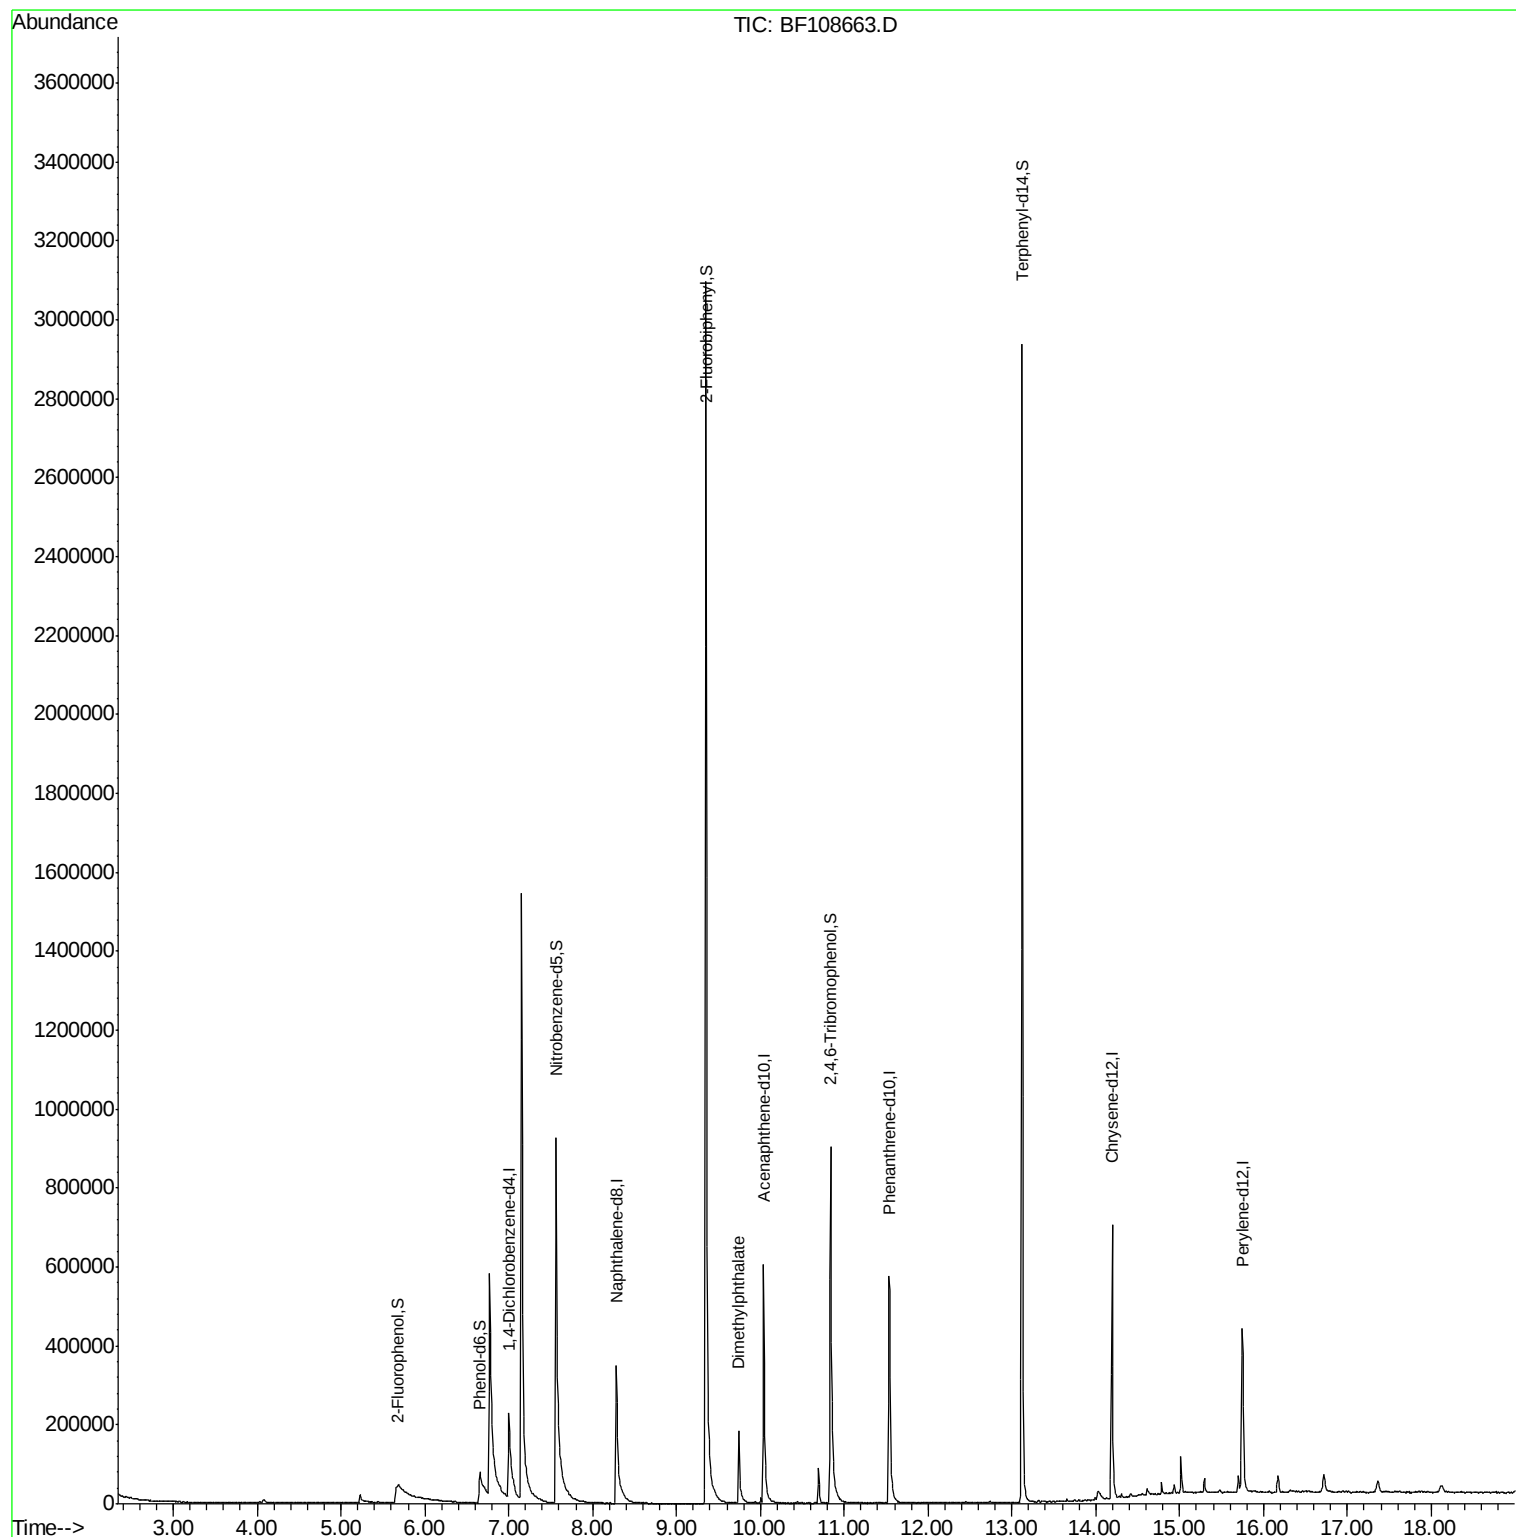



#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.00 min Scan# 793
Delta R.T. -0.01 min
Lab File: BF108663.D
Acq: 31 Aug 2018 1:43

Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-U-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	145.7	124.6	186.8
115	57.2	50.1	75.1

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:37 PM


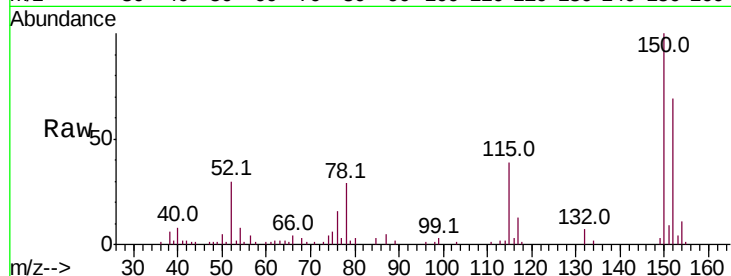


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

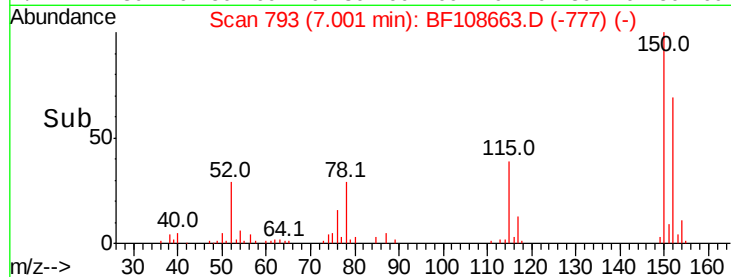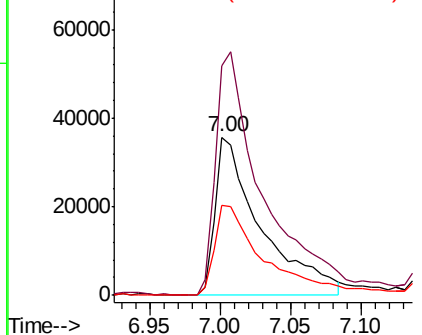

#5

2-Fluorophenol
Concen: 27.159 ng m
RT: 5.68 min Scan# 568
Delta R.T. 0.03 min
Lab File: BF108663.D
Acq: 31 Aug 2018 1:43




Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.6	47.9	71.9
63	35.6	23.7	35.5


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

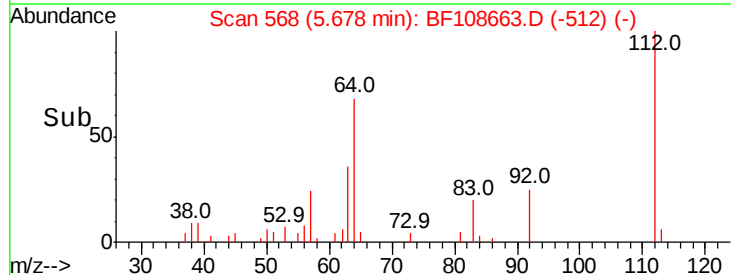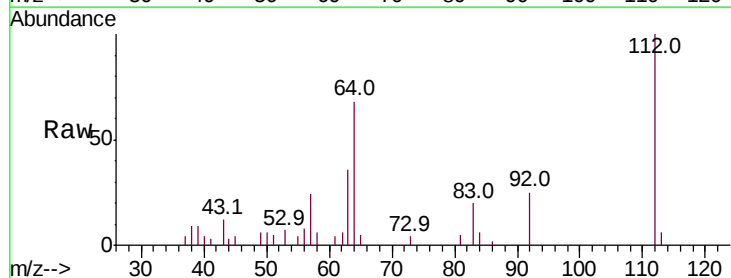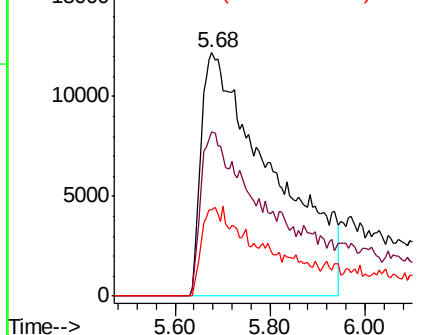

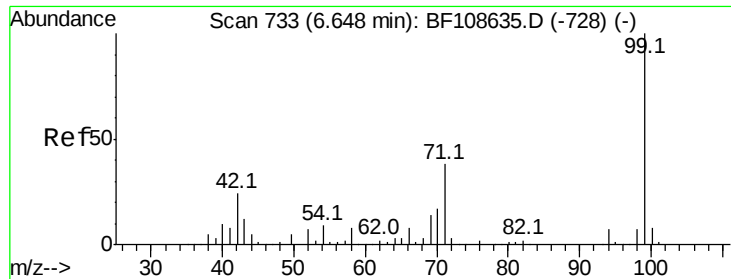

#7

Phenol-d6

Concen: 20.040 ng

RT: 6.66 min Scan# 735

Delta R.T. 0.01 min

Lab File: BF108663.D

Acq: 31 Aug 2018 1:43

Instrument :

BNA_F





ClientSampleId :

082818-SIDI-F-U-B

Tot Ion:	99	Resp:	133695
Ion Ratio	Lower	Upper	
99	100		
42	19.8	14.5	21.7
71	34.8	25.4	38.0

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:37 PM

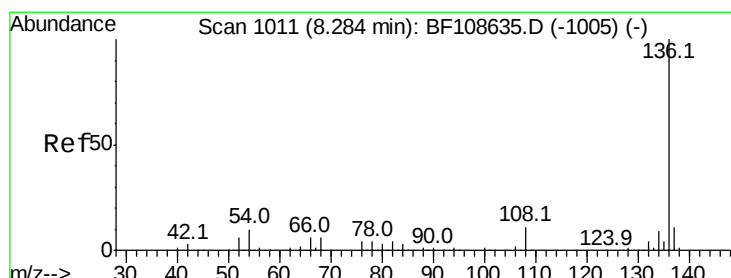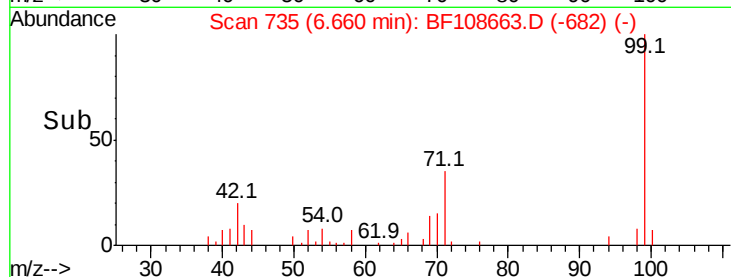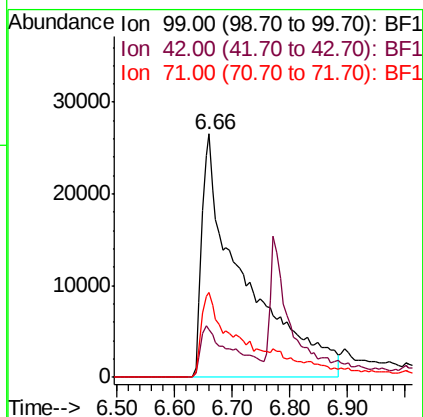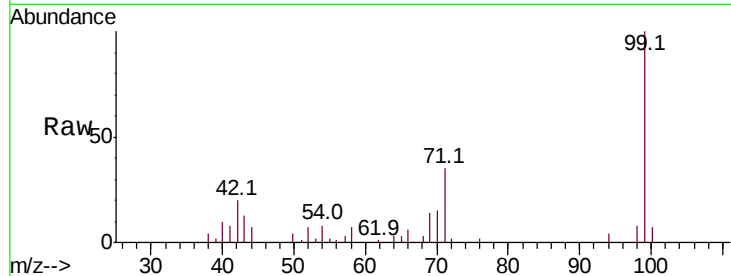

#21

Naphthalene-d8

Concen: 20.000 ng




RT: 8.28 min Scan# 1011

Delta R.T. -0.00 min

Lab File: BF108663.D

Acq: 31 Aug 2018 1:43

Tgt Ion:	136	Resp:	345520
Ion Ratio	Lower	Upper	
136	100		
137	10.8	8.9	13.3
54	9.3	6.6	9.8
68	5.9	5.0	7.4

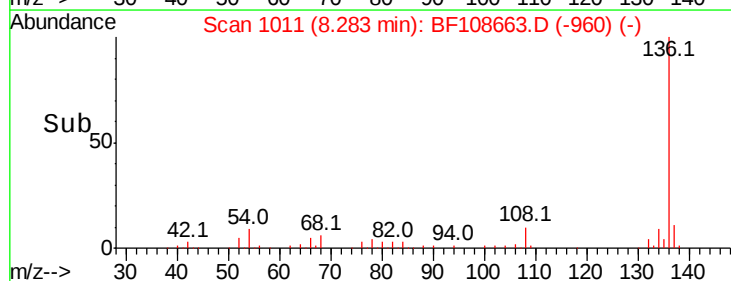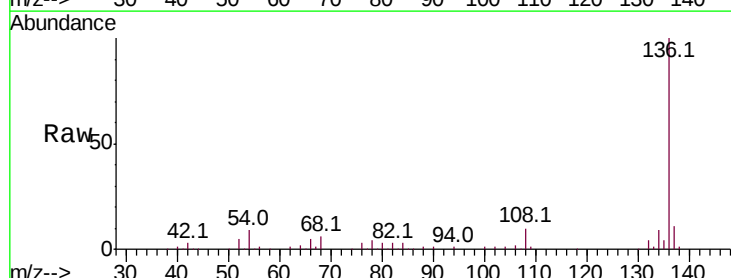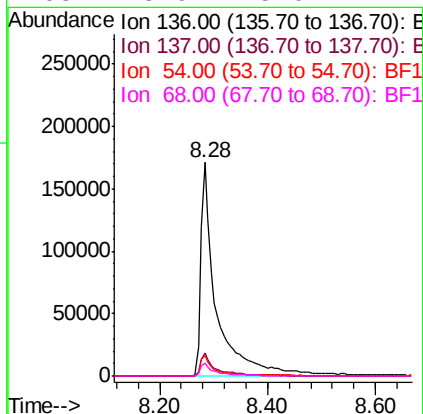







#23
Nitrobenzene-d5
Concen: 91.283 ng
RT: 7.57 min Scan# 889
Delta R.T. -0.01 min
Lab File: BF108663.D
Acq: 31 Aug 2018 1:43

Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-U-B

Tot Ion	Ratio	Lower	Upper
82	100		
128	41.9	36.1	54.1
54	58.3	41.4	62.2




Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:37 PM

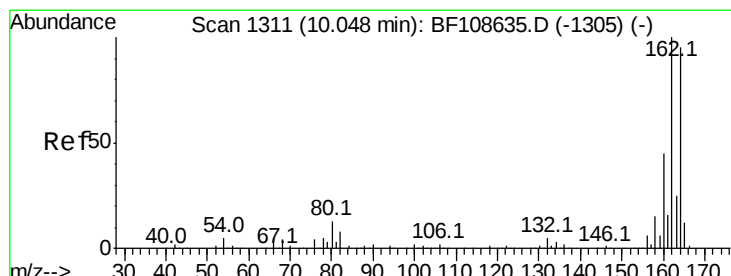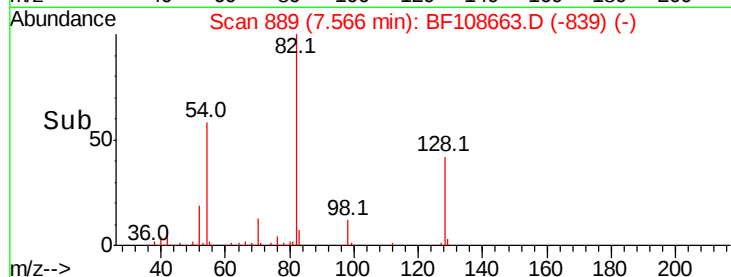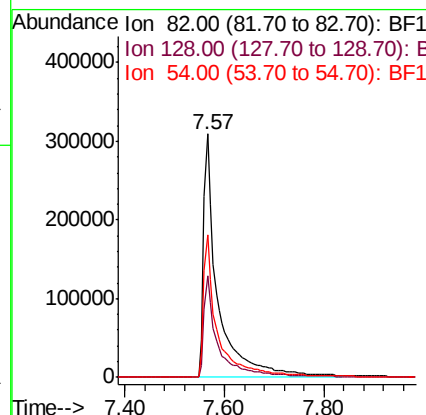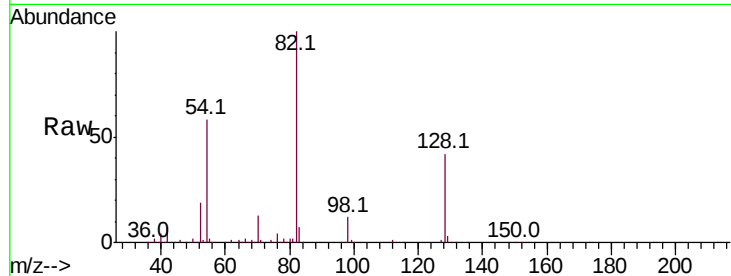

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.04 min Scan# 1310
Delta R.T. -0.01 min
Lab File: BF108663.D
Acq: 31 Aug 2018 1:43

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.2	86.1	129.1
160	46.3	38.3	57.5

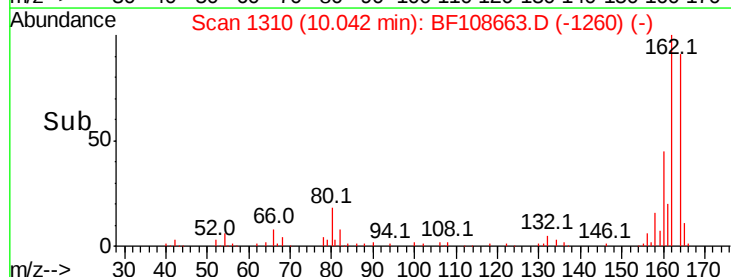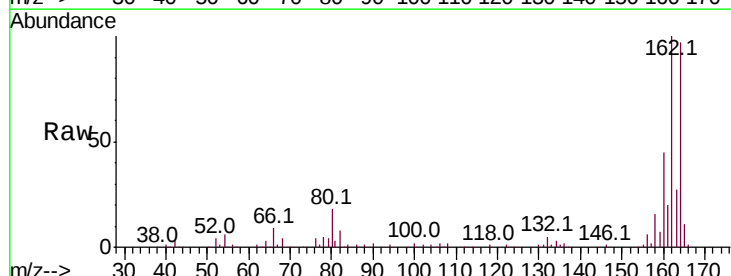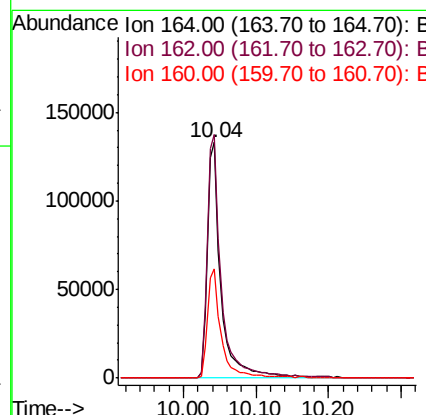




#41
 2,4,6-Tribromophenol
 Concen: 76.590 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108663.D
 Acq: 31 Aug 2018 1:43

Instrument :
 BNA_F
 ClientSampleId :
 082818-SIDI-F-U-B

Tot Ion	Ratio	Resp	Lower	Upper
330	100	177114		
332	96.9	77.0	115.6	
141	32.8	29.9	44.9	

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:18:37 PM



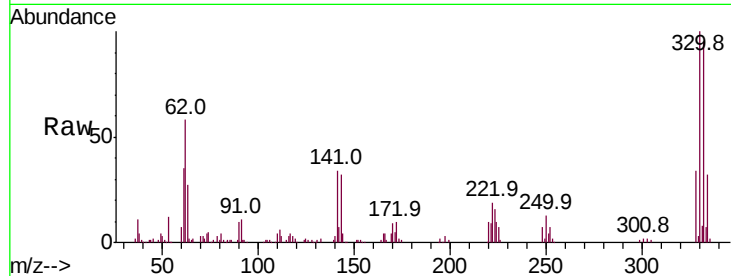


Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

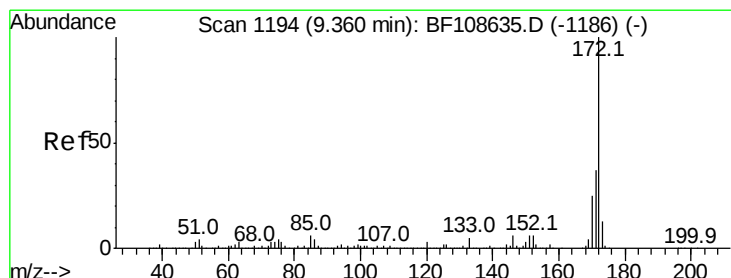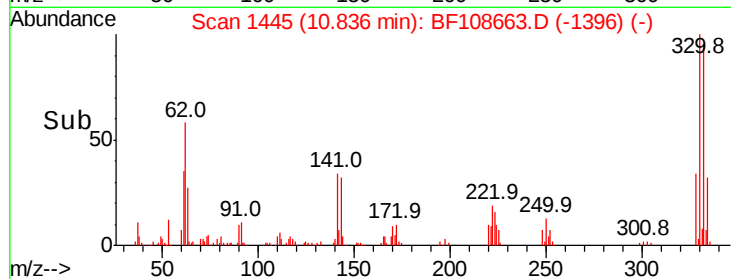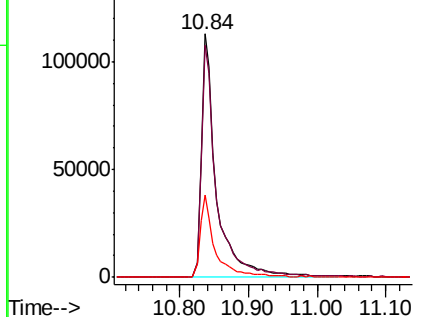

#44
 2-Fluorobiphenyl
 Concen: 96.105 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108663.D
 Acq: 31 Aug 2018 1:43




Tgt Ion	Ratio	Resp	Lower	Upper
172	100	1252064		
171	35.8	29.7	44.5	
170	24.3	19.6	29.4	

Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

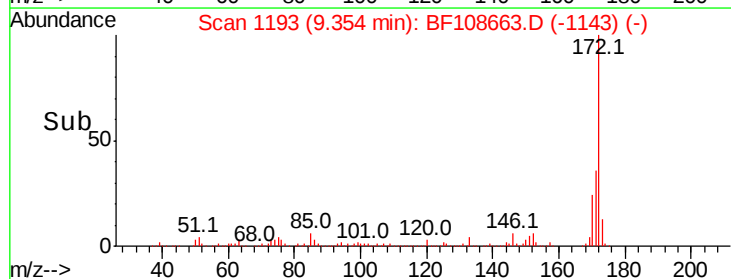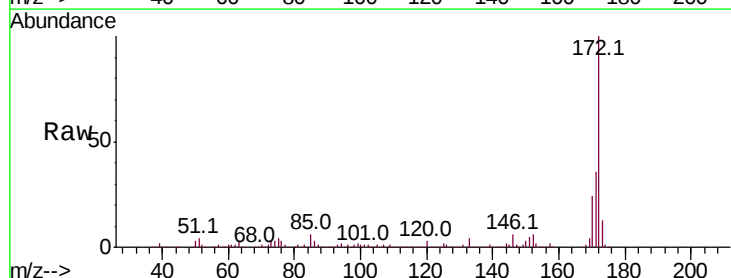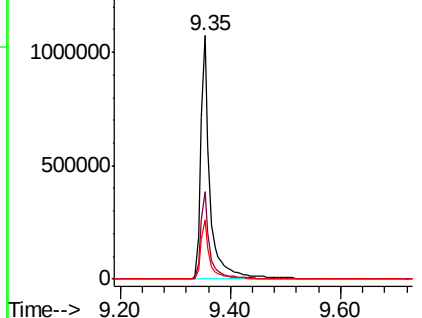







#49
Dimethylphthalate
Concen: 9.473 ng
RT: 9.74 min Scan# 1259
Delta R.T. -0.02 min
Lab File: BF108663.D
Acq: 31 Aug 2018 1:43

Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-U-B

Tot Ion	163	Resp	130678
Ion Ratio	Lower	Upper	
163	100		
194	3.9	2.7	4.1
164	10.9	8.2	12.2




Manual Integrations
APPROVED


Sohil
8/31/2018 12:18:37 PM

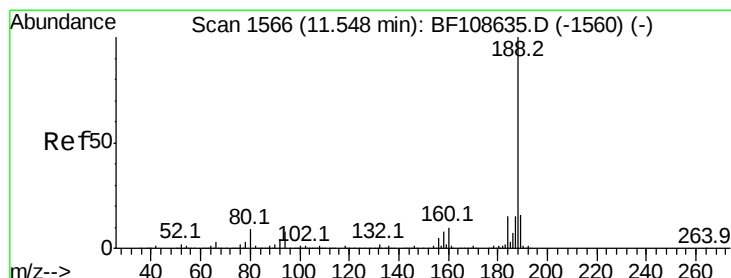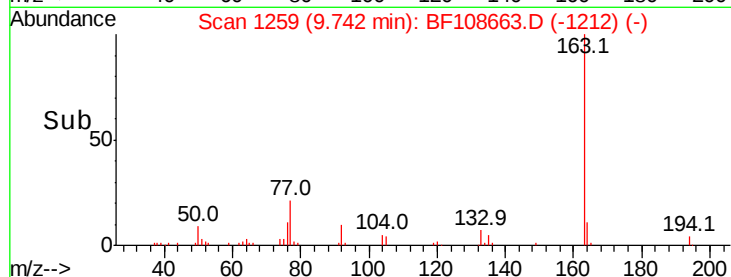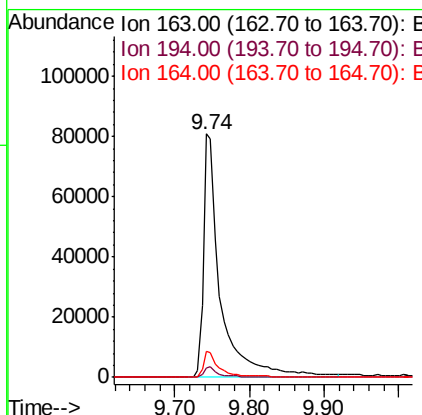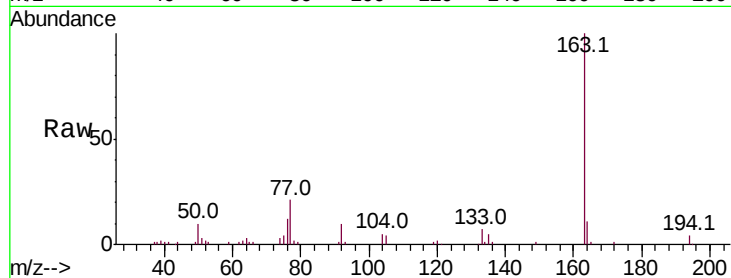

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1564
Delta R.T. -0.01 min
Lab File: BF108663.D
Acq: 31 Aug 2018 1:43

Tgt Ion	188	Resp	345373
Ion Ratio	Lower	Upper	
188	100		
94	8.9	8.5	12.7
80	10.1	9.2	13.8

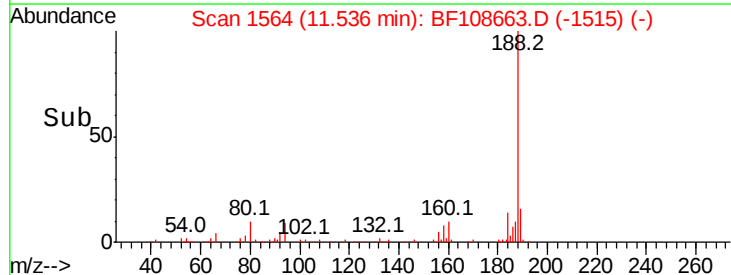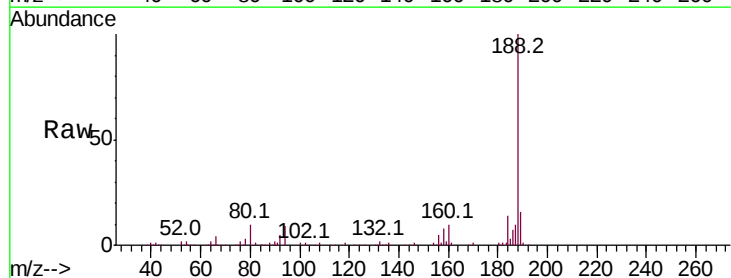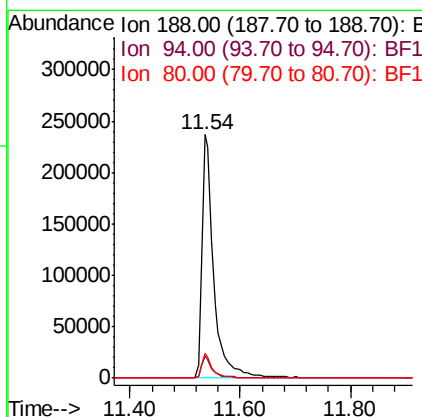

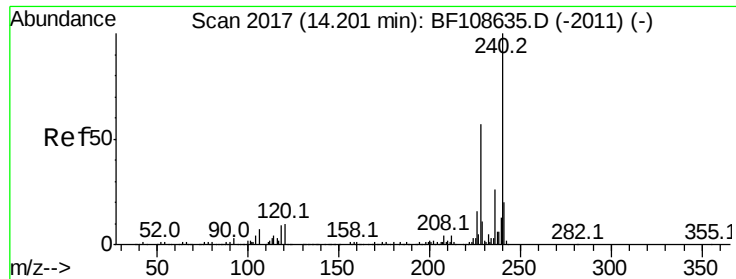

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 2016

Delta R.T. -0.01 min

Lab File: BF108663.D

Acq: 31 Aug 2018 1:43

Instrument :

BNA_F





ClientSampleId :

082818-SIDI-F-U-B

Tot Ion	Ratio	Lower	Upper
240	100		
120	8.1	9.5	14.3#
236	25.5	20.7	31.1

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:37 PM

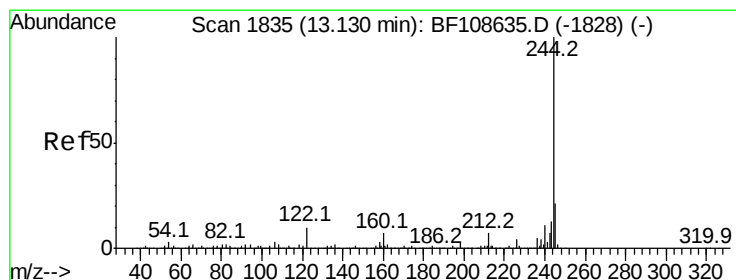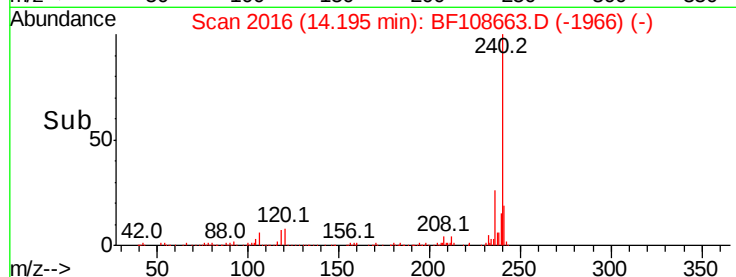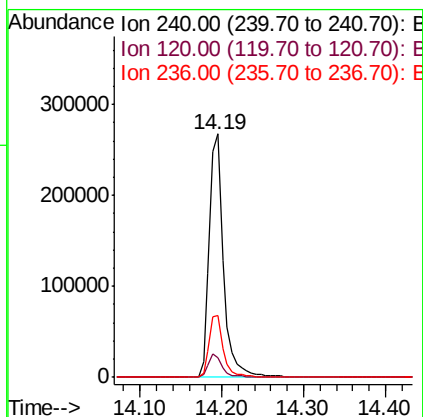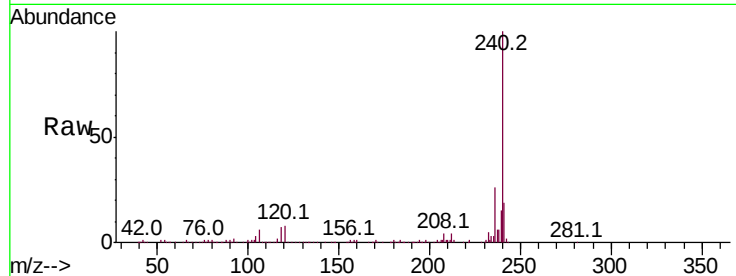

#78

Terphenyl-d14

Concen: 74.071 ng




RT: 13.12 min Scan# 1834




Delta R.T. -0.01 min

Lab File: BF108663.D

Acq: 31 Aug 2018 1:43

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.1	5.4	8.0
122	8.9	11.0	16.4#

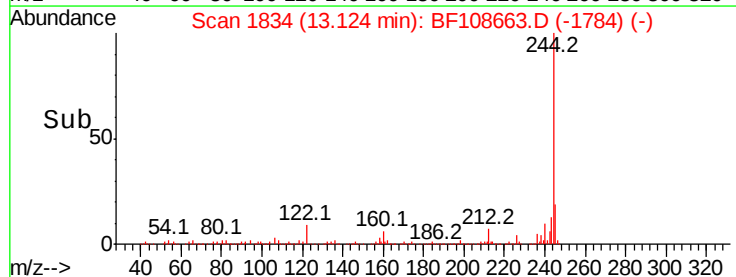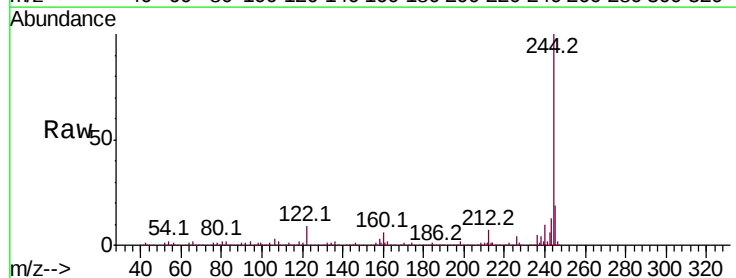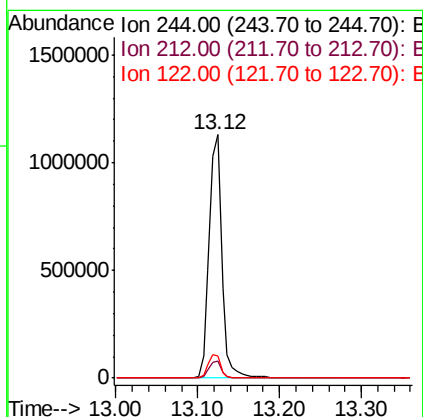

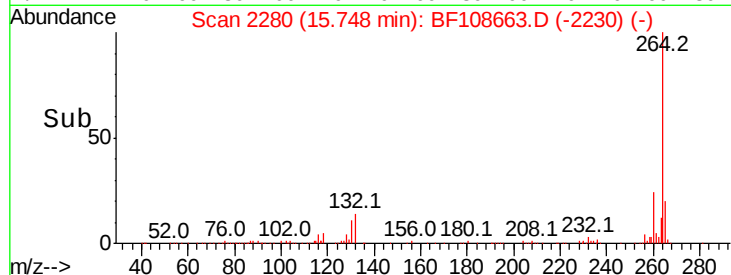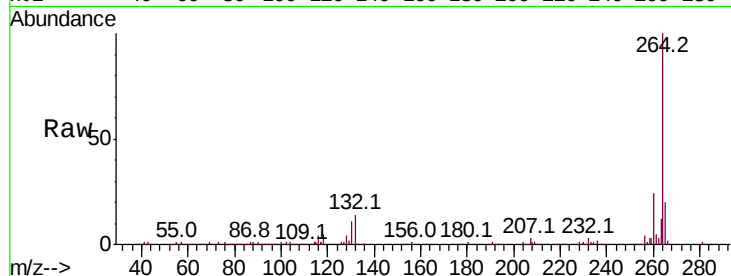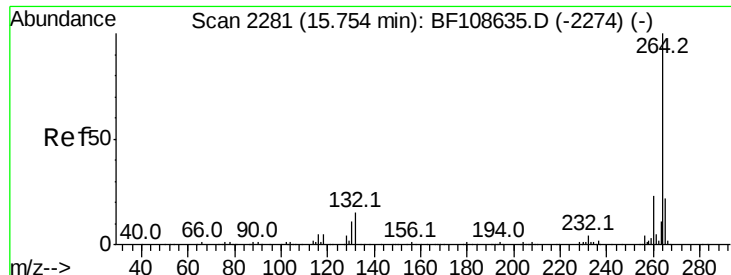

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.75 min Scan# 2280
Delta R.T. -0.01 min
Lab File: BF108663.D
Acq: 31 Aug 2018 1:43

Instrument :
BNA_F
ClientSampleId :
082818-SIDI-F-U-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.2	28.8
265	20.3	17.5	26.3

Manual Integrations
APPROVED

Sohil
8/31/2018 12:18:37 PM

