

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
 Data File : BF108676.D
 Acq On : 31 Aug 2018 8:07
 Operator : JU/SJ
 Sample : J4700-14
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082818-JETT-F-U-B

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:19:09 PM

Quant Time: Aug 31 11:05:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 30 15:06:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	82313	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	343126	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	166015	20.00	ng	0.00
63) Phenanthrene-d10	11.54	188	306454	20.00	ng	0.00
75) Chrysene-d12	14.19	240	304247	20.00	ng	-0.01
86) Perylene-d12	15.75	264	258512	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	132897m	28.05	ng	0.04
7) Phenol-d6	6.66	99	142420	20.99	ng	0.01
23) Nitrobenzene-d5	7.57	82	629890	93.18	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	168661	76.96	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	1266376	102.57	ng	0.00
78) Terphenyl-d14	13.12	244	1164822	74.39	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.74	163	166987	12.773	ng	Qvalue # 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
Data File : BF108676.D
Acq On : 31 Aug 2018 8:07
Operator : JU/SJ
Sample : J4700-14
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
082818-JETT-F-U-B

Manual Integrations
APPROVED

Sohil
8/31/2018 12:19:09 PM

Quant Time: Aug 31 11:05:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

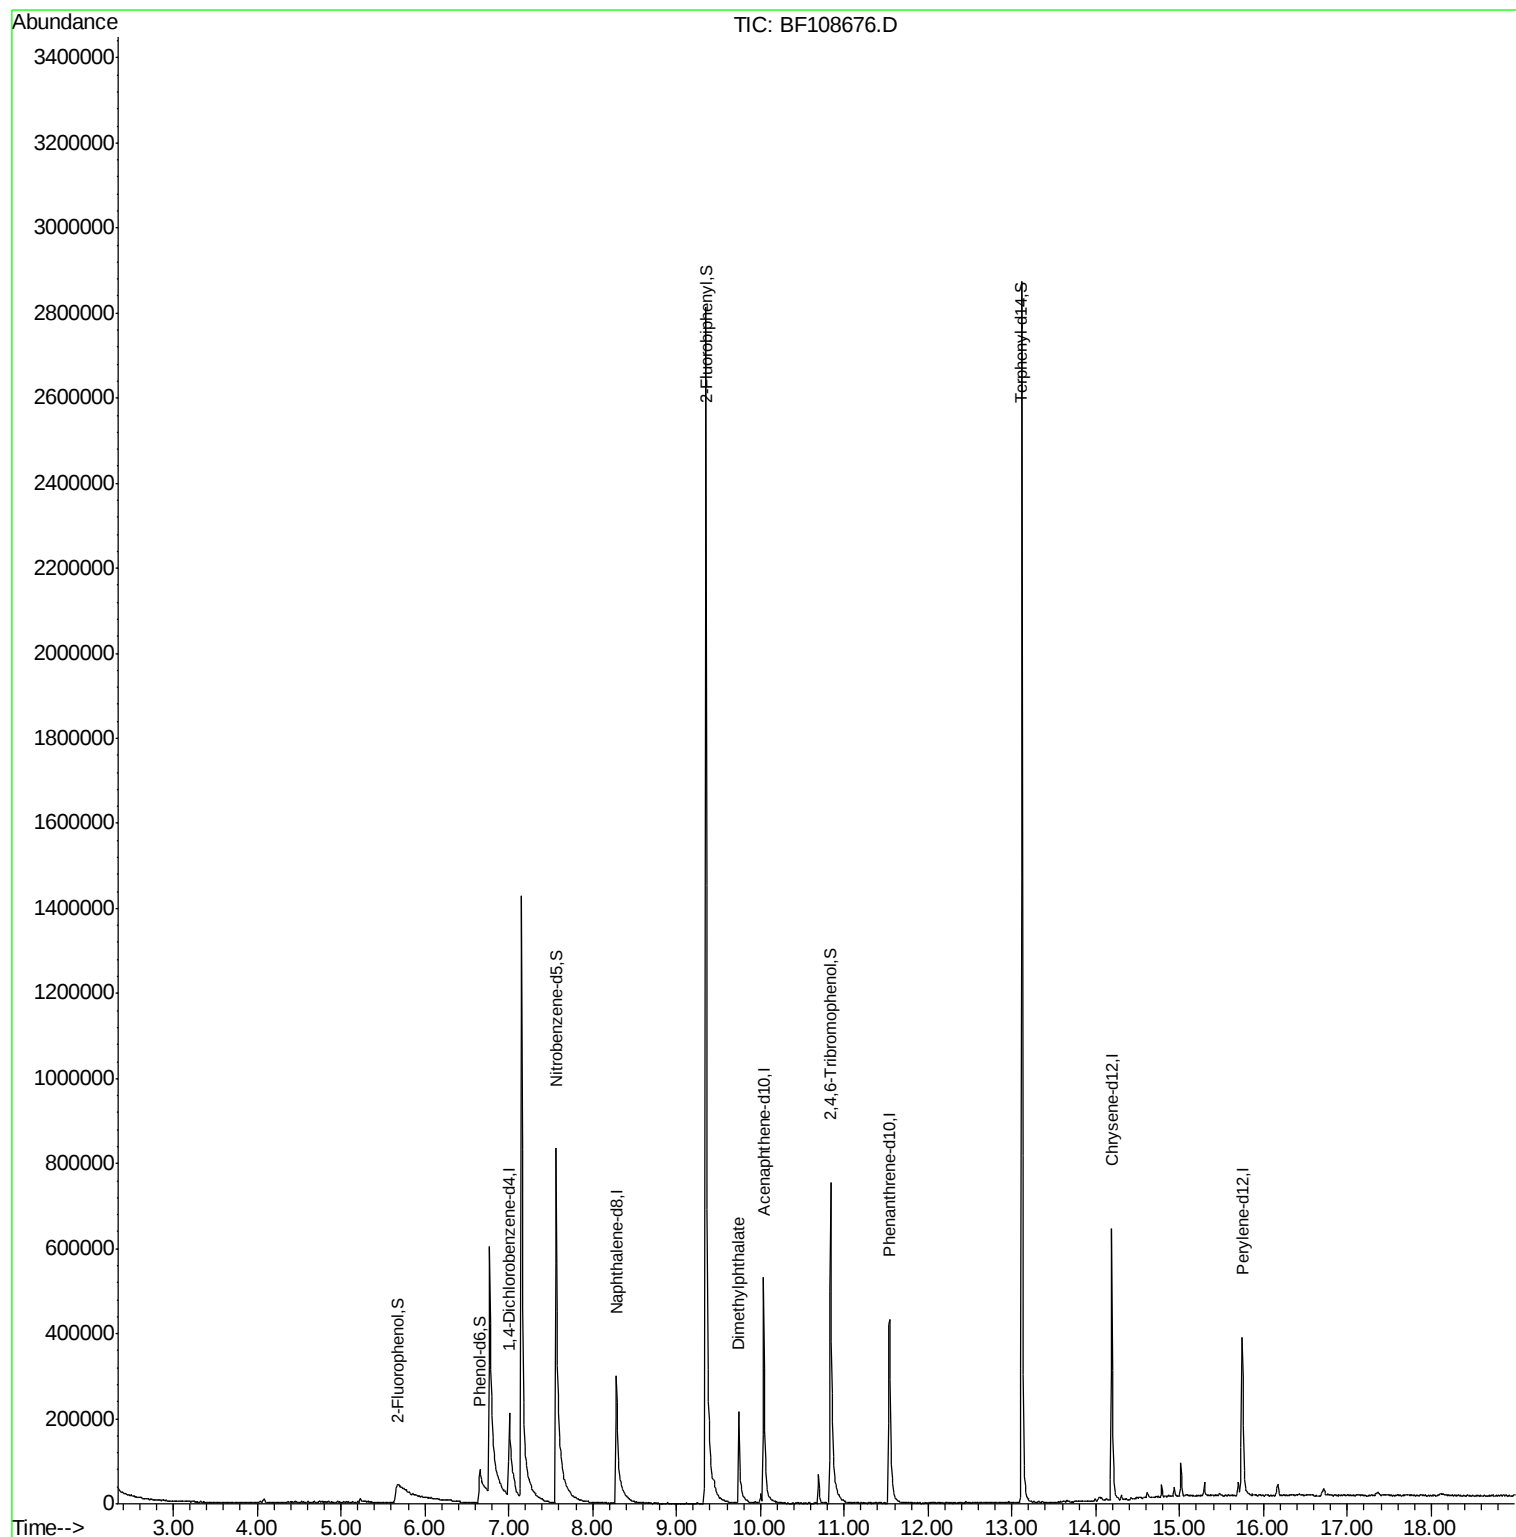

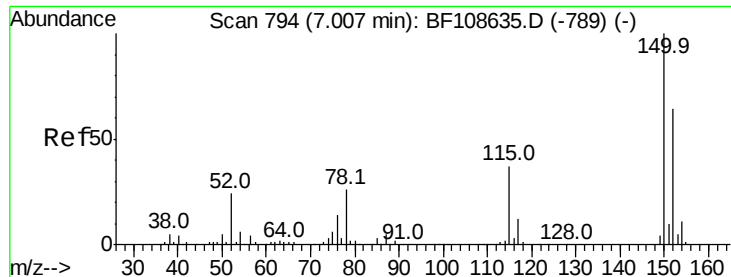

#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.01 min Scan# 794
Delta R.T. 0.00 min
Lab File: BF108676.D
Acq: 31 Aug 2018 8:07

Instrument :
BNA_F
ClientSampleId :
082818-JETT-F-U-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	163.3	124.6	186.8
115	60.4	50.1	75.1

Manual Integrations
APPROVED

Sohil
8/31/2018 12:19:09 PM


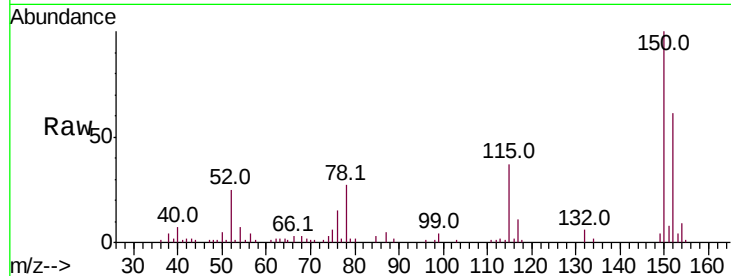


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

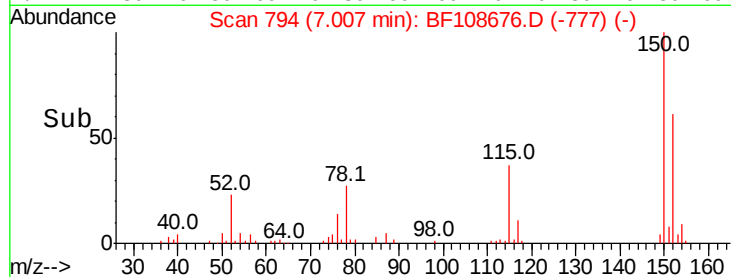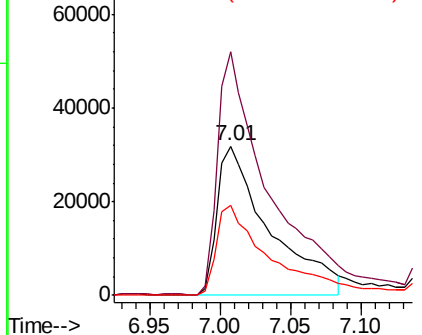

#5

2-Fluorophenol
Concen: 28.048 ng m
RT: 5.69 min Scan# 570
Delta R.T. 0.04 min
Lab File: BF108676.D
Acq: 31 Aug 2018 8:07




Tgt Ion	Ratio	Lower	Upper
112	100		
64	64.0	47.9	71.9
63	29.9	23.7	35.5


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

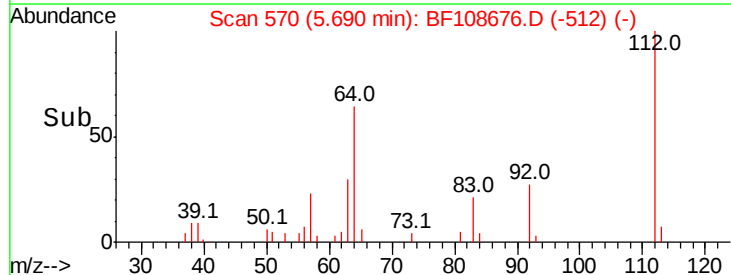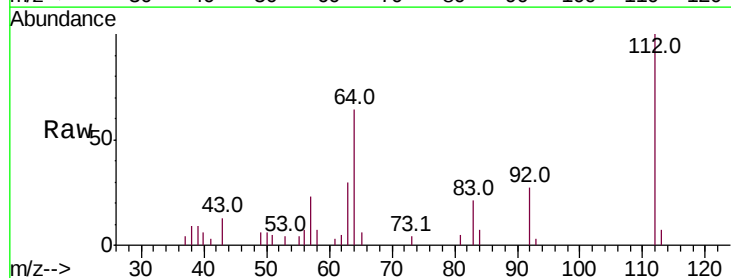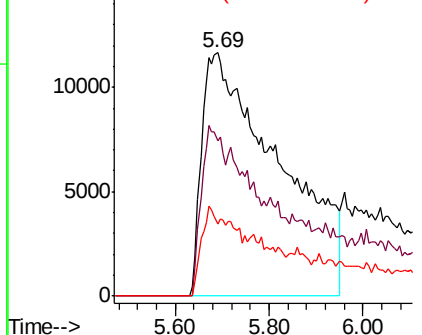

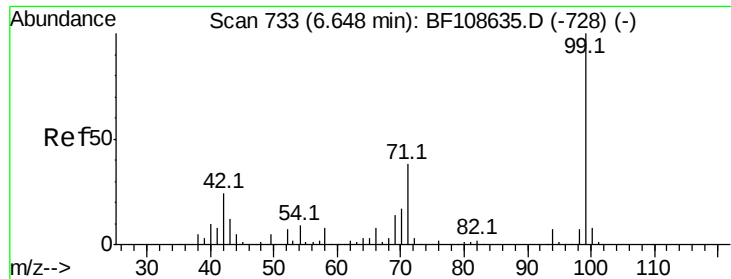

#7

Phenol-d6

Concen: 20.986 ng

RT: 6.66 min Scan# 735

Delta R.T. 0.01 min

Lab File: BF108676.D

Acq: 31 Aug 2018 8:07

Instrument :

BNA_F


ClientSampleId :

082818-JETT-F-U-B




Tot Ion:	99	Resp:	142420
Ion Ratio	Lower	Upper	
99	100		
42	20.6	14.5	21.7
71	32.4	25.4	38.0

Manual Integrations
APPROVED

Sohil
8/31/2018 12:19:09 PM

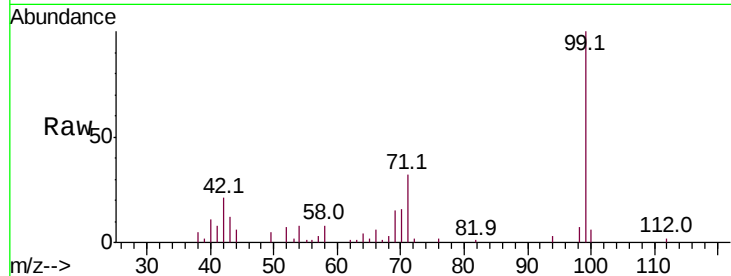

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

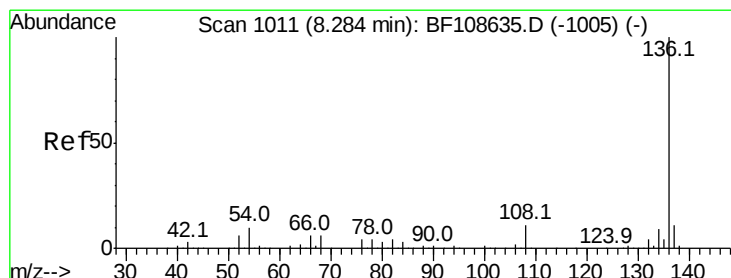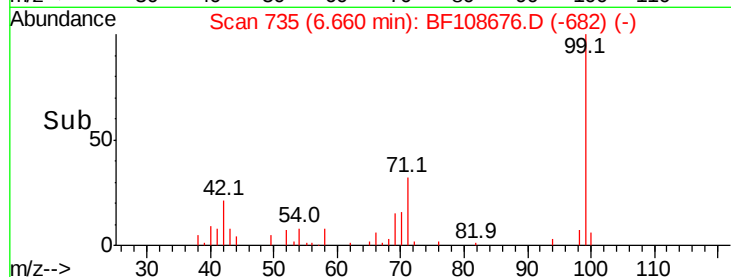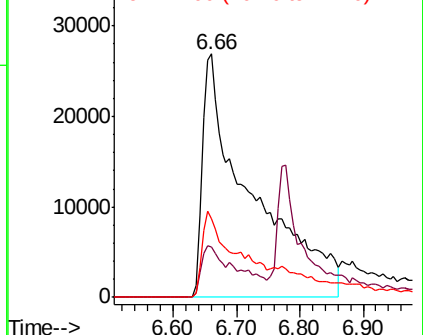

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.28 min Scan# 1011




Delta R.T. 0.00 min


Lab File: BF108676.D

Acq: 31 Aug 2018 8:07

Tgt Ion:	136	Resp:	343126
Ion Ratio	Lower	Upper	
136	100		
137	10.7	8.9	13.3
54	9.7	6.6	9.8
68	5.8	5.0	7.4

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

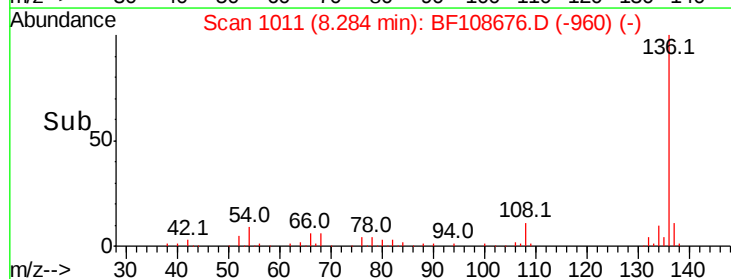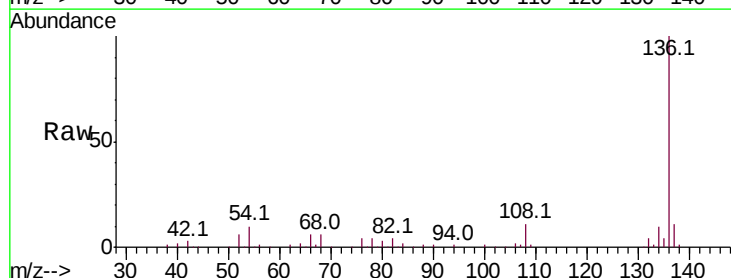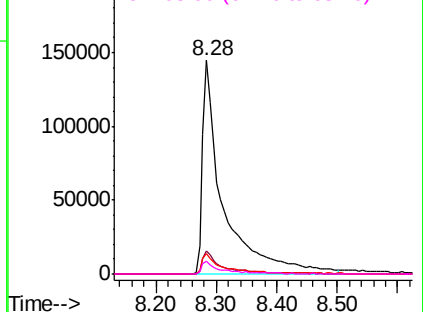

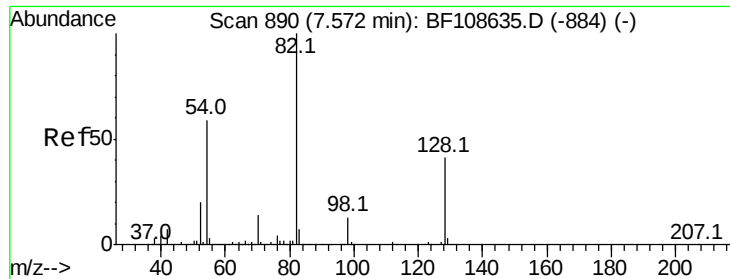


#23
 Nitrobenzene-d5
 Concen: 93.180 ng
 RT: 7.57 min Scan# 889
 Delta R.T. -0.01 min
 Lab File: BF108676.D
 Acq: 31 Aug 2018 8:07

Instrument :
 BNA_F
 ClientSampleId :
 082818-JETT-F-U-B

Tot Ion	Ratio	Lower	Upper
82	100		
128	40.9	36.1	54.1
54	56.3	41.4	62.2

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:19:09 PM



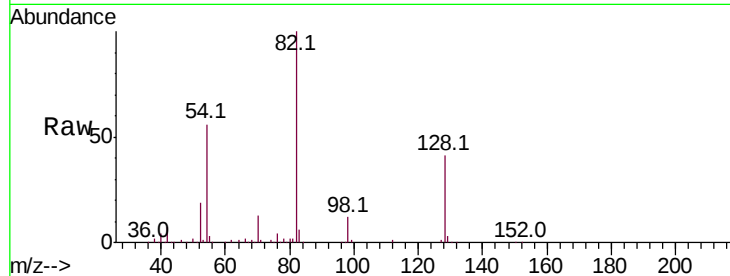


Abundance

Ion 82.00 (81.70 to 82.70): BF1


Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

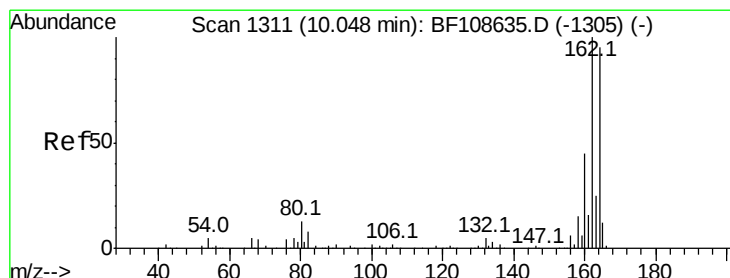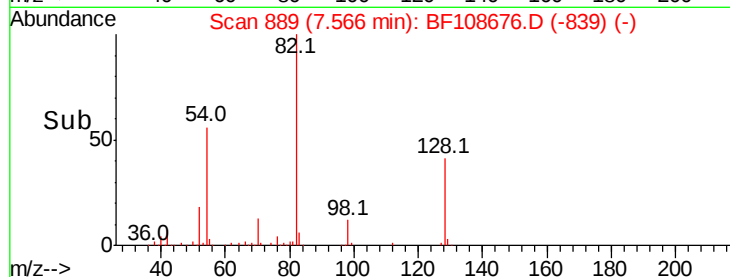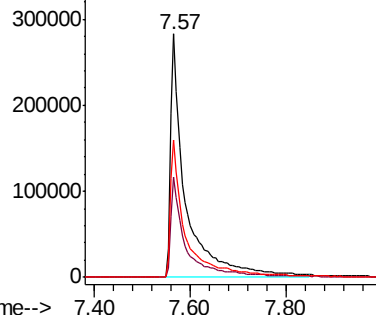

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.04 min Scan# 1310
 Delta R.T. -0.01 min
 Lab File: BF108676.D
 Acq: 31 Aug 2018 8:07

Tgt Ion	Ratio	Lower	Upper
164	100		
162	102.1	86.1	129.1
160	48.1	38.3	57.5


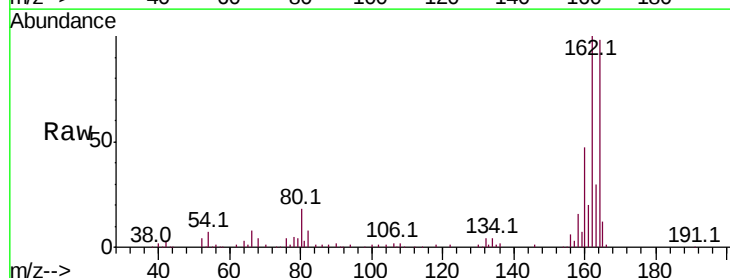



Abundance

Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1

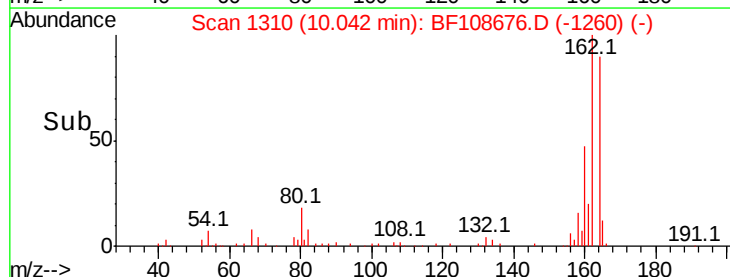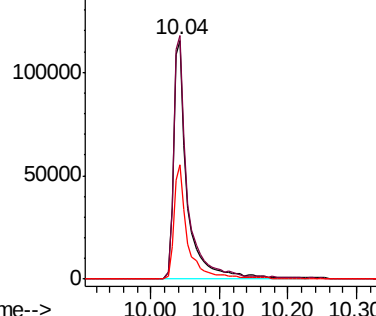

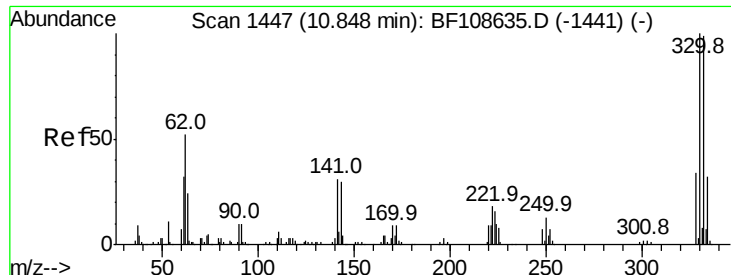


#41
 2,4,6-Tribromophenol
 Concen: 76.958 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108676.D
 Acq: 31 Aug 2018 8:07

Instrument :
 BNA_F
 ClientSampleId :
 082818-JETT-F-U-B

Tot Ion	Ratio	Resp	Lower	Upper
330	100	168661		
332	94.2	77.0	115.6	
141	32.1	29.9	44.9	

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:19:09 PM



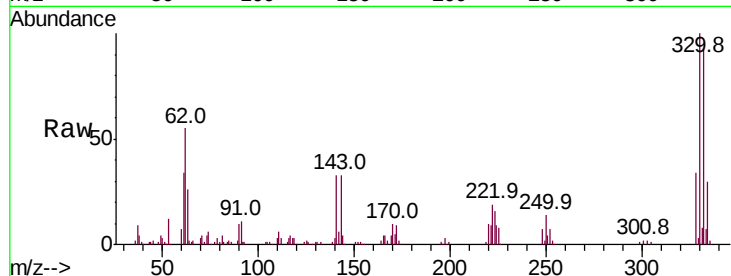


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

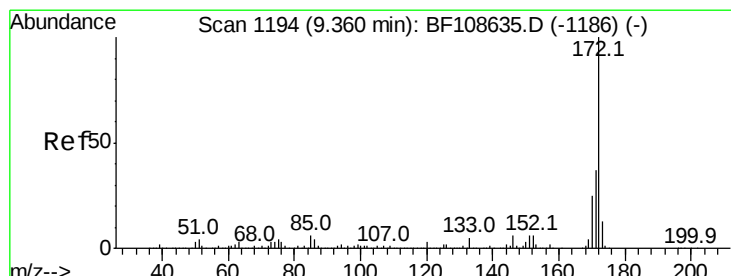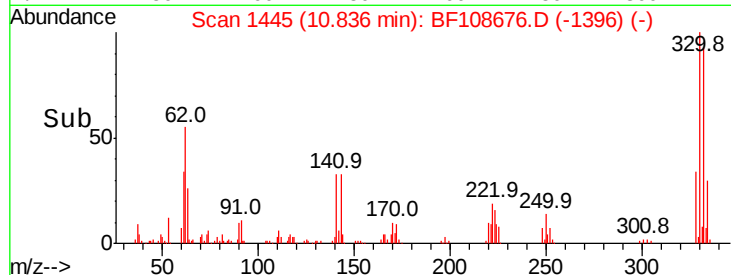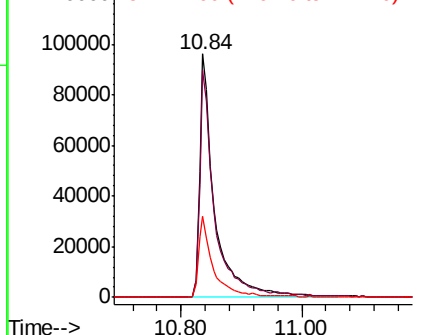

#44
 2-Fluorobiphenyl
 Concen: 102.565 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108676.D
 Acq: 31 Aug 2018 8:07

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	1266376		
171	36.5	29.7	44.5	
170	24.3	19.6	29.4	


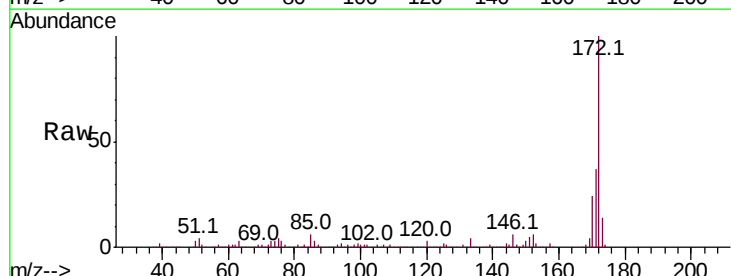


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

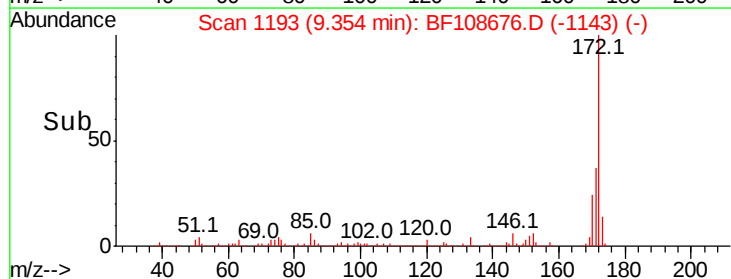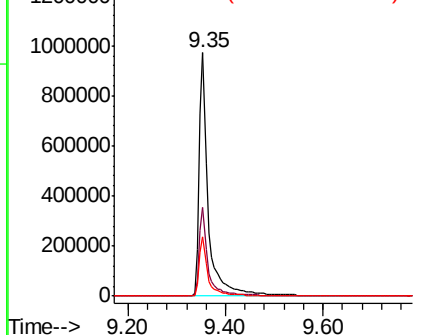




#49
Dimethylphthalate
Concen: 12.773 ng
RT: 9.74 min Scan# 1259
Delta R.T. -0.02 min
Lab File: BF108676.D
Acq: 31 Aug 2018 8:07

Instrument :
BNA_F
ClientSampleId :
082818-JETT-F-U-B




Tot Ion	Ratio	Resp	Lower	Upper
163	100	166987		
194	4.5	2.7	4.1#	
164	10.1	8.2	12.2	

Manual Integrations
APPROVED

Sohil
8/31/2018 12:19:09 PM

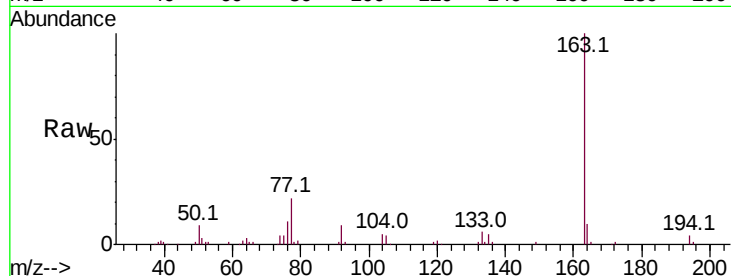


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

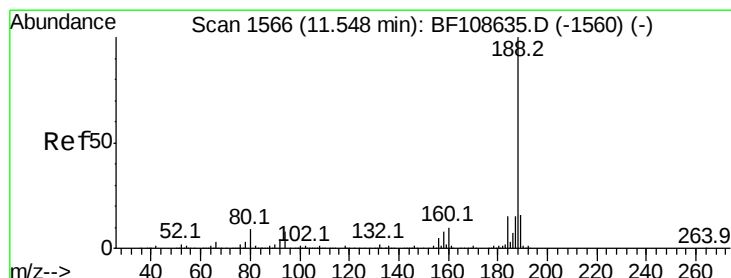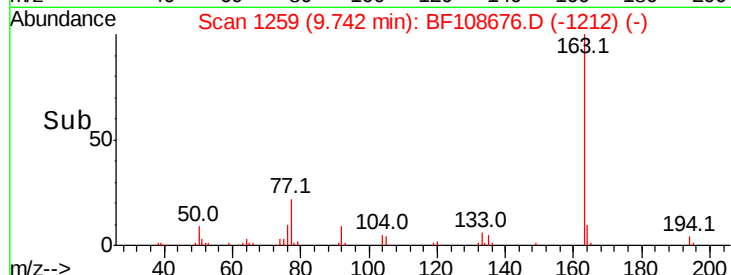
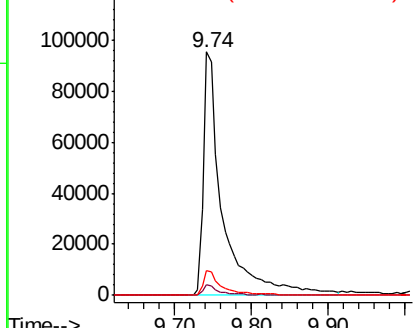



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1565
Delta R.T. -0.01 min
Lab File: BF108676.D
Acq: 31 Aug 2018 8:07

Tgt Ion	Ratio	Resp	Lower	Upper
188	100	306454		
94	8.5	8.5	12.7	
80	8.8	9.2	13.8#	

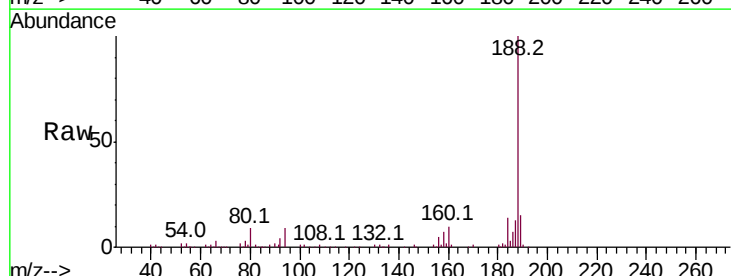

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

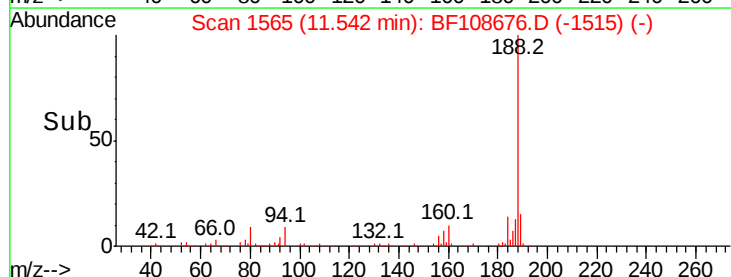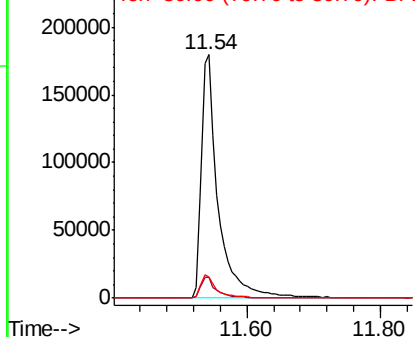

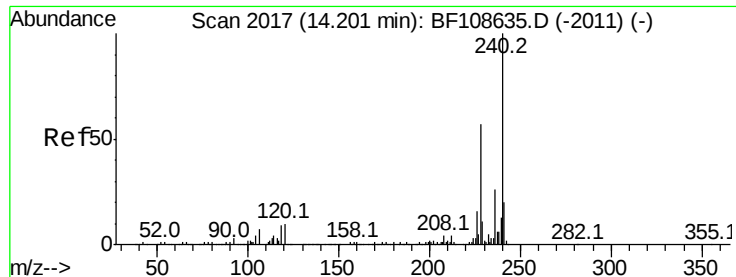

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 1015

Delta R.T. -0.01 min

Lab File: BF108676.D

Acq: 31 Aug 2018 8:07

Instrument :

BNA_F





ClientSampleId :

082818-JETT-F-U-B

Tot Ion:	240	Resp:	304247
Ion Ratio	Lower	Upper	
240	100		
120	10.5	9.5	14.3
236	26.3	20.7	31.1

Manual Integrations
APPROVED

Sohil
8/31/2018 12:19:09 PM

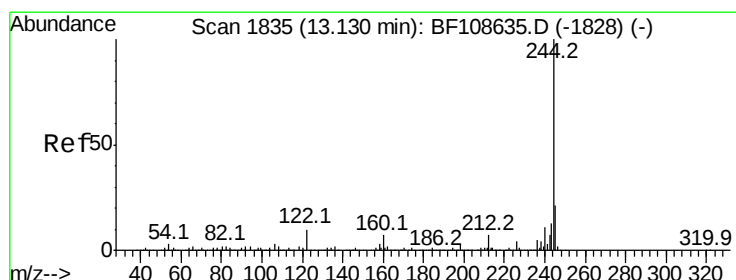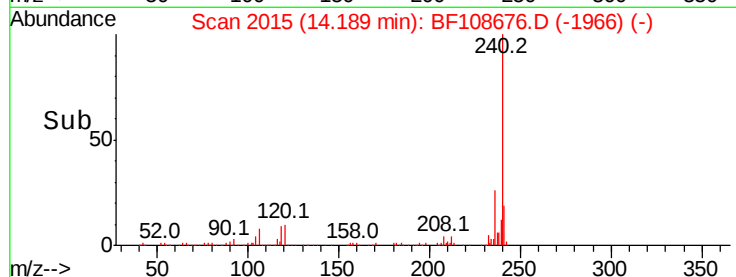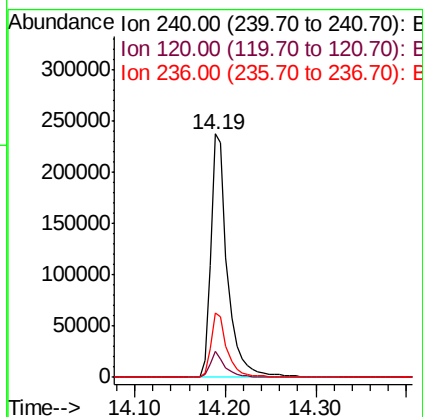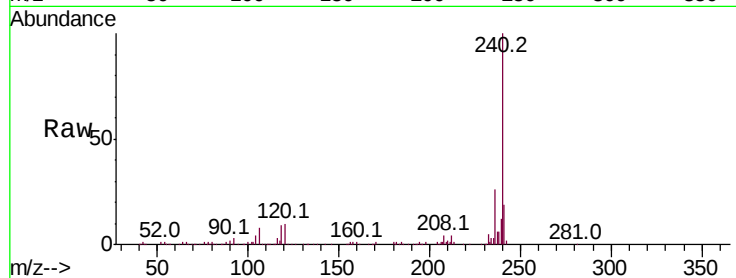

#78

Terphenyl-d14

Concen: 74.387 ng




RT: 13.12 min Scan# 1833


Delta R.T. -0.01 min

Lab File: BF108676.D

Acq: 31 Aug 2018 8:07

Tgt Ion:	244	Resp:	1164822
Ion Ratio	Lower	Upper	
244	100		
212	7.4	5.4	8.0
122	10.2	11.0	16.4#

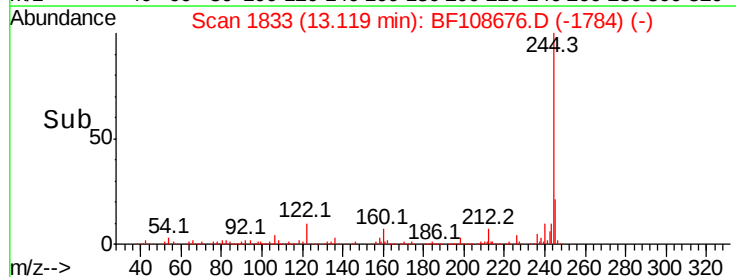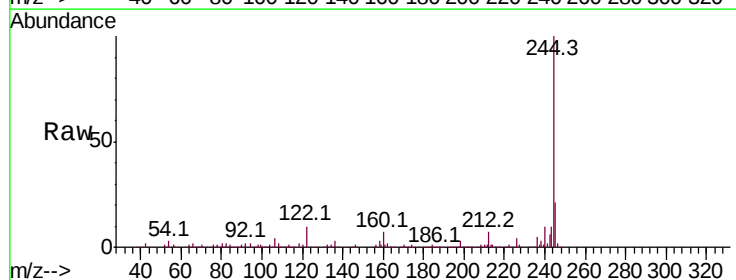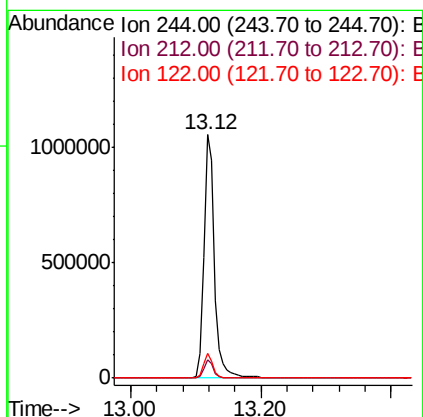

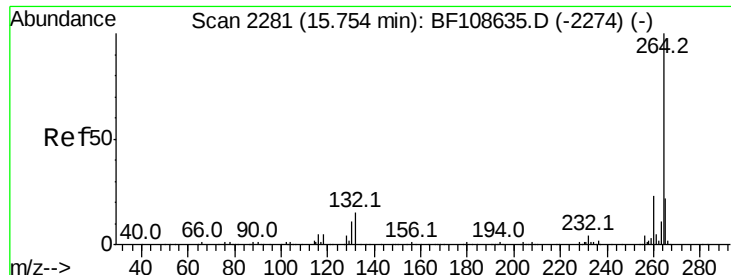

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.75 min Scan# 2280
 Delta R.T. -0.01 min
 Lab File: BF108676.D
 Acq: 31 Aug 2018 8:07

Instrument :
 BNA_F
 ClientSampleId :
 082818-JETT-F-U-B

Tot Ion	Ion	Ratio	Resp	Lower	Upper
264	100				
260	23.4	19.2	28.8		
265	21.2	17.5	26.3		

Manual Integrations
 APPROVED

Sohil
 8/31/2018 12:19:09 PM

