

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083018\
 Data File : BF108668.D
 Acq On : 31 Aug 2018 4:30
 Operator : JU/SJ
 Sample : J4700-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082818-DBRI-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.695	562	571	574	rBV3	42681	135368	3.88%	0.717%
2	6.660	730	735	742	rBV	71989	177703	5.09%	0.941%
3	6.777	751	755	790	rVV	524369	1272861	36.46%	6.743%
4	7.007	790	794	815	rVV	206194	511396	14.65%	2.709%
5	7.154	815	819	855	rVB	1589599	2231679	63.93%	11.822%
6	7.566	885	889	930	rBV	915999	1847494	52.92%	9.787%
7	8.283	1007	1011	1035	rBV	324216	662367	18.97%	3.509%
8	9.354	1189	1193	1226	rBV	2782896	3490910	100.00%	18.493%
9	9.748	1255	1260	1267	rBV	26770	44133	1.26%	0.234%
10	10.042	1306	1310	1323	rBV	594266	761046	21.80%	4.032%
11	10.695	1418	1421	1427	rBV	57166	53945	1.55%	0.286%
12	10.836	1441	1445	1474	rBV	824977	1339848	38.38%	7.098%
13	11.542	1561	1565	1586	rBV	561916	838127	24.01%	4.440%
14	13.124	1829	1834	1852	rBV	3224736	3411691	97.73%	18.074%
15	14.195	2012	2016	2028	rBV	794505	940831	26.95%	4.984%
16	14.936	2139	2142	2147	rVB	37297	39330	1.13%	0.208%
17	15.018	2152	2156	2162	rBV	39673	50071	1.43%	0.265%
18	15.294	2199	2203	2208	rBV	50656	61615	1.77%	0.326%
19	15.706	2268	2273	2275	rBV	50090	66219	1.90%	0.351%
20	15.747	2275	2280	2294	rVB	474328	763100	21.86%	4.043%
21	16.177	2347	2353	2359	rBV	43378	75982	2.18%	0.403%
22	16.718	2439	2445	2454	rBV5	31154	65743	1.88%	0.348%
23	18.035	2657	2669	2671	rBV10	12002	35154	1.01%	0.186%


Sum of corrected areas: 18876613

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083018\
Data File : BF108668.D
Acq On : 31 Aug 2018 4:30
Operator : JU/SJ
Sample : J4700-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082818-DBRI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

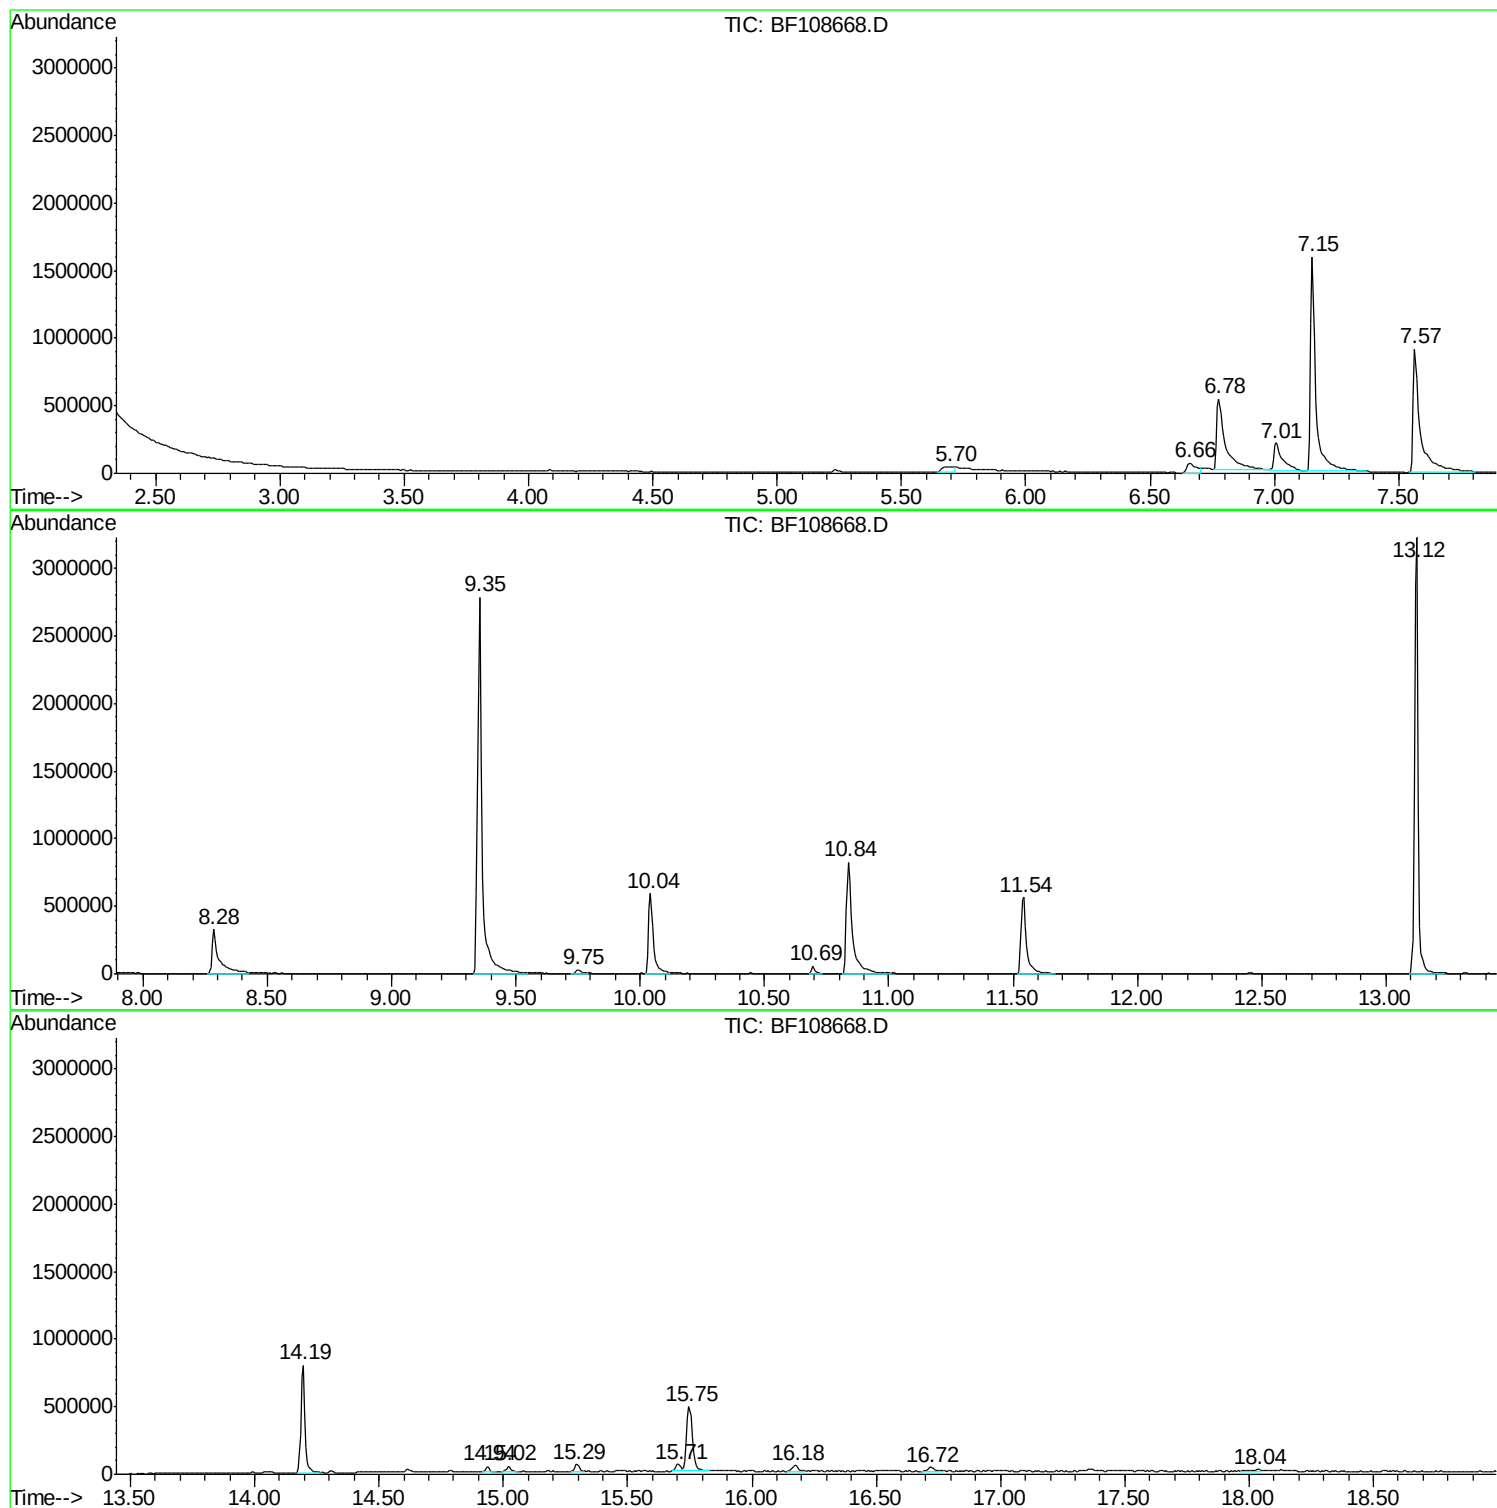

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083018\
Data File : BF108668.D
Acq On : 31 Aug 2018 4:30
Operator : JU/SJ
Sample : J4700-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082818-DBRI-F-D-M










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.78 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.78	49.78 ng	1272860	1,4-Dichlorobenzene-d4	7.01

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3			5-Aminoindole	132	C8H8N2	005192-03-0	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

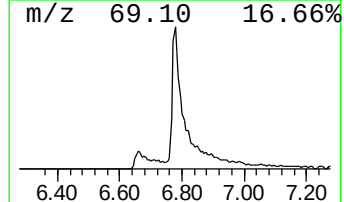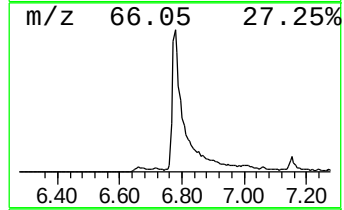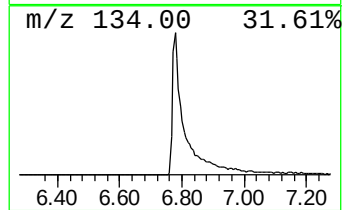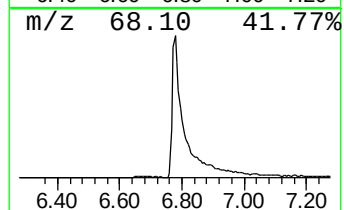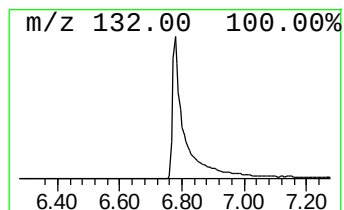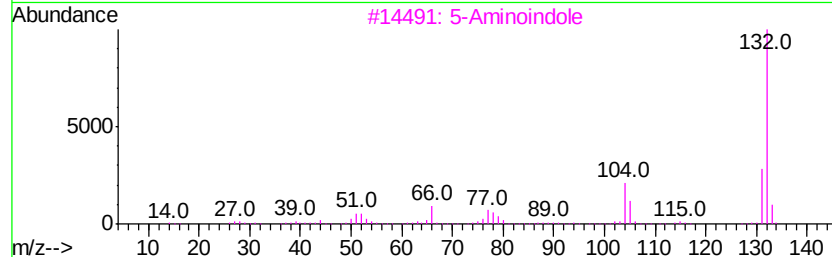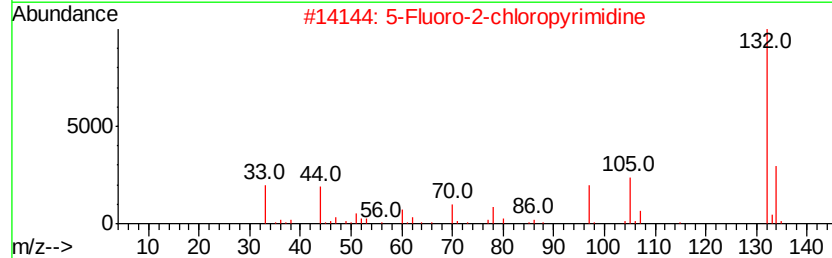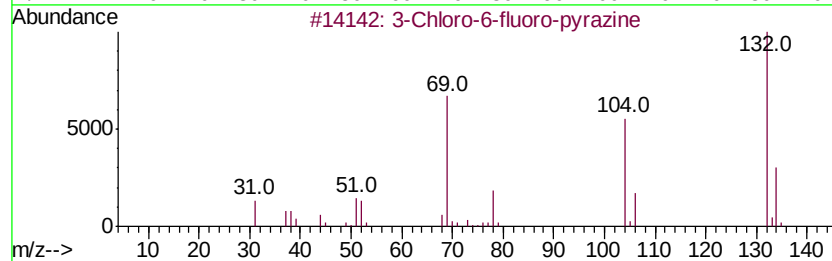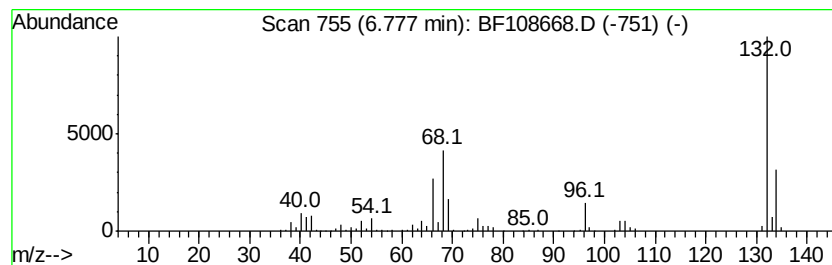

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083018\
Data File : BF108668.D
Acq On : 31 Aug 2018 4:30
Operator : JU/SJ
Sample : J4700-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082818-DBRI-F-D-M

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.78	6.78	49.8	ng	1272860	1	7.01	511396	20.0