


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF083018\  
 Data File : BF108631.D  
 Acq On : 30 Aug 2018 10:20  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF083018.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Aug 30 15:06:55 2018

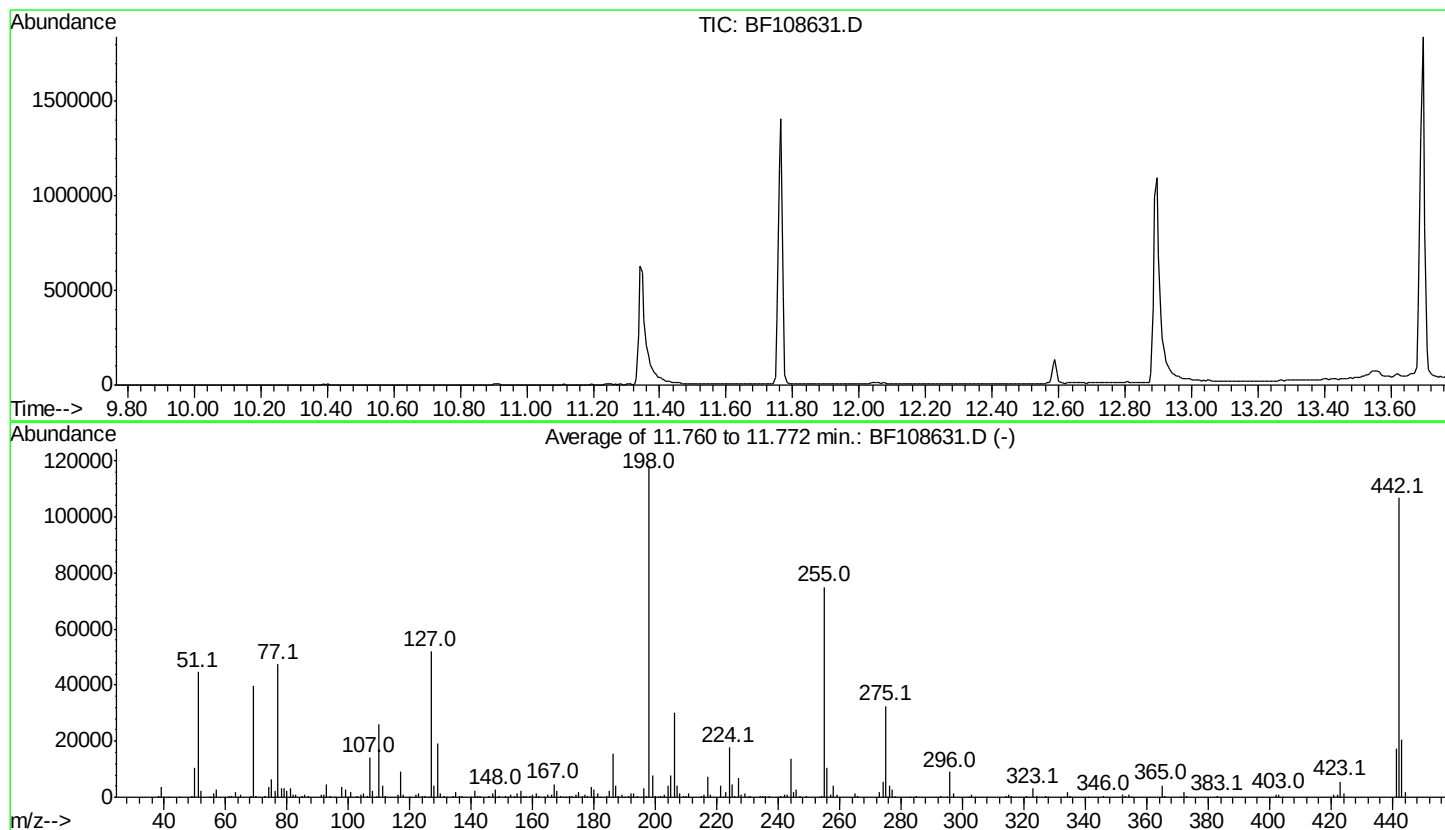

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1596

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 37.7         | 44622      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 643        | PASS                |
| 69             | 198             | 0.00            | 100             | 33.4         | 39545      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 288        | PASS                |
| 127            | 198             | 10              | 80              | 43.9         | 51960      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 666        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 118314     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 7886       | PASS                |
| 275            | 198             | 10              | 60              | 27.5         | 32493      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 4314       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.7         | 17435      | PASS                |
| 442            | 198             | 50              | 100             | 90.3         | 106861     | PASS                |
| 443            | 442             | 15              | 24              | 19.0         | 20345      | PASS                |