


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083018\
 Data File : BF108640.D
 Acq On : 30 Aug 2018 15:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 30 15:06:55 2018

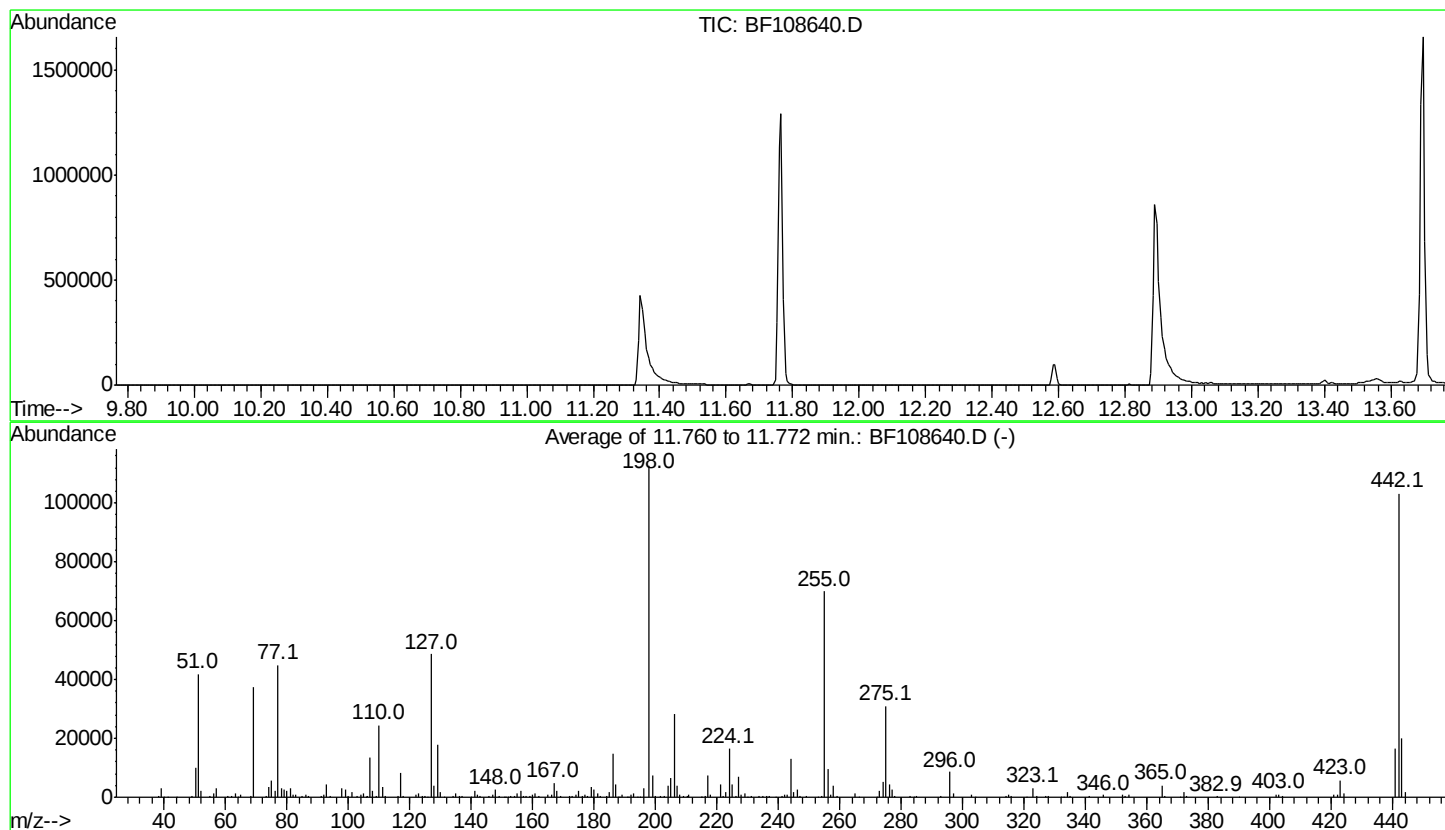

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	41934	PASS
68	69	0.00	2	1.4	509	PASS
69	198	0.00	100	33.1	37266	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	48716	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112733	PASS
199	198	5	9	6.4	7227	PASS
275	198	10	60	27.5	31039	PASS
365	198	1	100	3.6	4081	PASS
441	198	0.01	100	14.7	16616	PASS
442	198	50	100	91.6	103261	PASS
443	442	15	24	19.5	20158	PASS