


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083018\
 Data File : BF108666.D
 Acq On : 31 Aug 2018 3:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 30 15:06:55 2018

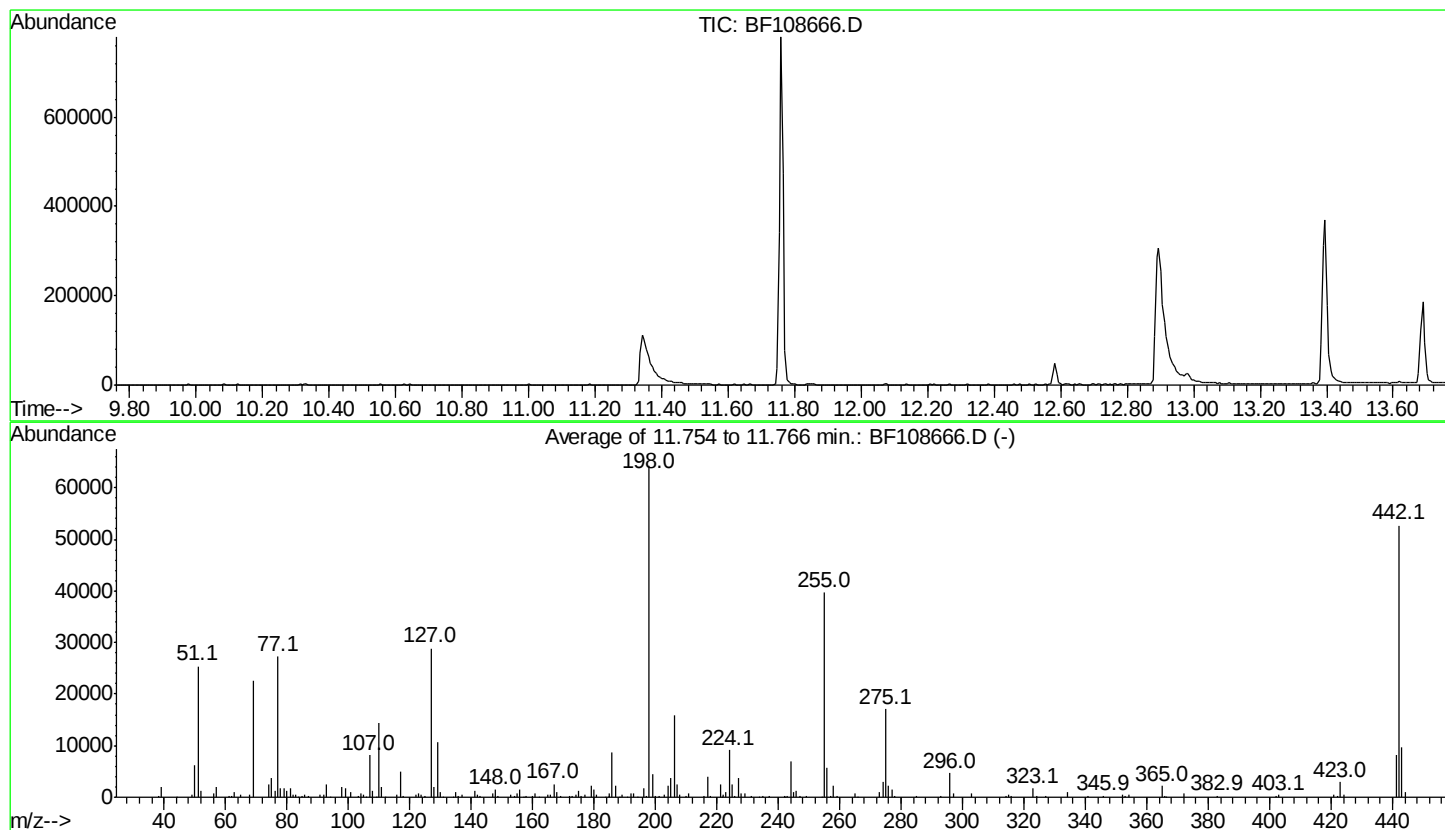

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	25383	PASS
68	69	0.00	2	1.8	399	PASS
69	198	0.00	100	35.2	22635	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	28872	PASS
197	198	0.00	2	0.4	272	PASS
198	198	100	100	100.0	64277	PASS
199	198	5	9	6.9	4457	PASS
275	198	10	60	26.6	17112	PASS
365	198	1	100	3.4	2177	PASS
441	198	0.01	100	12.7	8188	PASS
442	198	50	100	81.9	52659	PASS
443	442	15	24	18.5	9730	PASS