

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083019\
 Data File : BF116685.D
 Acq On : 31 Aug 2019 7:22
 Operator : HP/JU
 Sample : K4575-14 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S703A-N-1.0-1.5-082719

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	568	572	578	rVB	260832	221725	23.27%	2.685%
2	6.463	740	744	752	rBV	328731	269959	28.34%	3.269%
3	6.610	765	769	773	rBV	320308	253286	26.59%	3.067%
4	6.845	806	809	813	rBV	801594	616087	64.67%	7.461%
5	7.004	832	836	839	rBV	254350	210285	22.07%	2.547%
6	7.398	900	903	911	rBV	185012	143633	15.08%	1.739%
7	8.128	1023	1027	1030	rBV	1101374	843593	88.55%	10.216%
8	9.198	1206	1209	1213	rBV	373603	290451	30.49%	3.517%
9	9.592	1273	1276	1284	rBV	28218	24873	2.61%	0.301%
10	9.881	1321	1325	1328	rBV	1213410	952635	100.00%	11.536%
11	9.910	1328	1330	1334	rVB	15981	15067	1.58%	0.182%
12	10.663	1455	1458	1464	rBV	146444	131125	13.76%	1.588%
13	11.363	1573	1577	1579	rBV	1058557	912686	95.81%	11.053%
14	11.380	1579	1580	1584	rVV	134891	110959	11.65%	1.344%
15	11.433	1584	1589	1592	rVB2	27321	29668	3.11%	0.359%
16	11.586	1610	1615	1619	rBV2	18220	19141	2.01%	0.232%
17	11.863	1658	1662	1663	rBV2	14788	12952	1.36%	0.157%
18	11.886	1663	1666	1669	rVB2	26846	27378	2.87%	0.332%
19	11.975	1677	1681	1683	rBV	17581	17300	1.82%	0.210%
20	12.569	1778	1782	1785	rBV	199027	163698	17.18%	1.982%
21	12.798	1815	1821	1824	rBV	160761	155493	16.32%	1.883%
22	12.939	1842	1845	1851	rVB	332452	268594	28.19%	3.253%
23	13.121	1871	1876	1879	rBV	19964	21337	2.24%	0.258%
24	13.192	1883	1888	1892	rVV2	16554	23423	2.46%	0.284%
25	13.421	1924	1927	1934	rVB4	31991	35067	3.68%	0.425%
26	13.521	1942	1944	1947	rBV4	10318	12831	1.35%	0.155%
27	13.627	1959	1962	1968	rVB7	14338	22074	2.32%	0.267%
28	13.833	1994	1997	2003	rBV4	79972	106888	11.22%	1.294%
29	13.992	2016	2024	2027	rBV	875186	877898	92.15%	10.631%
30	14.016	2027	2028	2031	rVB	75152	40435	4.24%	0.490%
31	14.098	2039	2042	2046	rBV2	19401	21066	2.21%	0.255%
32	14.157	2050	2052	2058	rVB4	15773	23982	2.52%	0.290%
33	14.468	2102	2105	2109	rBV	124775	137883	14.47%	1.670%
34	14.768	2154	2156	2161	rVB2	30666	35379	3.71%	0.428%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083019\
Data File : BF116685.D
Acq On : 31 Aug 2019 7:22
Operator : HP/JU
Sample : K4575-14 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S703A-N-1.0-1.5-082719

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.910	2178	2180	2184	rVB4	25031	24553	2.58%	0.297%
36	15.021	2195	2199	2206	rBV	67823	141180	14.82%	1.710%
37	15.104	2210	2213	2215	rBV3	56191	64114	6.73%	0.776%
38	15.321	2247	2250	2254	rVB	36780	45616	4.79%	0.552%
39	15.380	2256	2260	2265	rBV	48056	58672	6.16%	0.711%
40	15.445	2266	2271	2275	rBV	597741	725080	76.11%	8.781%
41	15.915	2347	2351	2356	rBV	56326	71434	7.50%	0.865%
42	16.410	2431	2435	2442	rBV5	25815	51390	5.39%	0.622%
43	16.874	2512	2514	2519	rBV4	17364	26706	2.80%	0.323%


Sum of corrected areas: 8257596

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083019\
Data File : BF116685.D
Acq On : 31 Aug 2019 7:22
Operator : HP/JU
Sample : K4575-14 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S703A-N-1.0-1.5-082719

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

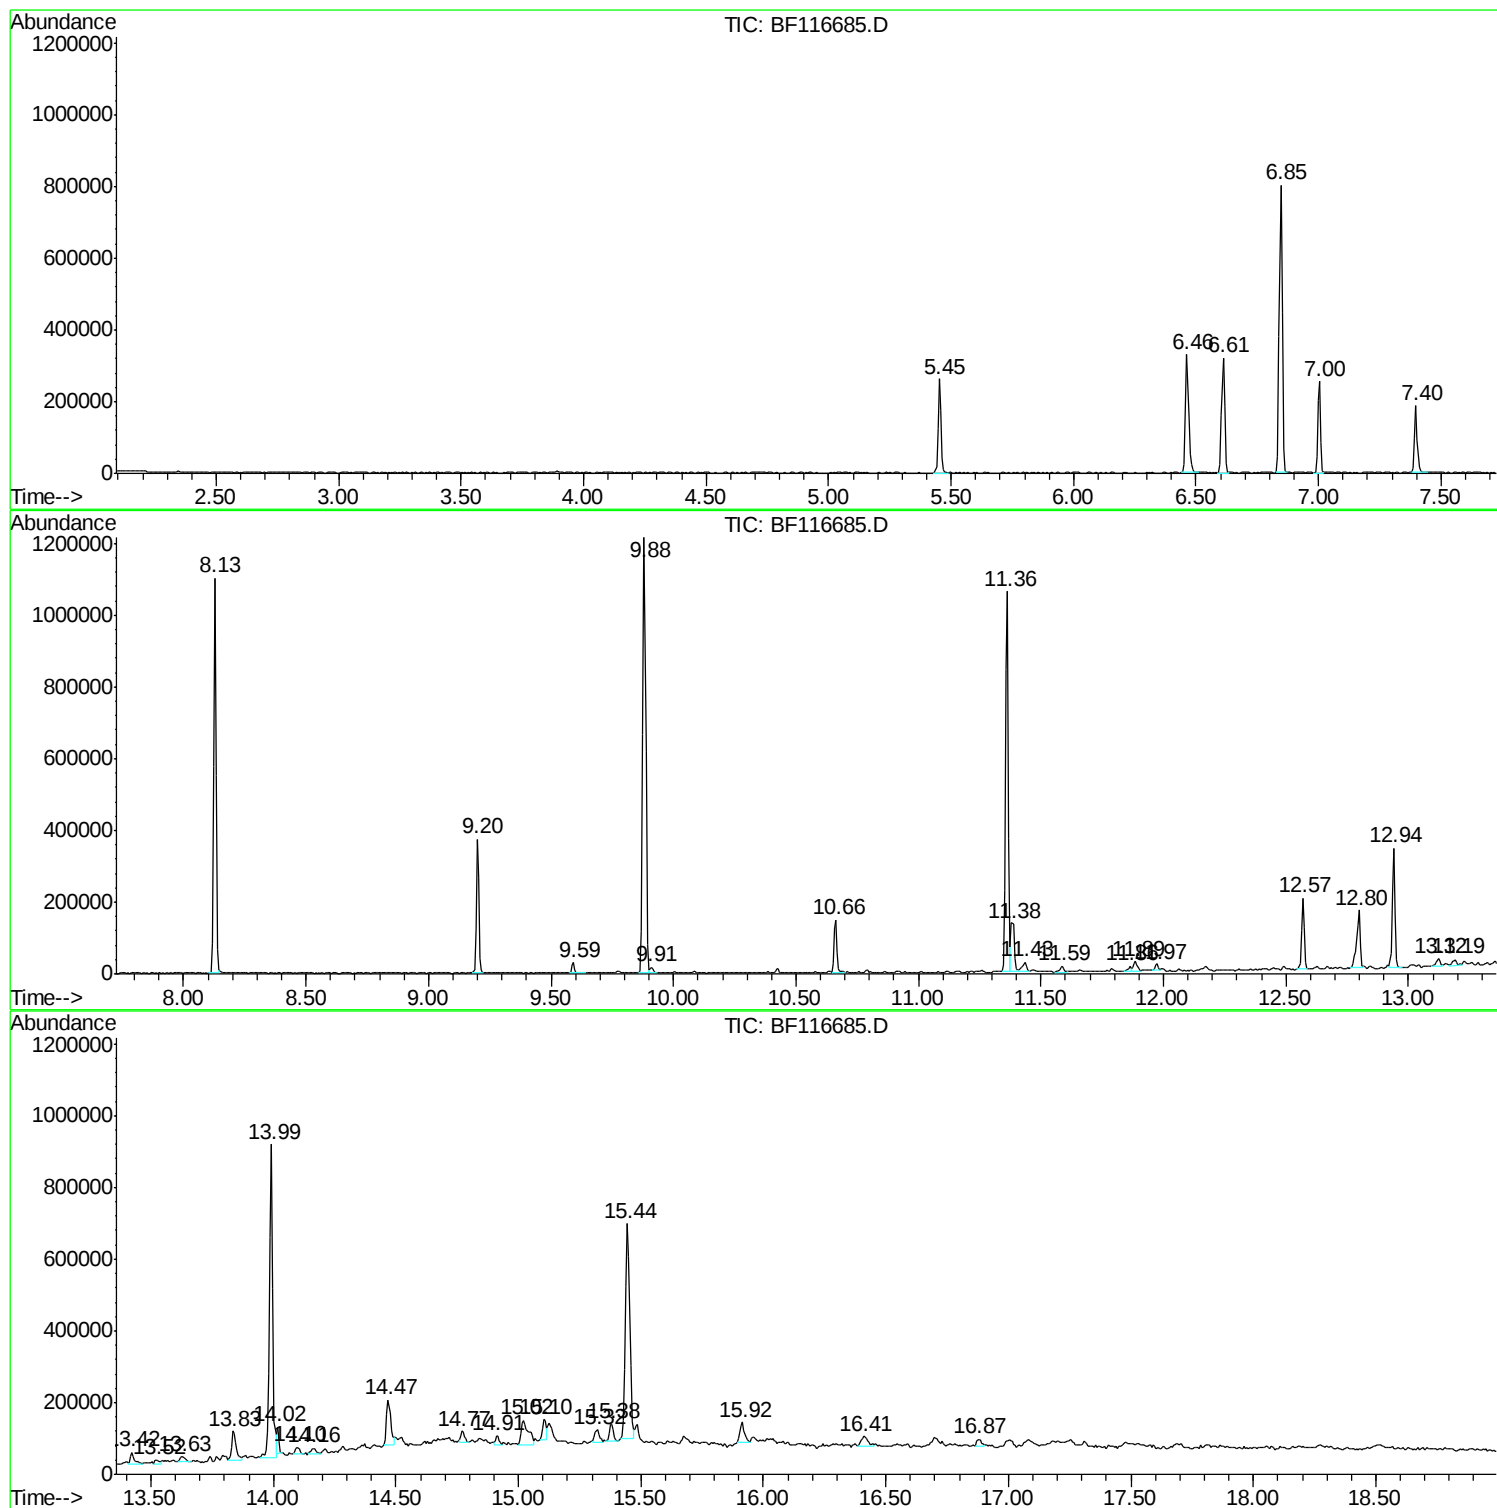

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083019\
Data_File : BF116685.D
Acq_On : 31_Aug_2019 7:222
Operator : HP/JUU
Sample : K4575-14 10XX
Misc :
ALS_Vial : 24 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
S703A-N-1.0-1.5-082719

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
