


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083019\
 Data File : BF116653.D
 Acq On : 30 Aug 2019 16:01
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 20:02:30 2019

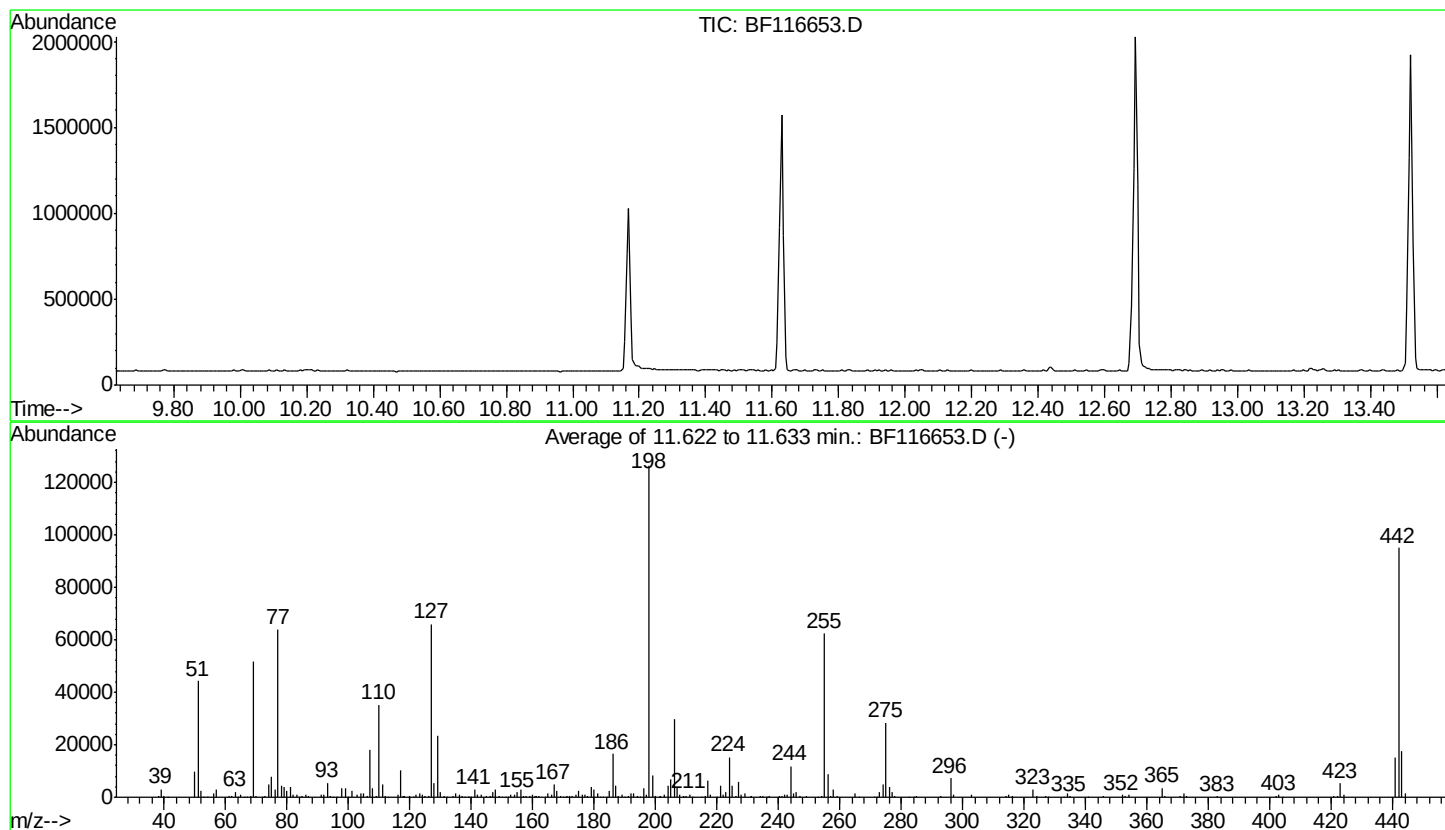

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	44386	PASS
68	69	0.00	2	0.7	361	PASS
69	198	0.00	100	41.0	51854	PASS
70	69	0.00	2	0.7	381	PASS
127	198	10	80	52.2	66021	PASS
197	198	0.00	2	0.8	1058	PASS
198	198	100	100	100.0	126386	PASS
199	198	5	9	6.4	8104	PASS
275	198	10	60	22.5	28394	PASS
365	198	1	100	2.8	3585	PASS
441	198	0.01	100	11.9	15022	PASS
442	198	50	100	75.1	94949	PASS
443	442	15	24	18.3	17337	PASS