


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083019\
 Data File : BF116662.D
 Acq On : 30 Aug 2019 20:52
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 30 20:02:30 2019

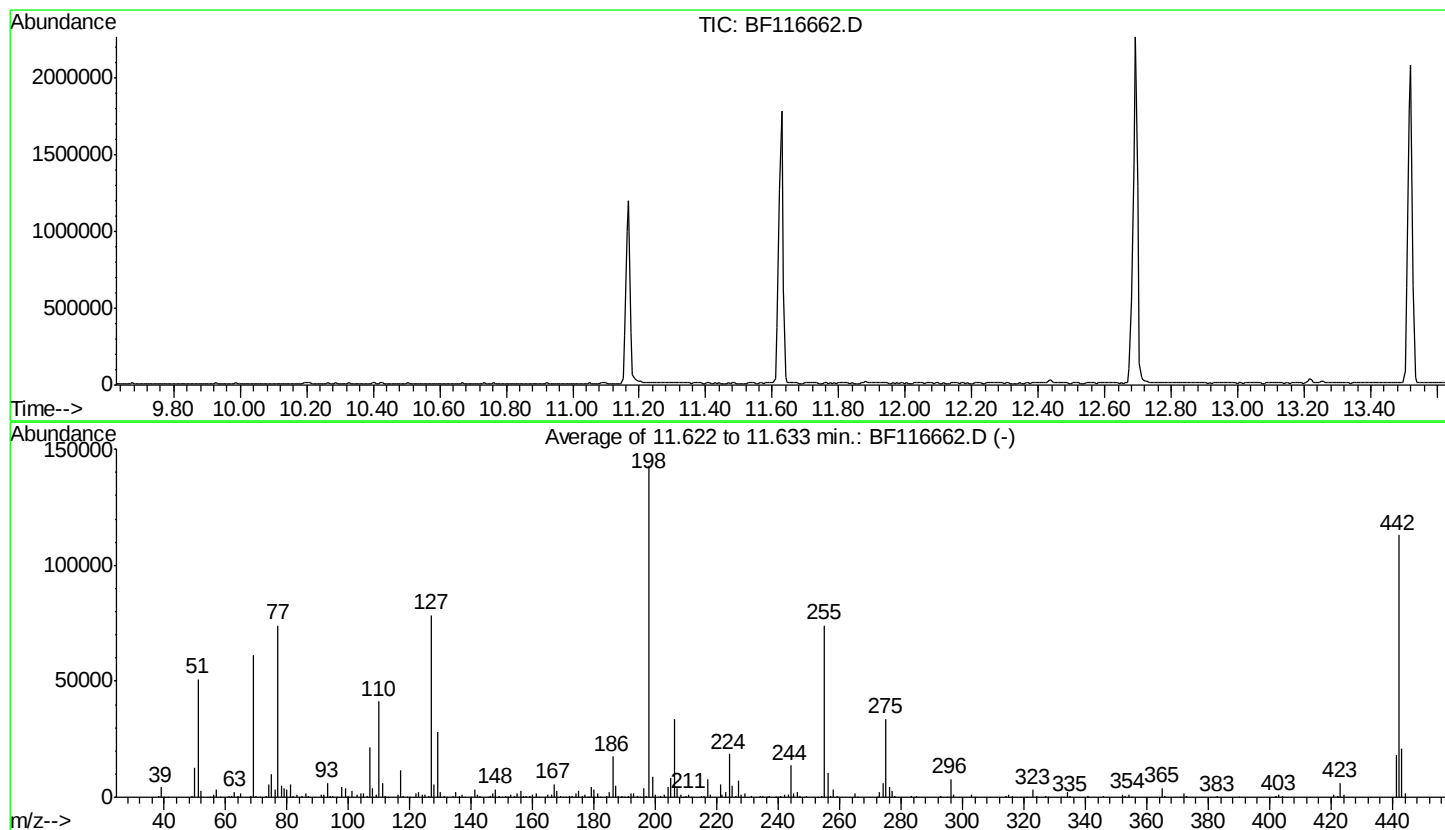

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	51024	PASS
68	69	0.00	2	1.1	689	PASS
69	198	0.00	100	42.8	61248	PASS
70	69	0.00	2	1.1	659	PASS
127	198	10	80	55.0	78610	PASS
197	198	0.00	2	0.6	835	PASS
198	198	100	100	100.0	142946	PASS
199	198	5	9	6.3	9029	PASS
275	198	10	60	23.7	33837	PASS
365	198	1	100	2.8	3959	PASS
441	198	0.01	100	12.7	18154	PASS
442	198	50	100	79.0	112874	PASS
443	442	15	24	18.3	20712	PASS