
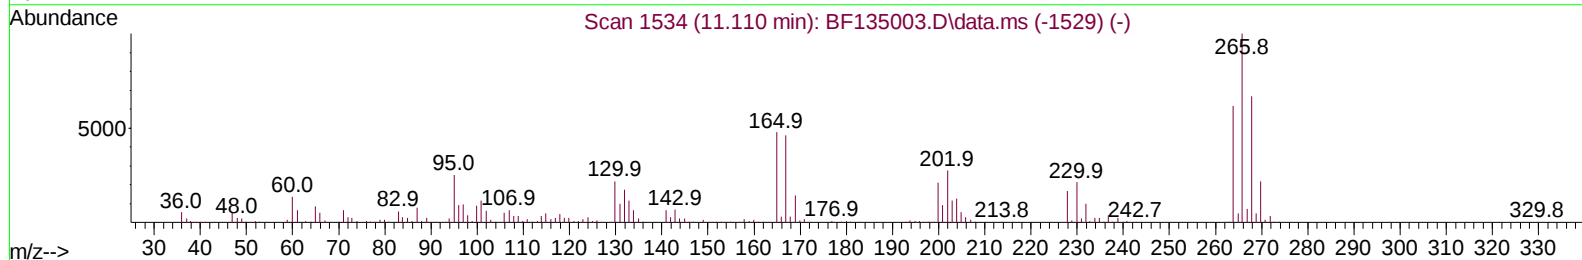
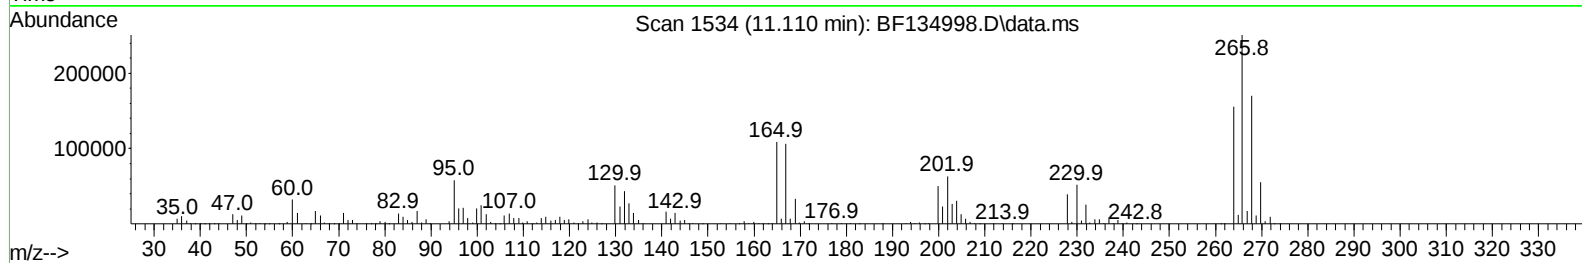


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF134998.D
Acq On : 30 Aug 2023 11:00
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 07:31:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

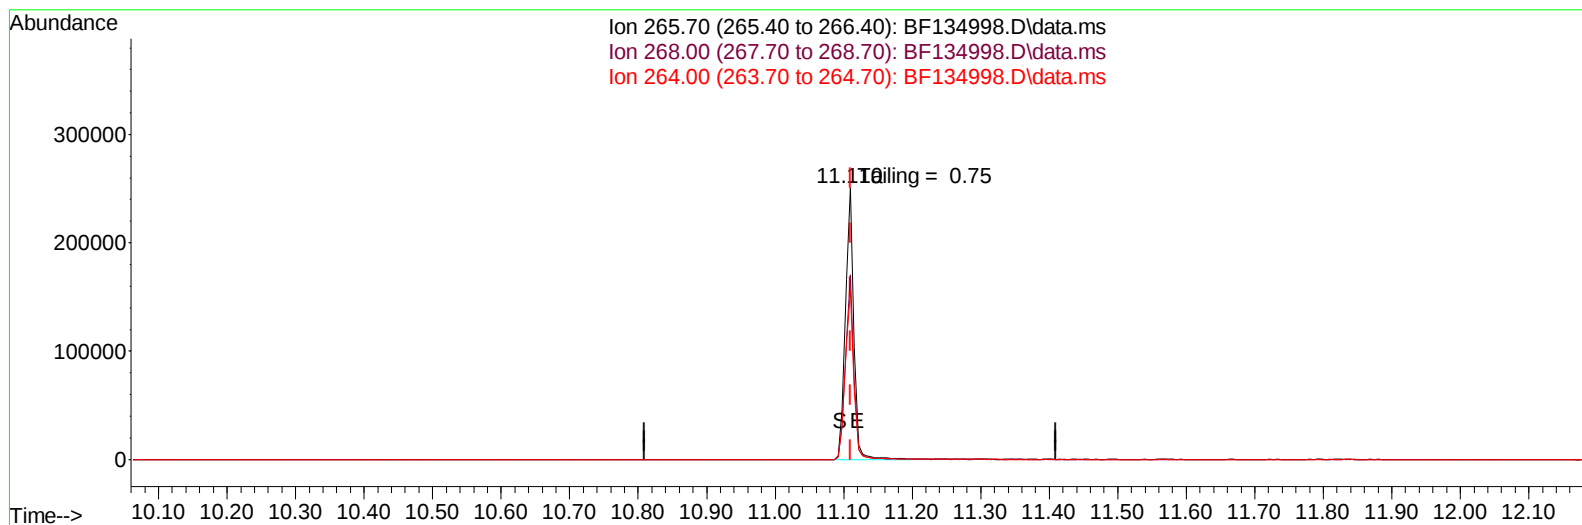

TIC: BF134998.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.000) 604890.37 ng

response 212717

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	67.93
264.00	61.60	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF134998.D
Acq On : 30 Aug 2023 11:00
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 07:31:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

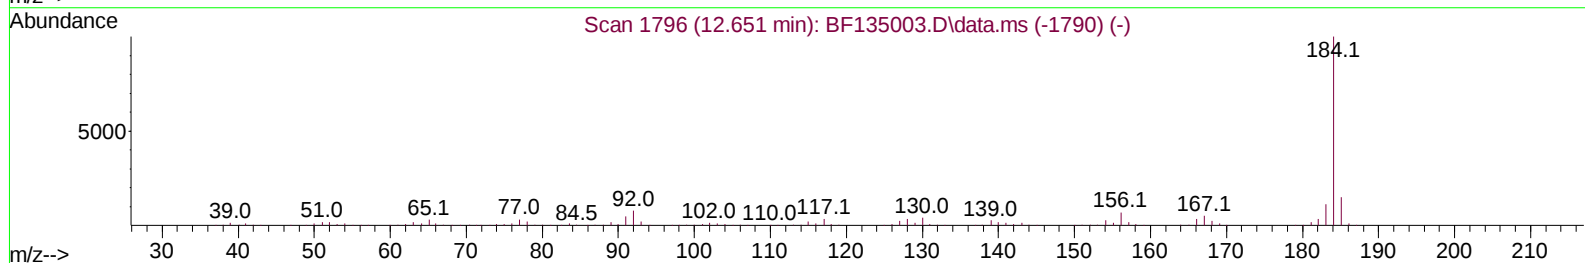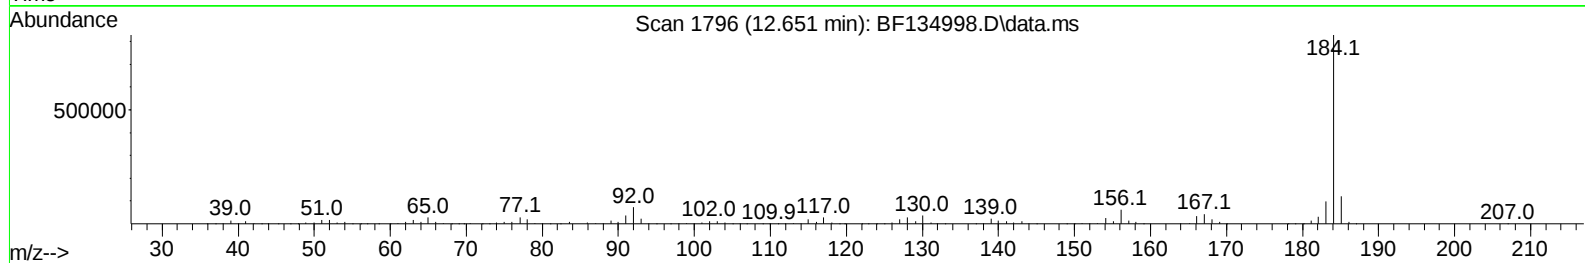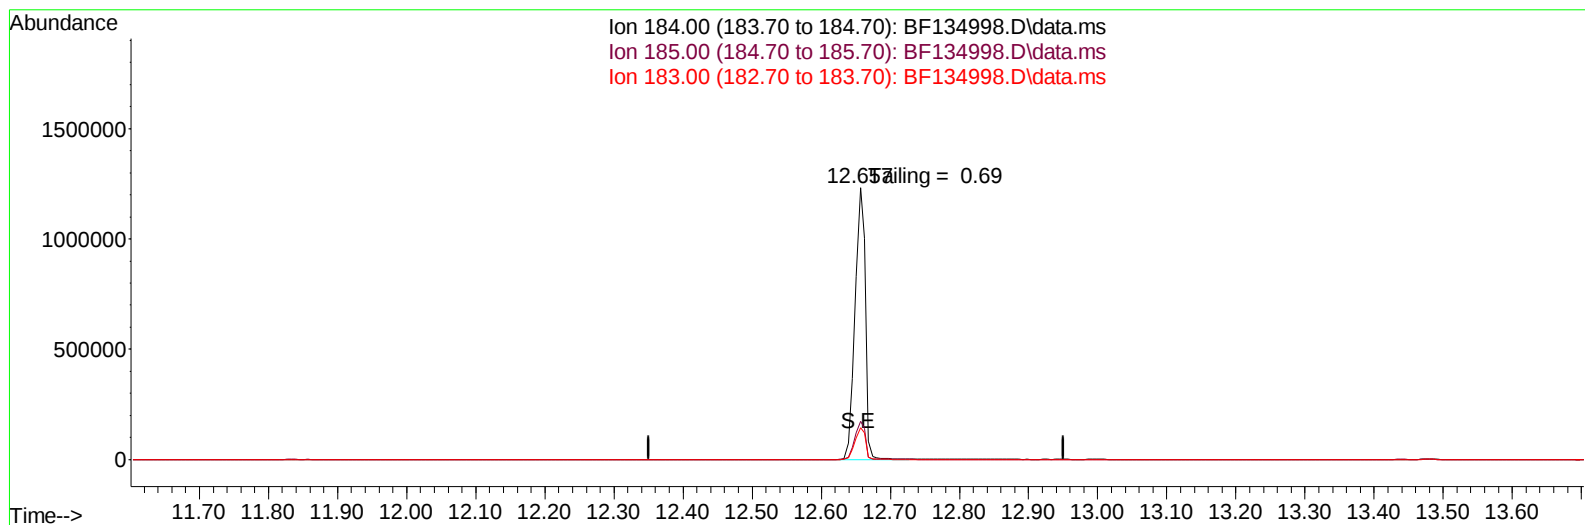

TIC: BF134998.D\data.ms

(77) Benzidine

12.651min (-12.651) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.00	0.00#
183.00	11.30	0.00#
0.00	0.00	0.00