
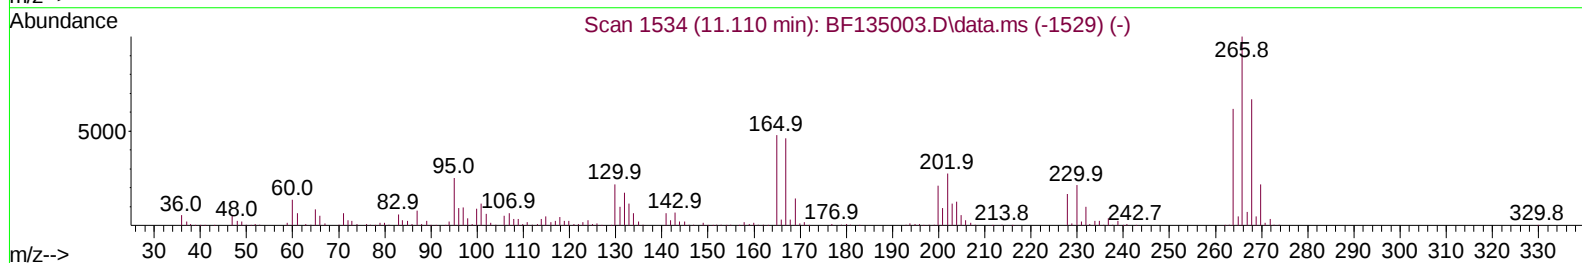
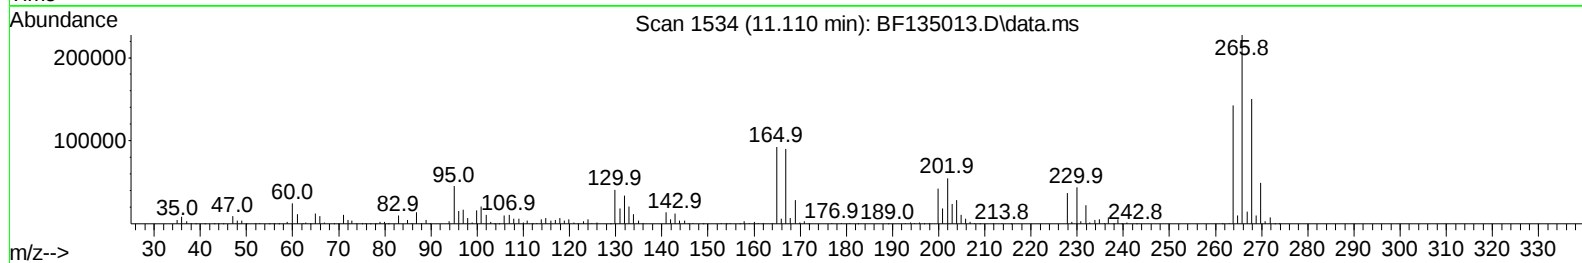


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF135013.D
Acq On : 30 Aug 2023 19:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 07:33:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration



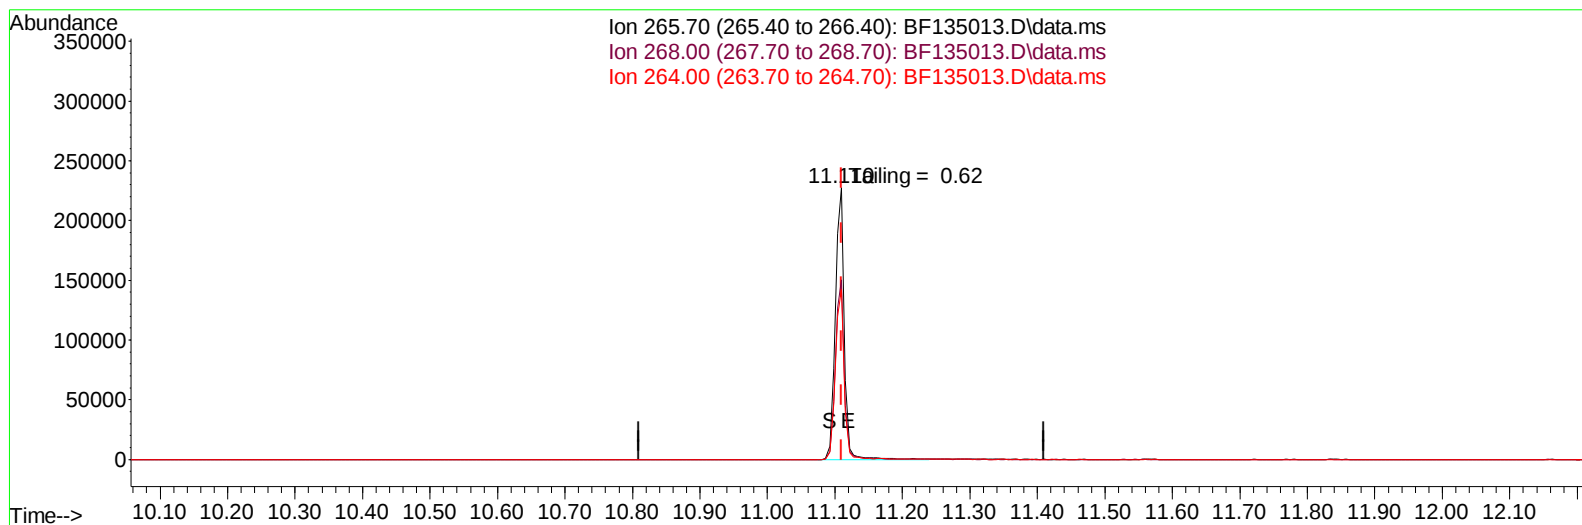


TIC: BF135013.D\data.ms

(70) Pentachlorophenol (C)**11.110min (-0.000) 159876.06 ng****response 211099**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	66.13
264.00	61.60	62.73
0.00	0.00	0.00

Quant Time: Aug 31 07:33:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

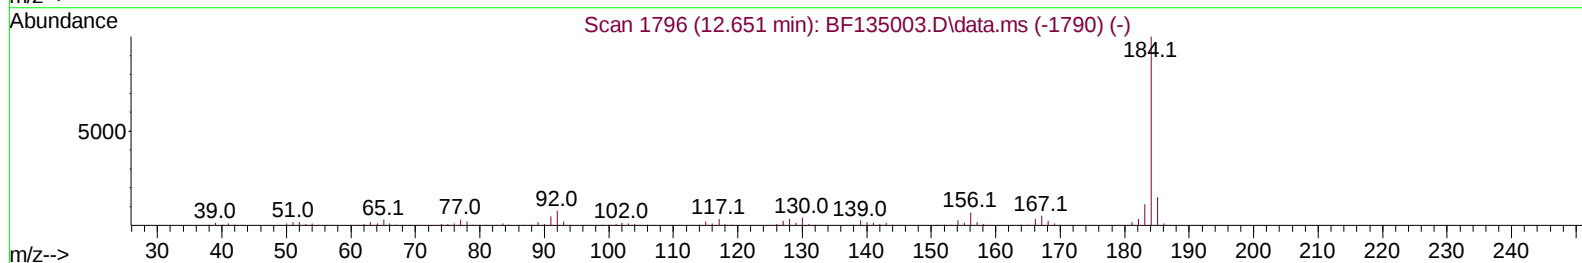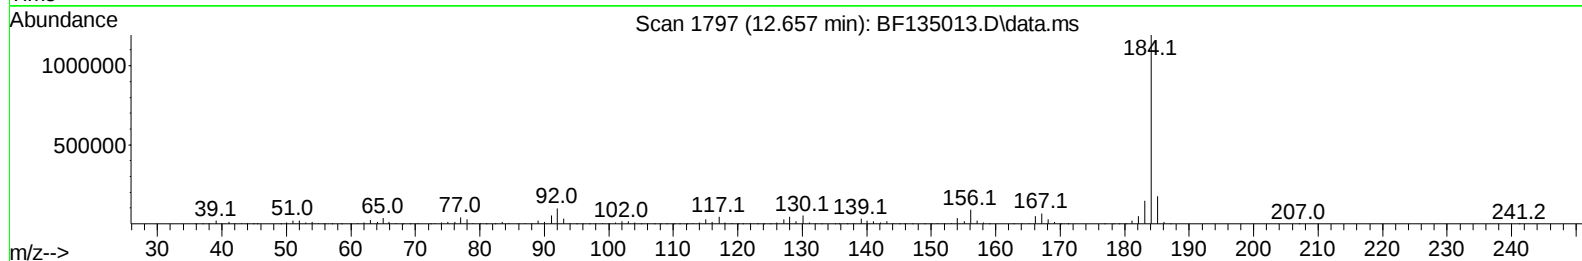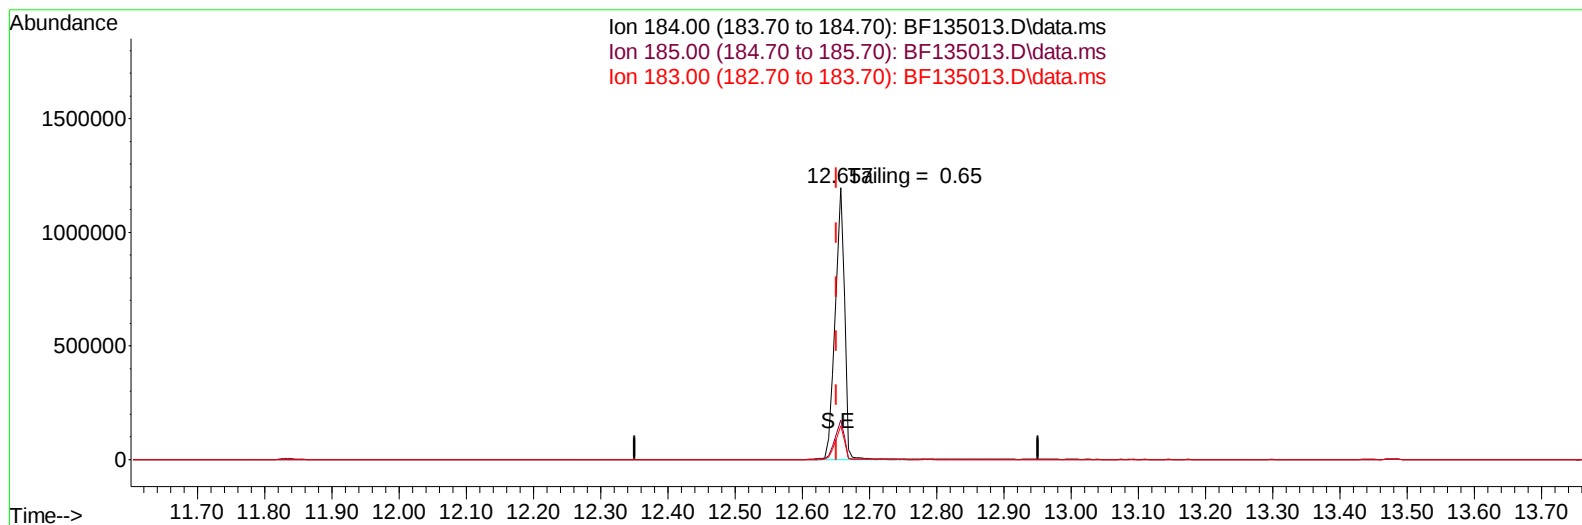

TIC: BF135013.D\data.ms

(77) **Benzidine**

12.657min (+ 0.006) 991443.38 ng

response **1161694**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.51
183.00	11.30	12.29
0.00	0.00	0.00