

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
 Data File : BF135027.D
 Acq On : 31 Aug 2023 03:28
 Operator : CG\JU
 Sample : 04198-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-309-OK-370-COMP-24

Quant Time: Aug 31 06:01:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 03:48:08 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.769	152	138624	20.000	ng	0.00
21) Naphthalene-d8	8.051	136	538693	20.000	ng	0.00
39) Acenaphthene-d10	9.810	164	246492	20.000	ng	0.00
64) Phenanthrene-d10	11.298	188	356239	20.000	ng	-0.01
76) Chrysene-d12	13.957	240	252236	20.000	ng	0.00
86) Perylene-d12	15.427	264	243462	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.404	112	747495	83.290	ng	0.00
7) Phenol-d6	6.410	99	917864	82.052	ng	0.00
23) Nitrobenzene-d5	7.334	82	552915	57.664	ng	-0.01
42) 2,4,6-Tribromophenol	10.598	330	185912	71.101	ng	-0.01
45) 2-Fluorobiphenyl	9.134	172	961365	63.499	ng	0.00
79) Terphenyl-d14	12.898	244	717322	46.409	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF135027.D
Acq On : 31 Aug 2023 03:28
Operator : CG\JU
Sample : 04198-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-309-OK-370-COMP-24

Quant Time: Aug 31 06:01:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration




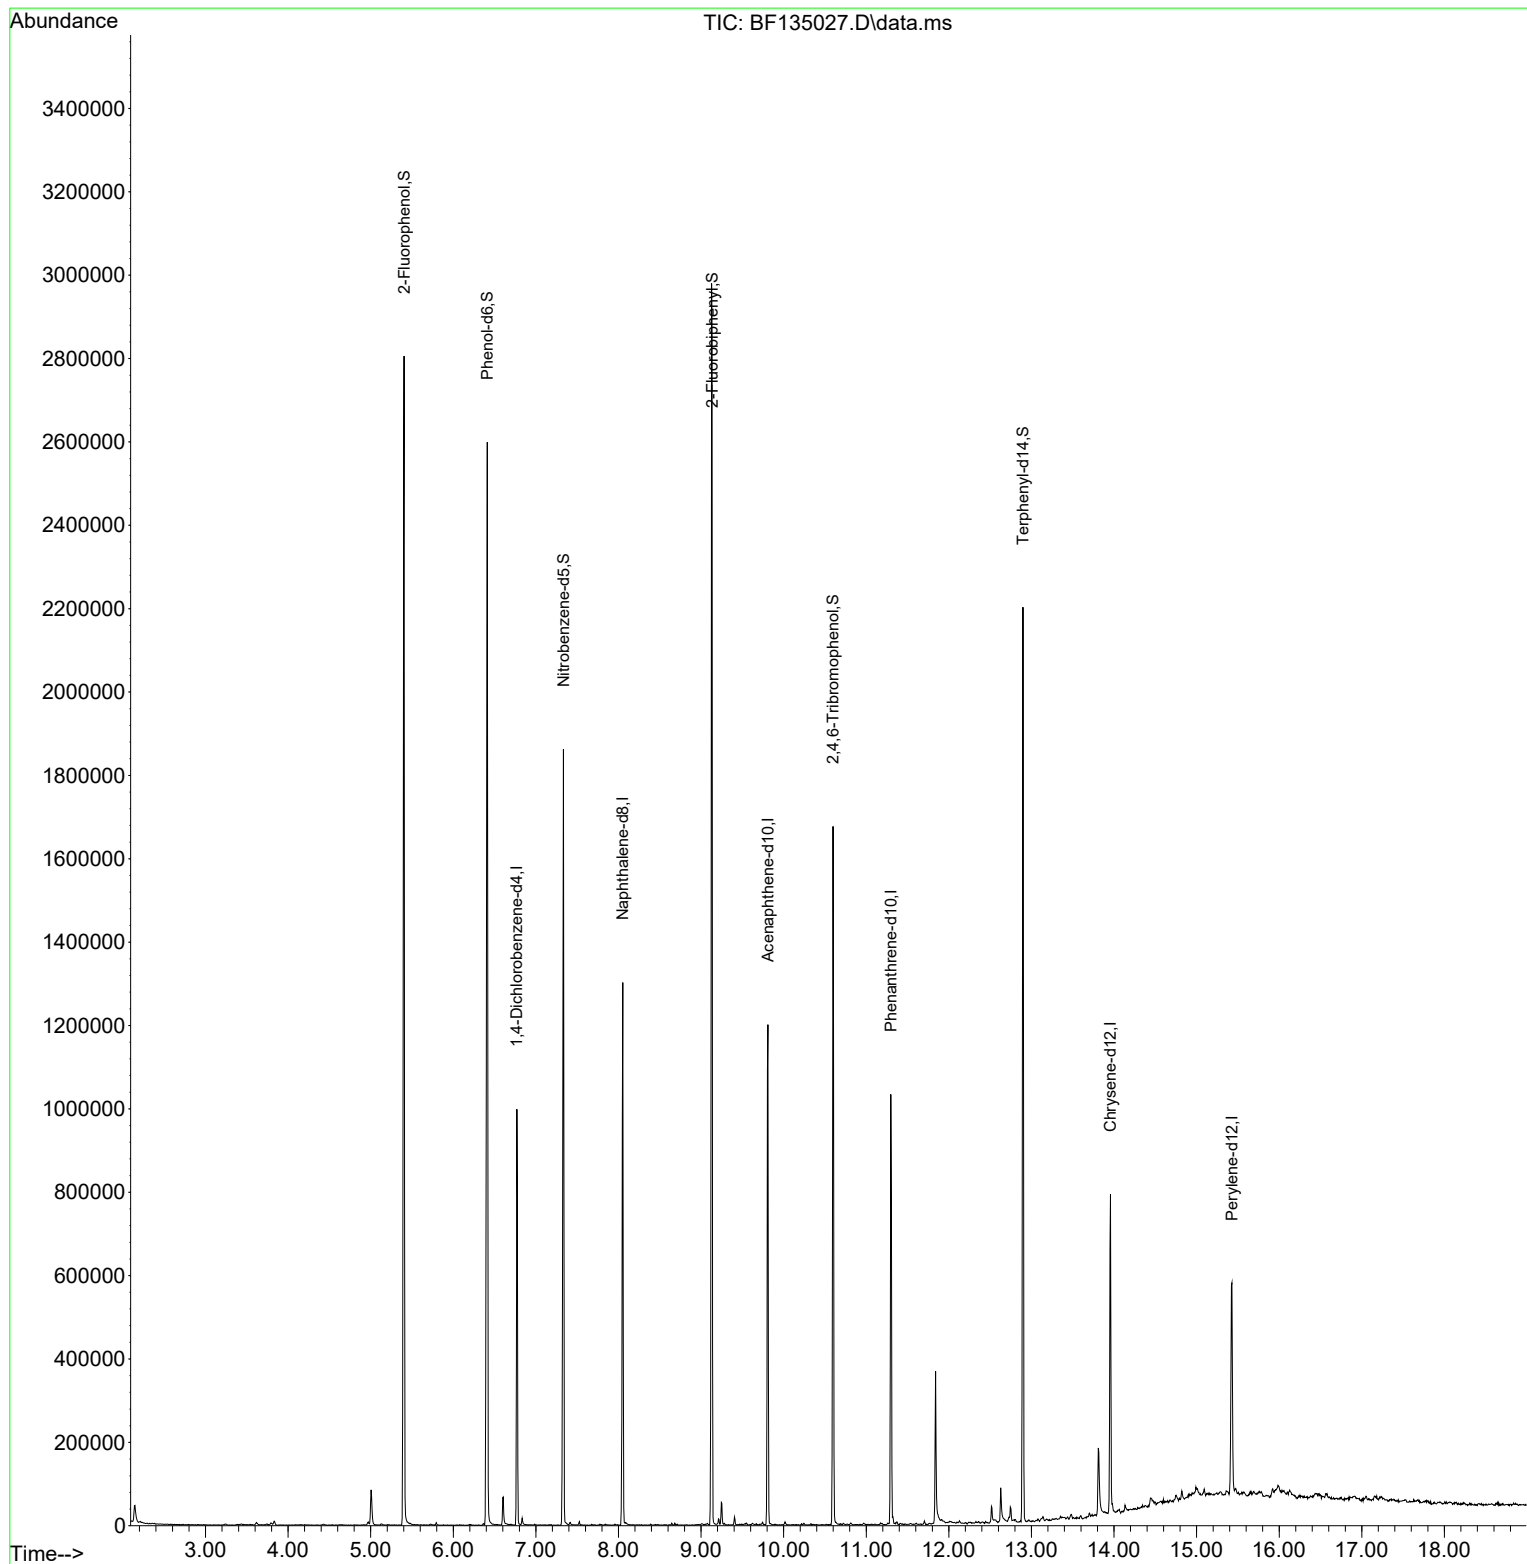


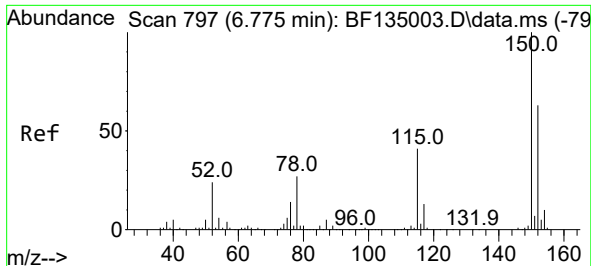

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.769 min Scan# 797
Delta R.T. -0.006 min
Lab File: BF135027.D
Acq: 31 Aug 2023 03:28




Instrument :
BNA_F
ClientSampleId :
OR-309-OK-370-COMP-24

Tgt Ion:152 Resp: 138624
Ion Ratio Lower Upper
152 100
150 156.6 126.2 189.4
115 66.1 51.2 76.8

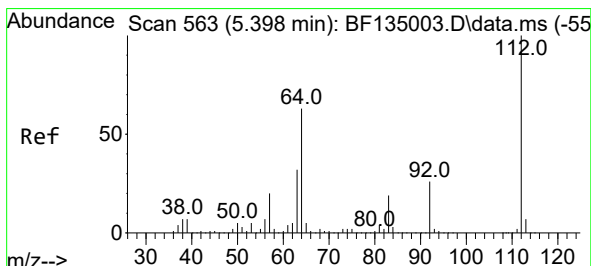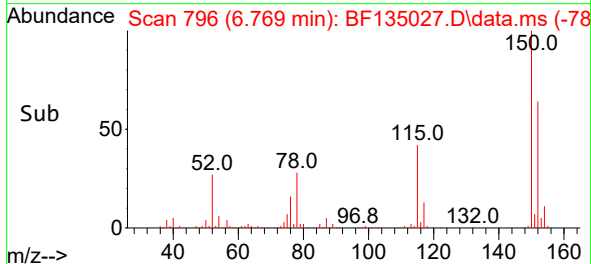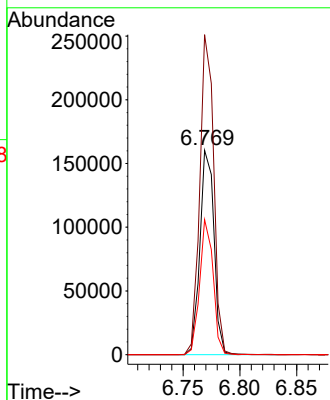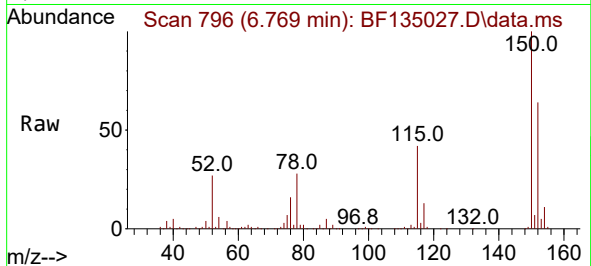

#5
2-Fluorophenol
Concen: 83.290 ng
RT: 5.404 min Scan# 564
Delta R.T. 0.006 min
Lab File: BF135027.D
Acq: 31 Aug 2023 03:28

Tgt Ion:112 Resp: 747495
Ion Ratio Lower Upper
112 100
64 60.8 50.5 75.7
63 31.1 25.9 38.9


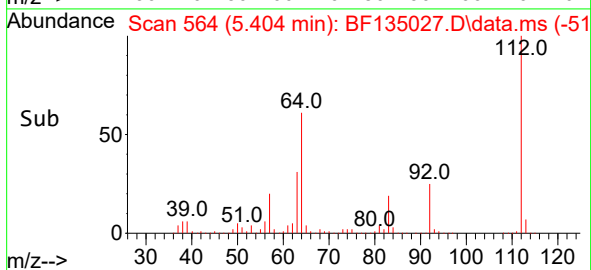
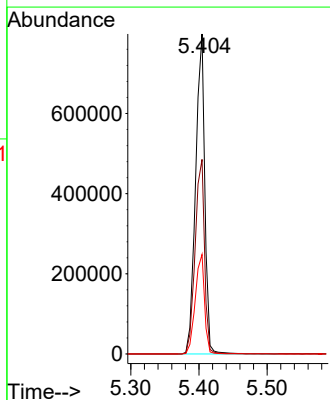
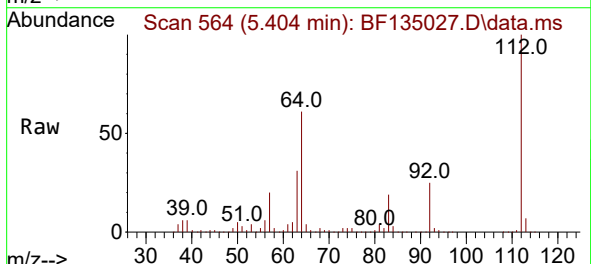




#7
Phenol-d6
Concen: 82.052 ng
RT: 6.410 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF135027.D
Acq: 31 Aug 2023 03:28




Instrument :
BNA_F
ClientSampleId :
OR-309-OK-370-COMP-24

Tgt Ion: 99 Resp: 917864
Ion Ratio Lower Upper
99 100
42 21.0 16.6 25.0
71 34.6 27.0 40.6

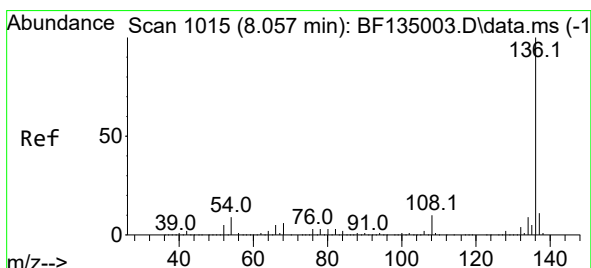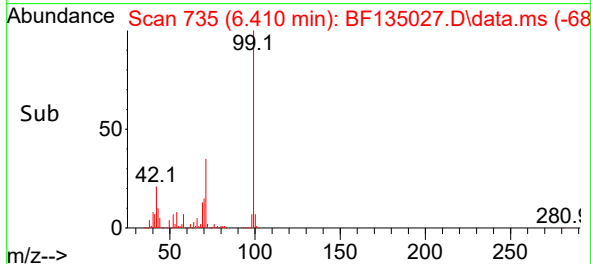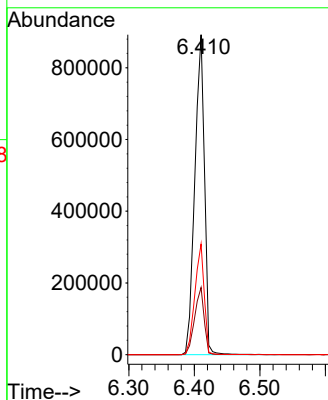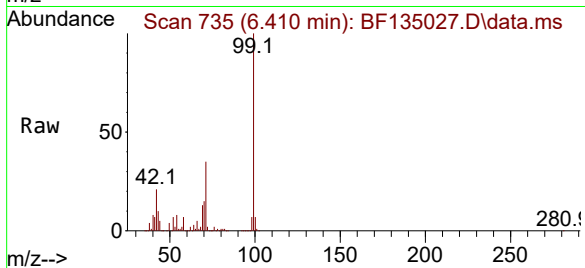

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.051 min Scan# 1014
Delta R.T. -0.006 min
Lab File: BF135027.D
Acq: 31 Aug 2023 03:28

Tgt Ion: 136 Resp: 538693
Ion Ratio Lower Upper
136 100
137 10.7 8.8 13.2
54 8.4 7.0 10.4
68 5.5 4.6 6.8

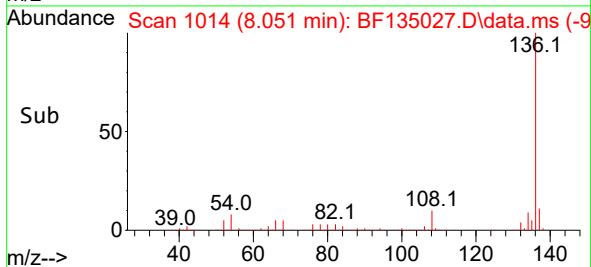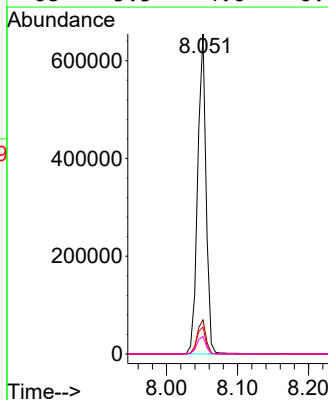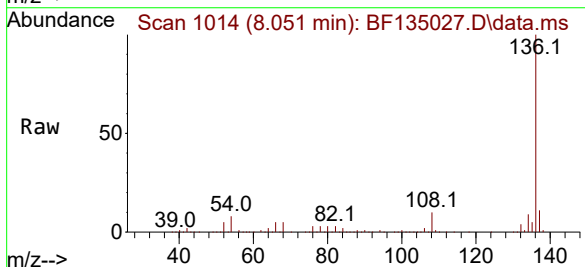



#23

Nitrobenzene-d5

Concen: 57.664 ng

RT: 7.334 min Scan# 894

Delta R.T. -0.012 min

Lab File: BF135027.D


Acq: 31 Aug 2023 03:28

Instrument :

BNA_F

ClientSampleId :

OR-309-OK-370-COMP-24

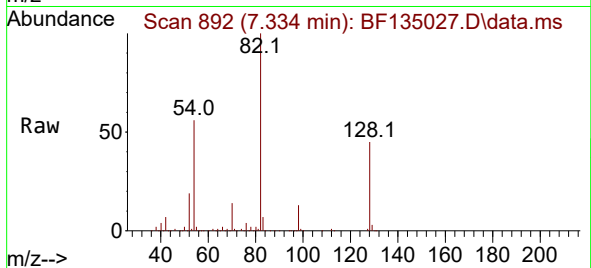




Tgt Ion: 82 Resp: 552915

Ion Ratio Lower Upper

82 100

128 45.3 37.8 56.8

54 56.3 45.0 67.6

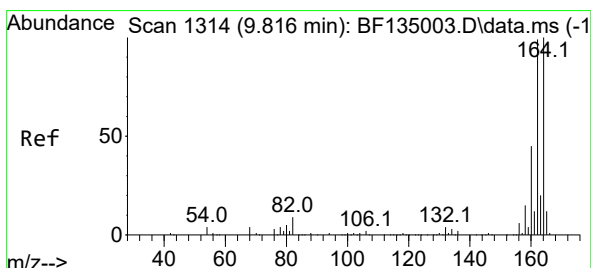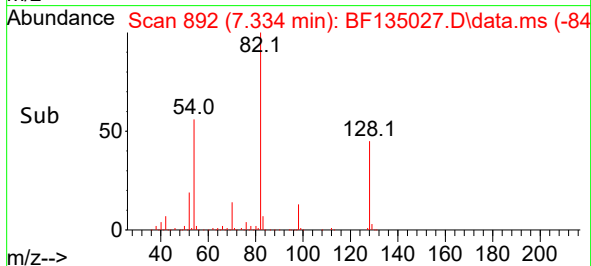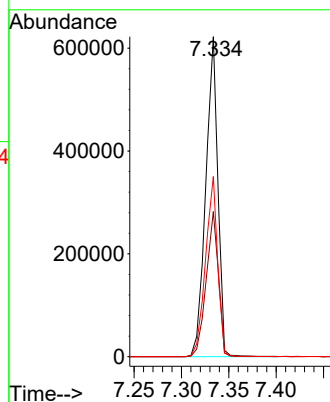

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.810 min Scan# 1313

Delta R.T. -0.006 min

Lab File: BF135027.D

Acq: 31 Aug 2023 03:28




Tgt Ion: 164 Resp: 246492

Ion Ratio Lower Upper

164 100

162 103.3 79.5 119.3

160 46.2 36.0 54.0

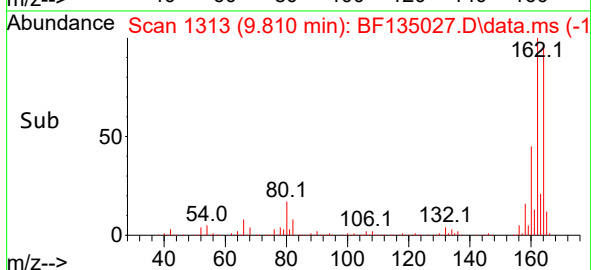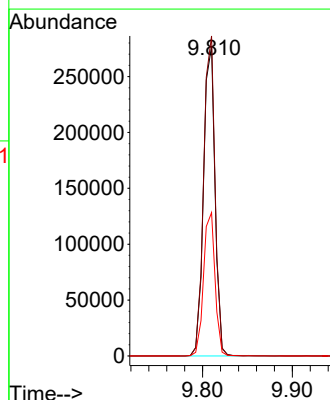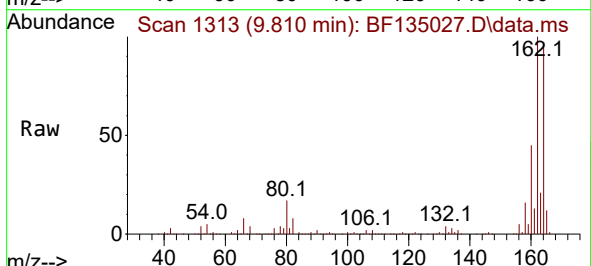



#42

2,4,6-Tribromophenol

Concen: 71.101 ng

RT: 10.598 min Scan# 1447

Delta R.T. -0.012 min

Lab File: BF135027.D


Acq: 31 Aug 2023 03:28

Instrument :

BNA_F

ClientSampleId :

OR-309-OK-370-COMP-24

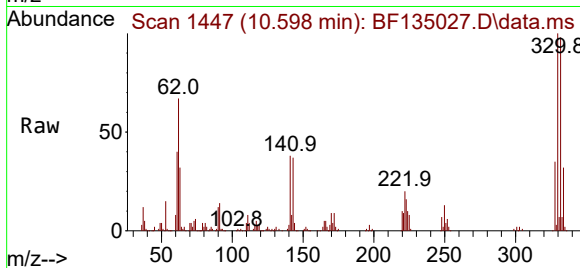




Tgt Ion:330 Resp: 185912

Ion Ratio Lower Upper

330 100

332 97.0 77.6 116.4

141 32.6 26.3 39.5

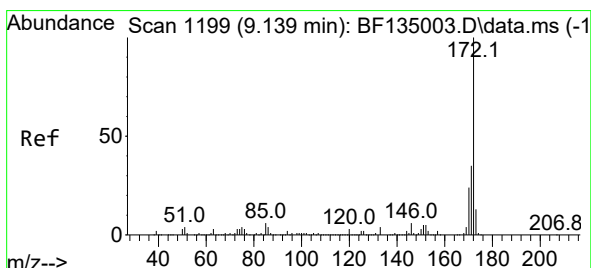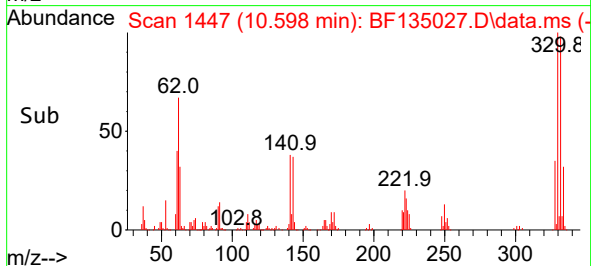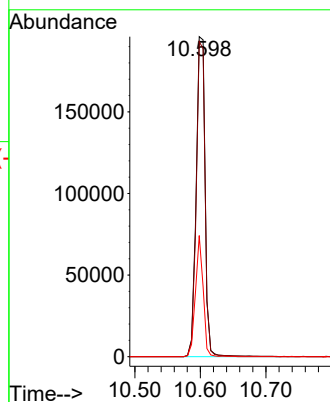

#45

2-Fluorobiphenyl

Concen: 63.499 ng

RT: 9.134 min Scan# 1198

Delta R.T. -0.006 min

Lab File: BF135027.D

Acq: 31 Aug 2023 03:28




Tgt Ion:172 Resp: 961365


Ion Ratio Lower Upper

172 100

171 34.8 28.2 42.2

170 23.2 19.0 28.4

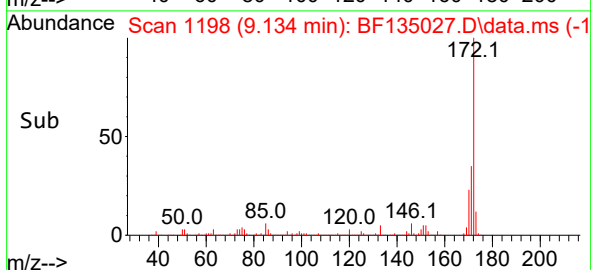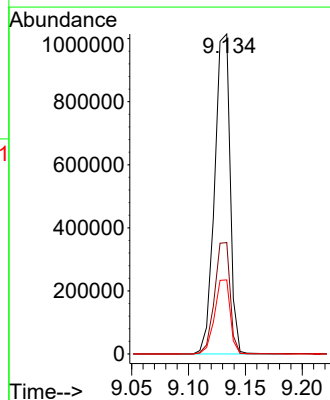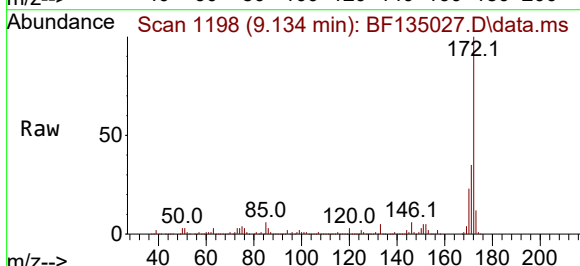

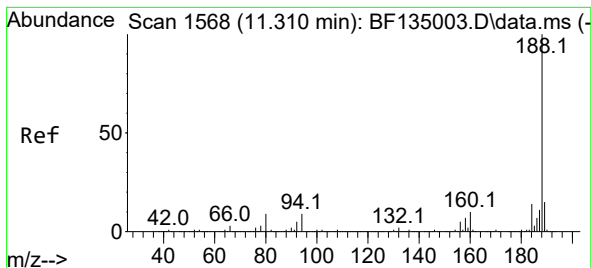

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.298 min Scan# 1

Delta R.T. -0.012 min

Lab File: BF135027.D

Acq: 31 Aug 2023 03:28

Instrument :

BNA_F

ClientSampleId :

OR-309-OK-370-COMP-24





Tgt Ion:188 Resp: 356239

Ion Ratio Lower Upper

188 100

94 9.9 7.0 10.4

80 10.3 7.4 11.2

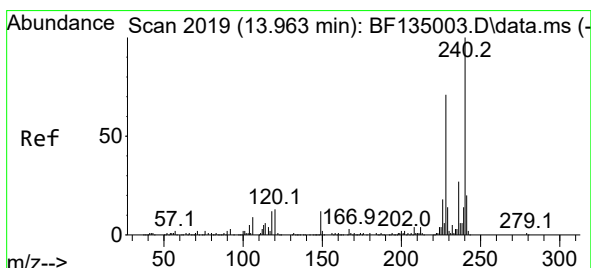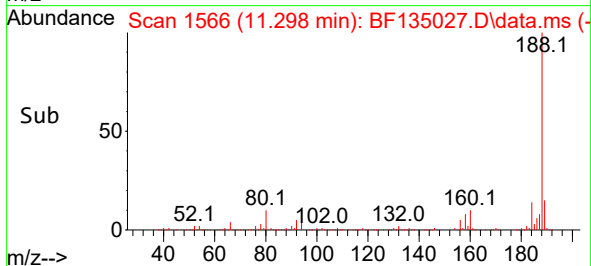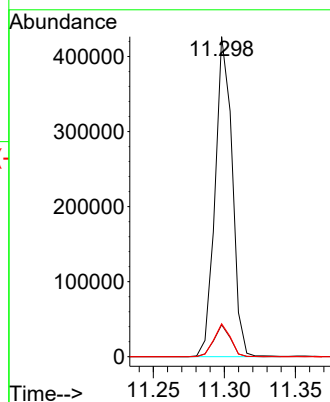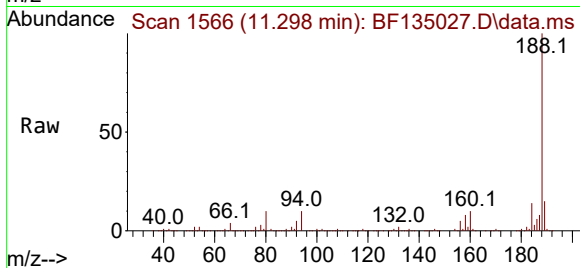

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.957 min Scan# 2018

Delta R.T. -0.006 min

Lab File: BF135027.D

Acq: 31 Aug 2023 03:28




Tgt Ion:240 Resp: 252236

Ion Ratio Lower Upper

240 100

120 11.0 10.2 15.2


236 26.4 21.3 31.9

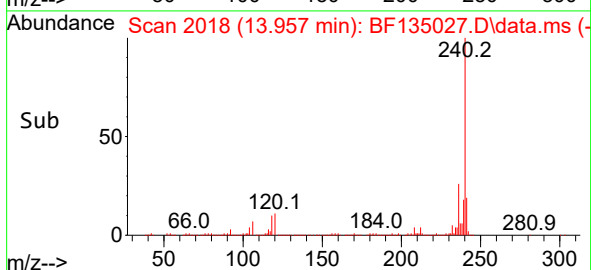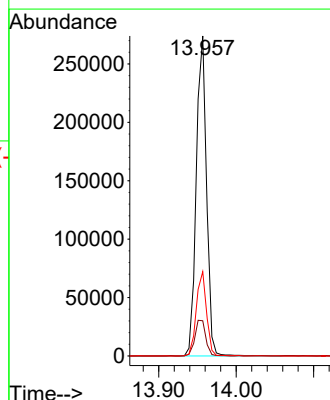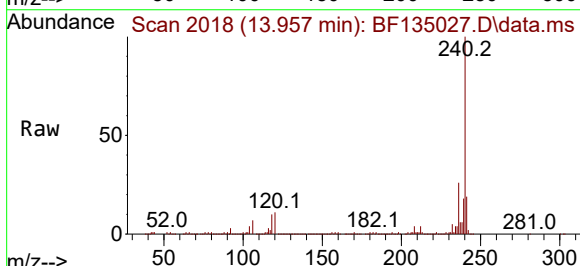






#79
 Terphenyl-d14
 Concen: 46.409 ng
 RT: 12.898 min Scan# 1838
 Delta R.T. -0.006 min
 Lab File: BF135027.D
 Acq: 31 Aug 2023 03:28

Instrument :
 BNA_F
 ClientSampleId :
 OR-309-OK-370-COMP-24

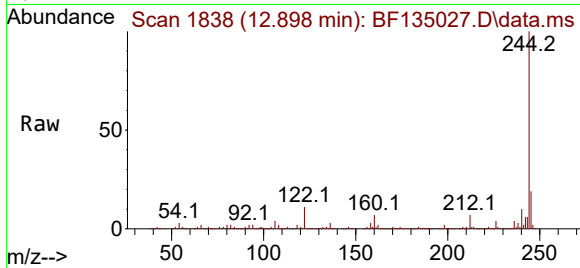

Tgt Ion:244 Resp: 717322
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.6 8.4
 122 11.3 9.8 14.6

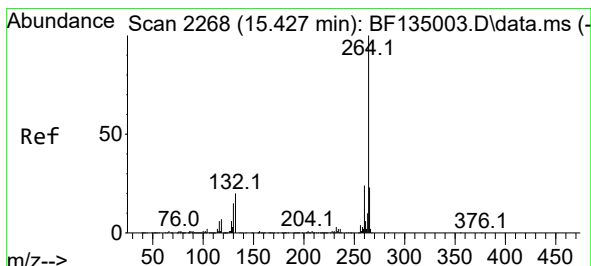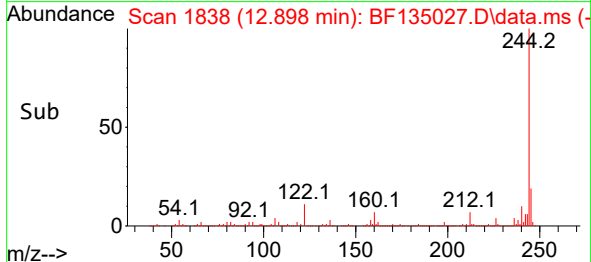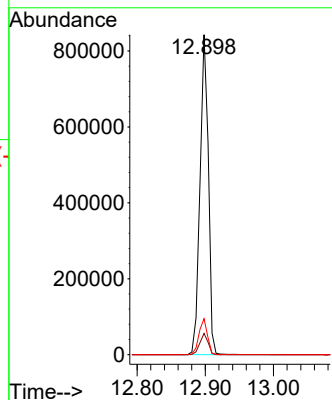

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.427 min Scan# 2268
 Delta R.T. 0.000 min
 Lab File: BF135027.D
 Acq: 31 Aug 2023 03:28

Tgt Ion:264 Resp: 243462
 Ion Ratio Lower Upper
 264 100
 260 24.7 19.0 28.6
 265 21.6 18.2 27.2

