

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
 Data File : BF135011.D
 Acq On : 30 Aug 2023 18:27
 Operator : CG\JU
 Sample : PB155120BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155120BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.010	491	497	508	rVB	1529419	2179613	44.22%	7.610%
2	5.410	560	565	568	rBV	3082854	2868672	58.20%	10.016%
3	6.410	730	735	738	rBV	2897172	2816977	57.15%	9.836%
4	6.769	793	796	800	rBV	926931	776045	15.74%	2.710%
5	7.339	887	893	895	rBV	2367909	2755388	55.90%	9.621%
6	8.051	1009	1014	1017	rBV	1194687	1073555	21.78%	3.748%
7	9.133	1192	1198	1201	rBV	4716712	4712599	95.61%	16.455%
8	9.810	1307	1313	1316	rBV	1396177	1239185	25.14%	4.327%
9	10.604	1443	1448	1451	rBV	2209218	2149466	43.61%	7.505%
10	11.304	1562	1567	1570	rBV	1450175	1337607	27.14%	4.670%
11	12.904	1834	1839	1842	rBV	4518029	4928881	100.00%	17.210%
12	13.957	2014	2018	2021	rBV	1228467	1043164	21.16%	3.642%
13	15.427	2262	2268	2273	rBV	599997	758480	15.39%	2.648%




Sum of corrected areas: 28639632

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF135011.D
Acq On : 30 Aug 2023 18:27
Operator : CG\JU
Sample : PB155120BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155120BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

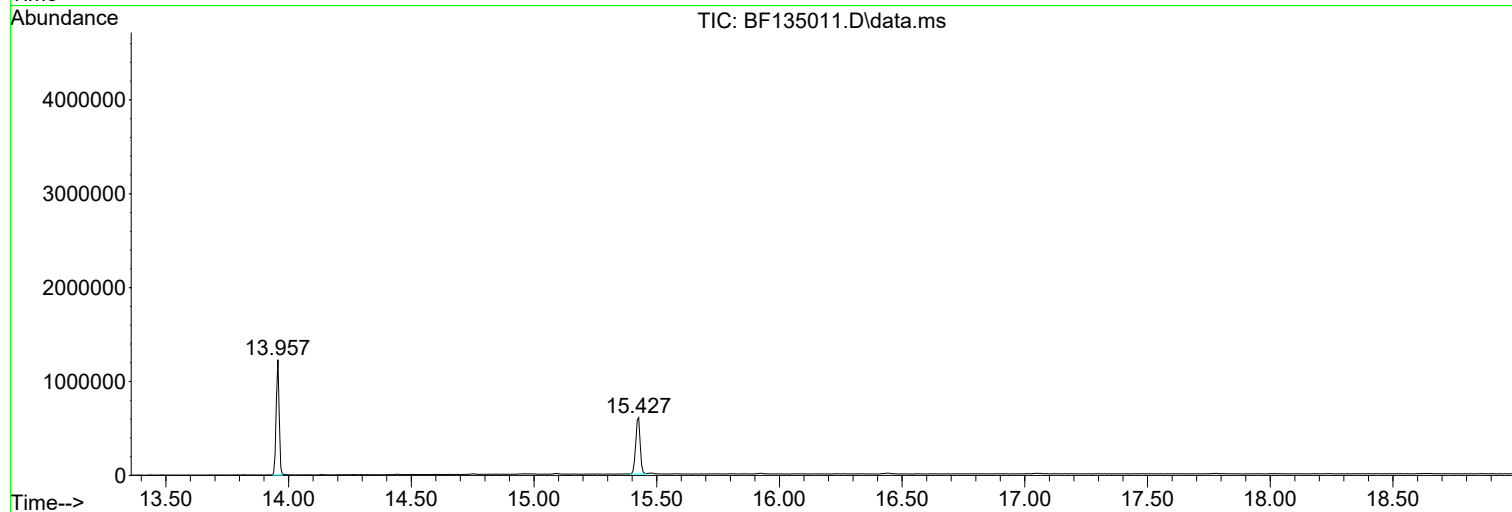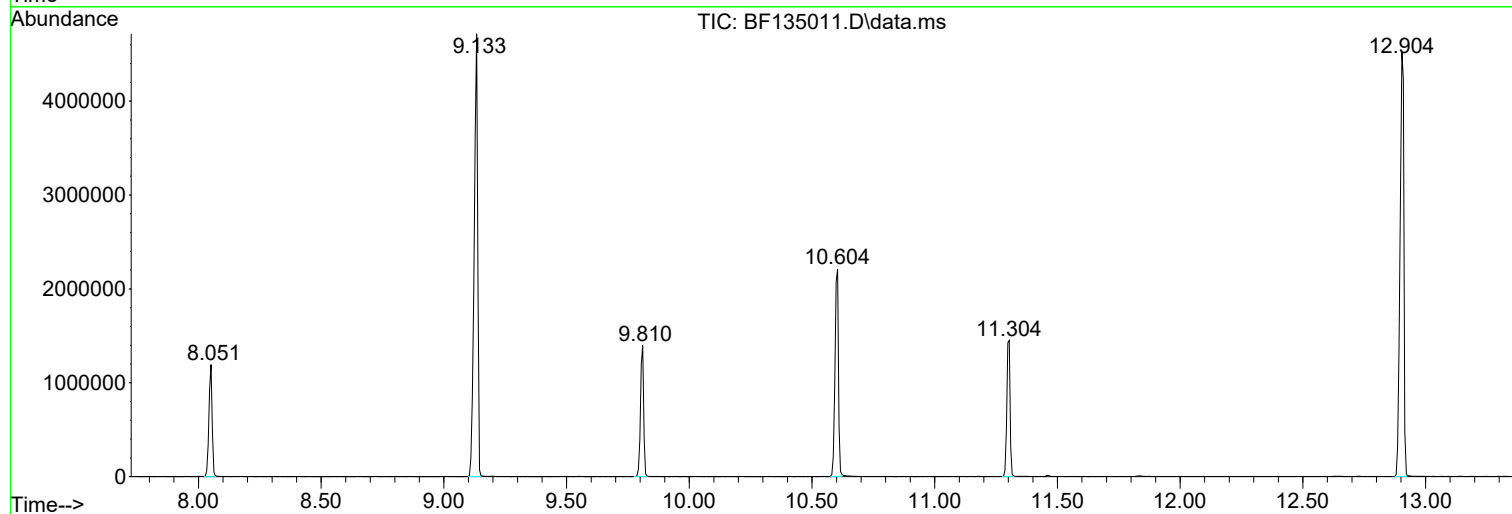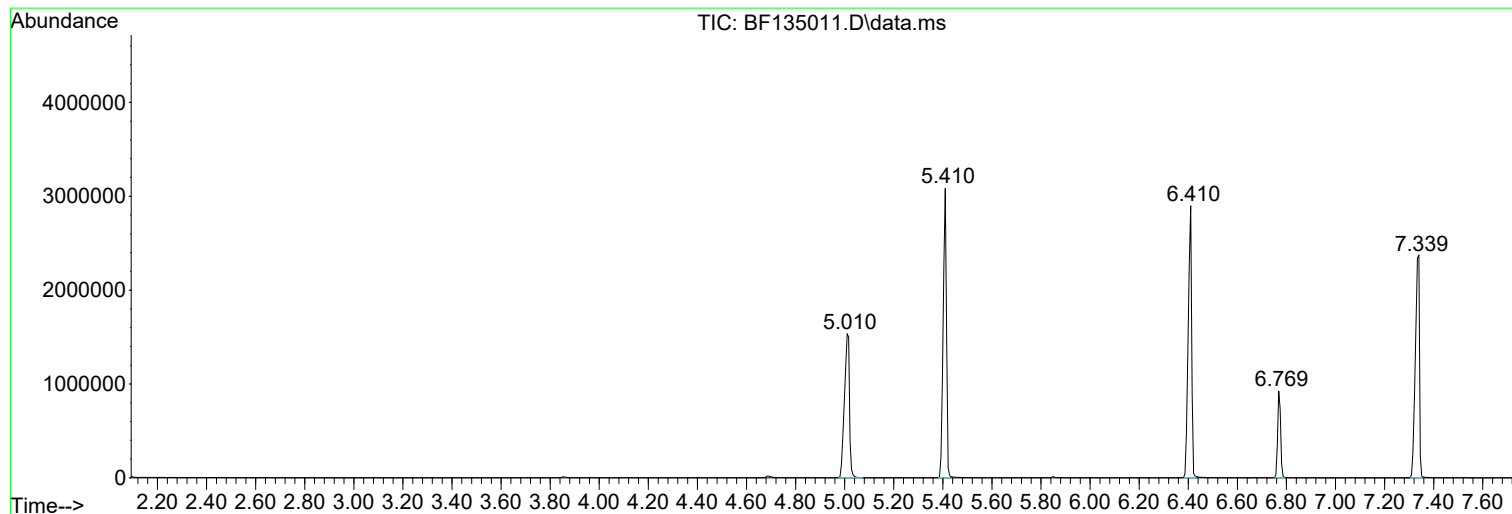

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF135011.D
Acq On : 30 Aug 2023 18:27
Operator : CG\JU
Sample : PB155120BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155120BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.010 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.010	56.17 ng	2179610	1,4-Dichlorobenzene-d4	6.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45		
2	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

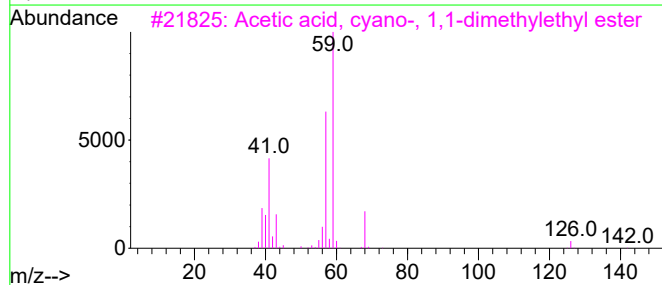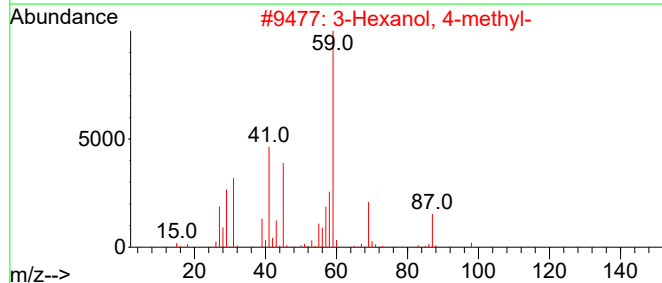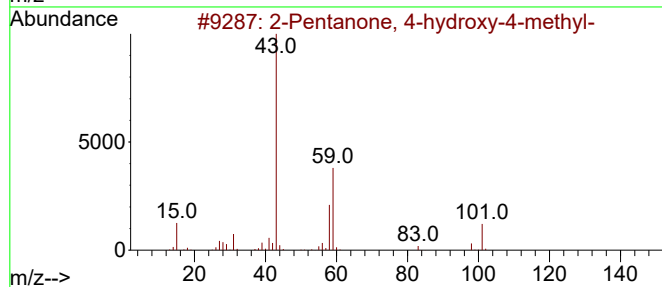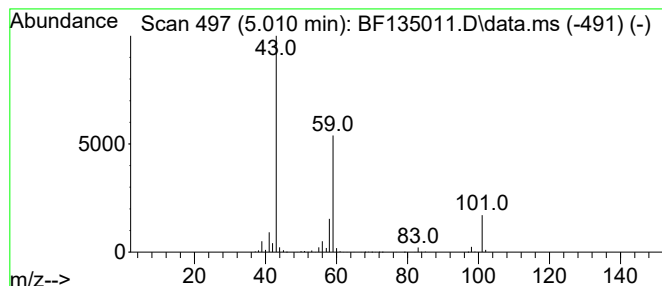

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF135011.D
Acq On : 30 Aug 2023 18:27
Operator : CG\JU
Sample : PB155120BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155120BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.010	5.010	56.2	ng	2179610	1	6.769	776045	20.0