


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF135013.D
Acq On : 30 Aug 2023 19:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 31 03:48:08 2023

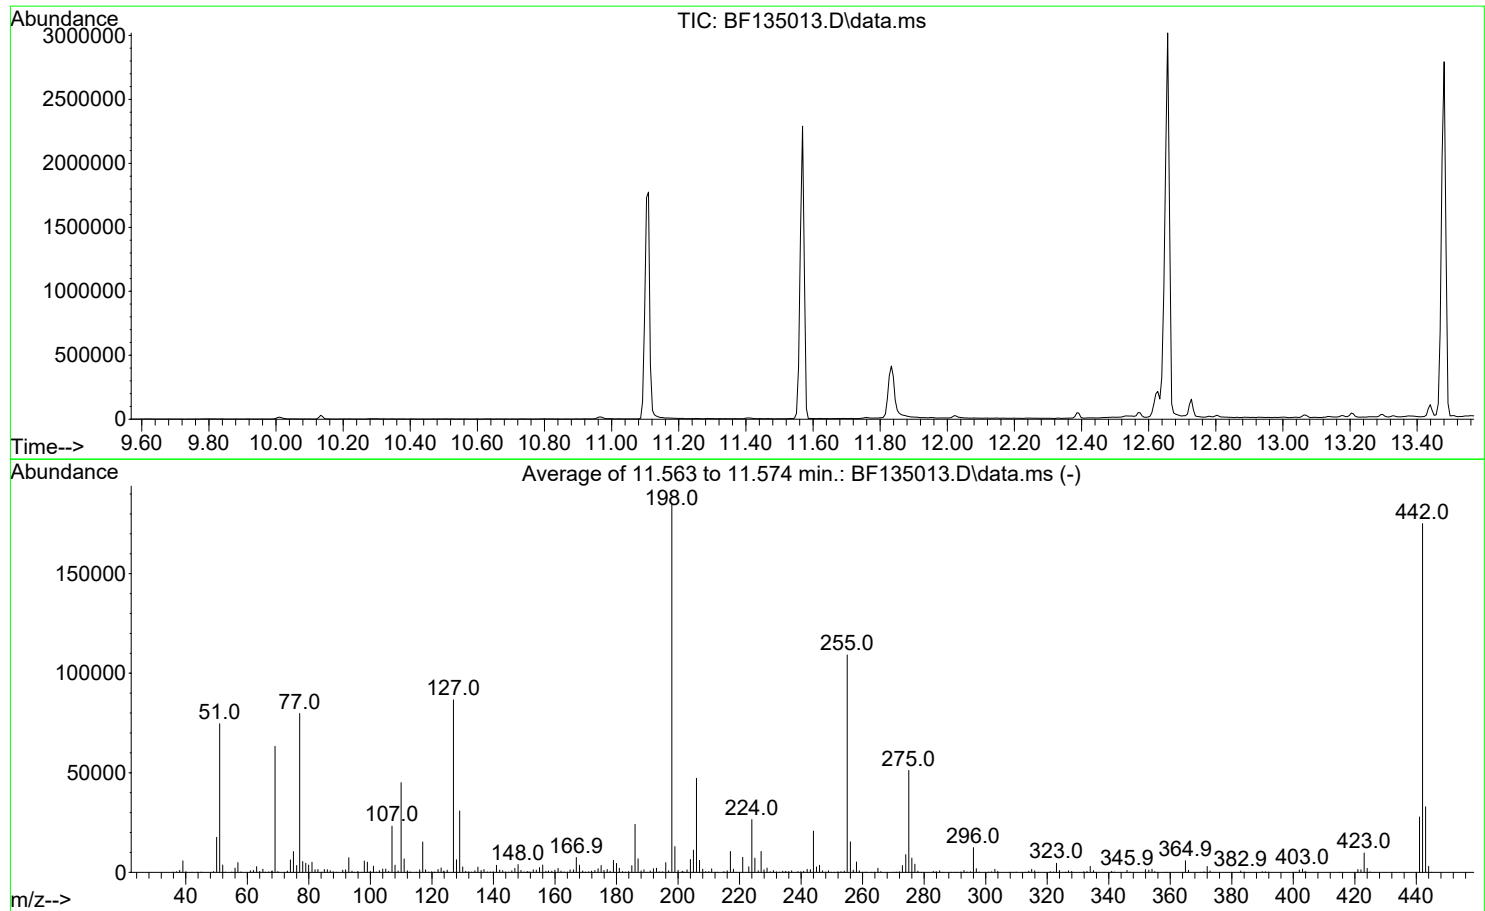




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	74651	PASS
68	69	0.00	2	1.2	729	PASS
69	198	0.00	100	34.3	63301	PASS
70	69	0.00	2	0.6	397	PASS
127	198	10	80	46.9	86608	PASS
197	198	0.00	2	0.4	803	PASS
198	198	100	100	100.0	184725	PASS
199	198	5	9	7.0	12973	PASS
275	198	10	60	27.7	51181	PASS
365	198	1	100	3.2	5896	PASS
441	198	0.01	100	15.1	27839	PASS
442	442	50	100	100.0	175176	PASS
443	442	15	24	18.8	32984	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF135013.D
Acq On : 30 Aug 2023 19:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 31 07:33:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

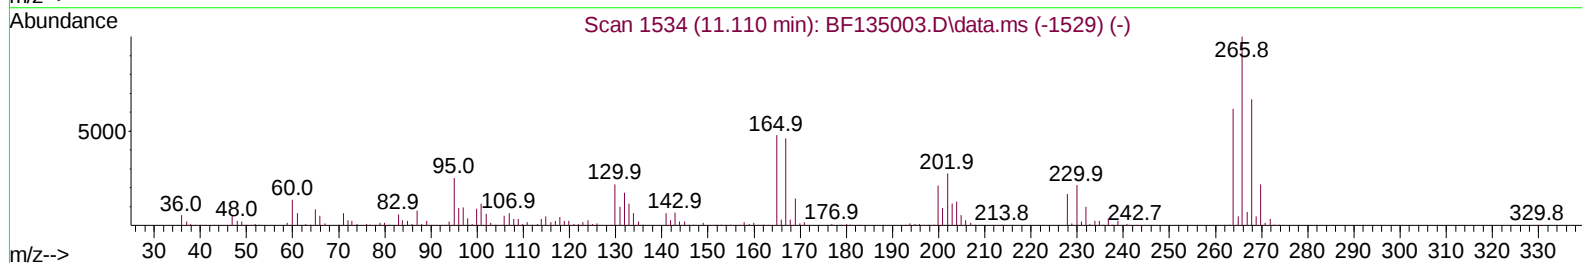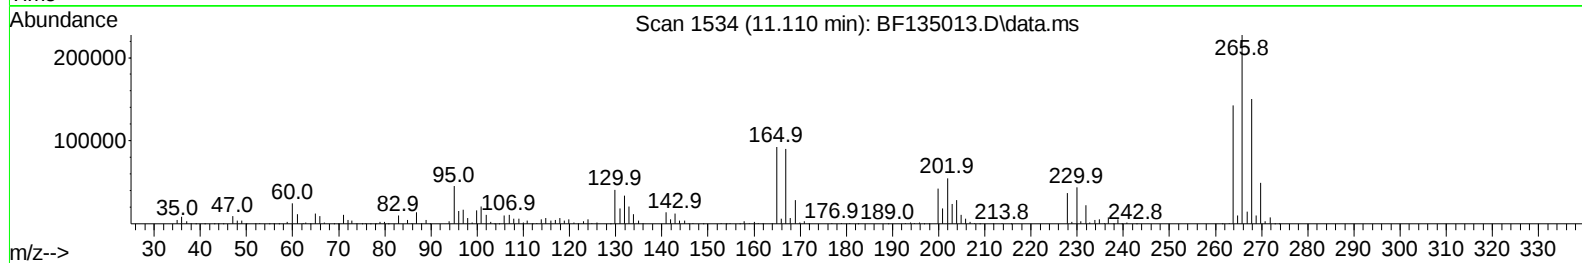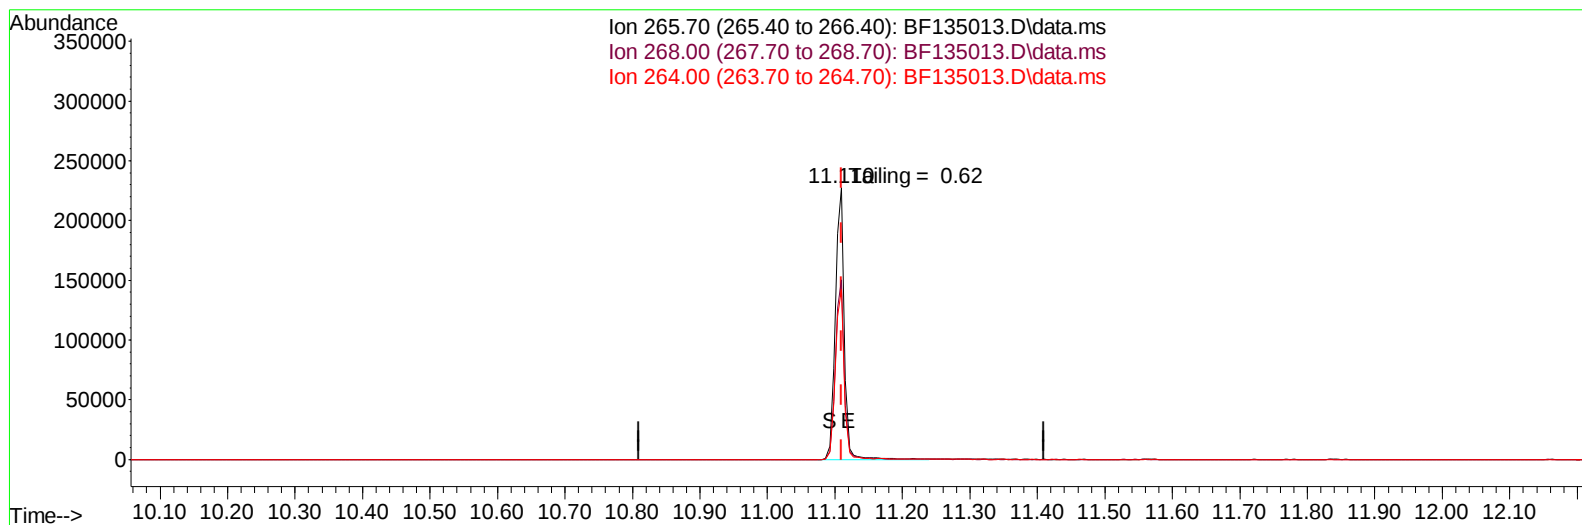

TIC: BF135013.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.000) 159876.06 ng




response 211099

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	66.13
264.00	61.60	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083023\
Data File : BF135013.D
Acq On : 30 Aug 2023 19:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 31 07:33:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

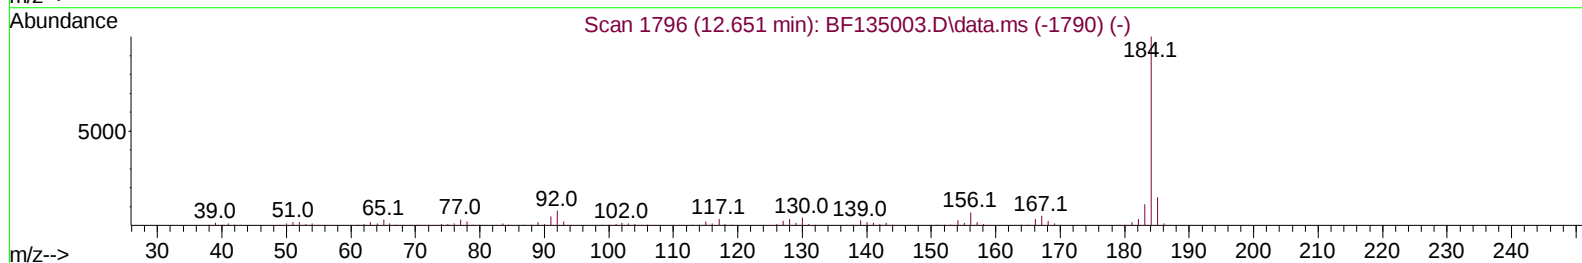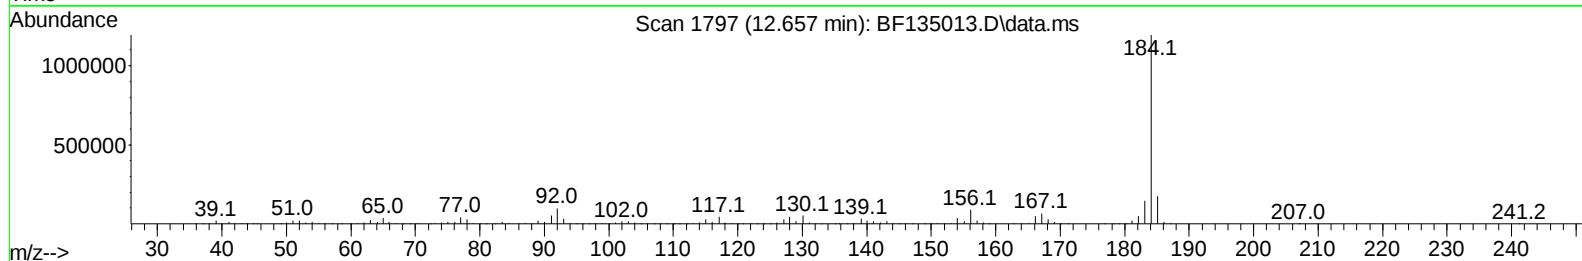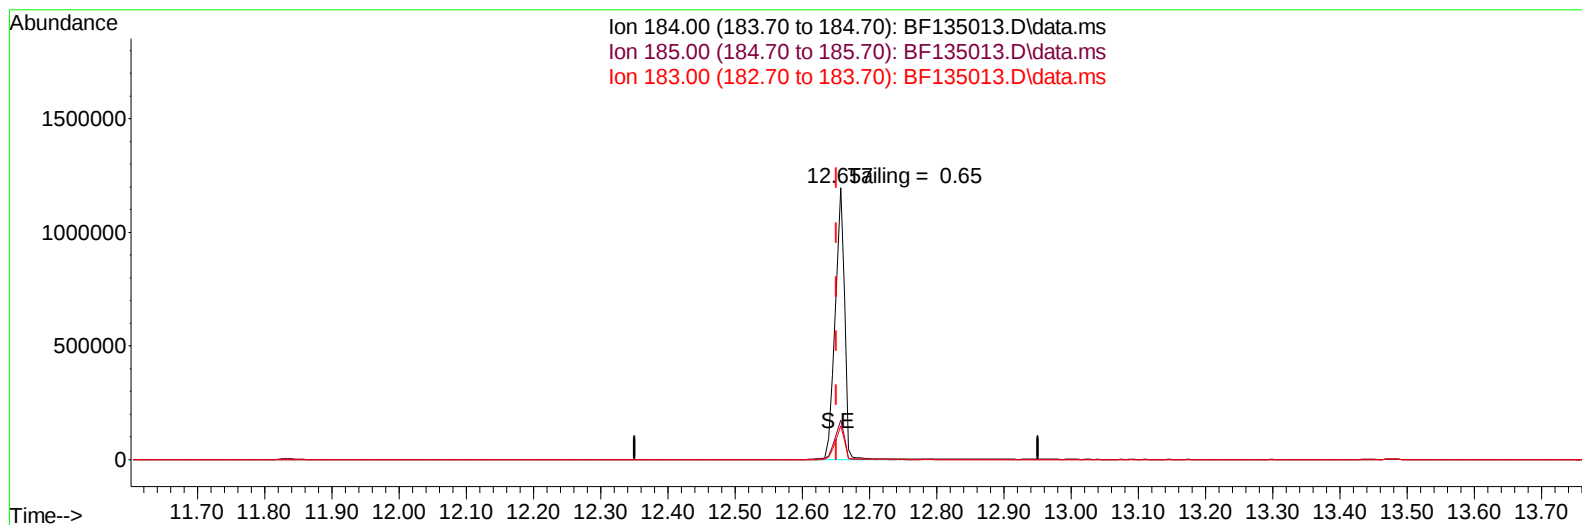

TIC: BF135013.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 991443.38 ng

response 1161694

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.51
183.00	11.30	12.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/30/2023	BNA_F	<u>BF135013.D</u>
Compound Name	Response	Retention Time
DDT	491054	13.48
DDD	7910	13.204
DDE	4098	11.568
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12008	503062	2.39

Instrument :
BNA_F
ClientSampleId :
DFTPP