

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
 Data File : BF108729.D
 Acq On : 1 Sep 2018 10:06
 Operator : JU/SJ
 Sample : J4729-15
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 04 02:03:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 30 15:06:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	60650	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	231656	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	111209	20.00	ng	-0.01
63) Phenanthrene-d10	11.54	188	251816	20.00	ng	0.00
75) Chrysene-d12	14.19	240	242394	20.00	ng	0.00
86) Perylene-d12	15.75	264	161477	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.68	112	20766	5.95	ng	0.04
7) Phenol-d6	6.66	99	52705	10.54	ng	0.01
23) Nitrobenzene-d5	7.57	82	472844	103.61	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	121961	83.07	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	943227	114.04	ng	0.00
78) Terphenyl-d14	13.12	244	1082142	86.74	ng	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.78	77	6318	2.044	ng	# 66
15) Benzyl Alcohol	7.15	79	8460	2.352	ng	# 42
19) n-Nitroso-di-n-propylamine	7.57	70	55359	16.532	ng	# 83
25) Isophorone	7.57	82	472844	62.369	ng	# 64
49) Dimethylphthalate	9.75	163	33246	3.796	ng	100
50) 2,6-Dinitrotoluene	10.04	165	12890	6.678	ng	# 24
56) 2,4-Dinitrotoluene	10.04	165	13536	5.296	ng	# 21
66) 4-Bromophenyl-phenylether	10.84	248	7677	2.481	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
Data File : BF108729.D
Acq On : 1 Sep 2018 10:06
Operator : JU/SJ
Sample : J4729-15
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 04 02:03:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

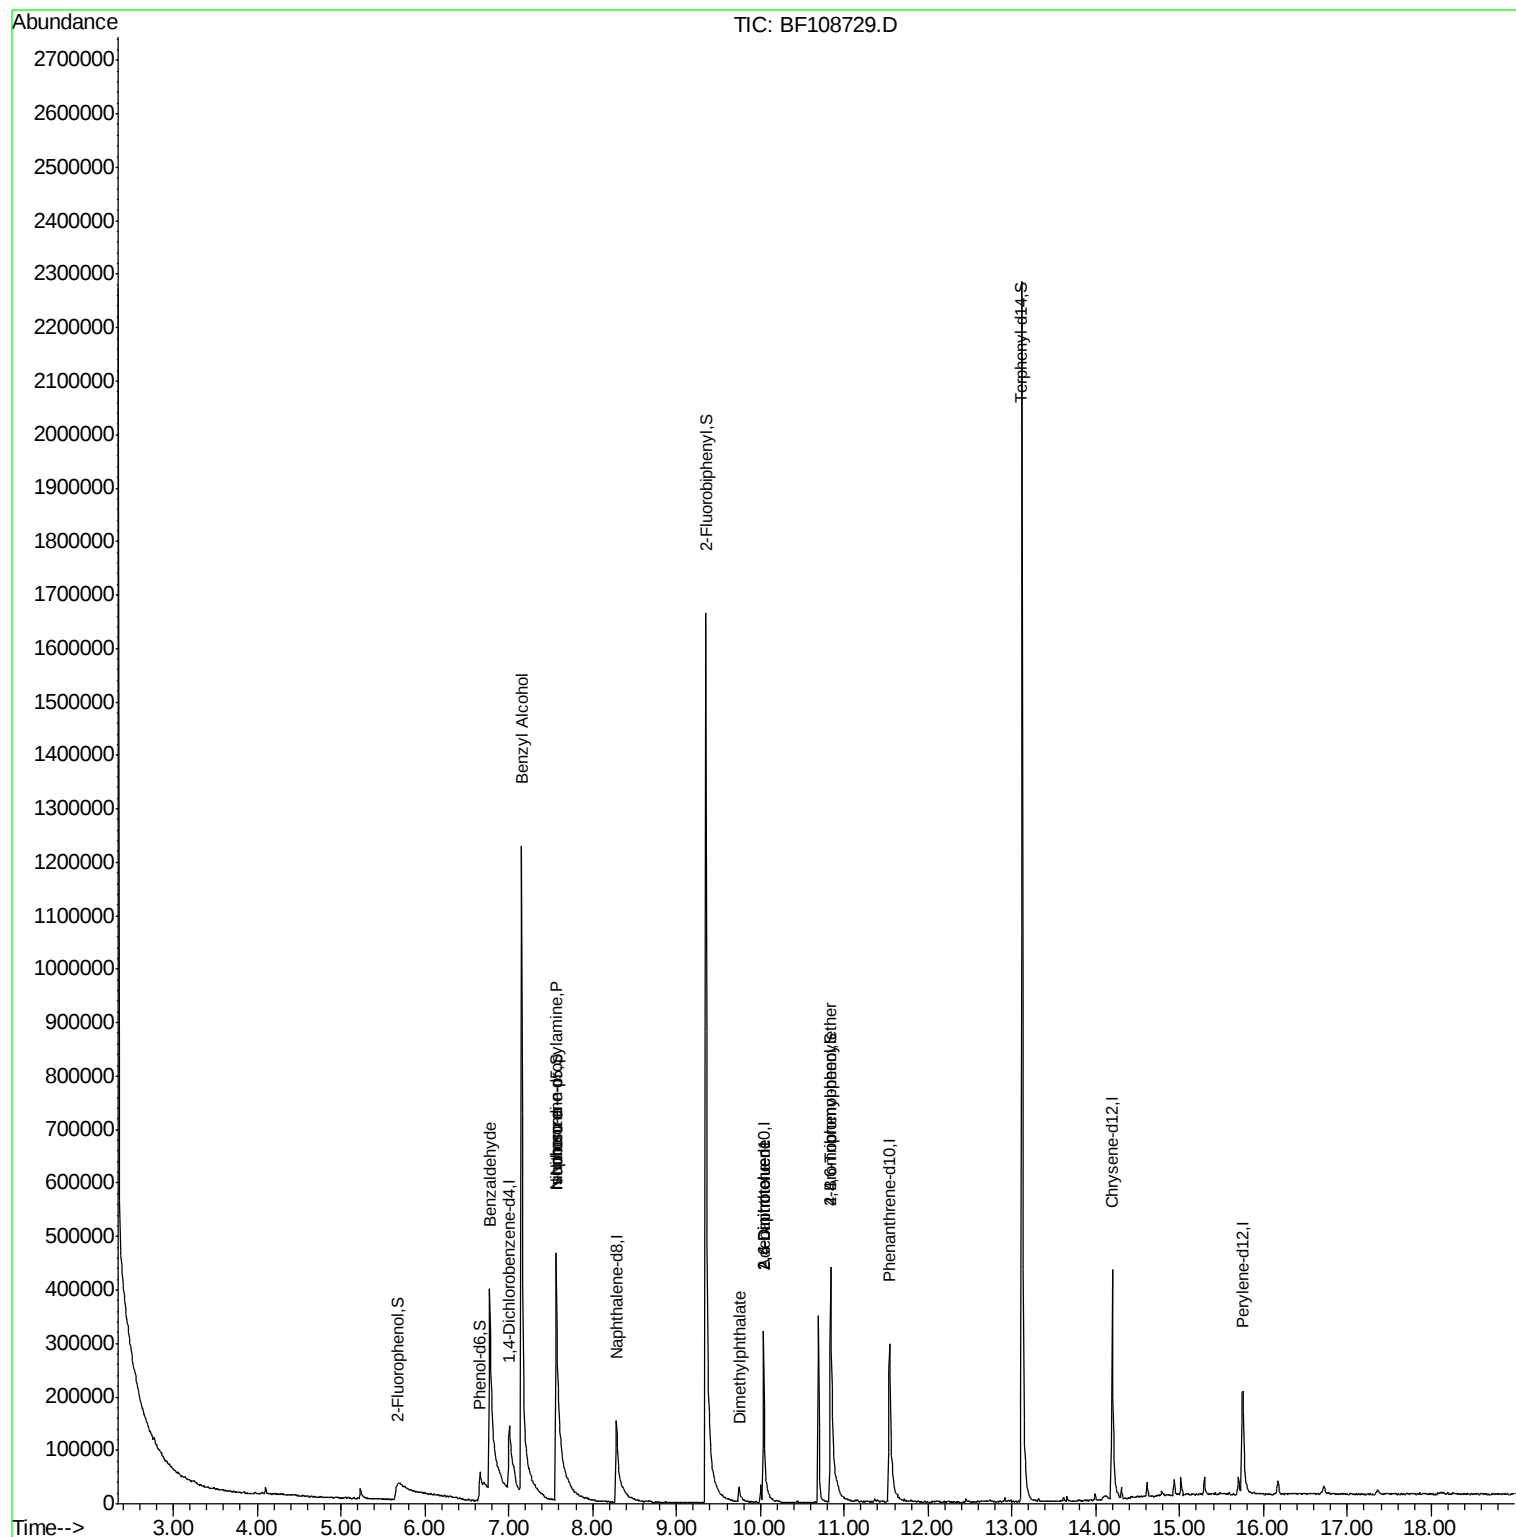

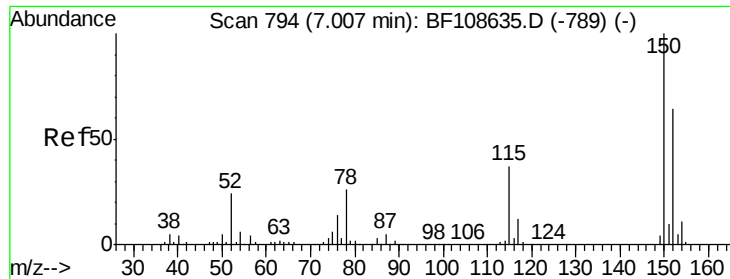


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.01 min Scan# 794
Delta R.T. 0.00 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 60650
Ion Ratio Lower Upper
152 100
150 153.8 124.6 186.8
115 59.4 50.1 75.1

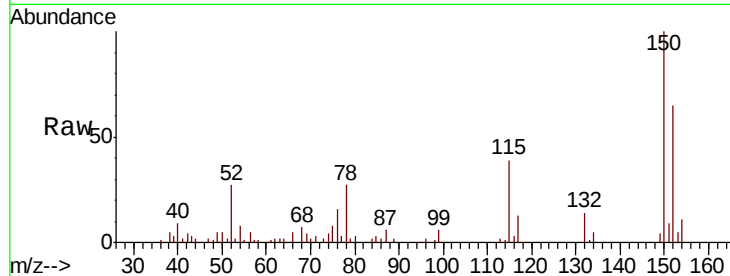


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

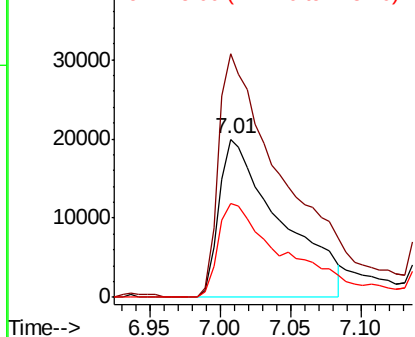



#5


2-Fluorophenol
Concen: 5.948 ng
RT: 5.68 min Scan# 569
Delta R.T. 0.04 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06

Tgt Ion:112 Resp: 20766
Ion Ratio Lower Upper
112 100
64 66.4 47.9 71.9
63 29.8 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

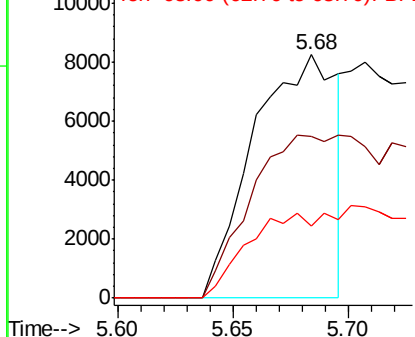

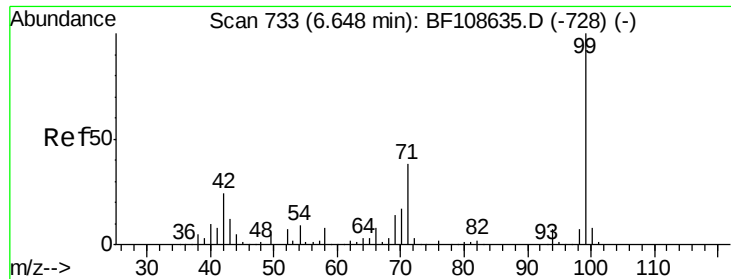

#7

Phenol-d6

Concen: 10.540 ng

RT: 6.66 min Scan# 735

Delta R.T. 0.01 min

Lab File: BF108729.D

Acq: 1 Sep 2018 10:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 52705

Ion Ratio Lower Upper




99 100

42 22.2 14.5 21.7#

71 38.7 25.4 38.0#

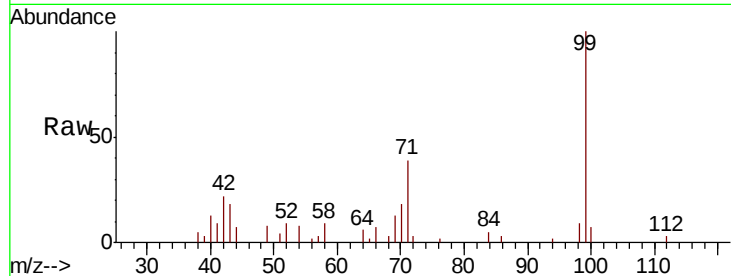

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

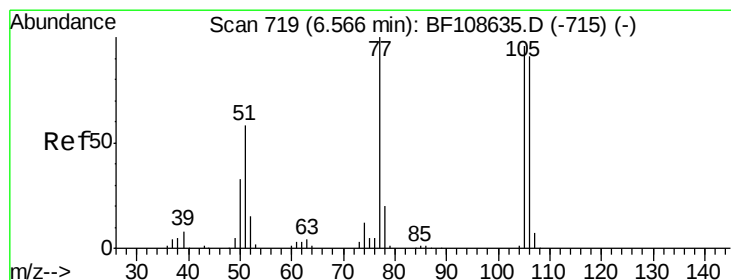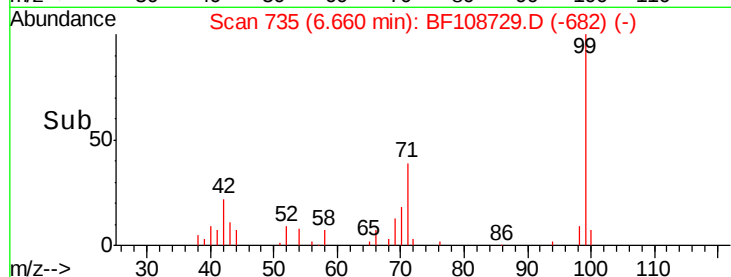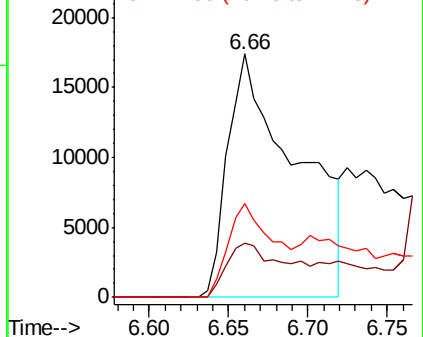

#9

Benzaldehyde

Concen: 2.044 ng

RT: 6.78 min Scan# 755

Delta R.T. 0.21 min

Lab File: BF108729.D

Acq: 1 Sep 2018 10:06


Tgt Ion: 77 Resp: 6318

Ion Ratio Lower Upper



77 100


105 64.9 81.1 121.1#

106 64.6 74.5 114.5#

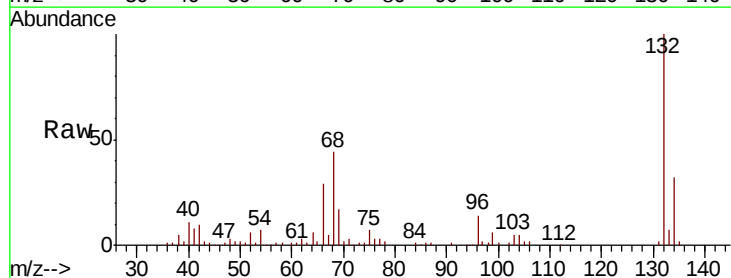

Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 105.00 (104.70 to 105.70): E
Ion 106.00 (105.70 to 106.70): E

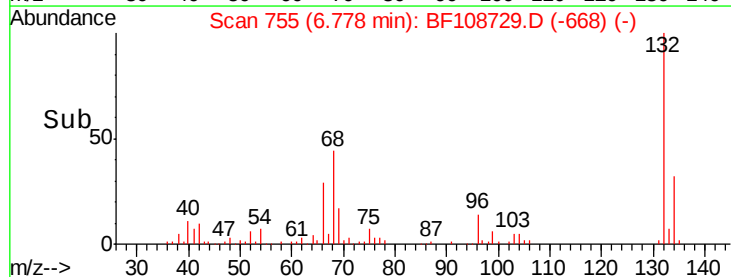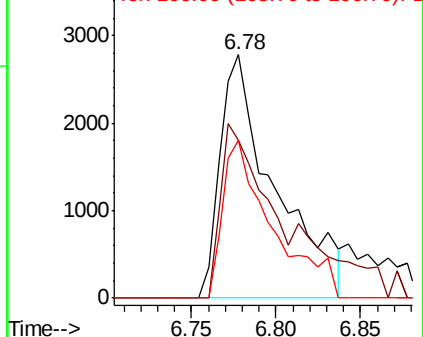

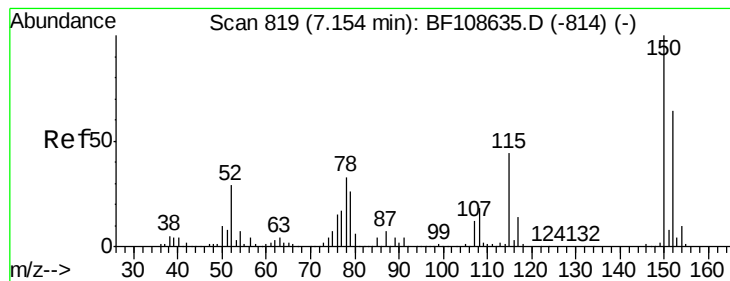

#15

Benzyl Alcohol

Concen: 2.352 ng

RT: 7.15 min Scan# 819

Delta R.T. 0.00 min

Lab File: BF108729.D

Acq: 1 Sep 2018 10:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 79 Resp: 8460

Ion Ratio Lower Upper

79 100

108 28.2 65.1 97.7#

77 107.2 50.6 75.8#






Abundance

Ion 79.00 (78.70 to 79.70): BF1

Ion 108.00 (107.70 to 108.70): BF1

Ion 77.00 (76.70 to 77.70): BF1

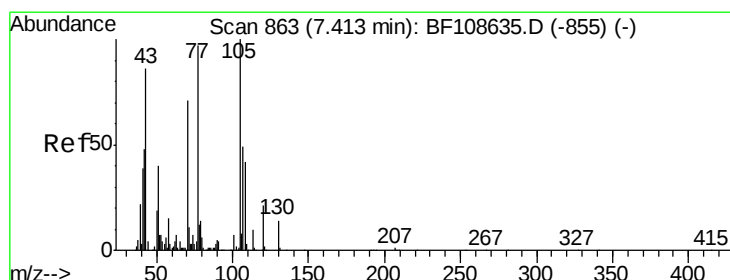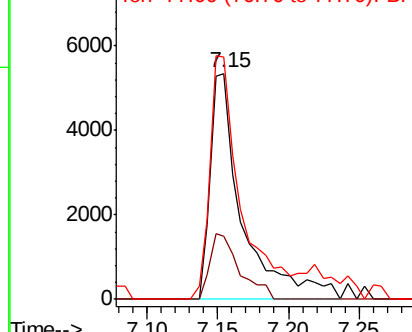

#19

n-Nitroso-di-n-propylamine

Concen: 16.532 ng

RT: 7.57 min Scan# 889

Delta R.T. 0.15 min

Lab File: BF108729.D

Acq: 1 Sep 2018 10:06

Tgt Ion: 70 Resp: 55359


Ion Ratio Lower Upper

70 100

42 53.4 47.5 71.3

101 0.0 7.4 11.2#

130 1.9 16.6 25.0#

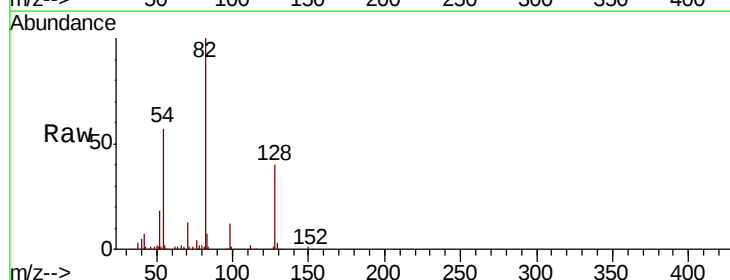



Abundance


Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1



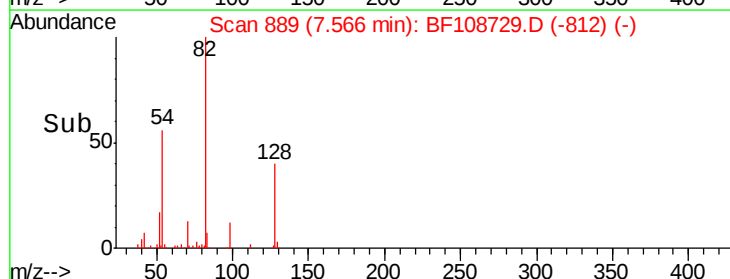
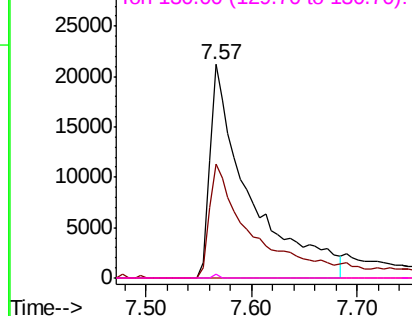


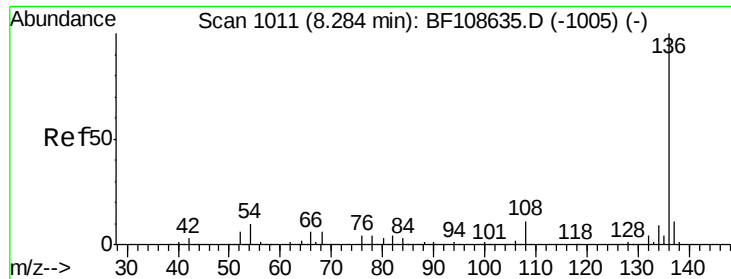

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.28 min Scan# 1011
Delta R.T. 0.00 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06




Instrument :
BNA_F
ClientSampleId :


Tot Ion:136	Resp:	231656
Ion Ratio	Lower	Upper
136	100	
137	11.1	8.9 13.3
54	9.8	6.6 9.8
68	5.7	5.0 7.4

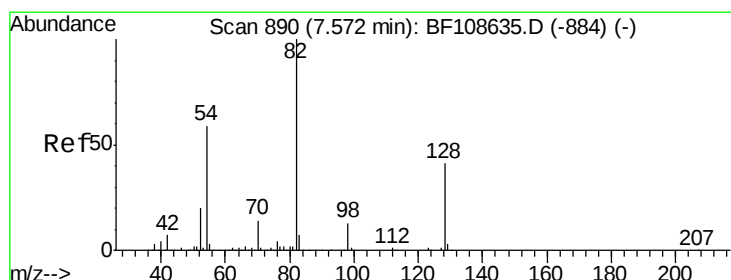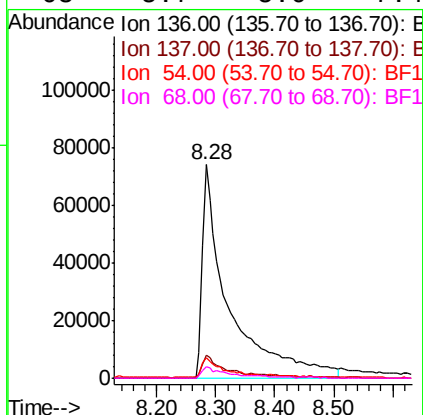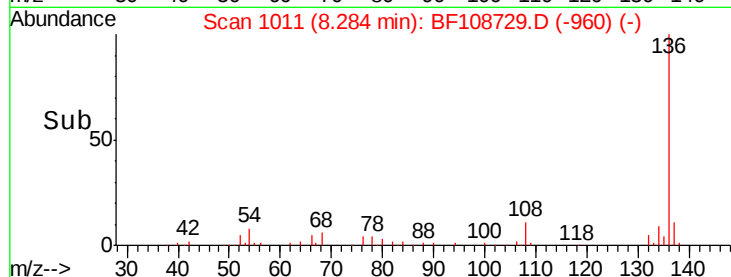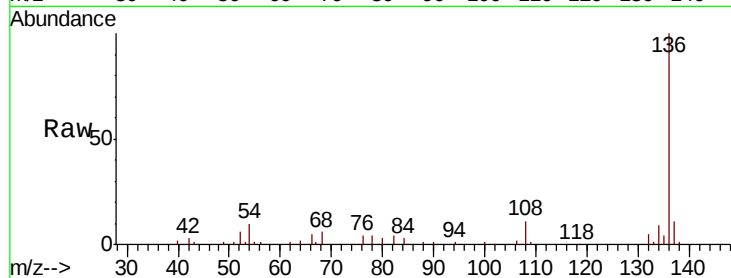

#23
Nitrobenzene-d5
Concen: 103.606 ng
RT: 7.57 min Scan# 889
Delta R.T. -0.01 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06

Tgt Ion: 82	Resp:	472844
Ion Ratio	Lower	Upper
82	100	
128	40.1	36.1 54.1
54	56.8	41.4 62.2

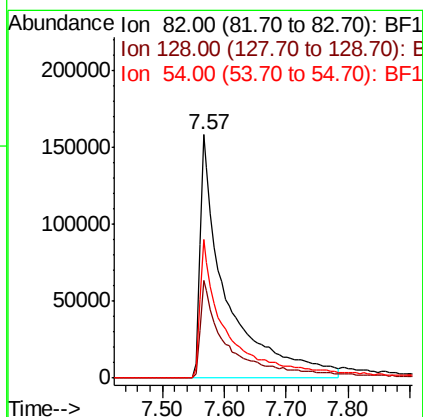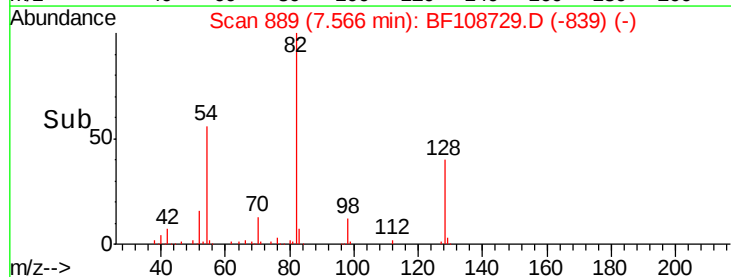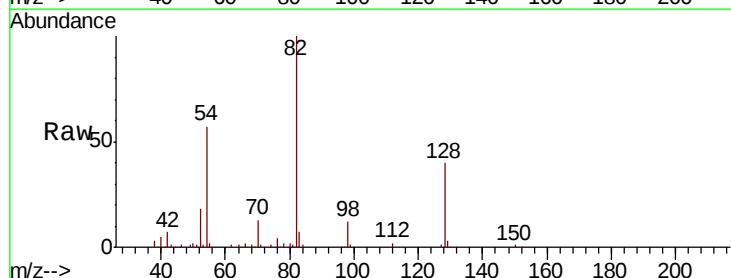

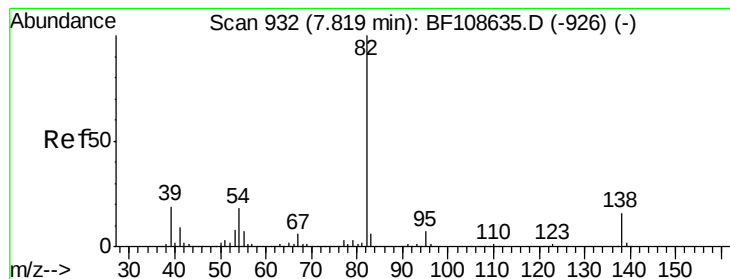

#25

Isophorone

Concen: 62.369 ng

RT: 7.57 min Scan# 889

Delta R.T. -0.25 min

Lab File: BF108729.D

Acq: 1 Sep 2018 10:06

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 472844

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

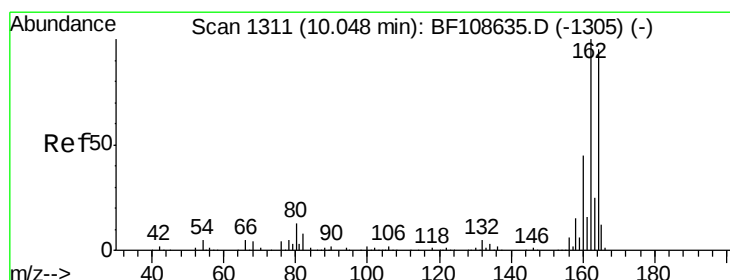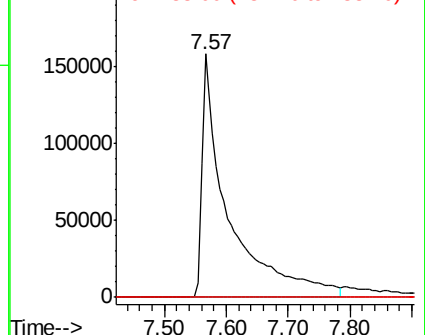

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.04 min Scan# 1309

Delta R.T. -0.01 min

Lab File: BF108729.D

Acq: 1 Sep 2018 10:06


Tgt Ion:164 Resp: 111209

Ion Ratio Lower Upper



164 100


162 103.2 86.1 129.1

160 44.8 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

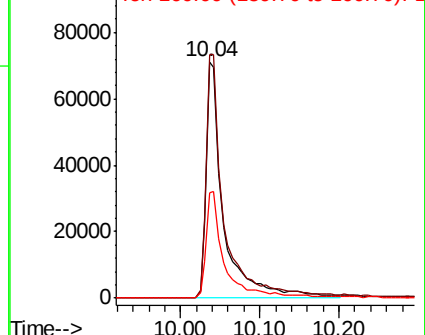







#41
 2,4,6-Tribromophenol
 Concen: 83.074 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108729.D
 Acq: 1 Sep 2018 10:06

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	99.8	77.0	115.6
141	31.0	29.9	44.9

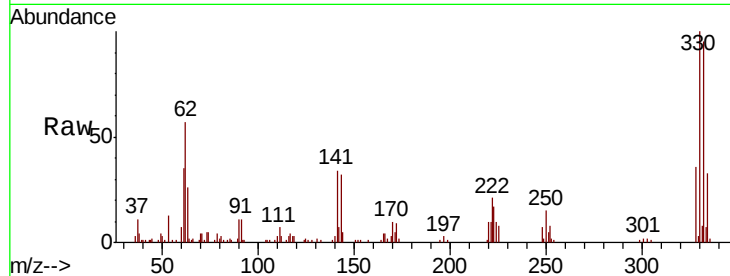


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

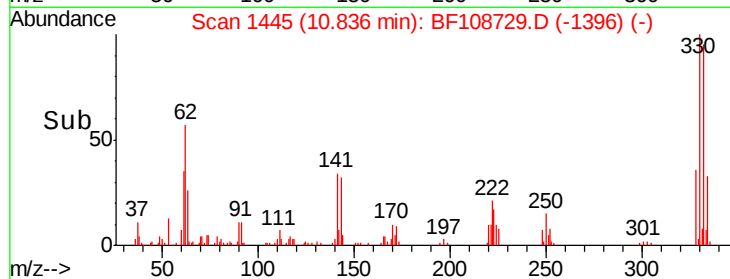
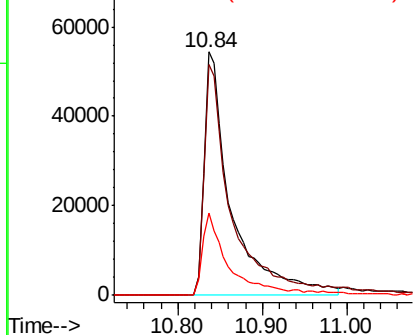



#44
 2-Fluorobiphenyl
 Concen: 114.041 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108729.D
 Acq: 1 Sep 2018 10:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	29.7	44.5
170	23.6	19.6	29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

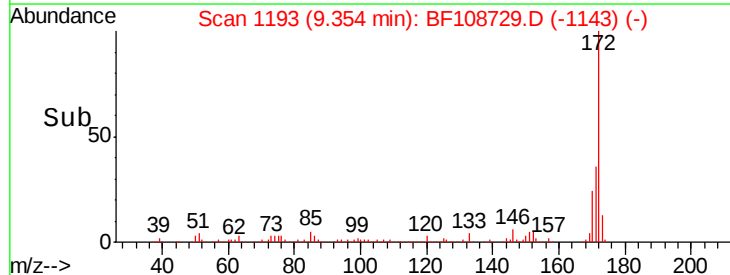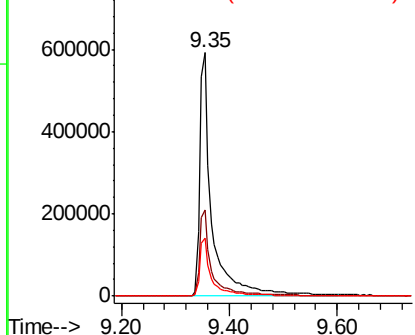


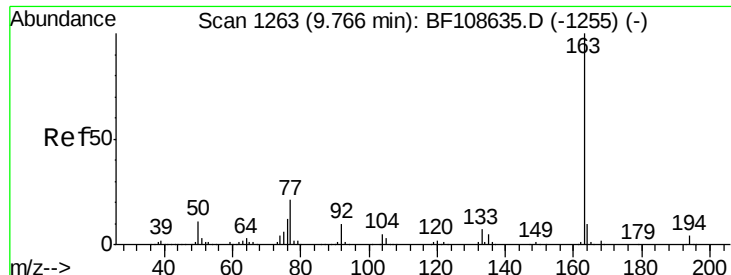




#49
Dimethylphthalate
Concen: 3.796 ng
RT: 9.75 min Scan# 1260
Delta R.T. -0.02 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06

Instrument :
BNA_F
ClientSampleId :

Tot Ion:163 Resp: 33246
Ion Ratio Lower Upper
163 100
194 3.5 2.7 4.1
164 10.4 8.2 12.2

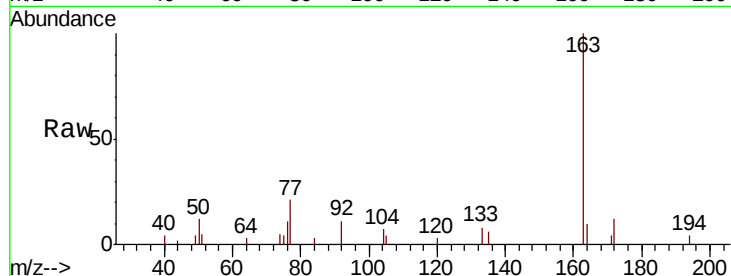


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

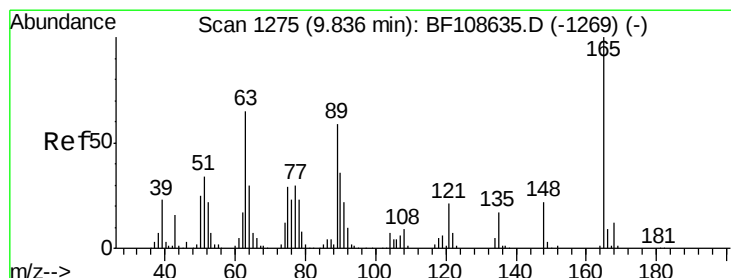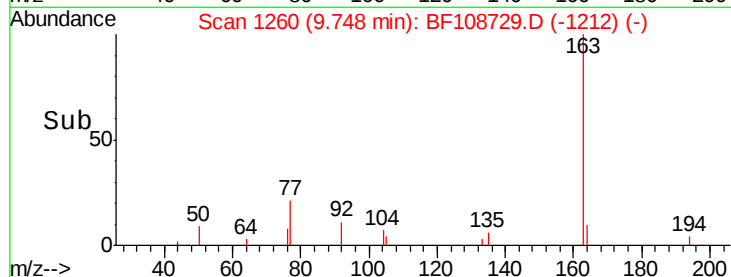
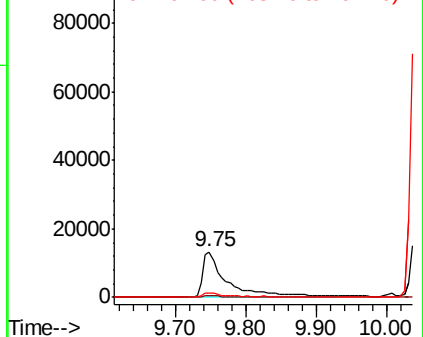



#50
2,6-Dinitrotoluene
Concen: 6.678 ng
RT: 10.04 min Scan# 1309
Delta R.T. 0.20 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06

Tgt Ion:165 Resp: 12890
Ion Ratio Lower Upper
165 100
63 0.0 44.7 67.1#
89 0.0 44.0 66.0#

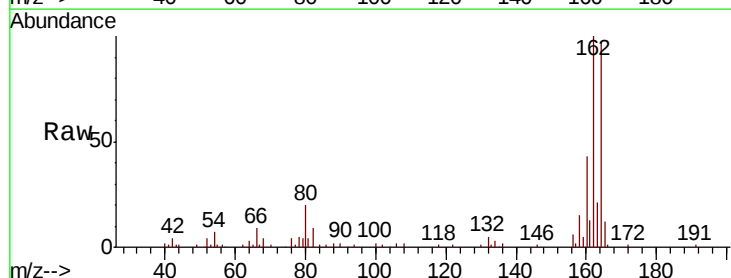

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

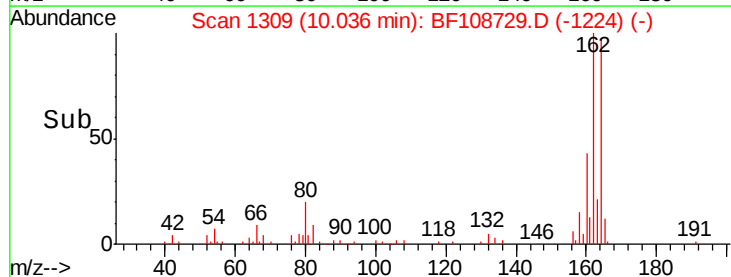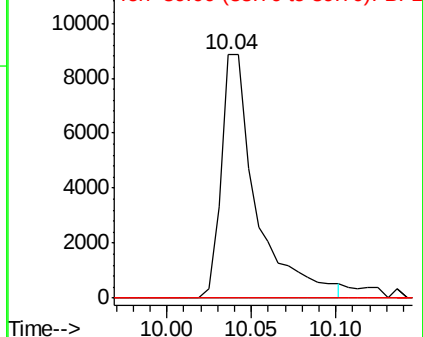


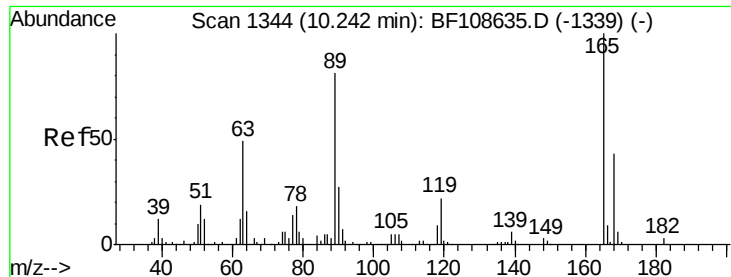

#56
2,4-Dinitrotoluene
Concen: 5.296 ng
RT: 10.04 min Scan# 1309
Delta R.T. -0.21 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06

Instrument :
BNA_F
ClientSampled :

Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#



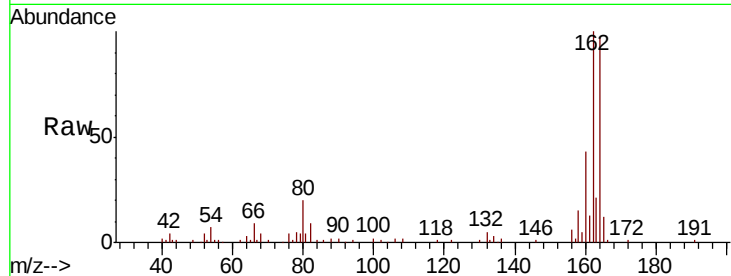


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

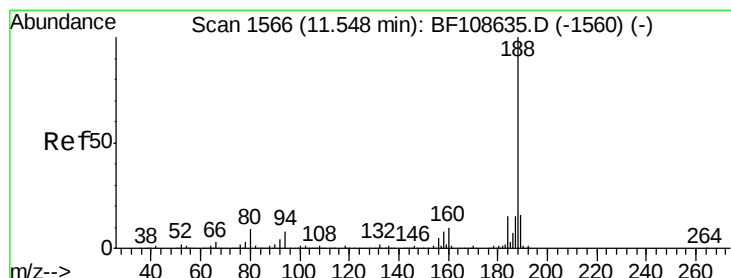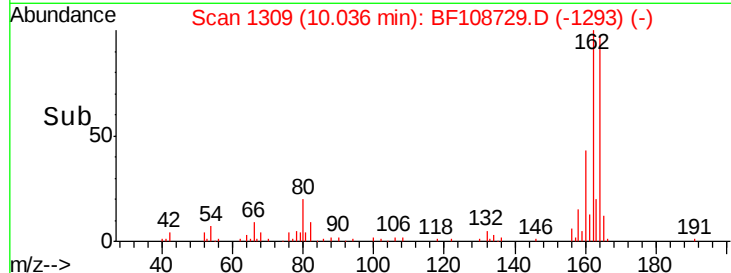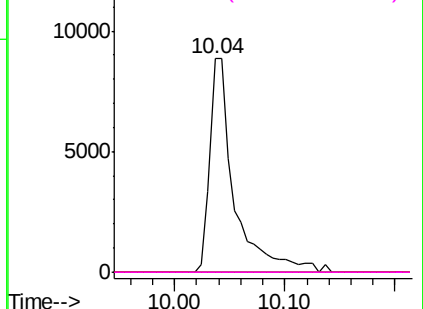

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1565
Delta R.T. -0.01 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06



Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.7	8.5	12.7#
80	9.1	9.2	13.8#

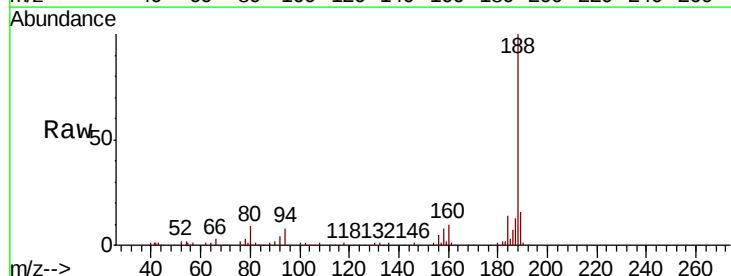


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

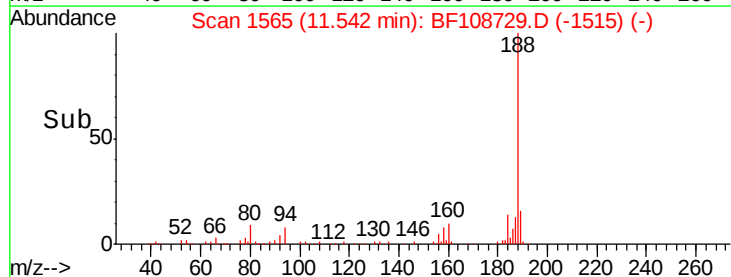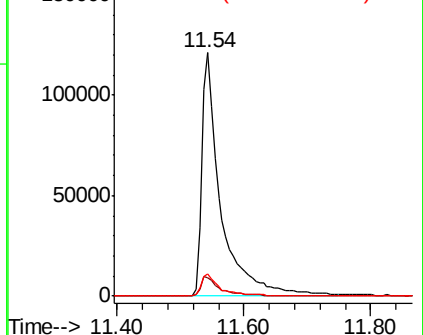


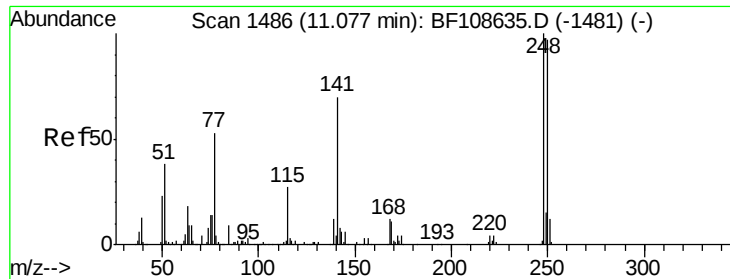




#66
4-Bromophenyl-phenylether
Concen: 2.481 ng
RT: 10.84 min Scan# 1445
Delta R.T. -0.24 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06

Instrument :
BNA_F
ClientSampled :

Tot Ion:248 Resp: 7677
Ion Ratio Lower Upper
248 100
250 198.8 76.9 115.3#
141 464.1 74.4 111.6#

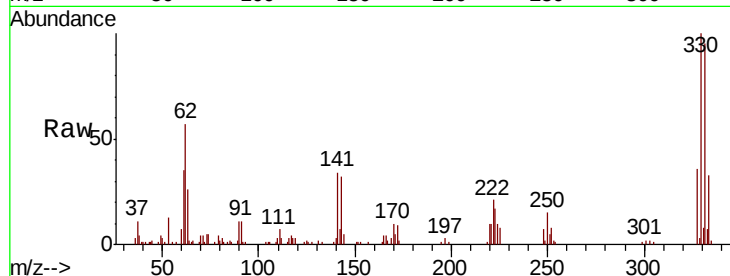


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E


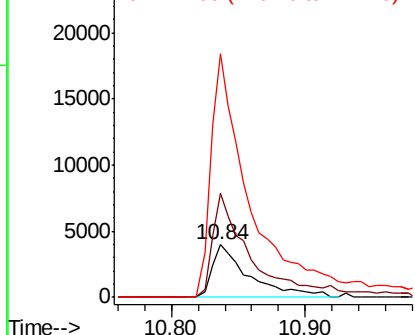



#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.19 min Scan# 2016
Delta R.T. -0.01 min
Lab File: BF108729.D
Acq: 1 Sep 2018 10:06

Tgt Ion:240 Resp: 242394
Ion Ratio Lower Upper
240 100
120 9.5 9.5 14.3#
236 25.2 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

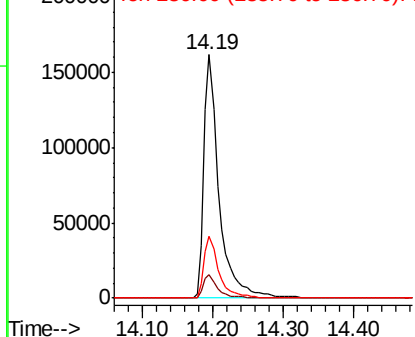



#78

Terphenyl-d14

Concen: 86.741 ng

RT: 13.12 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BF108729.D

Acq: 1 Sep 2018 10:06

Instrument :

BNA_F

ClientSampleId :





Tot Ion:244 Resp: 1082142

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0

122 10.5 11.0 16.4#

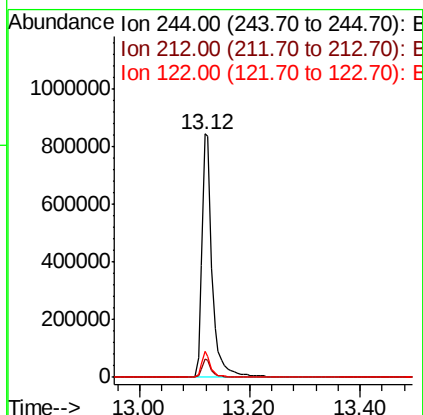

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.75 min Scan# 2281

Delta R.T. 0.00 min

Lab File: BF108729.D

Acq: 1 Sep 2018 10:06

Tgt Ion:264 Resp: 161477

Ion Ratio Lower Upper

264 100

260 24.4 19.2 28.8

265 21.1 17.5 26.3

