

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
 Data File : BF108732.D
 Acq On : 1 Sep 2018 11:28
 Operator : JU/SJ
 Sample : J4729-18
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 04 02:04:03 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 30 15:06:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.01	152	69071	20.00	ng	0.00
21) Naphthalene-d8	8.28	136	270367	20.00	ng	0.00
38) Acenaphthene-d10	10.04	164	124247	20.00	ng	-0.01
63) Phenanthrene-d10	11.54	188	265966	20.00	ng	0.00
75) Chrysene-d12	14.19	240	257120	20.00	ng	0.00
86) Perylene-d12	15.75	264	172516	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.68	112	29650	7.46	ng	0.04
7) Phenol-d6	6.66	99	113578	19.94	ng	0.01
23) Nitrobenzene-d5	7.57	82	525515	98.66	ng	0.00
41) 2,4,6-Tribromophenol	10.84	330	134555	82.04	ng	-0.01
44) 2-Fluorobiphenyl	9.35	172	998809	108.09	ng	0.00
78) Terphenyl-d14	13.12	244	1015652	76.75	ng	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.77	77	7100	2.017	ng	# 79
15) Benzyl Alcohol	7.15	79	9124	2.227	ng	# 47
19) n-Nitroso-di-n-propylamine	7.57	70	59002	15.472	ng	# 86
25) Isophorone	7.57	82	538961	60.911	ng	# 64
49) Dimethylphthalate	9.74	163	94134	9.621	ng	# 98
50) 2,6-Dinitrotoluene	10.04	165	14698	6.815	ng	# 24
56) 2,4-Dinitrotoluene	10.04	165	15129	5.298	ng	# 21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
Data File : BF108732.D
Acq On : 1 Sep 2018 11:28
Operator : JU/SJ
Sample : J4729-18
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 04 02:04:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

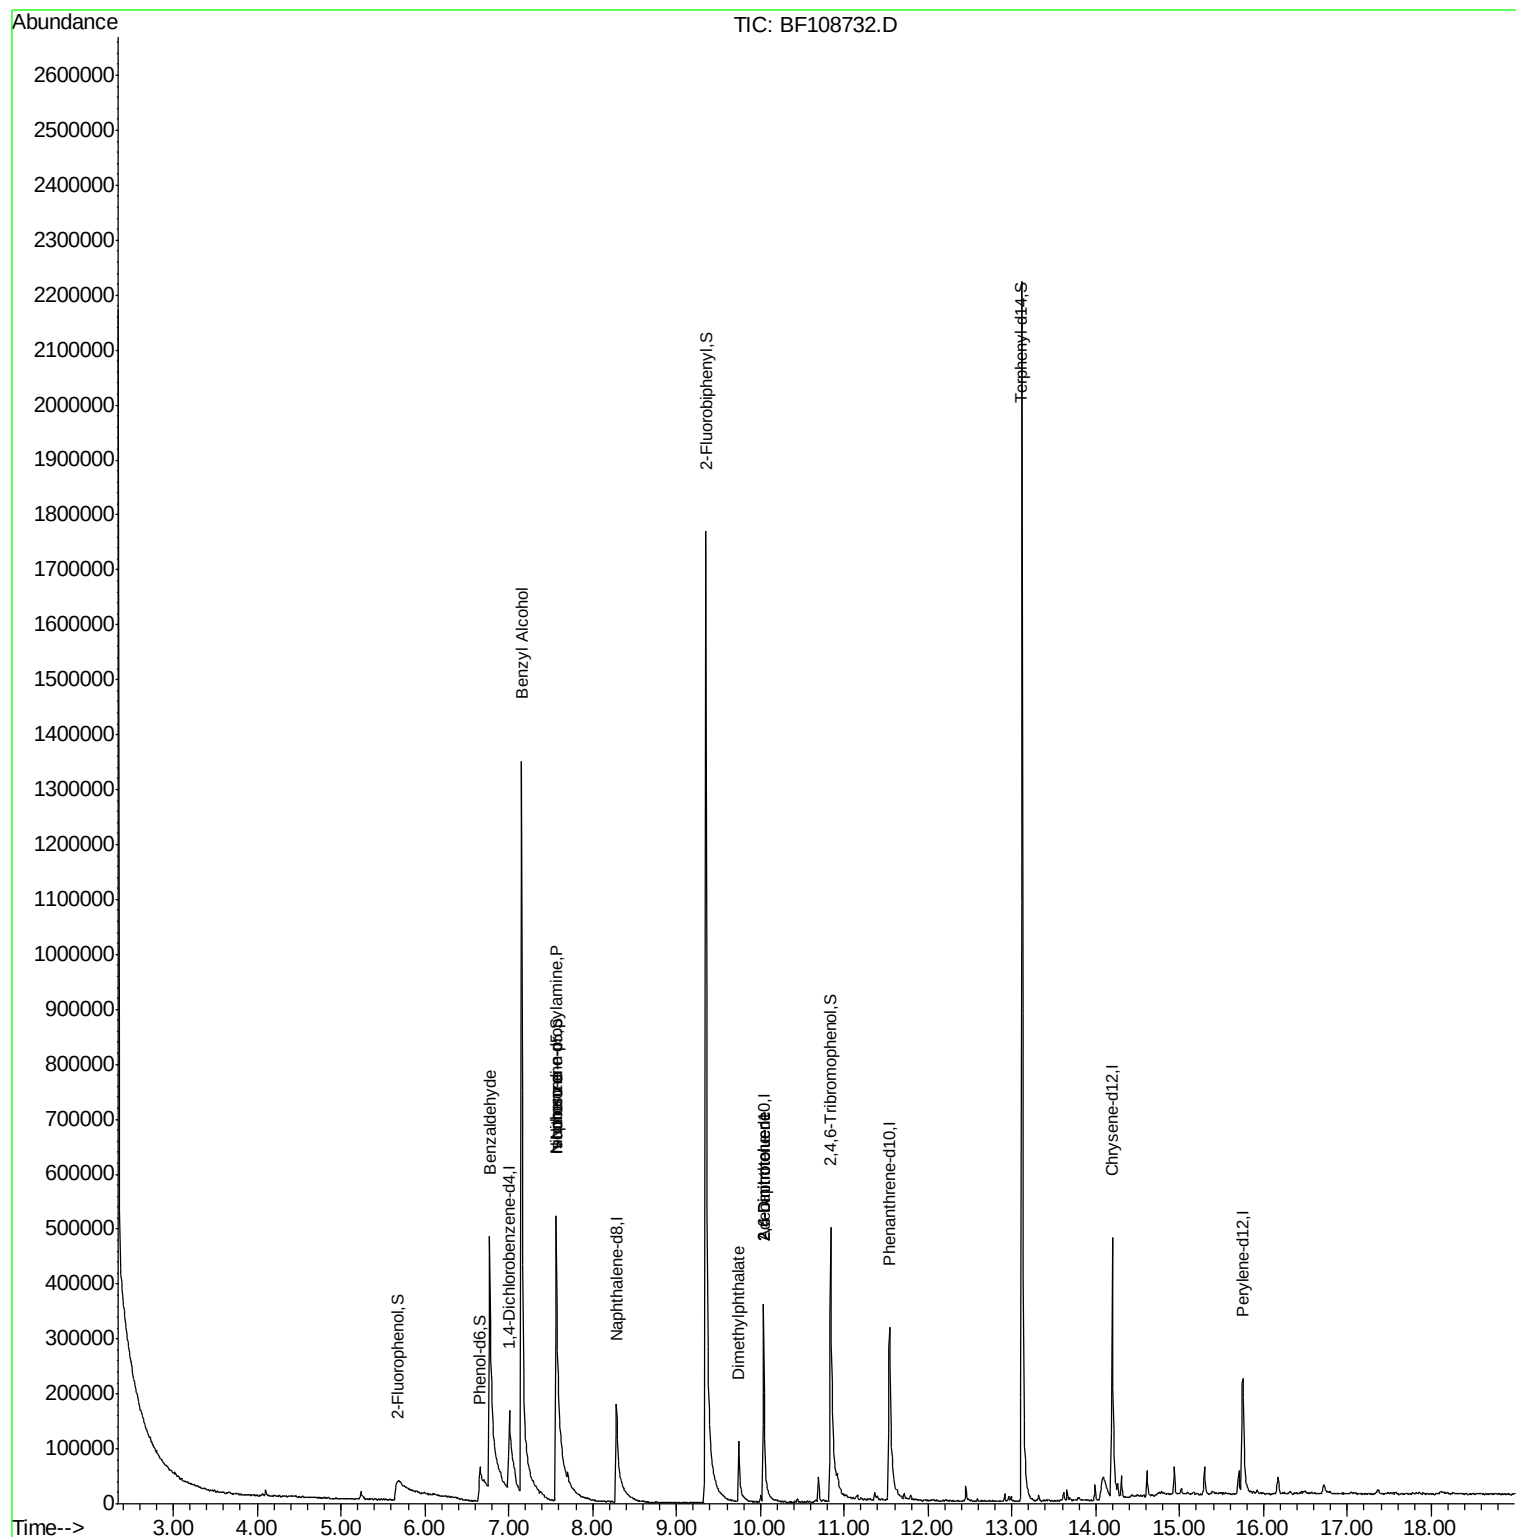

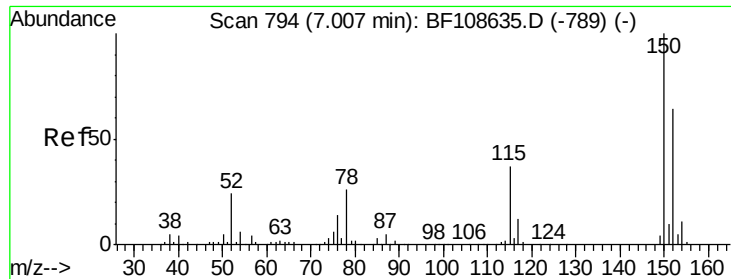


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.01 min Scan# 794
Delta R.T. 0.00 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 69071
Ion Ratio Lower Upper
152 100
150 158.0 124.6 186.8
115 61.7 50.1 75.1

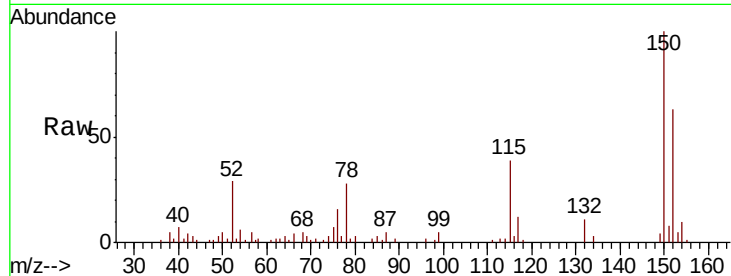


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

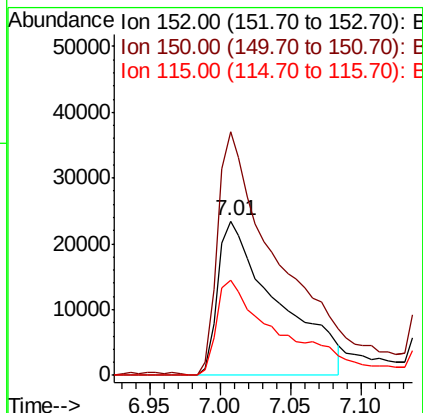



#5


2-Fluorophenol
Concen: 7.457 ng
RT: 5.68 min Scan# 569
Delta R.T. 0.04 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Tgt Ion:112 Resp: 29650
Ion Ratio Lower Upper
112 100
64 62.6 47.9 71.9
63 31.5 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

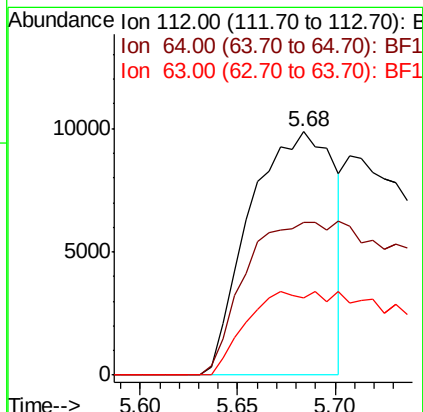

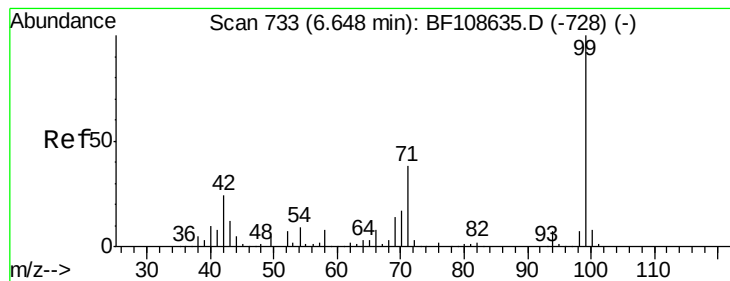

#7

Phenol-d6

Concen: 19.945 ng

RT: 6.66 min Scan# 735

Delta R.T. 0.01 min

Lab File: BF108732.D

Acq: 1 Sep 2018 11:28

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 113578

Ion Ratio Lower Upper




99 100

42 23.0 14.5 21.7#

71 35.7 25.4 38.0

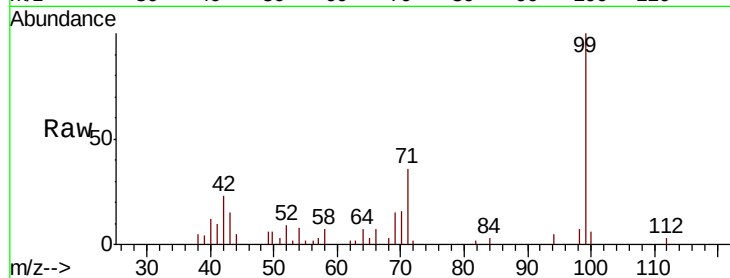

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

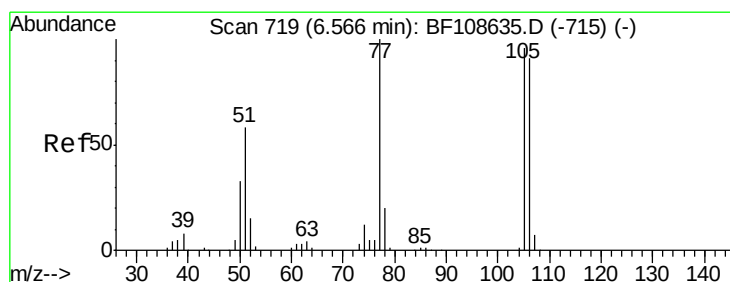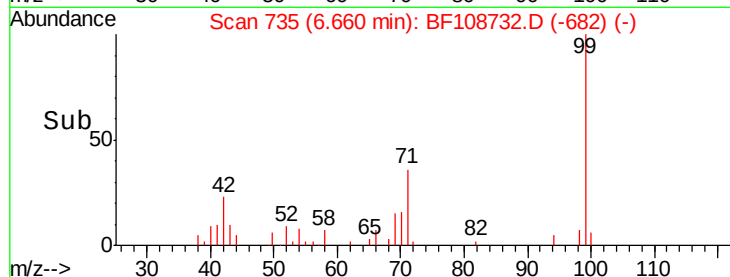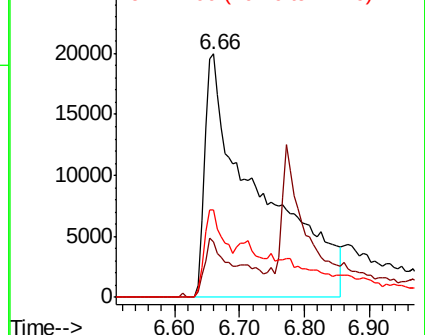

#9

Benzaldehyde

Concen: 2.017 ng

RT: 6.77 min Scan# 754

Delta R.T. 0.21 min

Lab File: BF108732.D

Acq: 1 Sep 2018 11:28


Tgt Ion: 77 Resp: 7100

Ion Ratio Lower Upper



77 100


105 83.4 81.1 121.1

106 70.1 74.5 114.5#

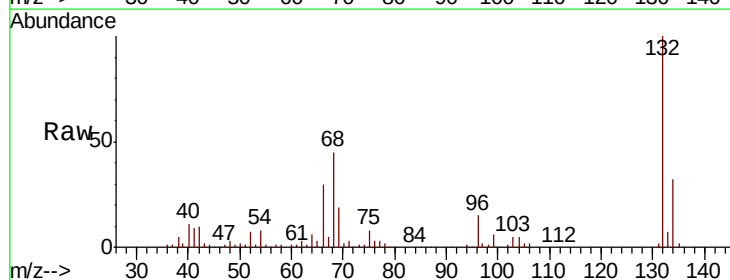

Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 105.00 (104.70 to 105.70): E
Ion 106.00 (105.70 to 106.70): E

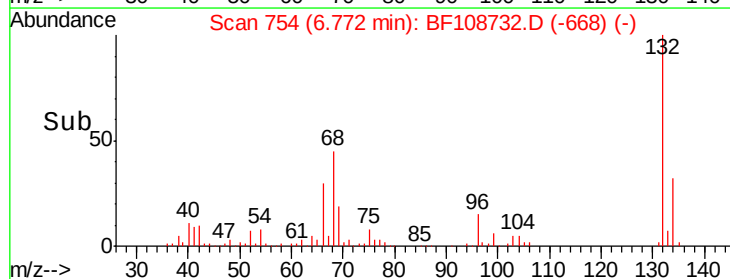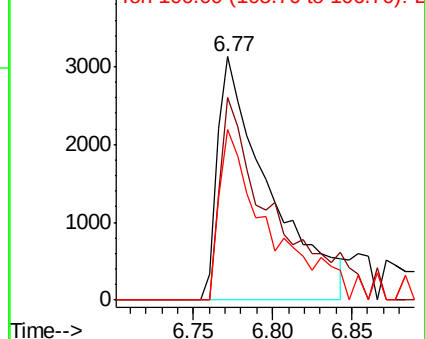


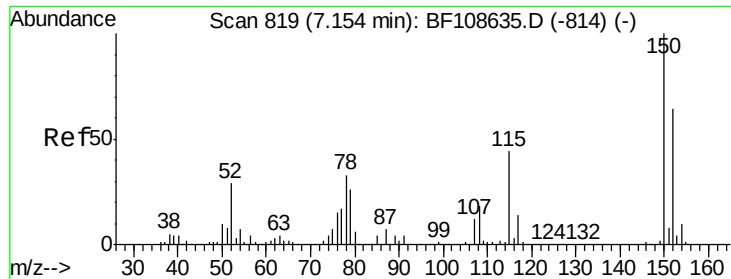




#15
Benzyl Alcohol
Concen: 2.227 ng
RT: 7.15 min Scan# 819
Delta R.T. 0.00 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 79 Resp: 9124
Ion Ratio Lower Upper
79 100
108 28.7 65.1 97.7#
77 98.4 50.6 75.8#

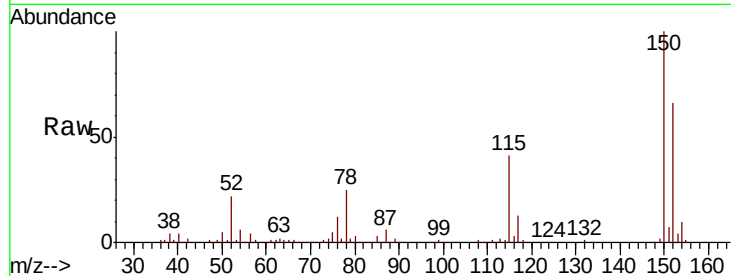


Abundance Ion 79.00 (78.70 to 79.70): BF1
Ion 108.00 (107.70 to 108.70): BF1
Ion 77.00 (76.70 to 77.70): BF1


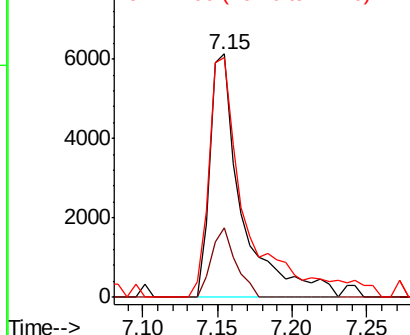



#19
n-Nitroso-di-n-propylamine
Concen: 15.472 ng
RT: 7.57 min Scan# 889
Delta R.T. 0.15 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Tgt Ion: 70 Resp: 59002
Ion Ratio Lower Upper
70 100
42 56.9 47.5 71.3
101 0.0 7.4 11.2#
130 2.2 16.6 25.0#



Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1




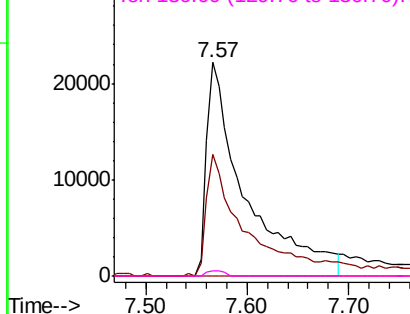


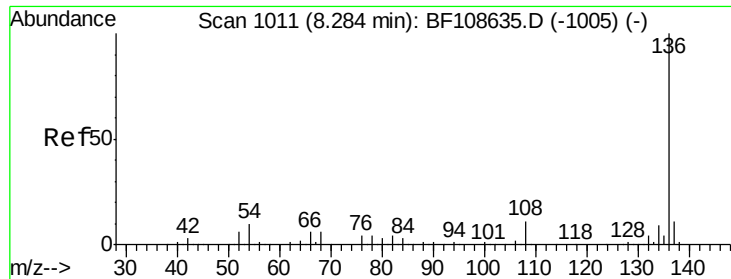

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.28 min Scan# 1011
Delta R.T. 0.00 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28




Instrument :
BNA_F
ClientSampleId :


Tot Ion:	136	Resp:	270367
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.9	13.3
54	9.7	6.6	9.8
68	5.4	5.0	7.4

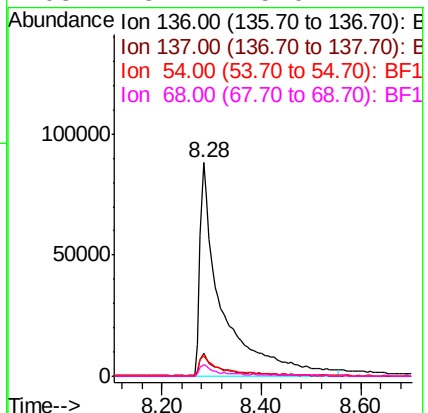

#23
Nitrobenzene-d5
Concen: 98.660 ng
RT: 7.57 min Scan# 889
Delta R.T. -0.01 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Tgt Ion:	82	Resp:	525515
Ion	Ratio	Lower	Upper
82	100		
128	41.6	36.1	54.1
54	57.5	41.4	62.2

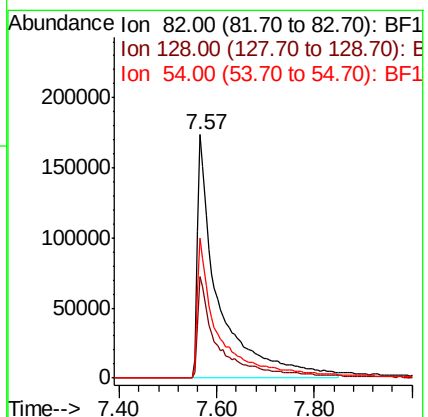

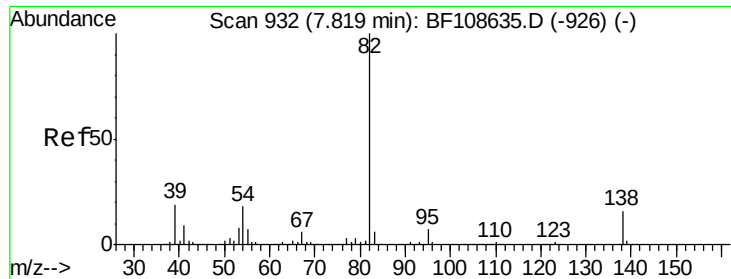

#25

Isophorone

Concen: 60.911 ng

RT: 7.57 min Scan# 889

Delta R.T. -0.25 min

Lab File: BF108732.D

Acq: 1 Sep 2018 11:28

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 538961

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

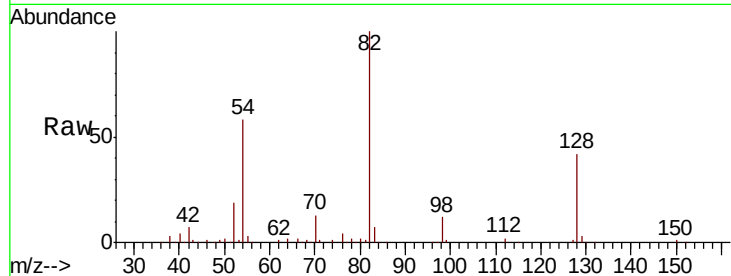

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

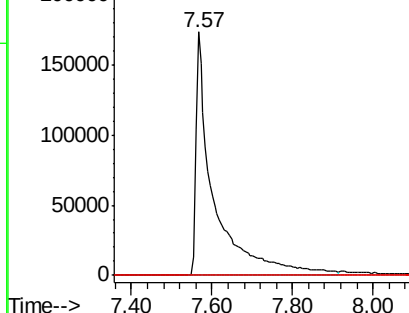

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.04 min Scan# 1309

Delta R.T. -0.01 min

Lab File: BF108732.D

Acq: 1 Sep 2018 11:28


Tgt Ion:164 Resp: 124247

Ion Ratio Lower Upper



164 100


162 104.3 86.1 129.1

160 47.0 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

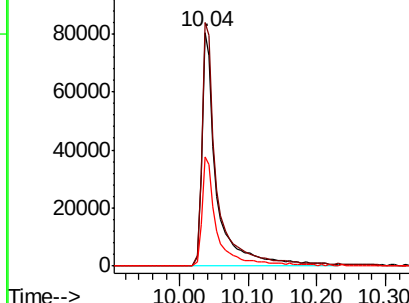


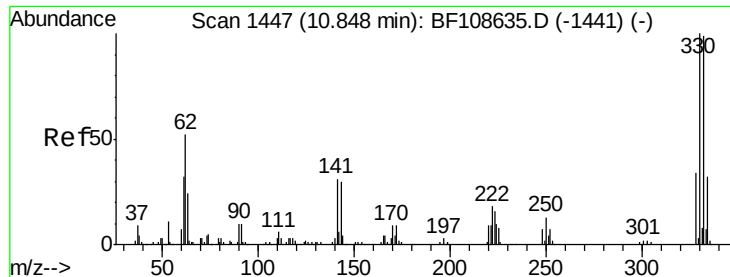

#41
 2,4,6-Tribromophenol
 Concen: 82.035 ng
 RT: 10.84 min Scan# 1445
 Delta R.T. -0.01 min
 Lab File: BF108732.D
 Acq: 1 Sep 2018 11:28

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.0	115.6
141	33.6	29.9	44.9



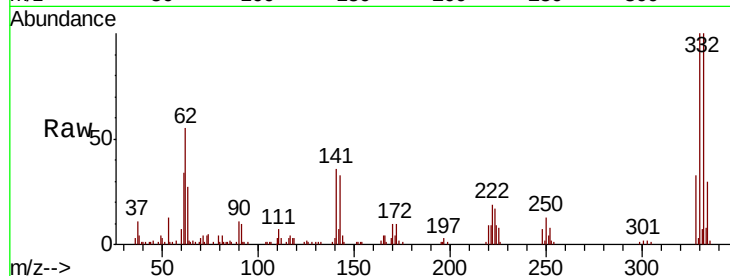


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

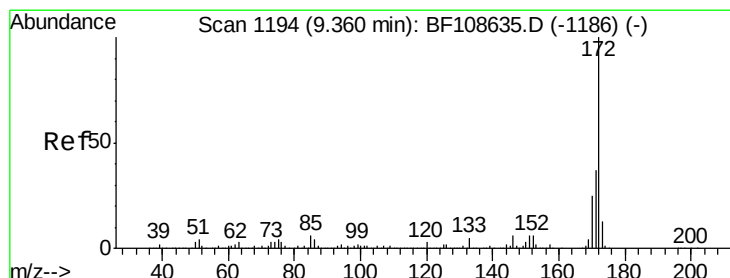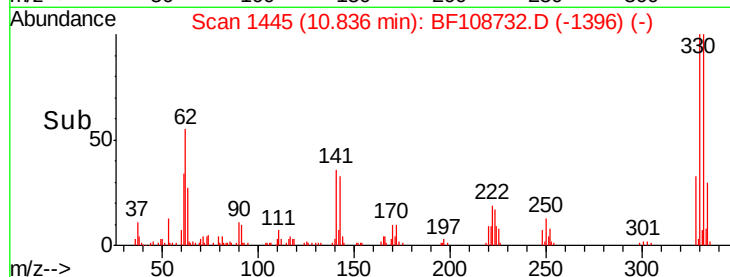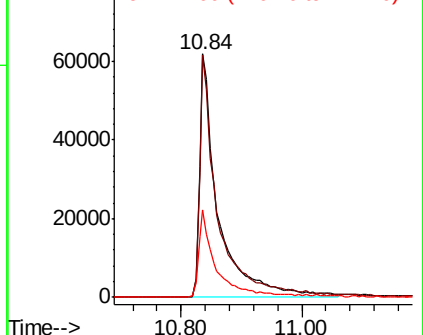

#44
 2-Fluorobiphenyl
 Concen: 108.089 ng
 RT: 9.35 min Scan# 1193
 Delta R.T. -0.01 min
 Lab File: BF108732.D
 Acq: 1 Sep 2018 11:28

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	29.7	44.5
170	23.4	19.6	29.4


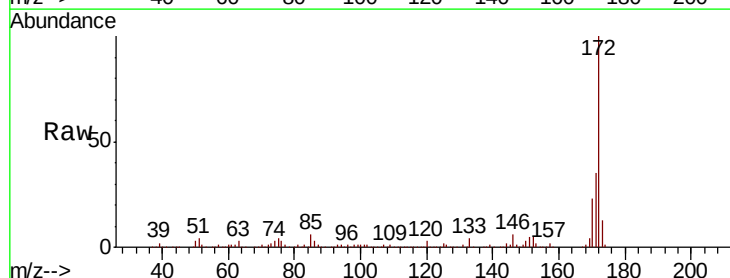



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

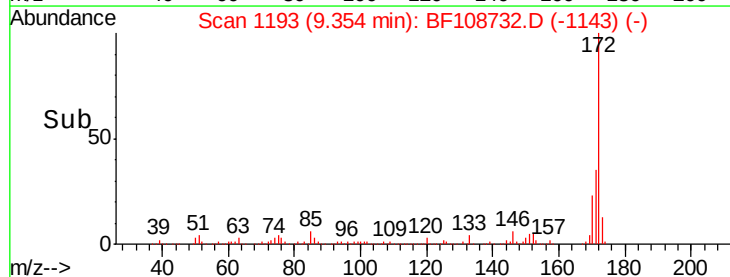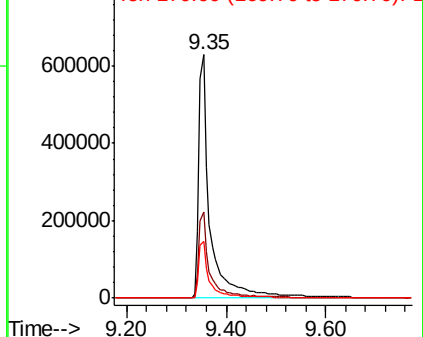


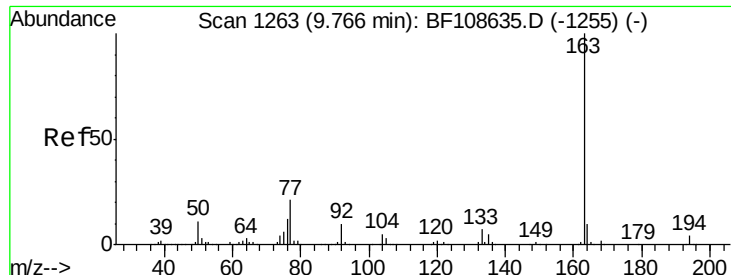



#49
Dimethylphthalate
Concen: 9.621 ng
RT: 9.74 min Scan# 1259
Delta R.T. -0.02 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Instrument :
BNA_F
ClientSampleId :

Tot Ion:163 Resp: 94134
Ion Ratio Lower Upper
163 100
194 4.3 2.7 4.1#
164 10.7 8.2 12.2

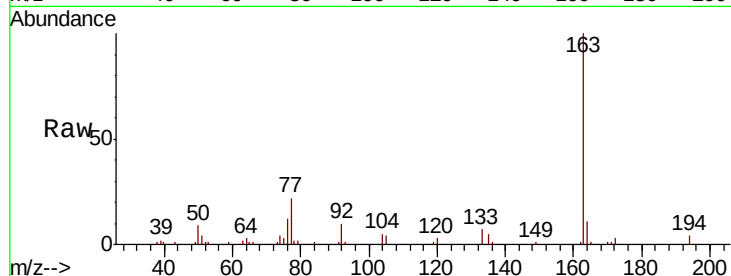


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

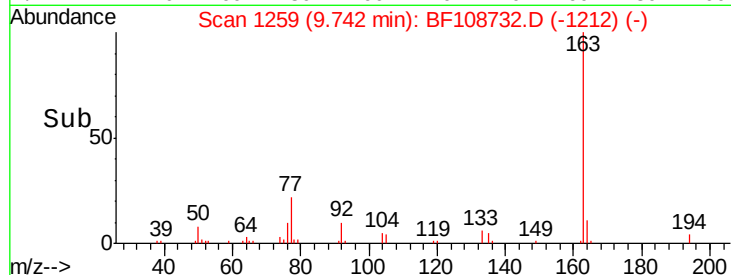
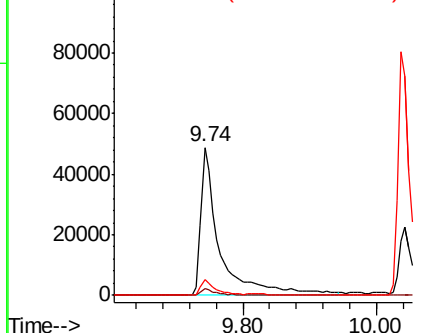



#50
2,6-Dinitrotoluene
Concen: 6.815 ng
RT: 10.04 min Scan# 1309
Delta R.T. 0.20 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Tgt Ion:165 Resp: 14698
Ion Ratio Lower Upper
165 100
63 0.0 44.7 67.1#
89 0.0 44.0 66.0#

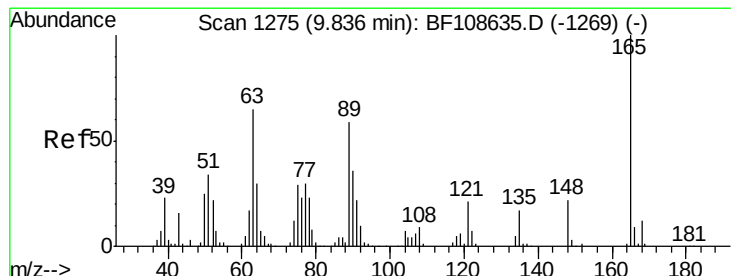

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

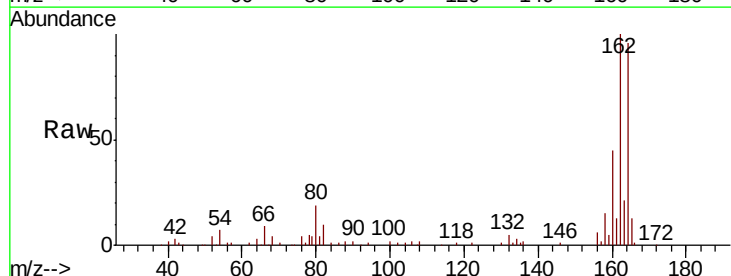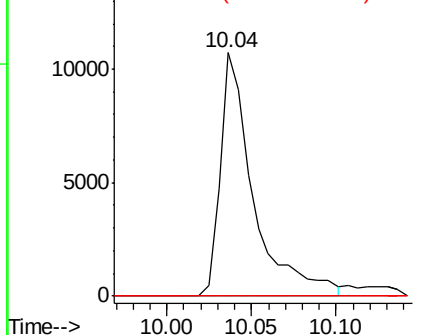


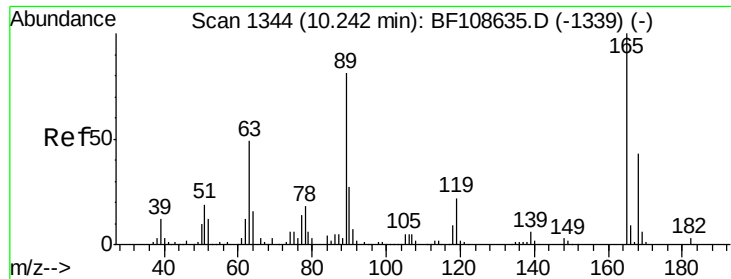

#56
2,4-Dinitrotoluene
Concen: 5.298 ng
RT: 10.04 min Scan# 1309
Delta R.T. -0.21 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#






Abundance

Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1


Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

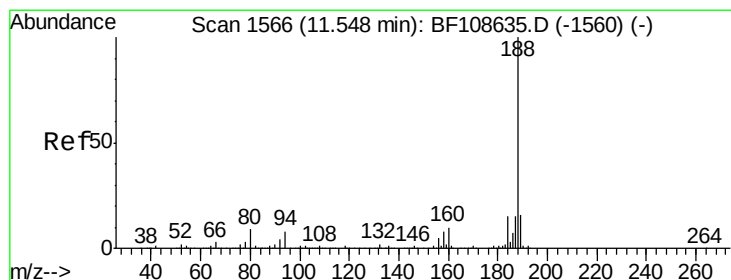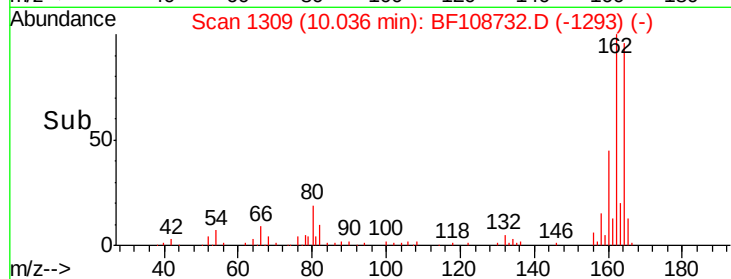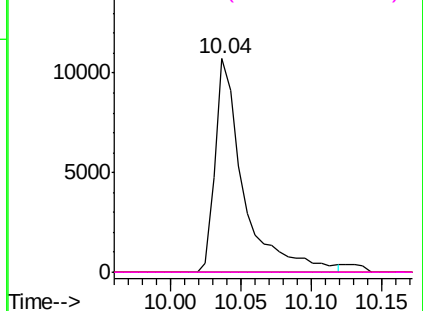

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.54 min Scan# 1565
Delta R.T. -0.01 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.0	8.5	12.7#
80	8.7	9.2	13.8#


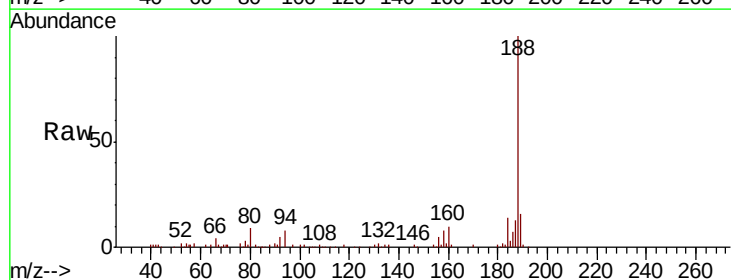



Abundance

Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

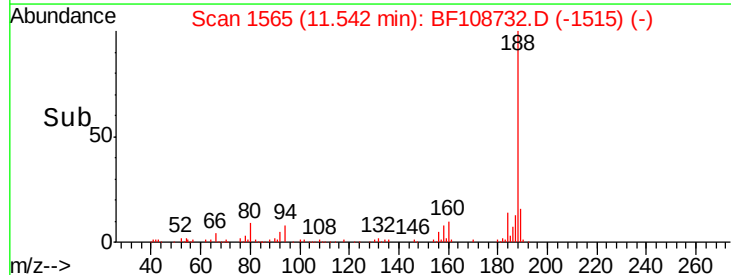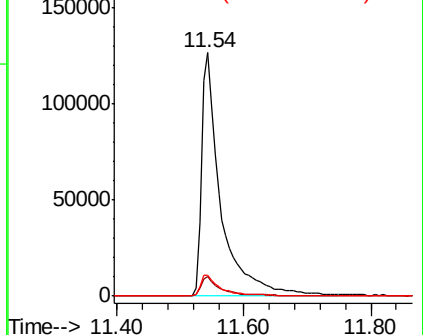



#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.19 min Scan# 2016

Delta R.T. -0.01 min

Lab File: BF108732.D

Acq: 1 Sep 2018 11:28

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 257120

Ion Ratio Lower Upper

240 100

120 9.2 9.5 14.3#




236 26.1 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

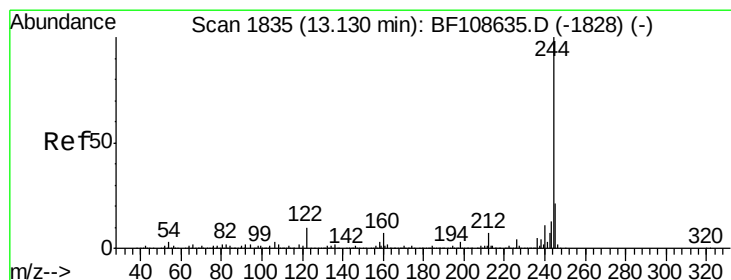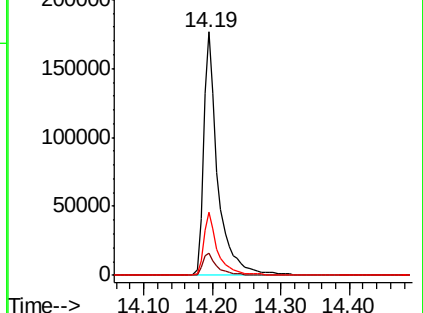

#78

Terphenyl-d14

Concen: 76.749 ng

RT: 13.12 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BF108732.D

Acq: 1 Sep 2018 11:28


Tgt Ion:244 Resp: 1015652

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0



122 9.8 11.0 16.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

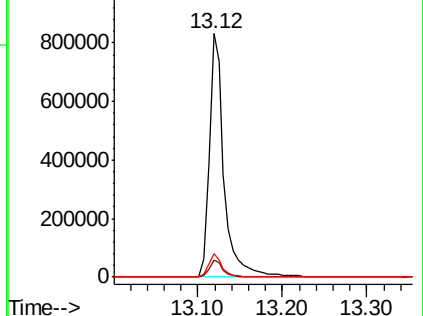


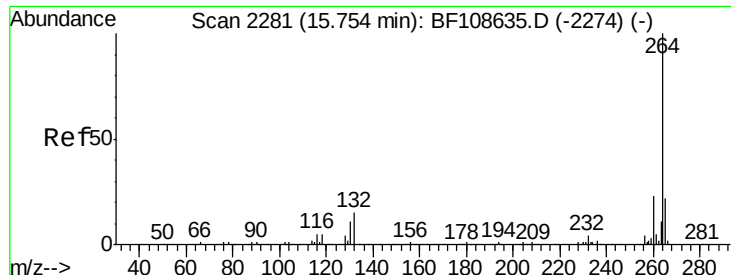

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.75 min Scan# 2281
Delta R.T. 0.00 min
Lab File: BF108732.D
Acq: 1 Sep 2018 11:28

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.2	28.8
265	20.4	17.5	26.3

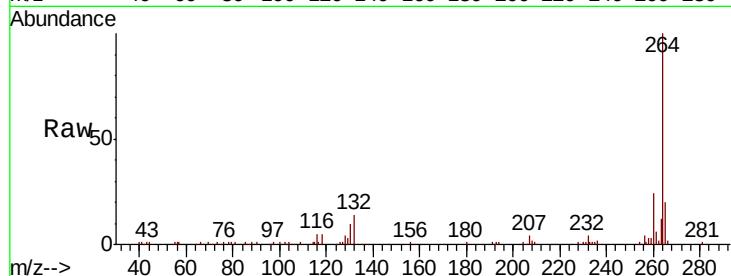

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

