
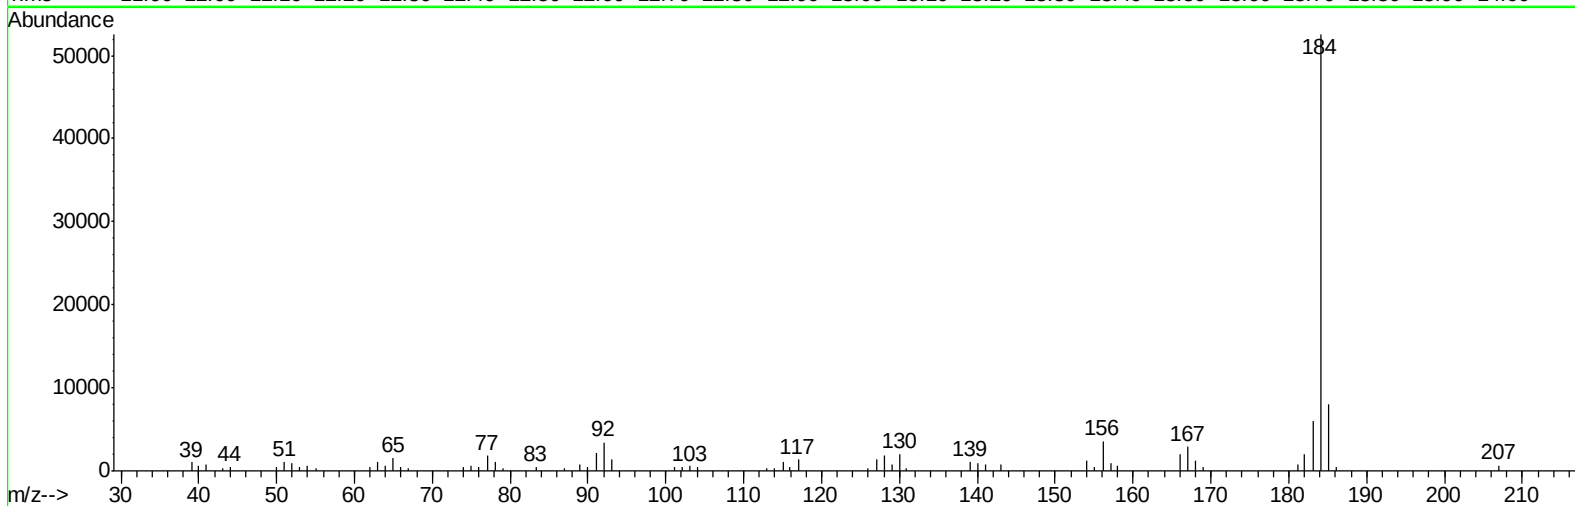


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF083118\
Data File : BF108712.D
Acq On : 1 Sep 2018 2:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 04 04:31:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 30 15:06:55 2018
Response via : Initial Calibration

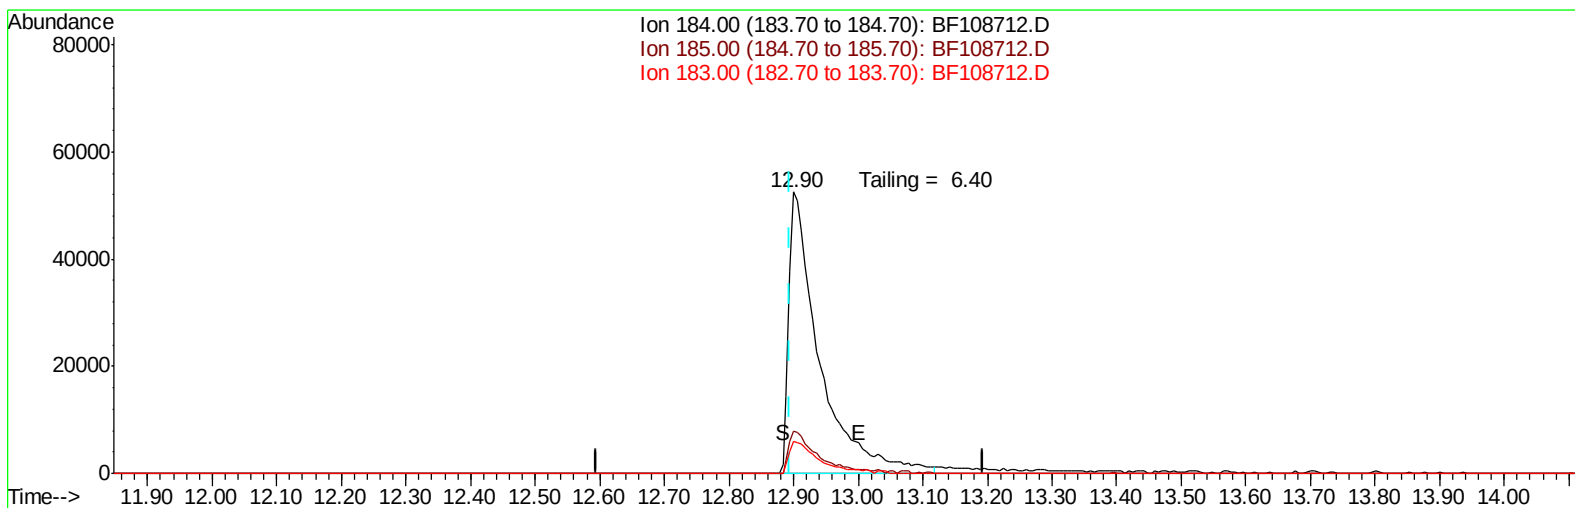

TIC: BF108712.D

(76) Benzidine

12.901min (+0.006) 0.00ng

response 171858

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.12
183.00	11.60	11.37
0.00	0.00	0.00