

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083118\
 Data File : BF108710.D
 Acq On : 1 Sep 2018 00:45
 Operator : JU/SJ
 Sample : J4729-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082918-JETT-E-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.231	490	492	502	rBV	28146	39342	1.34%	0.258%
2	5.660	559	565	583	rBV2	62189	337029	11.45%	2.207%
3	6.654	728	734	738	rBV	84648	168257	5.72%	1.102%
4	6.772	751	754	787	rVB	635511	1269202	43.12%	8.312%
5	7.001	790	793	815	rVB	187643	464308	15.78%	3.041%
6	7.154	815	819	848	rBV	1610272	2161561	73.44%	14.157%
7	7.566	885	889	916	rBV	744743	1623359	55.16%	10.632%
8	8.284	1007	1011	1026	rBV	256846	484033	16.45%	3.170%
9	9.354	1189	1193	1222	rBV	2302604	2943266	100.00%	19.276%
10	9.742	1256	1259	1271	rBV	99512	133097	4.52%	0.872%
11	10.042	1306	1310	1332	rVB	408295	515682	17.52%	3.377%
12	10.695	1417	1421	1430	rVB	82626	72757	2.47%	0.477%
13	10.836	1442	1445	1471	rBV	494583	906984	30.82%	5.940%
14	11.542	1561	1565	1579	rBV	308408	521556	17.72%	3.416%
15	13.124	1829	1834	1847	rBV	2193417	2591472	88.05%	16.972%
16	14.195	2012	2016	2026	rBV	456803	599156	20.36%	3.924%
17	15.707	2269	2273	2276	rBV3	24440	34882	1.19%	0.228%
18	15.754	2276	2281	2295	rVB	202671	370636	12.59%	2.427%
19	16.177	2349	2353	2359	rVB4	22005	32097	1.09%	0.210%


Sum of corrected areas: 15268676

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
Data File : BF108710.D
Acq On : 1 Sep 2018 00:45
Operator : JU/SJ
Sample : J4729-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082918-JETT-E-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

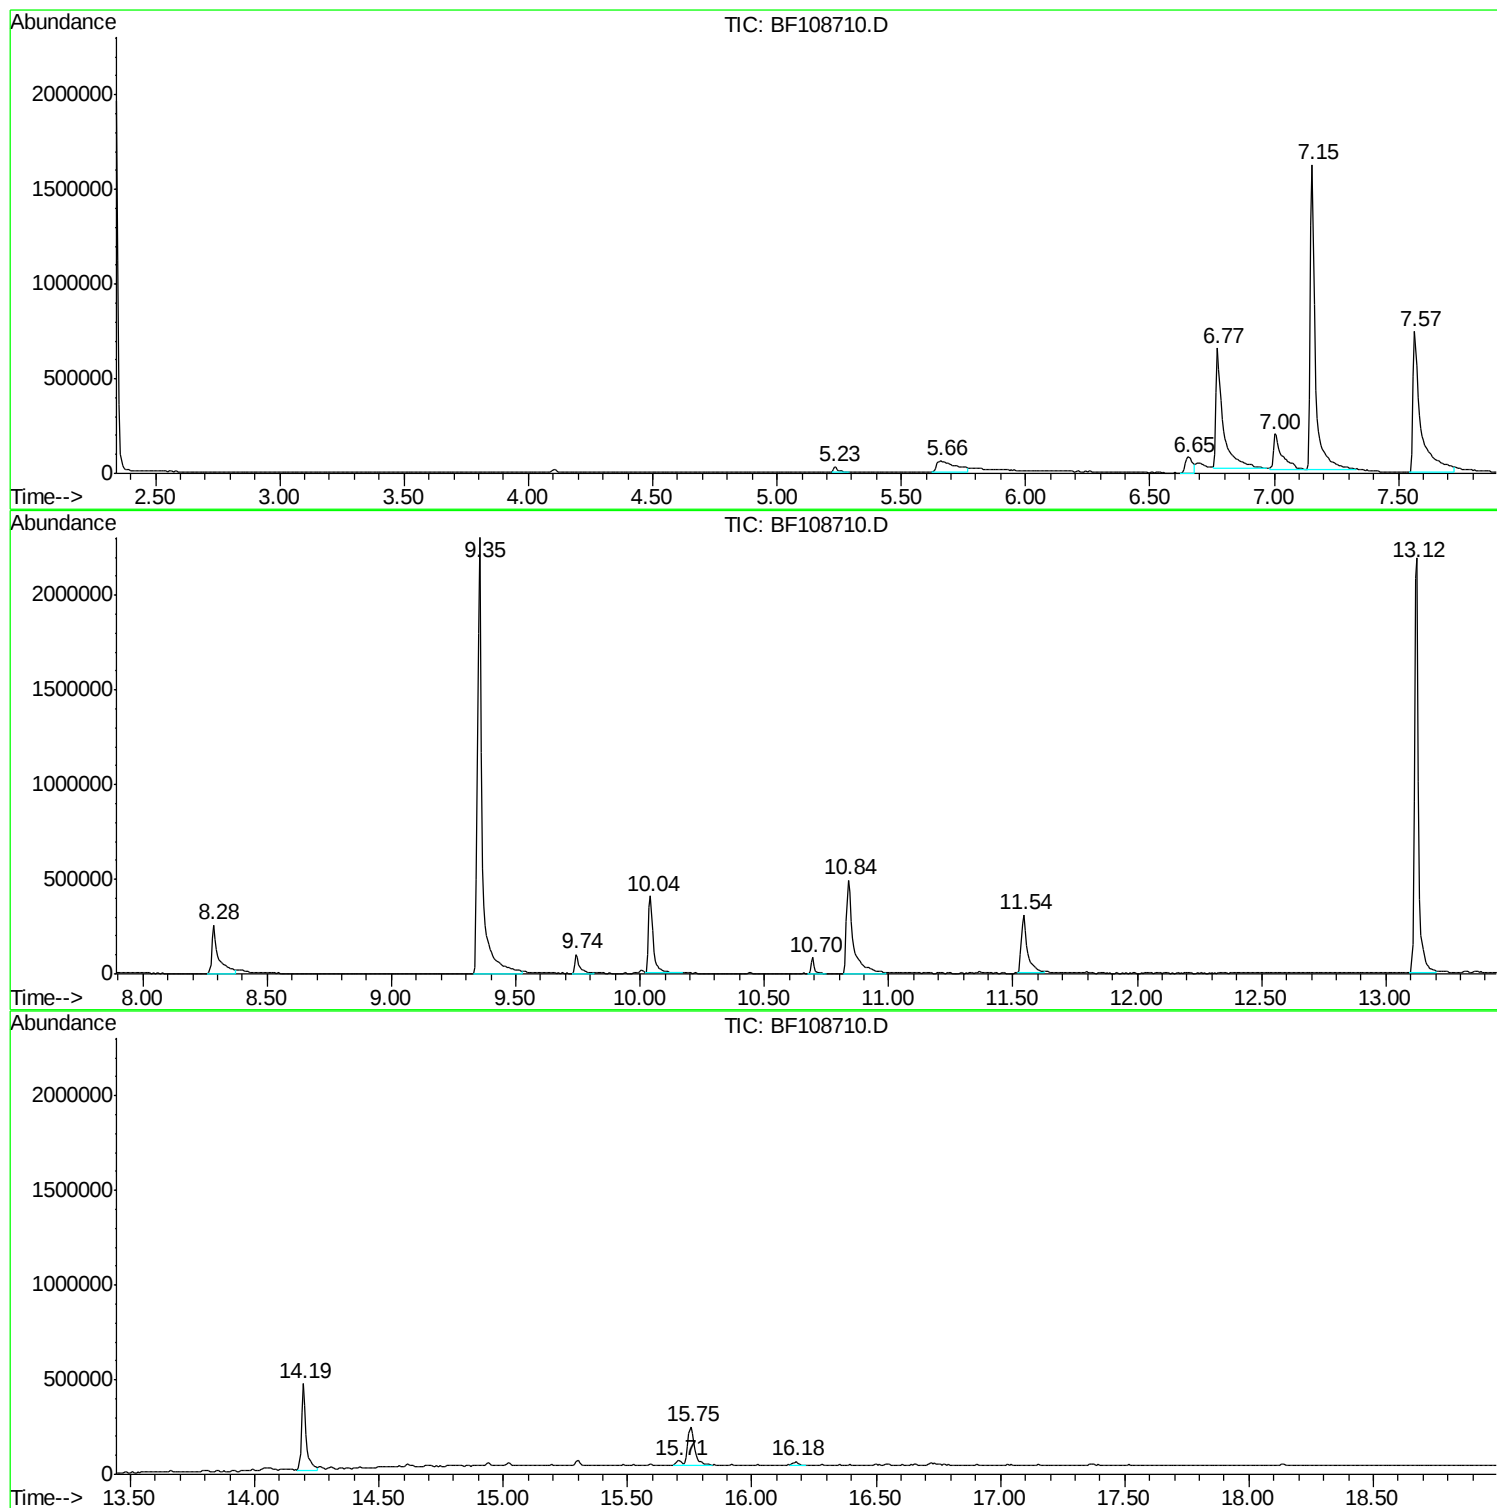

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
Data File : BF108710.D
Acq On : 1 Sep 2018 00:45
Operator : JU/SJ
Sample : J4729-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082918-JETT-E-D-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	54.67 ng	1269200	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

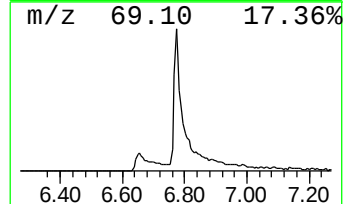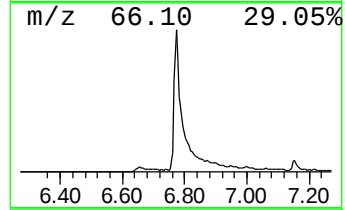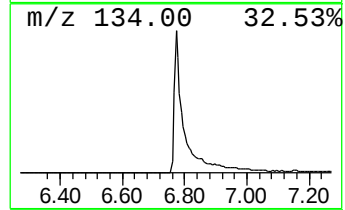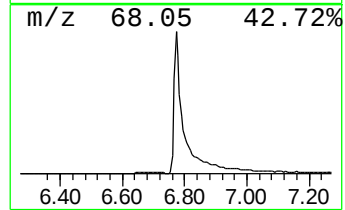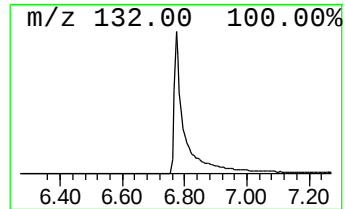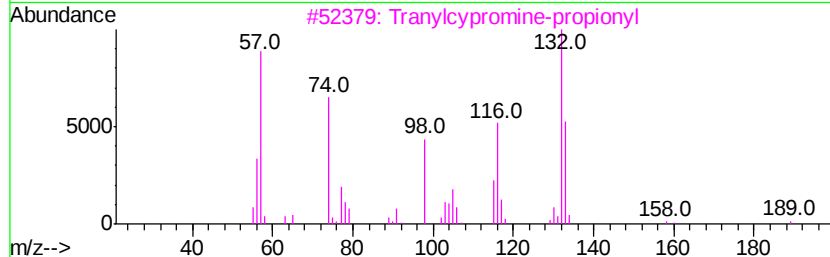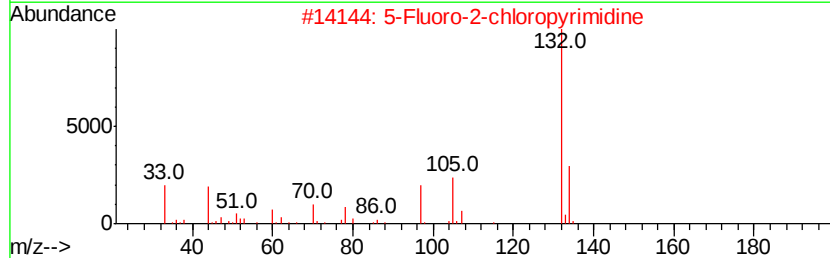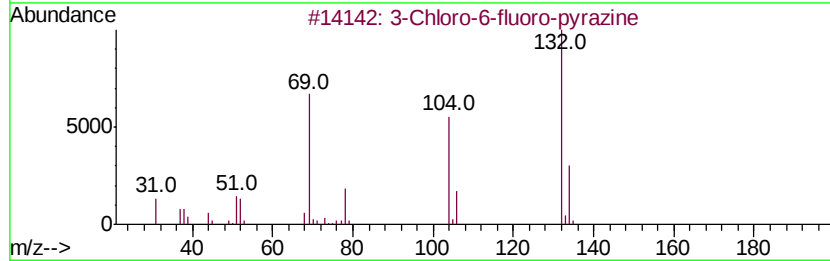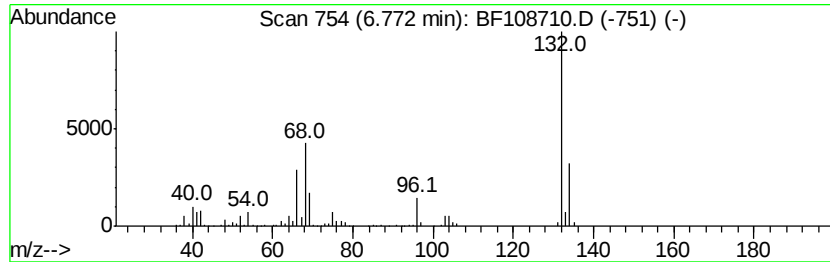

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
Data File : BF108710.D
Acq On : 1 Sep 2018 00:45
Operator : JU/SJ
Sample : J4729-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082918-JETT-E-D-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Triethyl citrate Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.70	2.82 ng	72757	Acenaphthene-d10	10.04

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Triethyl citrate	276	C12H20O7	000077-93-0	86
2		Ethylmalonic acid dipropyl ester	216	C11H20O4	001113-91-3	50
3		1-Amino-2-methylnaphthalene	157	C11H11N	002246-44-8	40
4		3-Chloro2-fluorobenzoic acid, 4-...	370	C21H32ClF02	1000338-64-7	36
5		3-Chloro2-fluorobenzoic acid, 3-...	342	C19H28ClF02	1000338-63-8	36

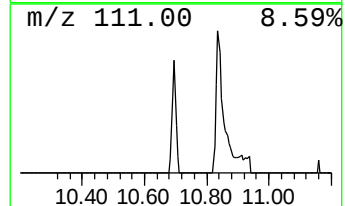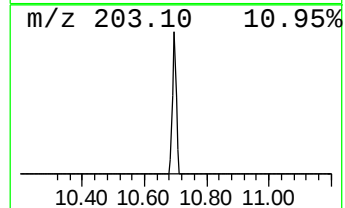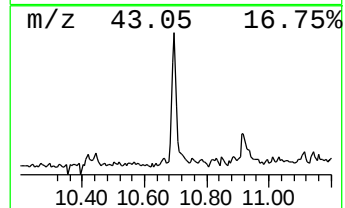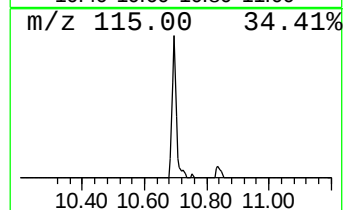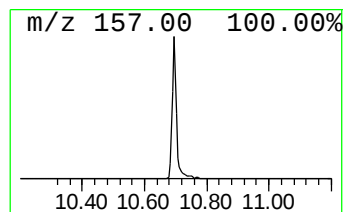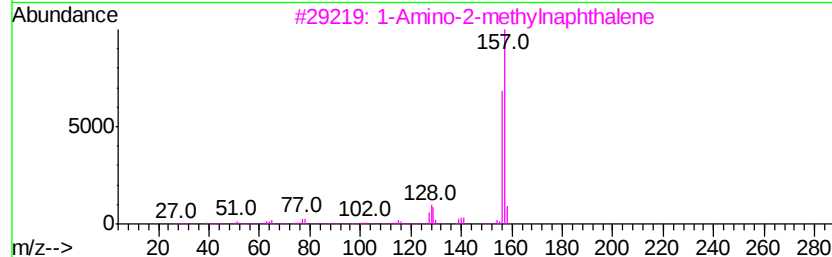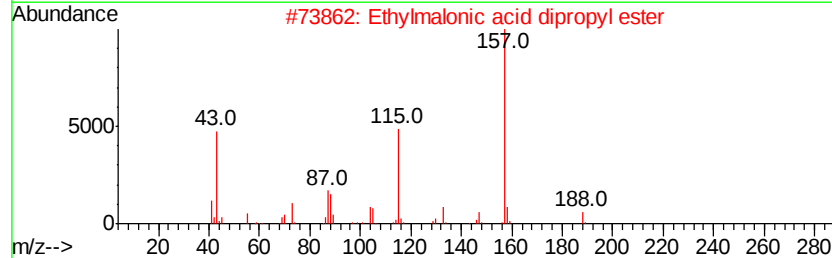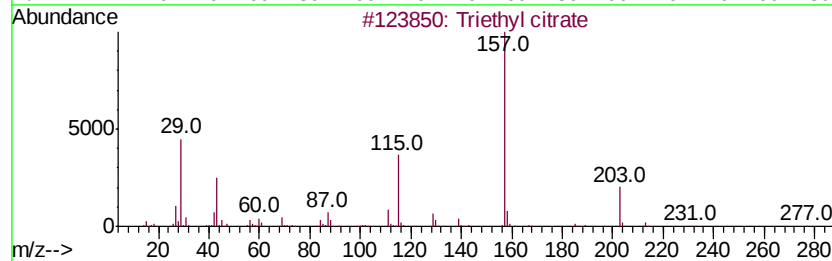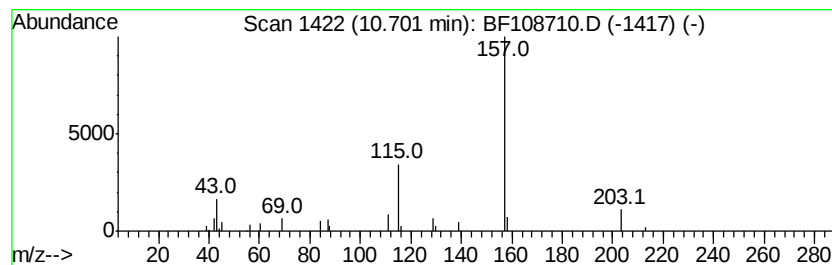

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083118\
Data File : BF108710.D
Acq On : 1 Sep 2018 00:45
Operator : JU/SJ
Sample : J4729-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082918-JETT-E-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	54.7	ng	1269200	1	7.00	464308	20.0
Triethyl citrate	10.70	2.8	ng	72757	3	10.04	515682	20.0