

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083118\
 Data File : BF108726.D
 Acq On : 1 Sep 2018 8:44
 Operator : JU/SJ
 Sample : J4729-12
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 082918-SIDI-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.684	561	569	570	rBV3	31775	70941	2.53%	0.505%
2	6.660	730	735	740	rBV	54916	117556	4.18%	0.837%
3	6.778	751	755	783	rBV	393861	1019323	36.28%	7.260%
4	7.007	790	794	815	rVB	124531	359471	12.80%	2.560%
5	7.154	815	819	861	rVB	1274450	1998668	71.14%	14.236%
6	7.566	886	889	922	rBV	472123	1389883	49.47%	9.900%
7	8.283	1007	1011	1040	rBV	145455	441859	15.73%	3.147%
8	9.354	1189	1193	1223	rBV	1796742	2689140	95.72%	19.154%
9	9.748	1256	1260	1271	rBV	32403	52375	1.86%	0.373%
10	10.042	1306	1310	1329	rBV	307035	469664	16.72%	3.345%
11	10.695	1418	1421	1427	rBV	42841	40919	1.46%	0.291%
12	10.836	1441	1445	1470	rBV	468104	984272	35.03%	7.011%
13	11.542	1561	1565	1586	rBV	285039	557758	19.85%	3.973%
14	13.124	1829	1834	1857	rBV	2238327	2809428	100.00%	20.010%
15	14.195	2012	2016	2026	rBV	387384	585472	20.84%	4.170%
16	15.295	2199	2203	2207	rBV	27489	32148	1.14%	0.229%
17	15.706	2268	2273	2276	rBV	25463	37191	1.32%	0.265%
18	15.754	2276	2281	2290	rVV	179362	350621	12.48%	2.497%
19	16.171	2348	2352	2359	rVB	20543	33200	1.18%	0.236%


Sum of corrected areas: 14039889

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
Data File : BF108726.D
Acq On : 1 Sep 2018 8:44
Operator : JU/SJ
Sample : J4729-12
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082918-SIDI-F-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

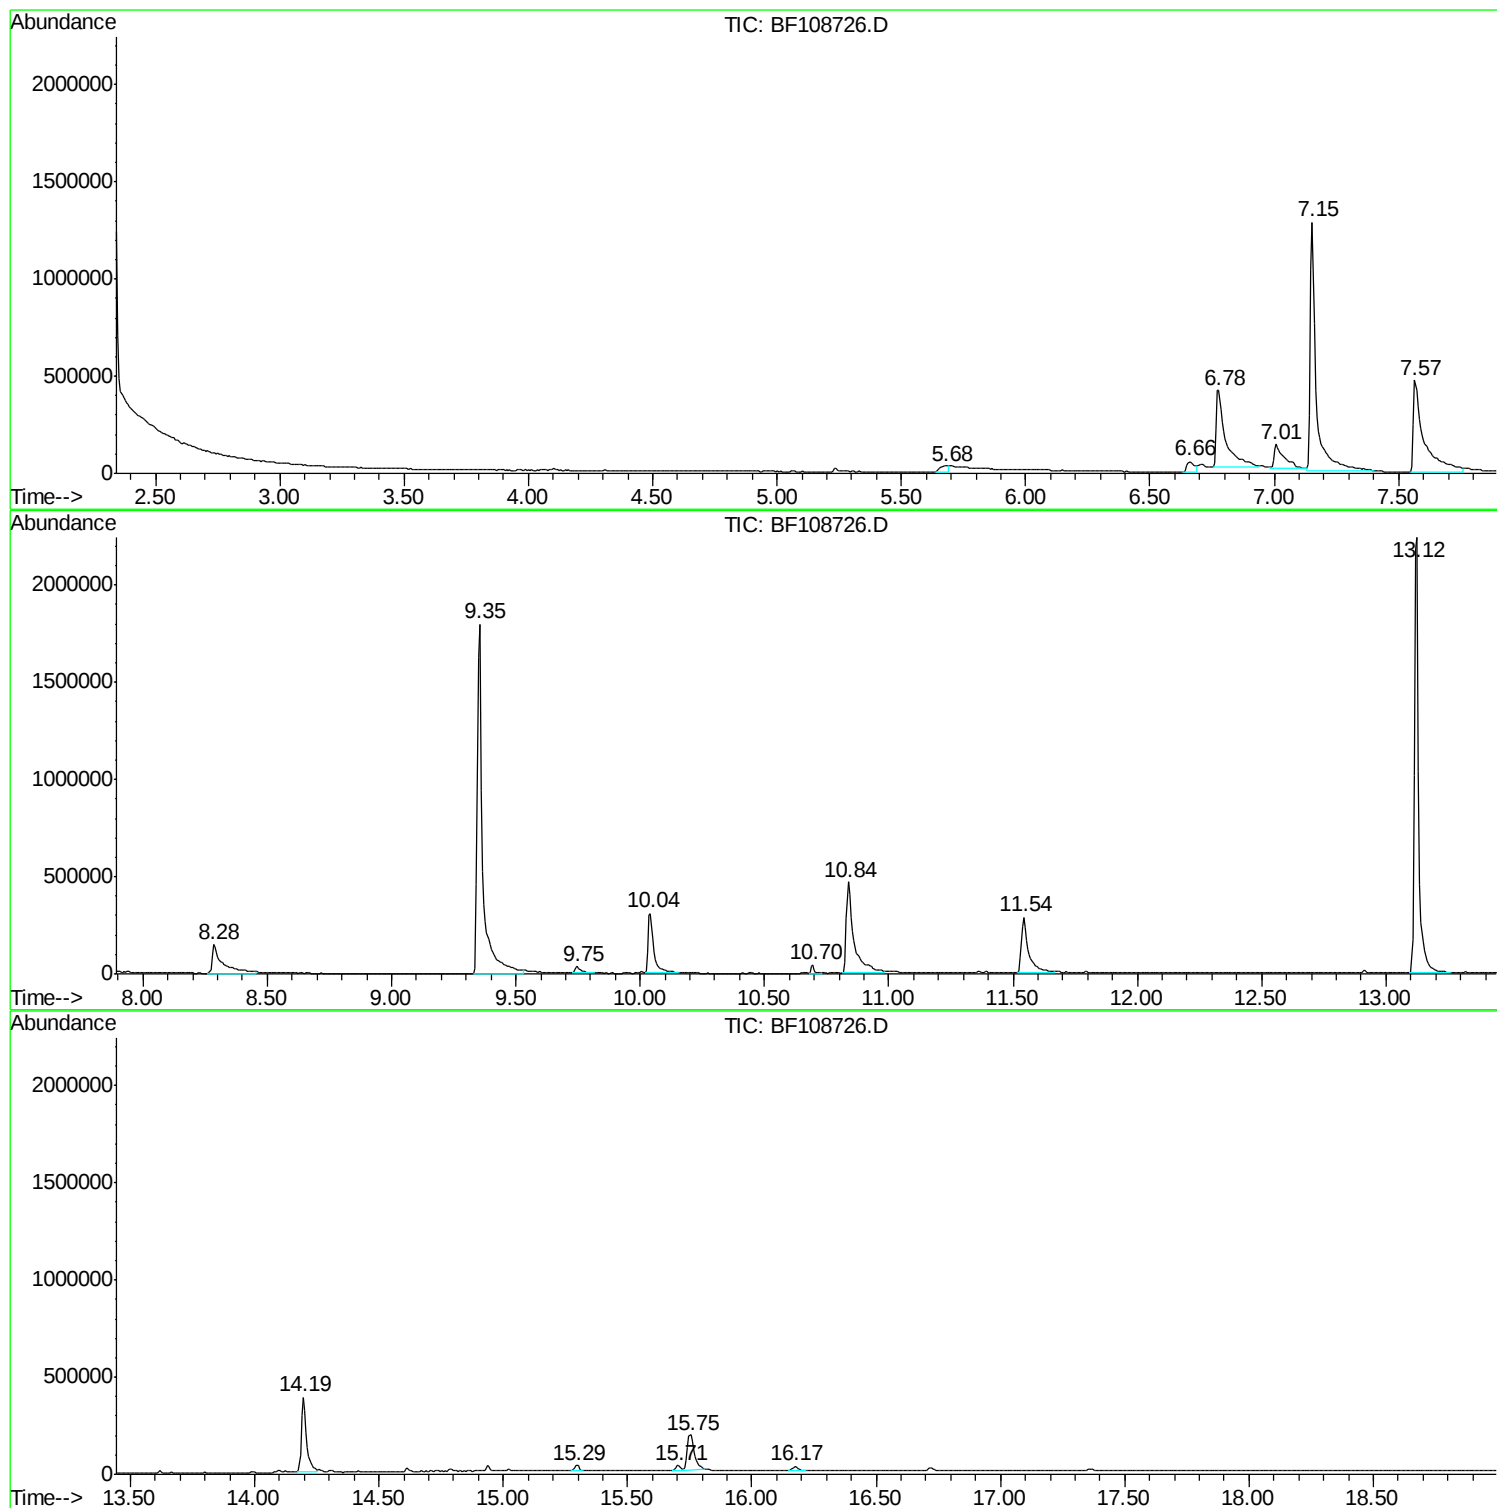

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF083118\
Data File : BF108726.D
Acq On : 1 Sep 2018 8:44
Operator : JU/SJ
Sample : J4729-12
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082918-SIDI-F-D-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.78 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.78	56.71 ng	1019320	1,4-Dichlorobenzene-d4	7.01

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16		
2	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12		
3	5-Aminoindole	132	C8H8N2	005192-03-0	10		
4	Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9		
5	1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9		

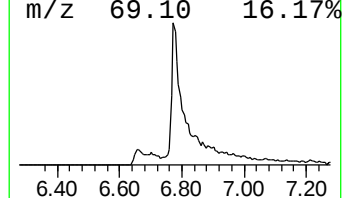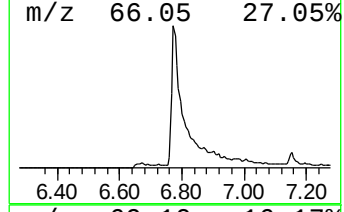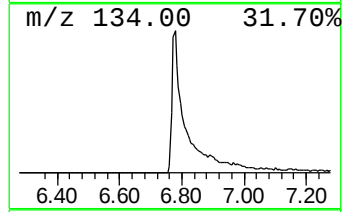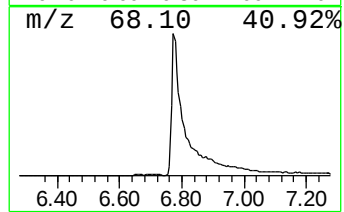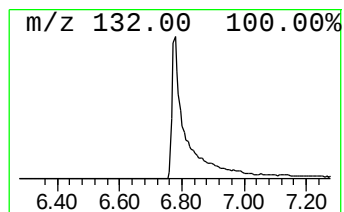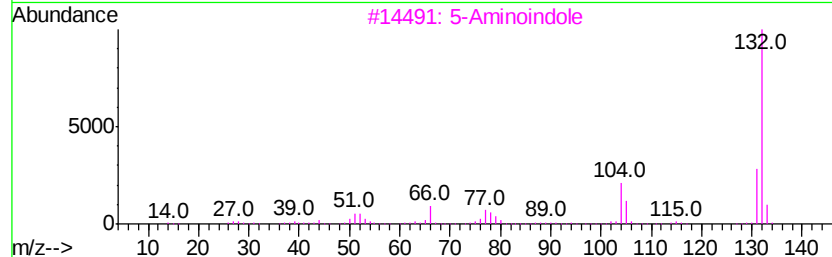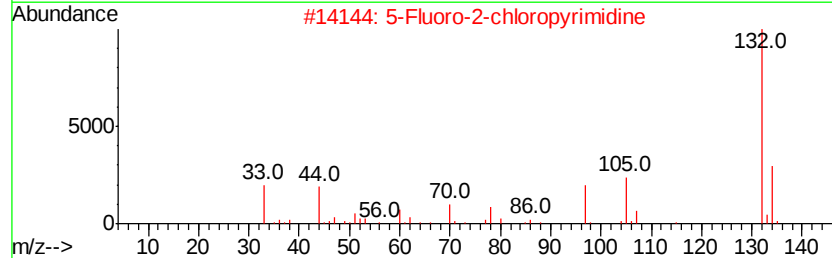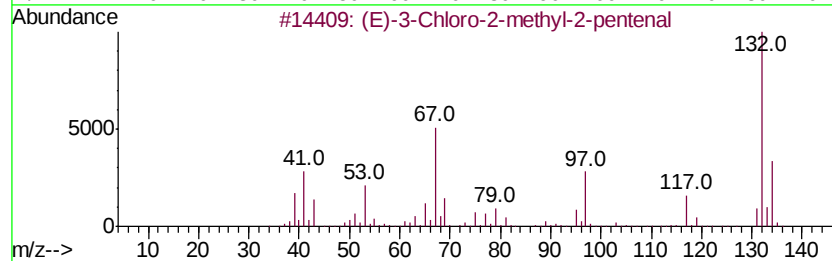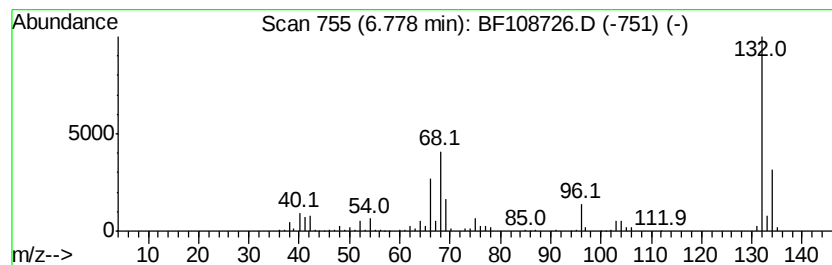

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF083118\
Data File : BF108726.D
Acq On : 1 Sep 2018 8:44
Operator : JU/SJ
Sample : J4729-12
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
082918-SIDI-F-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.78	6.78	56.7	ng	1019320	1	7.01	359471	20.0