


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083118\
 Data File : BF108712.D
 Acq On : 1 Sep 2018 2:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 30 15:06:55 2018

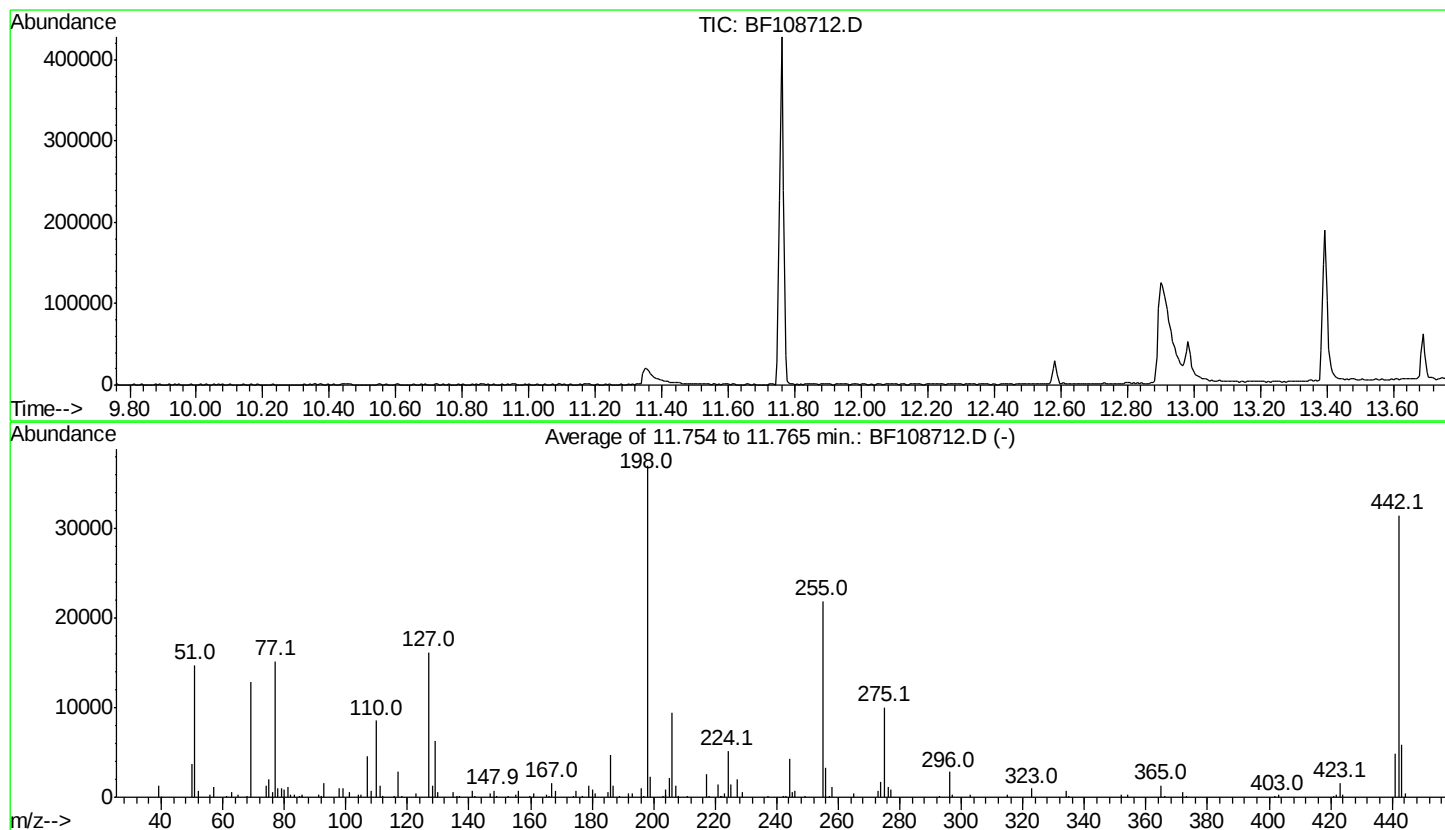

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	14728	PASS
68	69	0.00	2	1.1	138	PASS
69	198	0.00	100	34.8	12857	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.7	16152	PASS
197	198	0.00	2	0.4	133	PASS
198	198	100	100	100.0	36997	PASS
199	198	5	9	6.1	2263	PASS
275	198	10	60	27.1	10026	PASS
365	198	1	100	3.6	1334	PASS
441	198	0.01	100	13.1	4855	PASS
442	198	50	100	85.0	31429	PASS
443	442	15	24	18.6	5848	PASS