
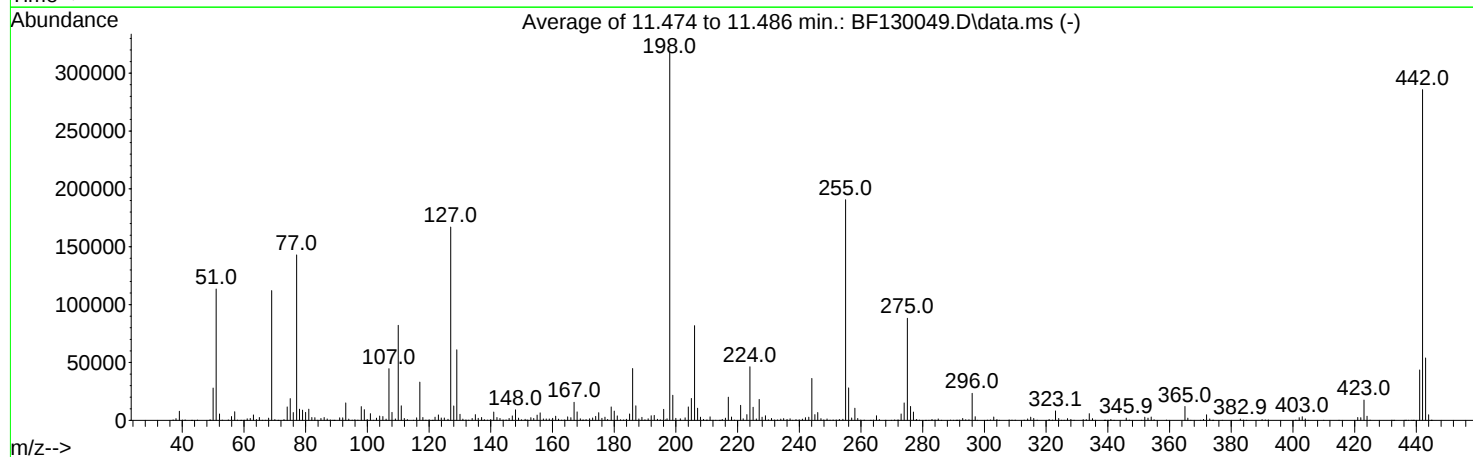


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083122\
 Data File : BF130049.D
 Acq On : 31 Aug 2022 13:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 31 18:15:32 2022

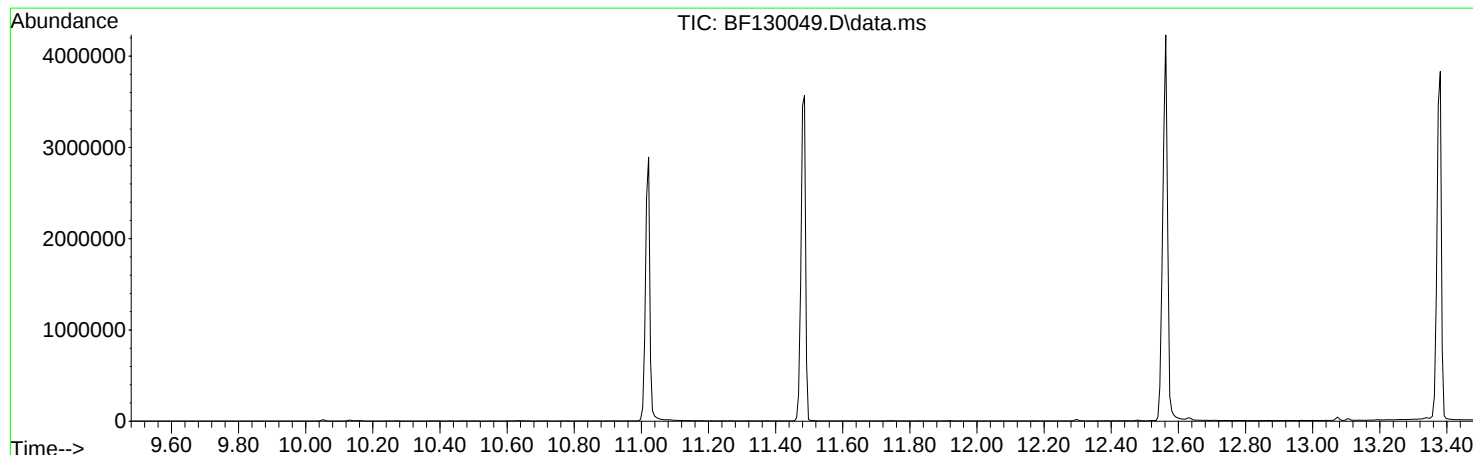




AutoFind: Scans 1562, 1563, 1564; Background Corrected with Scan 1556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	113536	PASS
68	69	0.00	2	1.7	1931	PASS
69	198	0.00	100	35.3	112136	PASS
70	69	0.00	2	0.6	679	PASS
127	198	10	80	52.6	167067	PASS
197	198	0.00	2	0.4	1388	PASS
198	198	100	100	100.0	317845	PASS
199	198	5	9	6.8	21671	PASS
275	198	10	60	27.8	88272	PASS
365	198	1	100	3.8	12028	PASS
441	198	0.01	100	13.7	43495	PASS
442	442	50	100	100.0	285725	PASS
443	442	15	24	18.9	53950	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083122\
Data File : BF130049.D
Acq On : 31 Aug 2022 13:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 31 16:36:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 31 15:58:13 2022
Response via : Initial Calibration

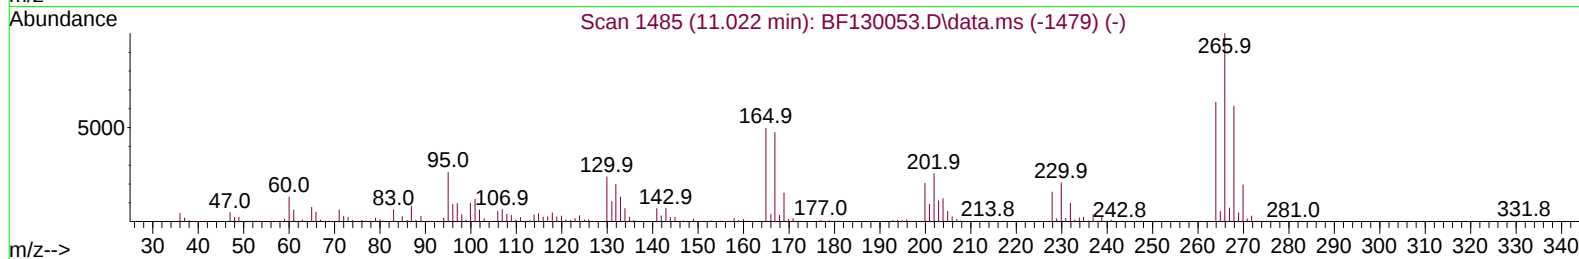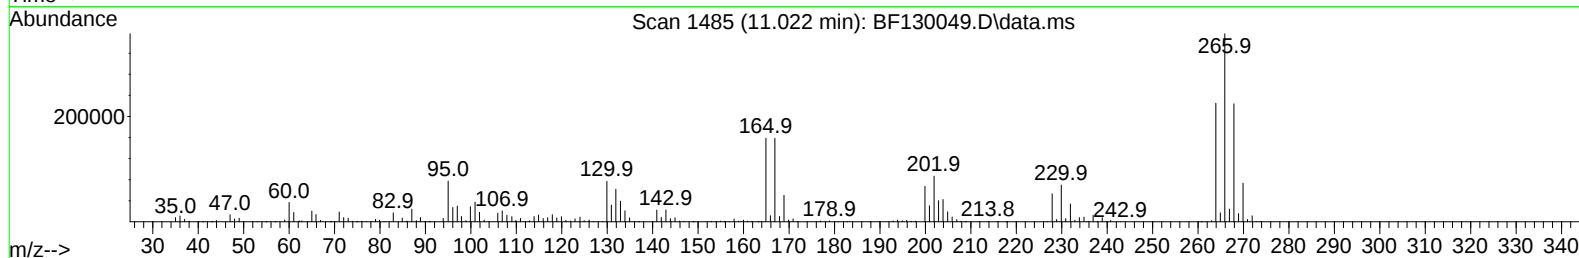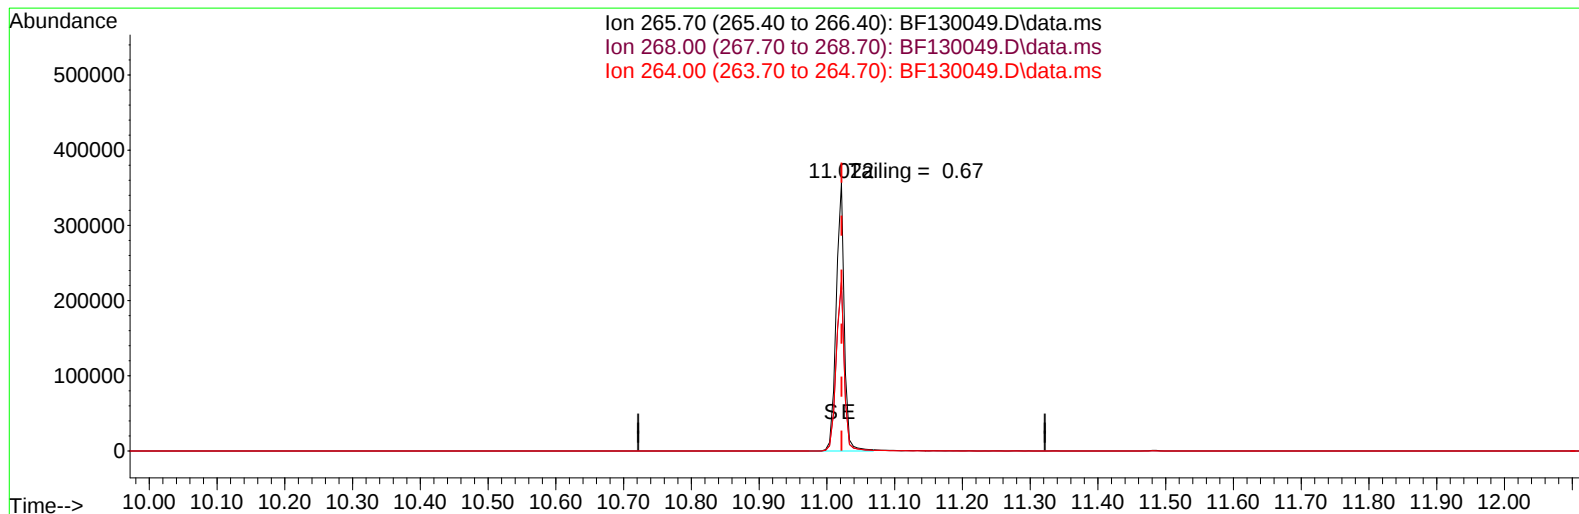

TIC: BF130049.D\data.ms

(70) Pentachlorophenol (C)

11.022min (-0.000) 844810.69 ng




response 300587

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.76
264.00	59.90	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083122\
 Data File : BF130049.D
 Acq On : 31 Aug 2022 13:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 31 16:36:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 31 15:58:13 2022
 Response via : Initial Calibration

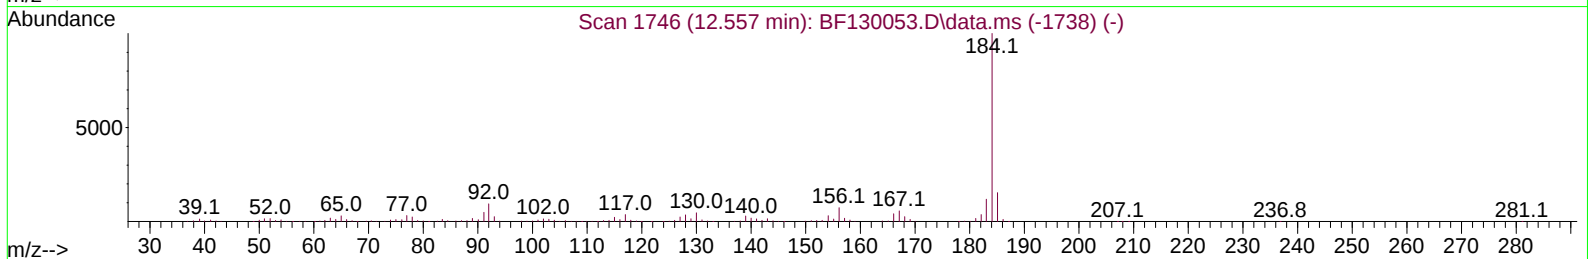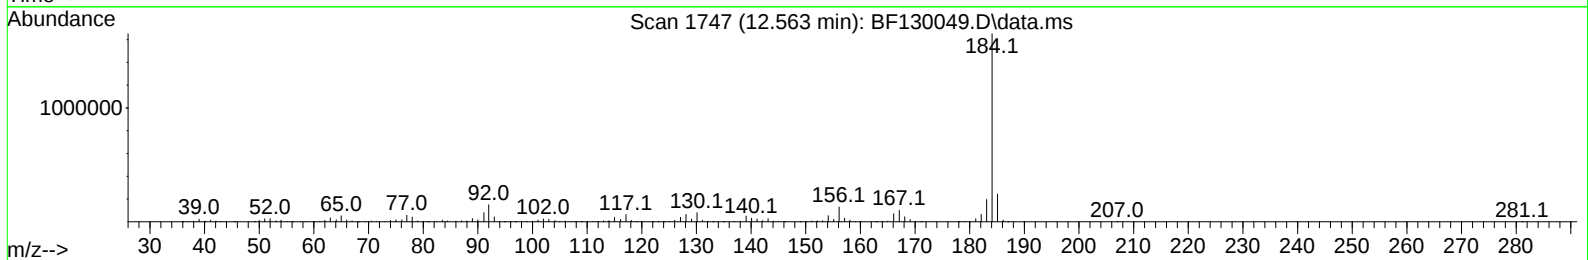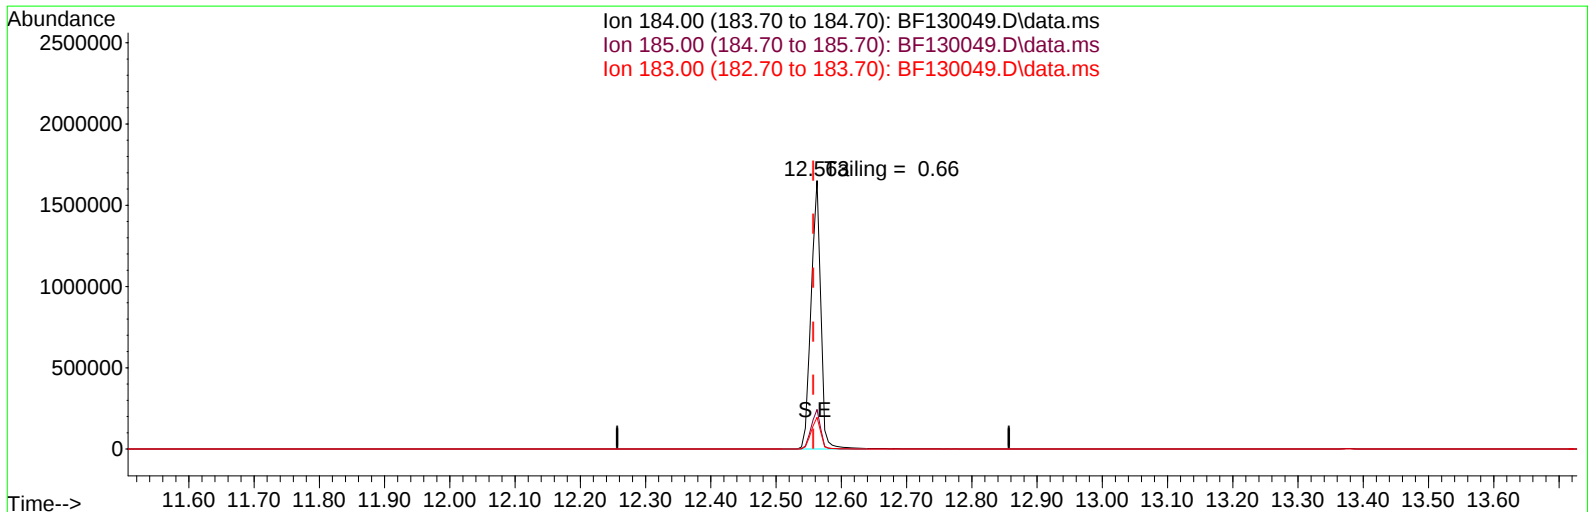

TIC: BF130049.D\data.ms

(77) Benzidine

12.563min (+ 0.006) 0.00 ng

response 1693933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.76
183.00	11.80	11.85
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/31/2022	BNA_F	<u>BF130049.D</u>
Compound Name	Response	Retention Time
DDT	594250	13.38
DDD	5173	13.07
DDE	0	12.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5173	599423	0.86

Instrument :
BNA_F
ClientSampleId :
DFTPP