
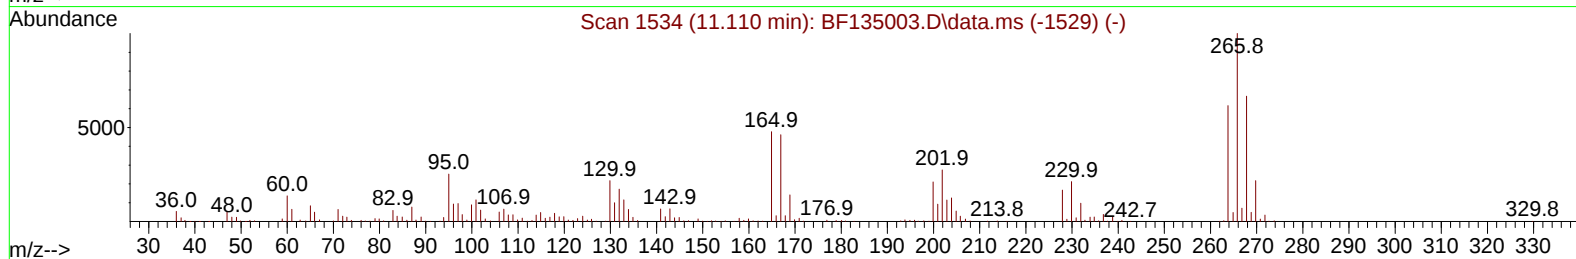
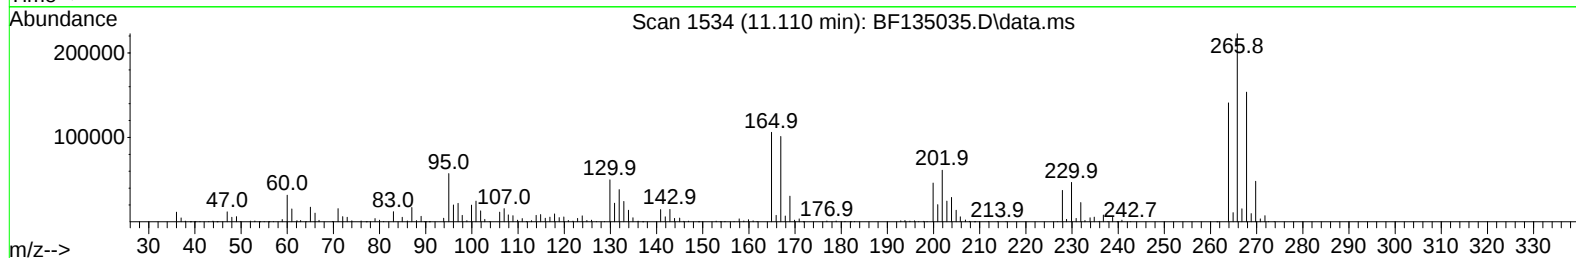


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
Data File : BF135035.D
Acq On : 31 Aug 2023 11:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 16:35:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

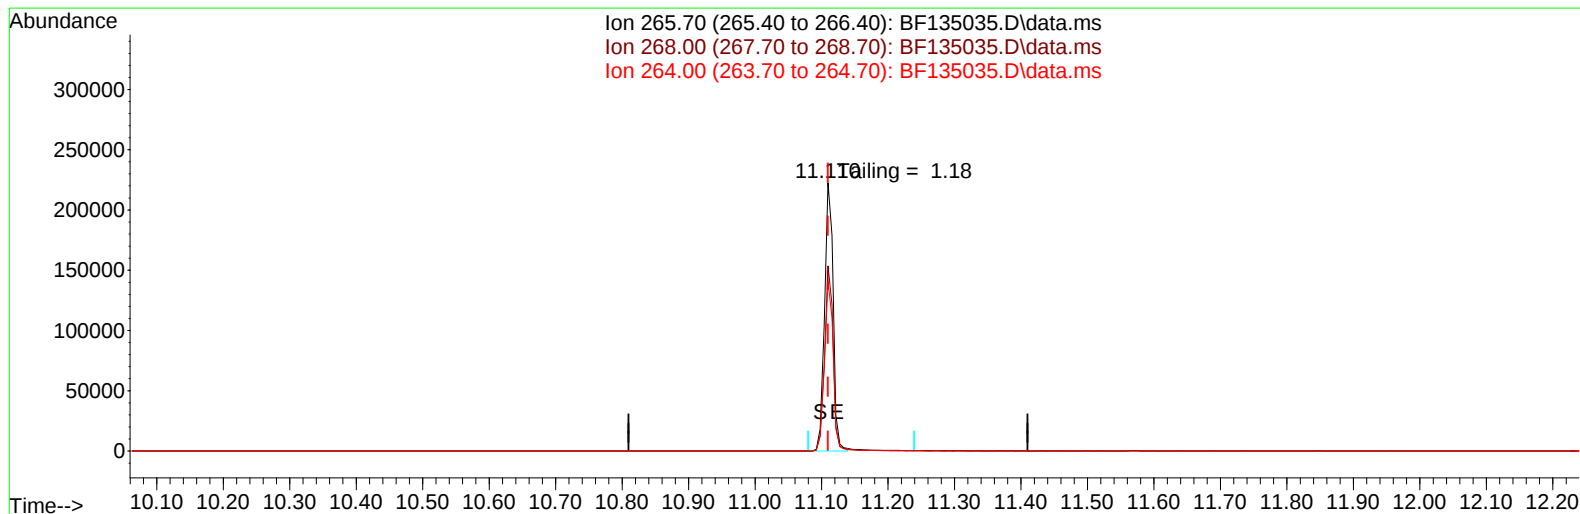

TIC: BF135035.D\data.ms




(70) Pentachlorophenol (C)

11.110min (-0.000) 39796.01 ng

response 203848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	68.94
264.00	61.60	63.28
0.00	0.00	0.00

Quant Time: Aug 31 16:35:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

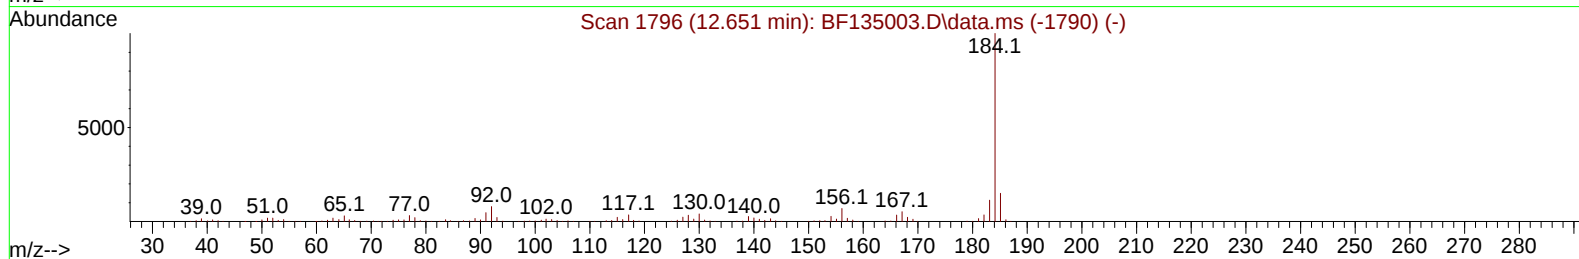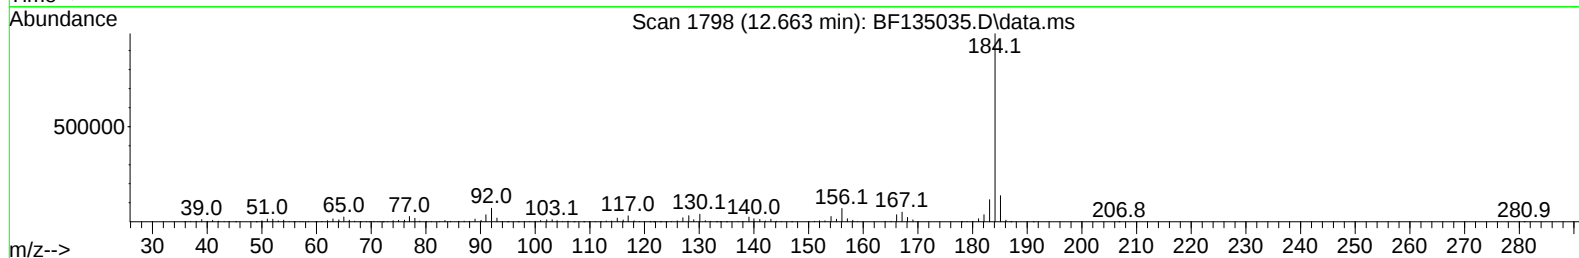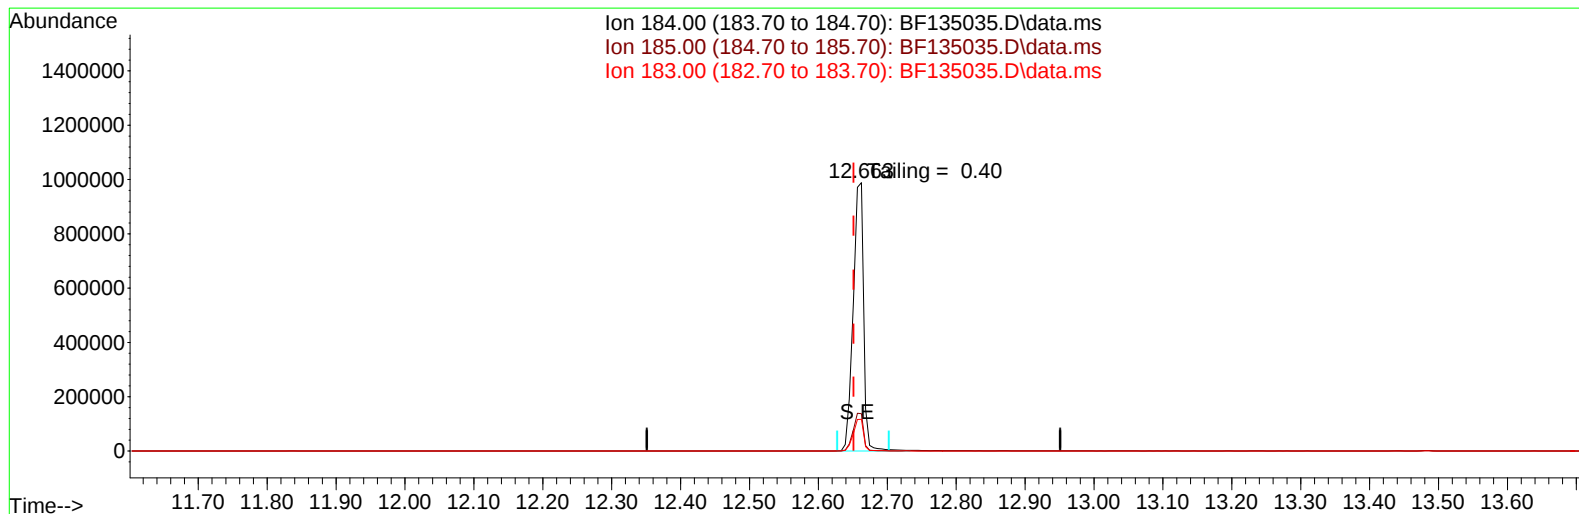

TIC: BF135035.D\data.ms

(77) Benzidine

12.663min (+ 0.012) 1086412.35 ng m

response **1037961**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.91
183.00	11.30	11.80
0.00	0.00	0.00