
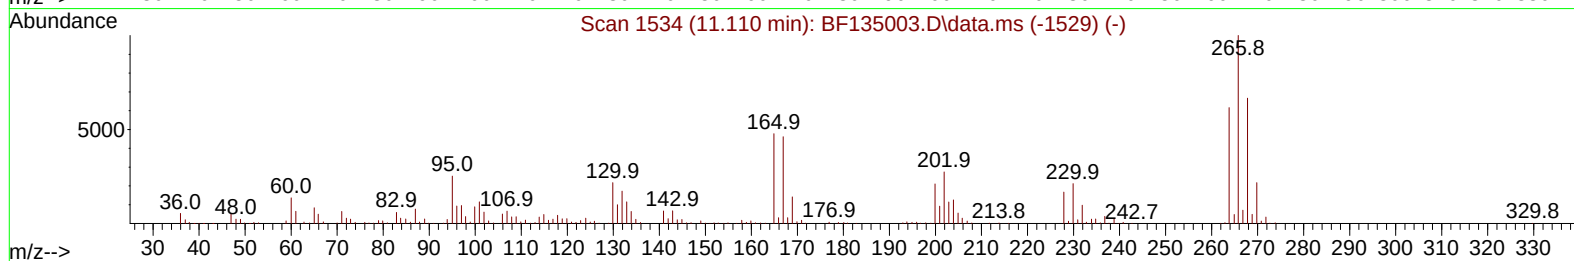
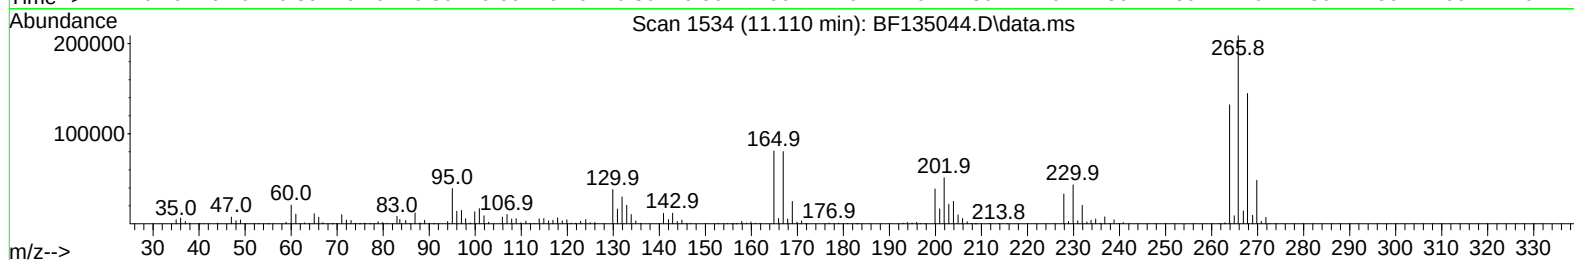


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
Data File : BF135044.D
Acq On : 31 Aug 2023 16:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 17:14:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

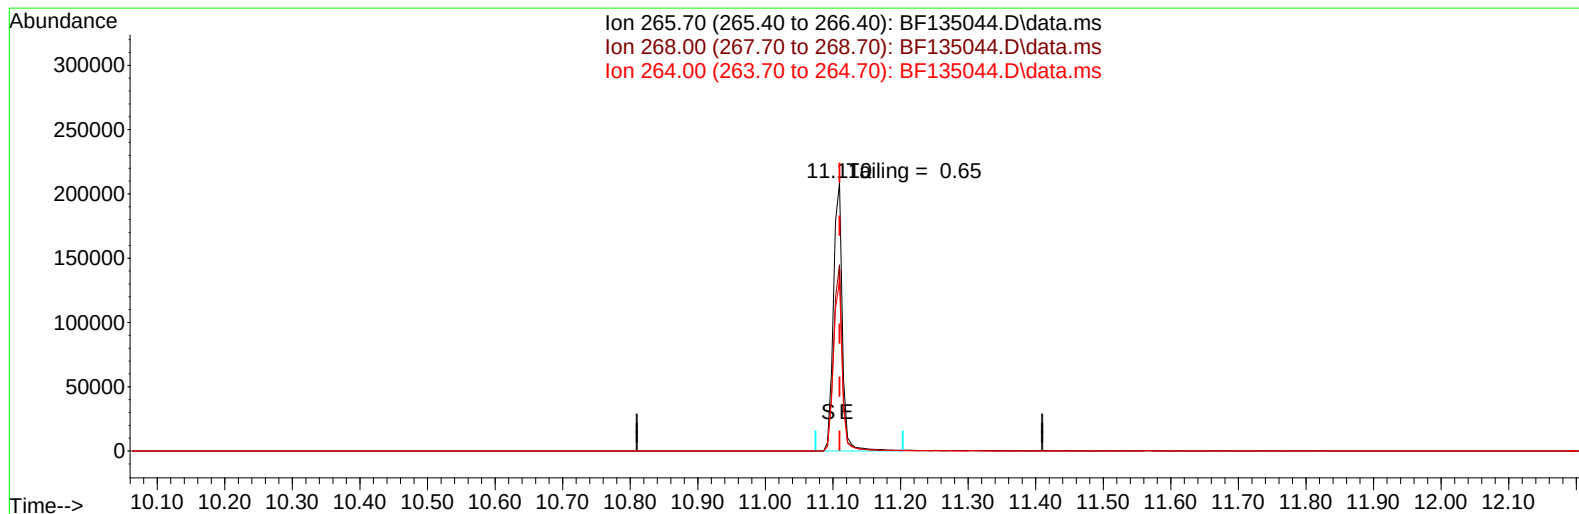

TIC: BF135044.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.000) 467020.29 ng

response 192122

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	69.34
264.00	61.60	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
Data File : BF135044.D
Acq On : 31 Aug 2023 16:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 31 17:14:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

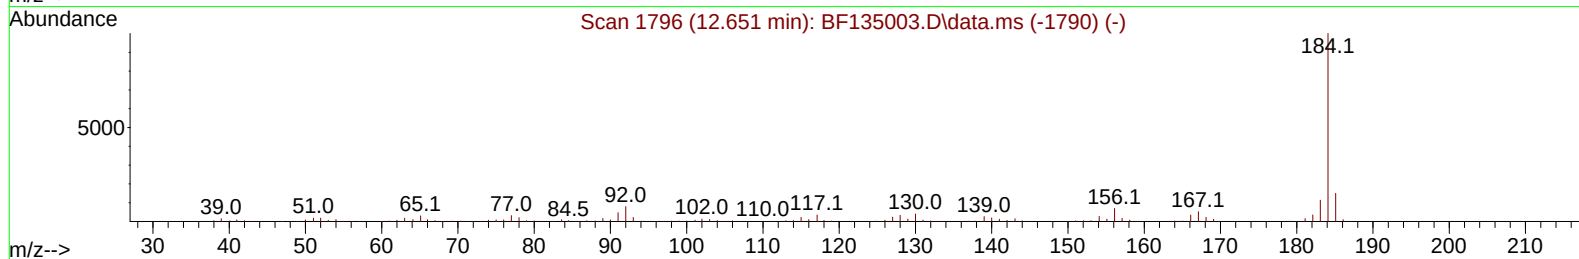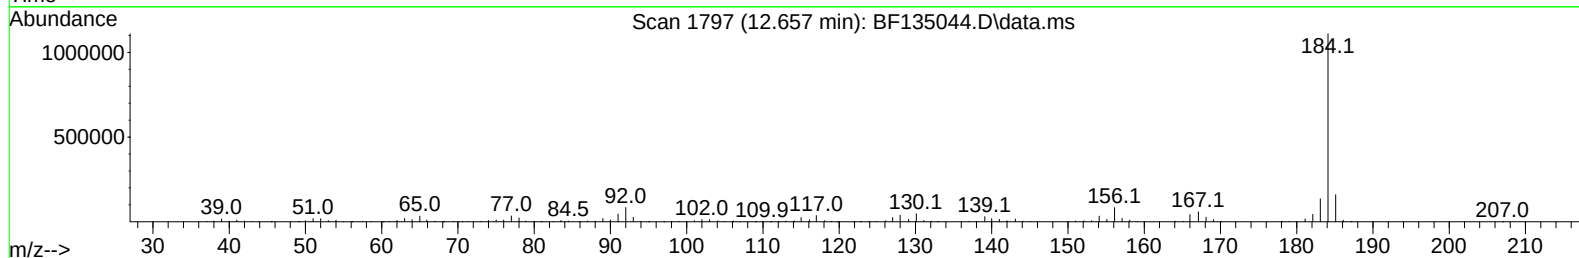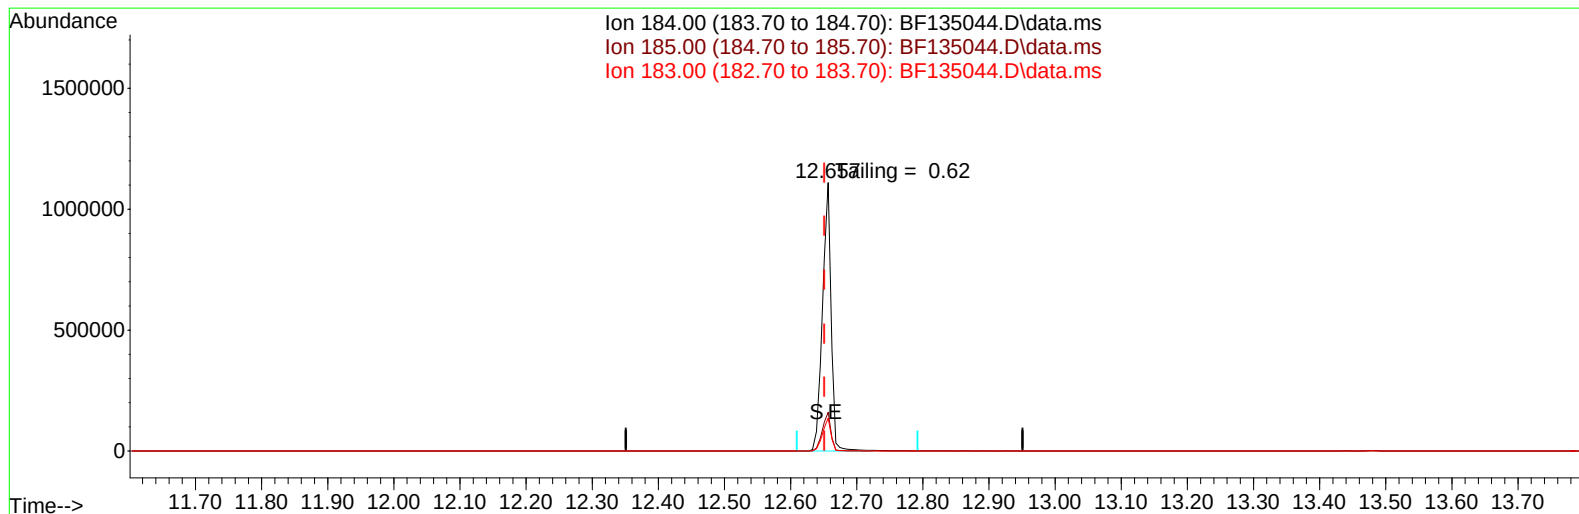

TIC: BF135044.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 0.00 ng

response 1015632

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.43
183.00	11.30	12.23
0.00	0.00	0.00