


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
Data File : BF135035.D
Acq On : 31 Aug 2023 11:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 31 03:48:08 2023

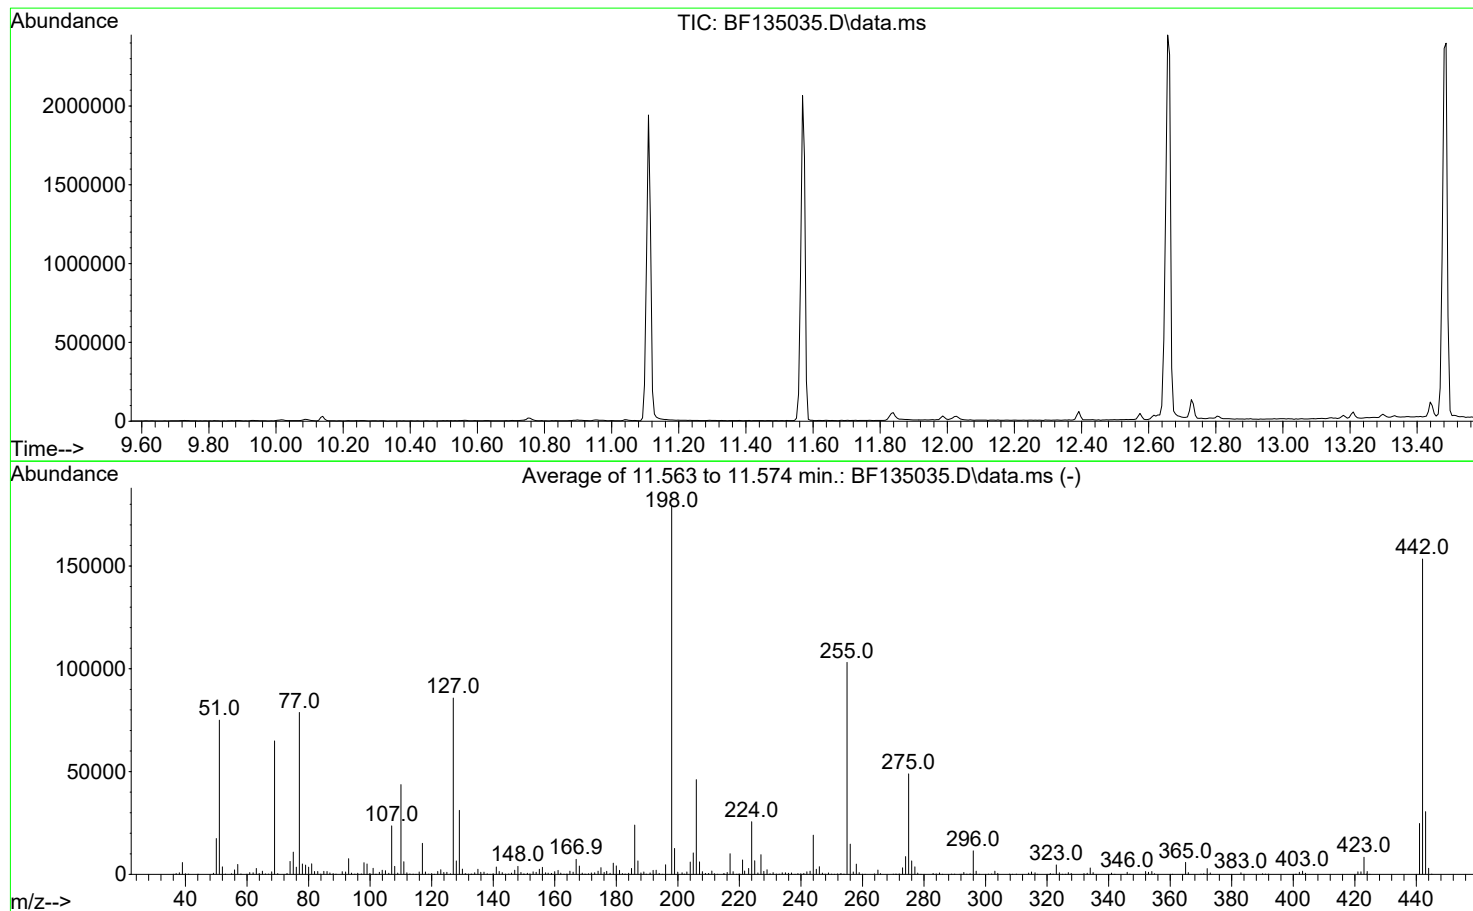




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	75003	PASS
68	69	0.00	2	1.9	1229	PASS
69	198	0.00	100	36.3	64933	PASS
70	69	0.00	2	0.7	426	PASS
127	198	10	80	47.9	85757	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	178941	PASS
199	198	5	9	7.0	12576	PASS
275	198	10	60	27.3	48875	PASS
365	198	1	100	3.3	5823	PASS
441	198	0.01	100	13.8	24770	PASS
442	442	50	100	100.0	153435	PASS
443	442	15	24	19.9	30511	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
Data File : BF135035.D
Acq On : 31 Aug 2023 11:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 31 16:35:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

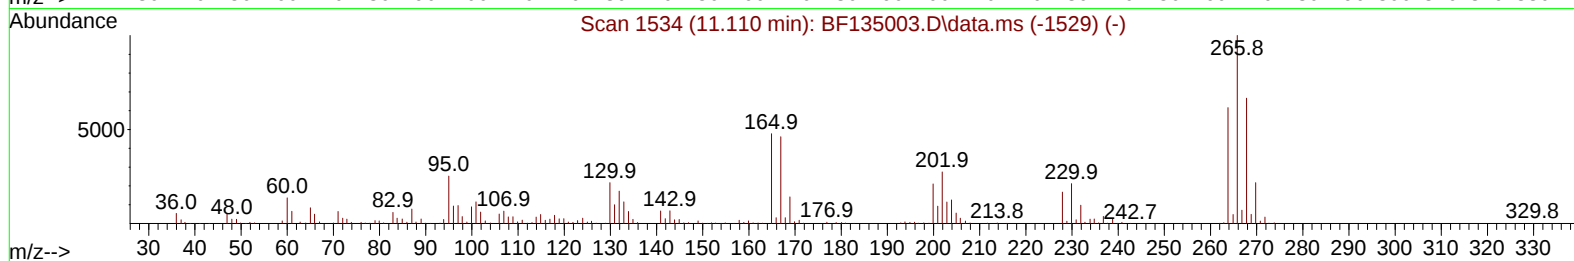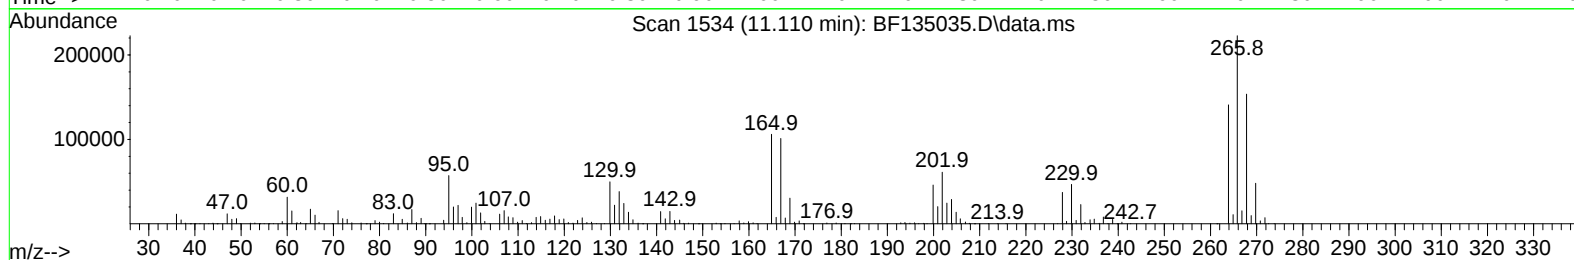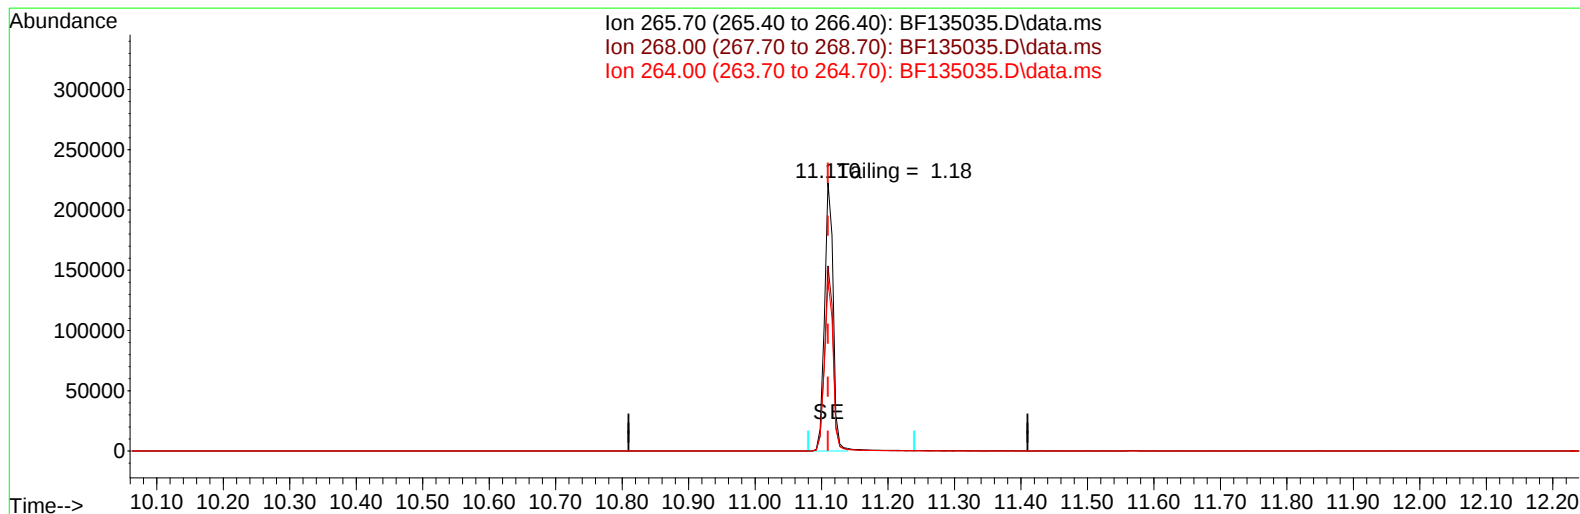

TIC: BF135035.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.000) 39796.01 ng




response 203848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	68.94
264.00	61.60	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
Data File : BF135035.D
Acq On : 31 Aug 2023 11:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 31 16:35:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

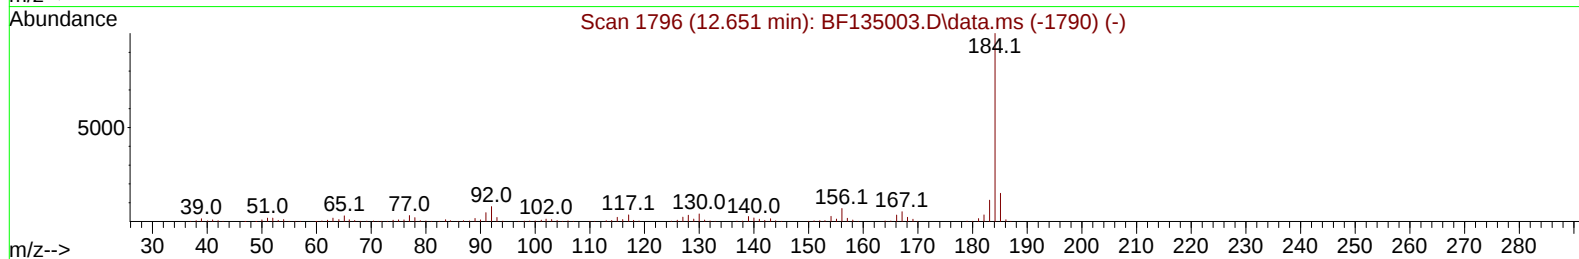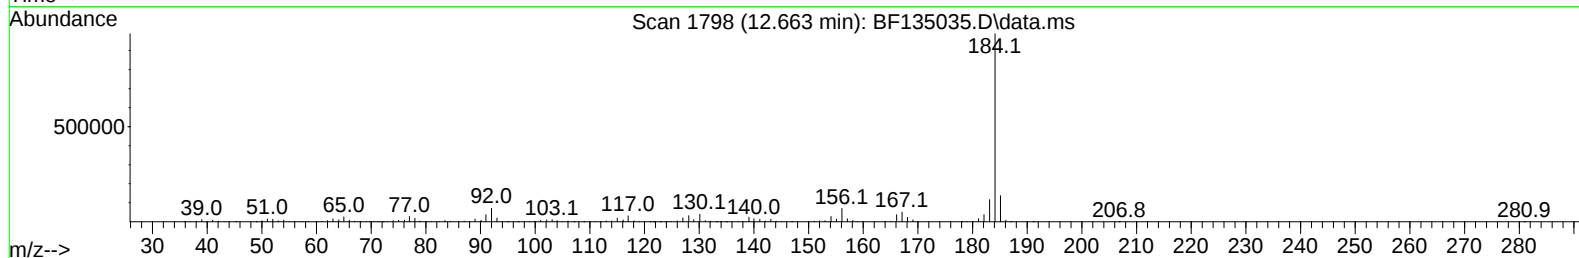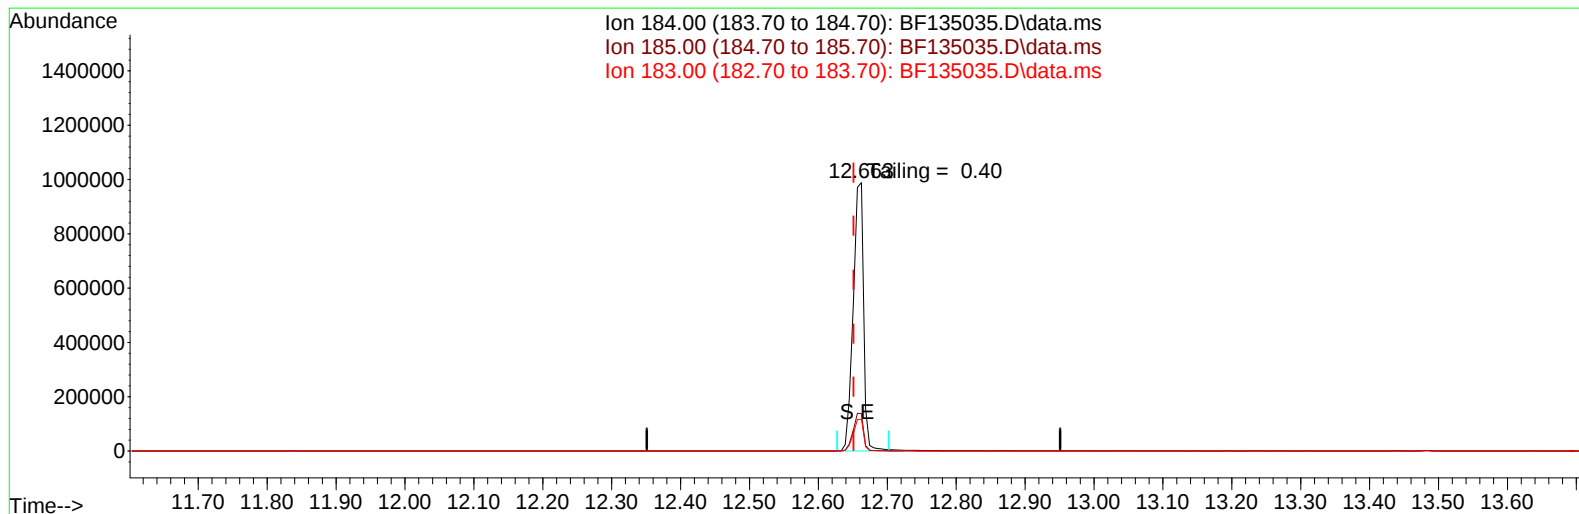

TIC: BF135035.D\data.ms

(77) Benzidine

12.663min (+ 0.012) 1086412.35 ng m

response **1037961**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	13.91
183.00	11.30	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/31/2023	BNA_F	<u>BF135035.D</u>
Compound Name	Response	Retention Time
DDT	467538	13.486
DDD	8082	13.21
DDE	4264	11.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12346	479884	2.57

Instrument :
BNA_F
ClientSampleId :
DFTPP