


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
Data File : BF135044.D
Acq On : 31 Aug 2023 16:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 31 03:48:08 2023

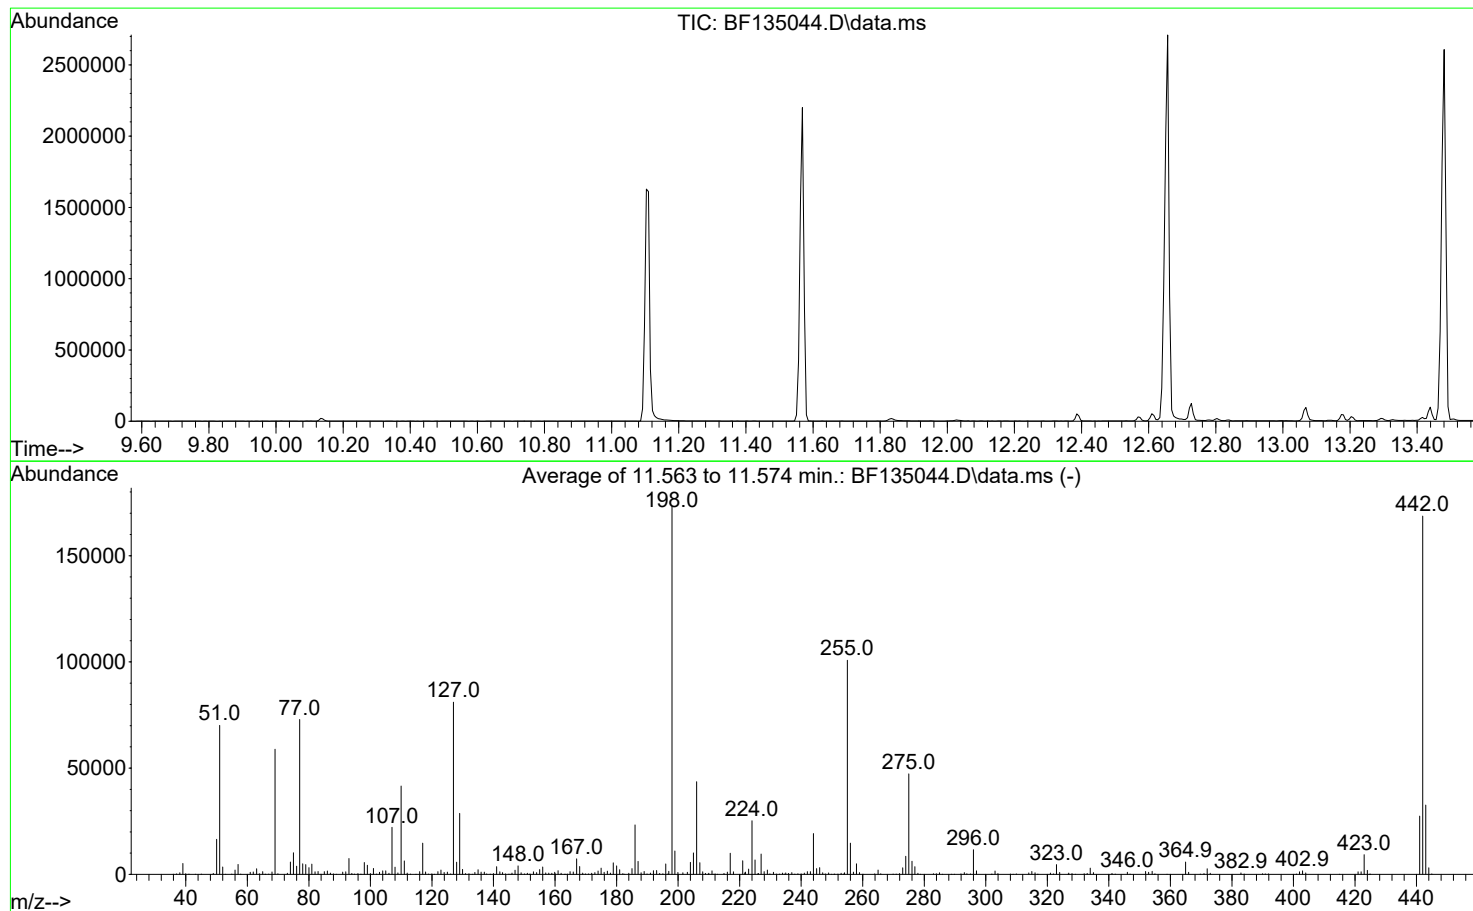




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	70133	PASS
68	69	0.00	2	2.0	1166	PASS
69	198	0.00	100	34.0	58939	PASS
70	69	0.00	2	0.6	335	PASS
127	198	10	80	46.8	81091	PASS
197	198	0.00	2	0.8	1417	PASS
198	198	100	100	100.0	173173	PASS
199	198	5	9	6.3	10996	PASS
275	198	10	60	27.3	47331	PASS
365	198	1	100	3.4	5815	PASS
441	198	0.01	100	15.9	27458	PASS
442	442	50	100	100.0	168632	PASS
443	442	15	24	19.3	32597	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
 Data File : BF135044.D
 Acq On : 31 Aug 2023 16:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 31 17:14:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 31 03:48:08 2023
 Response via : Initial Calibration

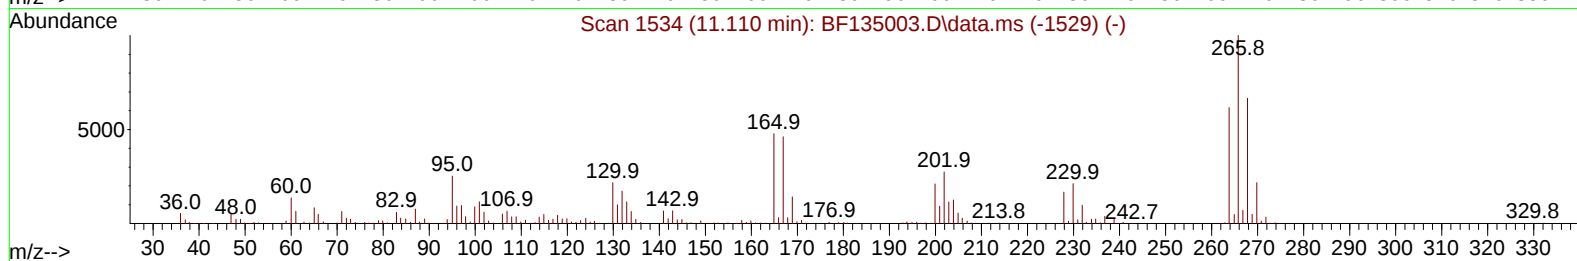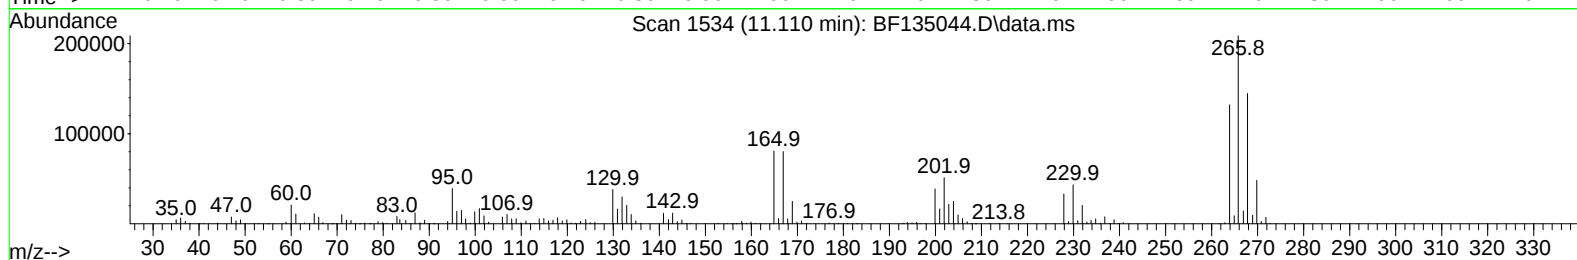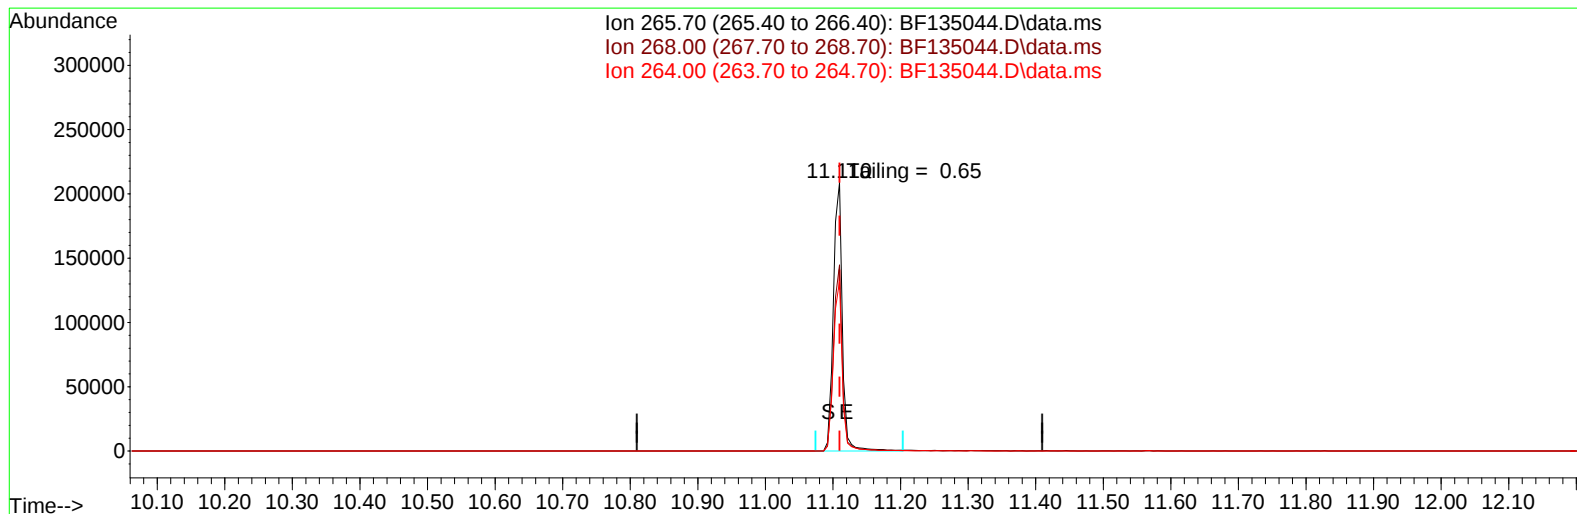

TIC: BF135044.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.000) 467020.29 ng




response 192122

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	69.34
264.00	61.60	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF083123\
Data File : BF135044.D
Acq On : 31 Aug 2023 16:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 31 17:14:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

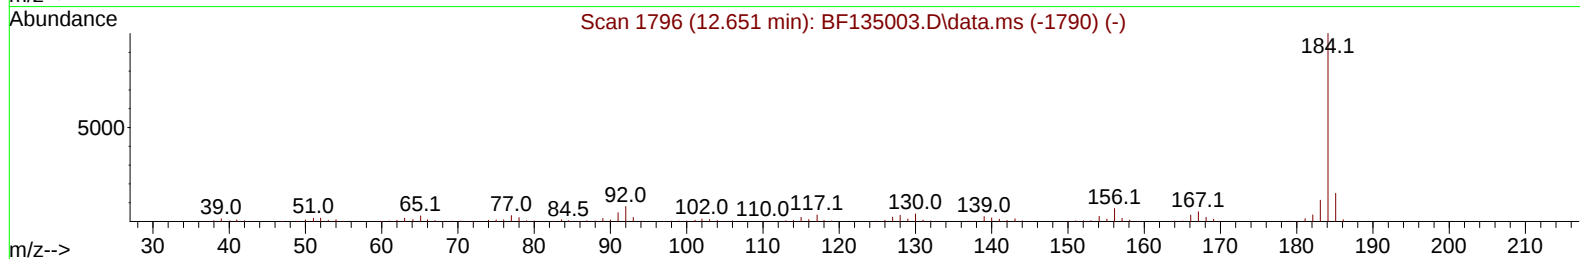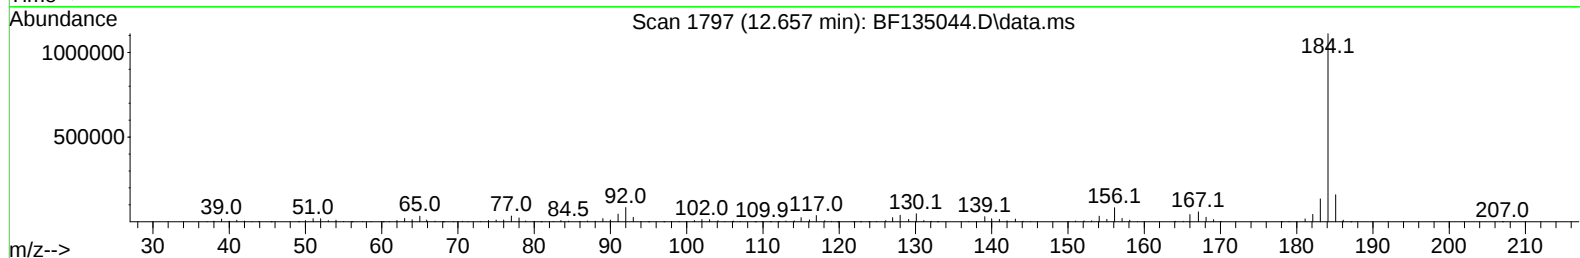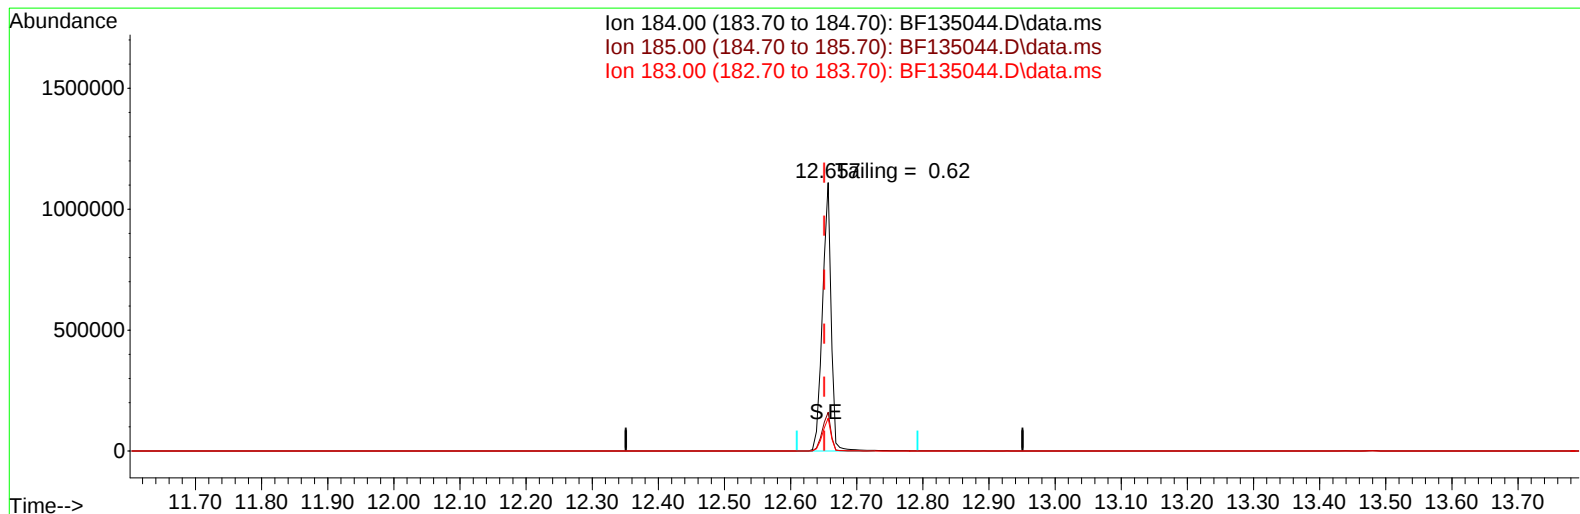

TIC: BF135044.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 0.00 ng

response 1015632

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.43
183.00	11.30	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/31/2023	BNA_F	<u>BF135044.D</u>
Compound Name	Response	Retention Time
DDT	462910	13.48
DDD	13050	13.174
DDE	3736	11.568
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16786	479696	3.50

Instrument :
BNA_F
ClientSampleId :
DFTPP