
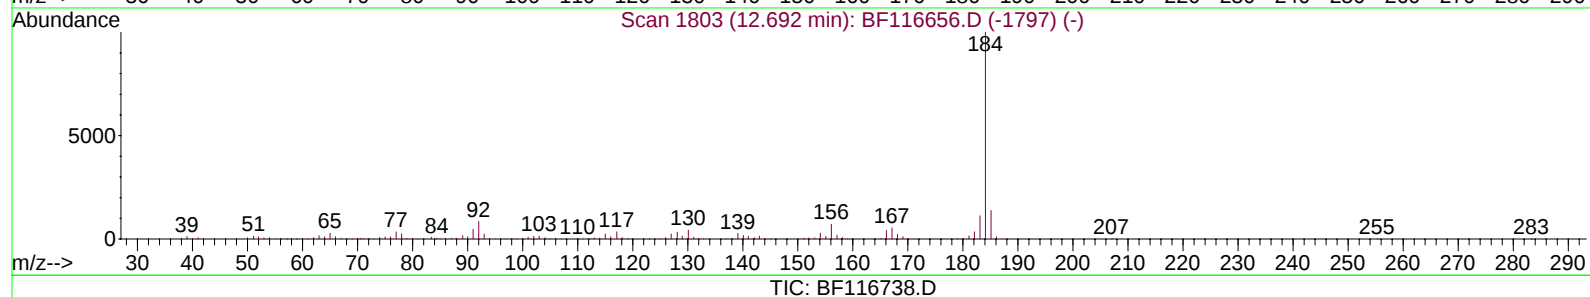
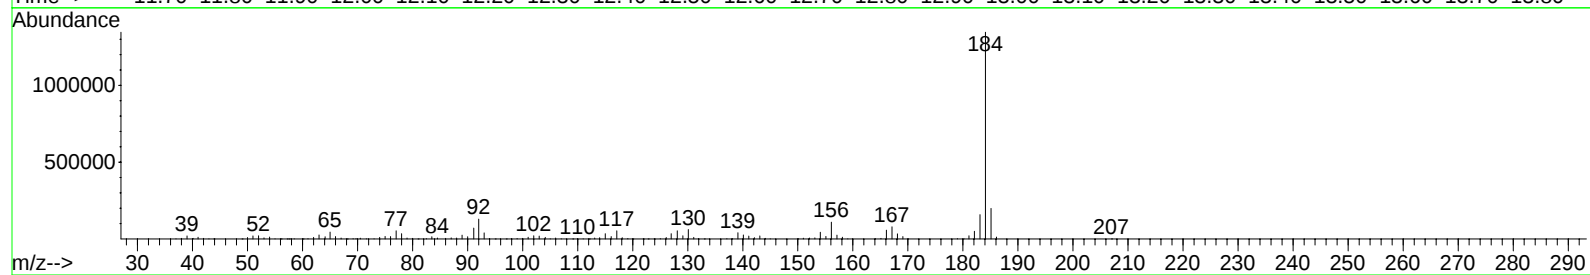


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090119\
 Data File : BF116738.D
 Acq On : 1 Sep 2019 13:04
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 11:55:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 30 20:02:30 2019
 Response via : Initial Calibration

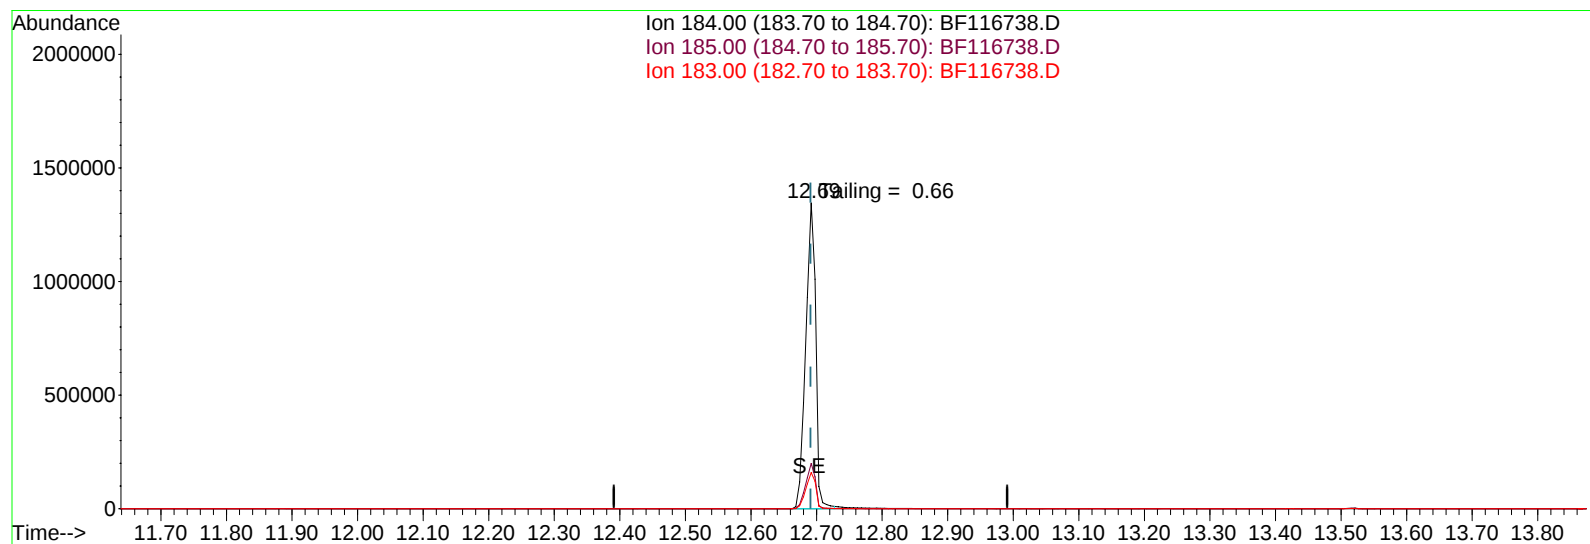

(77) Benzidine




12.692min (+0.001) 41098.65ng

response 1450791

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.80
183.00	11.50	11.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF090119\
Data File : BF116738.D
Acq On : 1 Sep 2019 13:04
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 11:55:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 30 20:02:30 2019
Response via : Initial Calibration

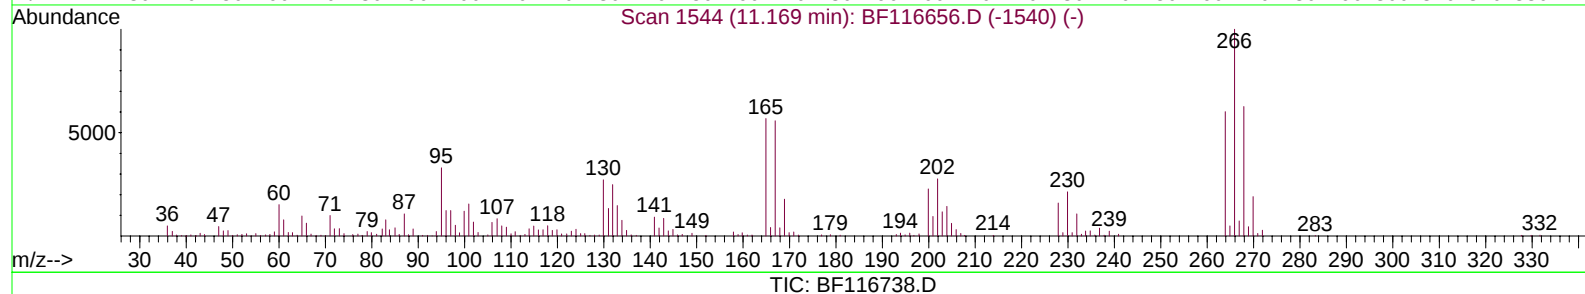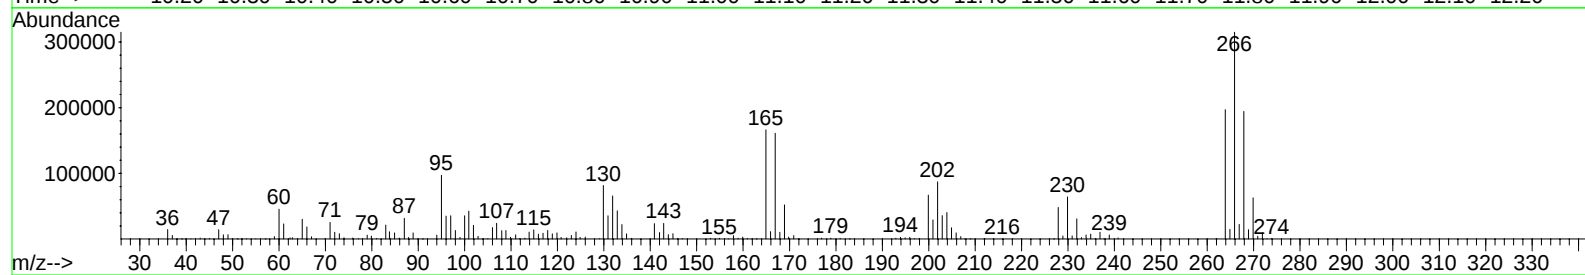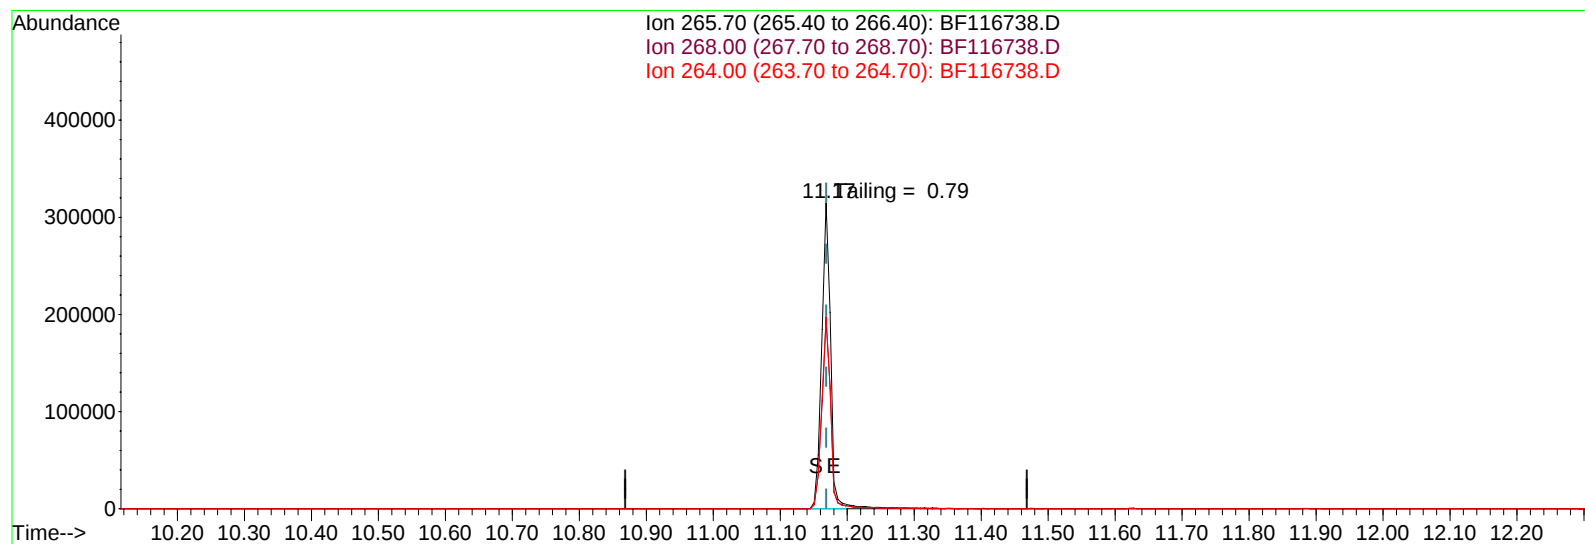

(70) Pentachlorophenol (C)

11.168min (-0.000) 45036.89ng

response 295933

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	61.71
264.00	64.90	62.57
0.00	0.00	0.00