

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090119\
 Data File : BF116759.D
 Acq On : 1 Sep 2019 22:46
 Operator : HP/JU
 Sample : K4583-01 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GS-STOCKPILE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	569	572	584	rBV	744200	735457	68.21%	5.594%
2	6.469	741	745	756	rBV	1026125	877235	81.36%	6.673%
3	6.610	766	769	773	rBV	958285	824619	76.48%	6.272%
4	6.845	806	809	813	rBV	718521	559724	51.91%	4.257%
5	7.004	832	836	839	rBV	697760	612018	56.76%	4.655%
6	7.398	900	903	908	rBV	561653	455288	42.23%	3.463%
7	8.128	1023	1027	1030	rBV	1048768	805977	74.75%	6.131%
8	8.886	1152	1156	1164	rVB2	9371	13779	1.28%	0.105%
9	9.198	1206	1209	1213	rBV	1290807	1016667	94.29%	7.733%
10	9.592	1272	1276	1280	rVB	110601	90287	8.37%	0.687%
11	9.880	1321	1325	1328	rBV	1308419	1047565	97.16%	7.968%
12	10.663	1454	1458	1469	rBV	617970	540401	50.12%	4.110%
13	10.751	1469	1473	1478	rBV2	26250	42147	3.91%	0.321%
14	11.321	1565	1570	1573	rBV5	8770	15784	1.46%	0.120%
15	11.363	1573	1577	1579	rVV	1253044	1059785	98.29%	8.061%
16	11.380	1579	1580	1584	rVV	91831	78466	7.28%	0.597%
17	11.433	1588	1589	1593	rVB	22106	18696	1.73%	0.142%
18	11.851	1657	1660	1663	rBV3	19417	27594	2.56%	0.210%
19	11.886	1663	1666	1670	rVV2	105353	105288	9.76%	0.801%
20	11.921	1670	1672	1678	rVV2	25176	33719	3.13%	0.256%
21	11.974	1678	1681	1688	rVB4	23504	37269	3.46%	0.283%
22	12.063	1693	1696	1701	rVB5	14875	16132	1.50%	0.123%
23	12.157	1709	1712	1714	rBV2	12845	16419	1.52%	0.125%
24	12.174	1714	1715	1719	rVB4	16838	13943	1.29%	0.106%
25	12.410	1752	1755	1760	rBV5	11595	13696	1.27%	0.104%
26	12.492	1767	1769	1774	rVB5	12357	14324	1.33%	0.109%
27	12.568	1779	1782	1787	rBV	223884	195922	18.17%	1.490%
28	12.668	1796	1799	1802	rBV3	31680	33428	3.10%	0.254%
29	12.798	1815	1821	1824	rBV	201105	205352	19.05%	1.562%
30	12.939	1841	1845	1851	rVB	1280854	1078226	100.00%	8.201%
31	13.063	1864	1866	1869	rBV3	15736	15444	1.43%	0.117%
32	13.092	1869	1871	1874	rBV4	27831	30751	2.85%	0.234%
33	13.227	1892	1894	1897	rBV3	21056	18635	1.73%	0.142%
34	13.415	1924	1926	1929	rBV2	24295	18606	1.73%	0.142%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090119\
Data File : BF116759.D
Acq On : 1 Sep 2019 22:46
Operator : HP/JU
Sample : K4583-01 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GS-STOCKPILE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.627	1960	1962	1966	rVB2	39653	34150	3.17%	0.260%
36	13.833	1994	1997	2004	rBV3	103835	139138	12.90%	1.058%
37	13.992	2019	2024	2027	rBV	955947	966868	89.67%	7.354%
38	14.015	2027	2028	2031	rVB	97418	56661	5.26%	0.431%
39	14.098	2040	2042	2045	rVB2	45537	38142	3.54%	0.290%
40	14.162	2050	2053	2058	rVV6	33144	43892	4.07%	0.334%
41	14.462	2102	2104	2108	rVB2	67693	67142	6.23%	0.511%
42	14.768	2153	2156	2159	rVB	65485	61603	5.71%	0.469%
43	15.021	2196	2199	2207	rVB	96007	181821	16.86%	1.383%
44	15.104	2210	2213	2215	rBV	109749	110943	10.29%	0.844%
45	15.445	2267	2271	2275	rBV	542709	673341	62.45%	5.122%
46	15.909	2347	2350	2354	rBV	72821	104543	9.70%	0.795%


Sum of corrected areas: 13146887

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090119\
Data File : BF116759.D
Acq On : 1 Sep 2019 22:46
Operator : HP/JU
Sample : K4583-01 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GS-STOCKPILE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

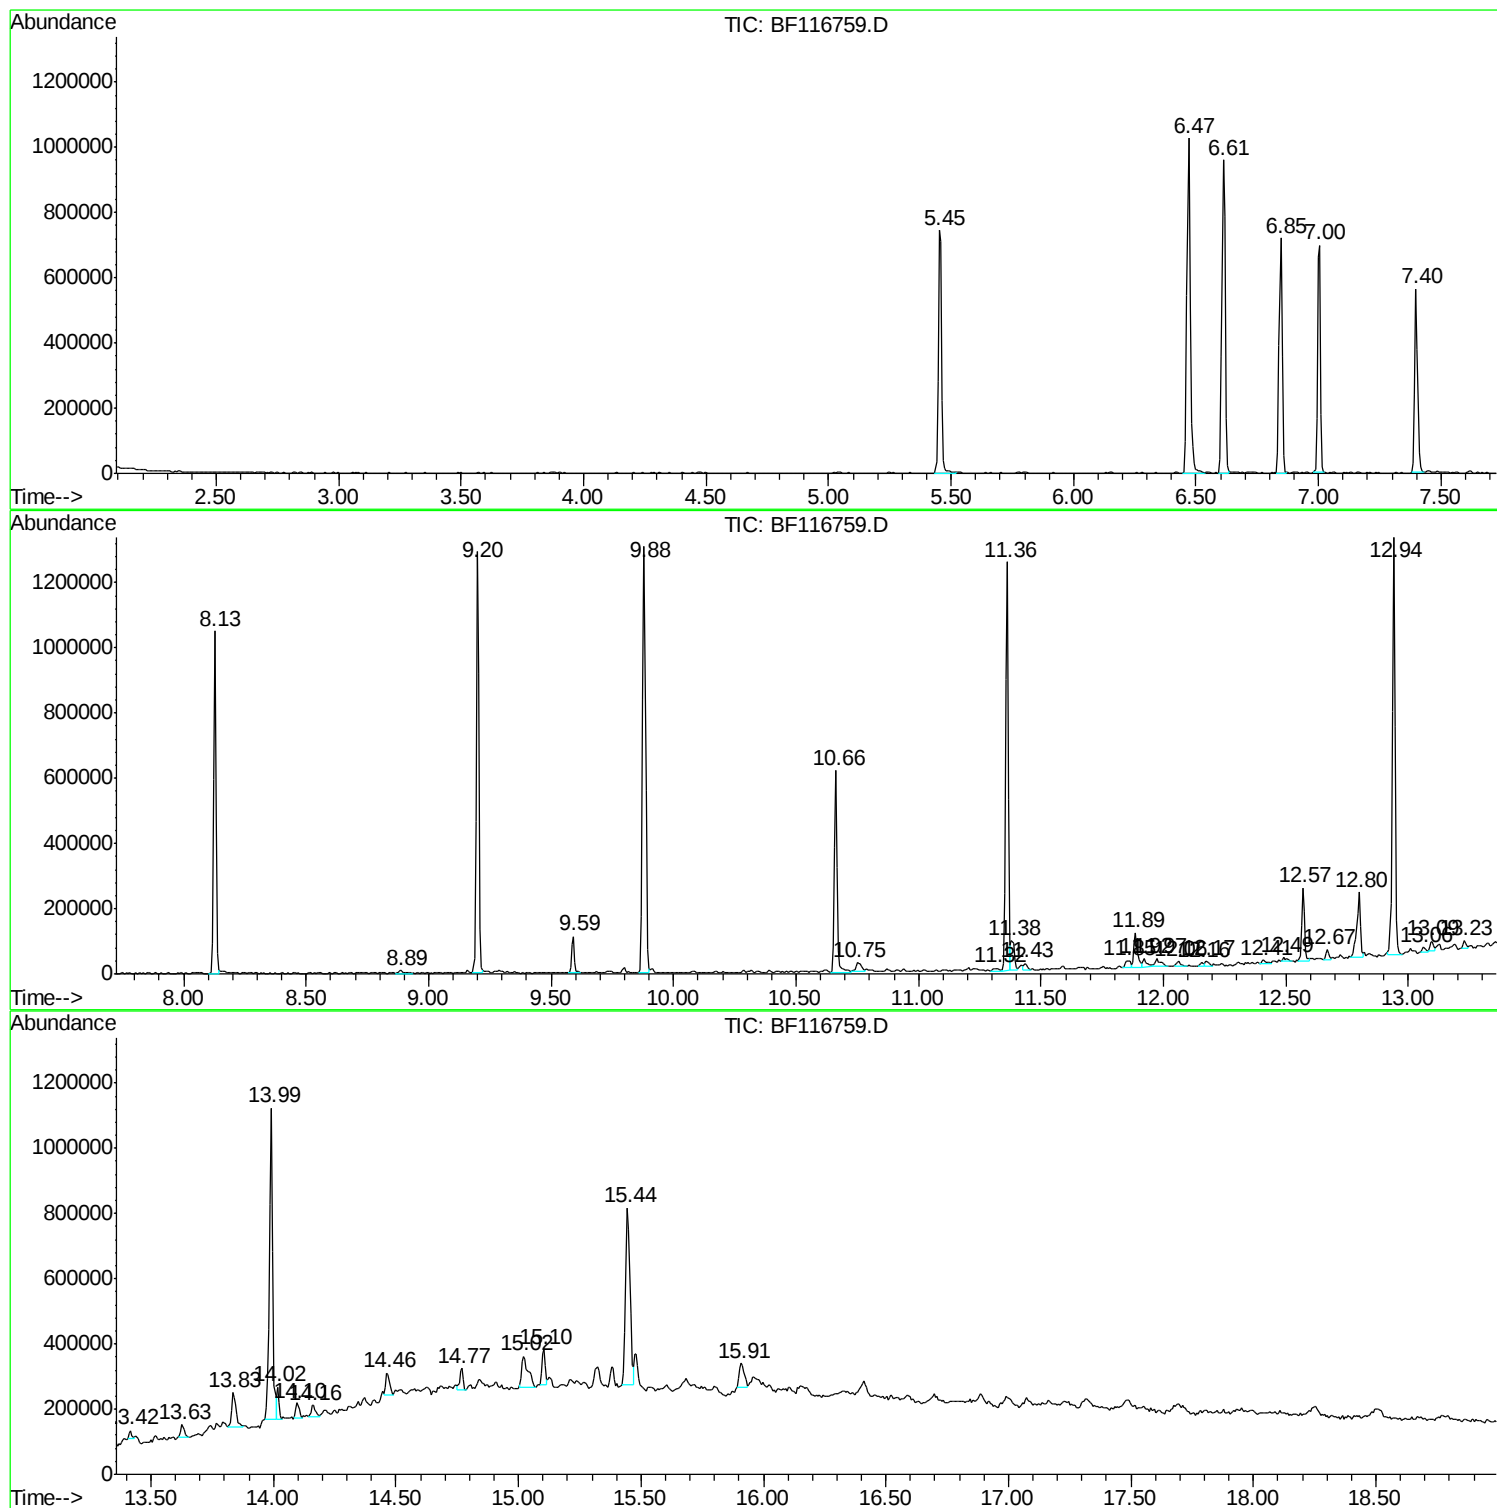

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090119\
Data_File : BF116759.D
Acq_On : 1-Sep-2019 22:466
Operator : HP/JUU
Sample : K4583-01_2XX
Misc :
ALS_Vial : 22 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
GS-STOCKPILE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
