


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF090119\
Data File : BF116738.D
Acq On : 1 Sep 2019 13:04
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 30 20:02:30 2019

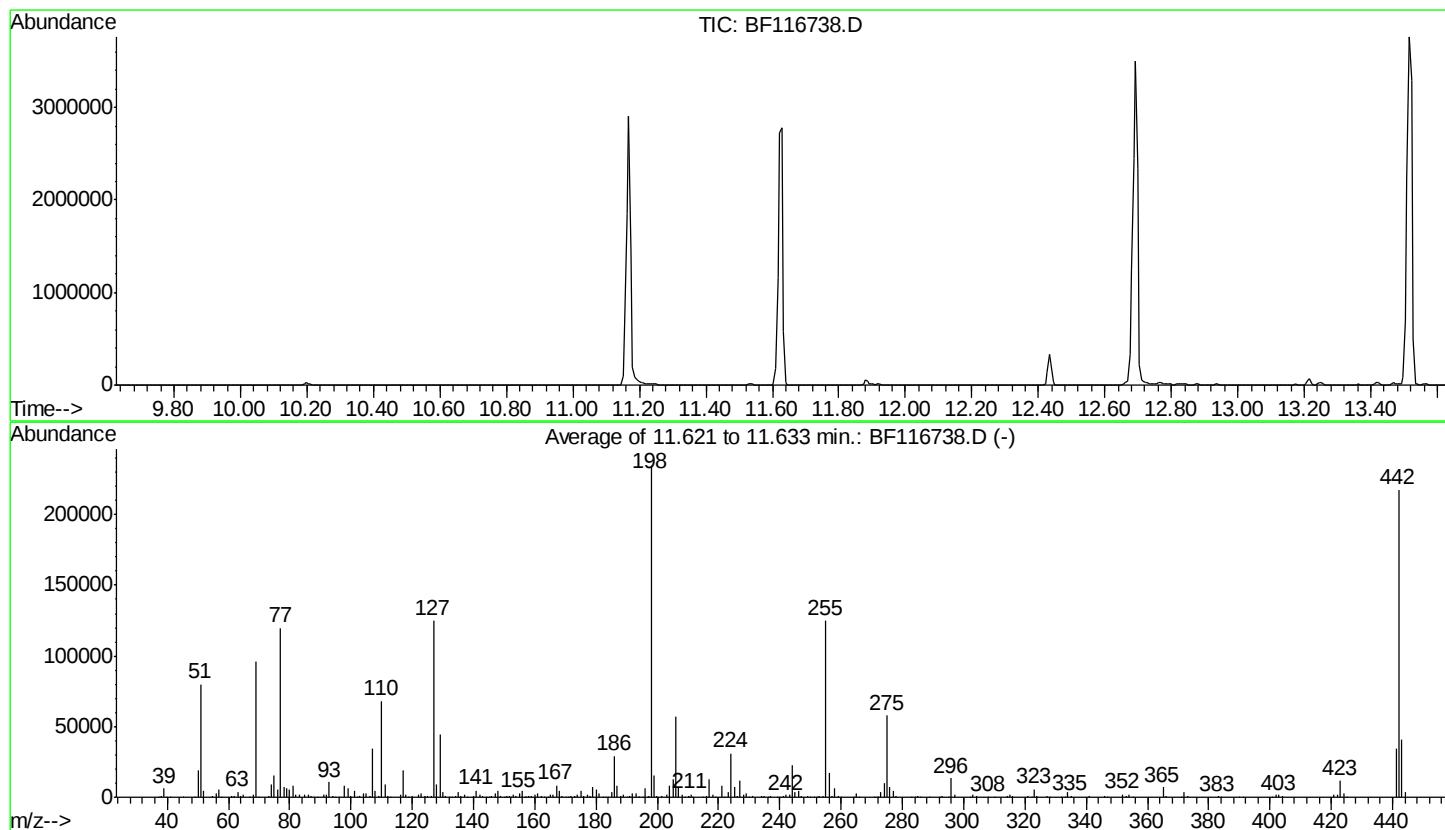

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	79905	PASS
68	69	0.00	2	1.5	1458	PASS
69	198	0.00	100	41.0	96148	PASS
70	69	0.00	2	0.5	474	PASS
127	198	10	80	53.2	124741	PASS
197	198	0.00	2	0.5	1082	PASS
198	198	100	100	100.0	234672	PASS
199	198	5	9	6.7	15777	PASS
275	198	10	60	24.5	57602	PASS
365	198	1	100	3.0	7120	PASS
441	198	0.01	100	14.7	34562	PASS
442	198	50	100	92.7	217472	PASS
443	442	15	24	18.8	40960	PASS