
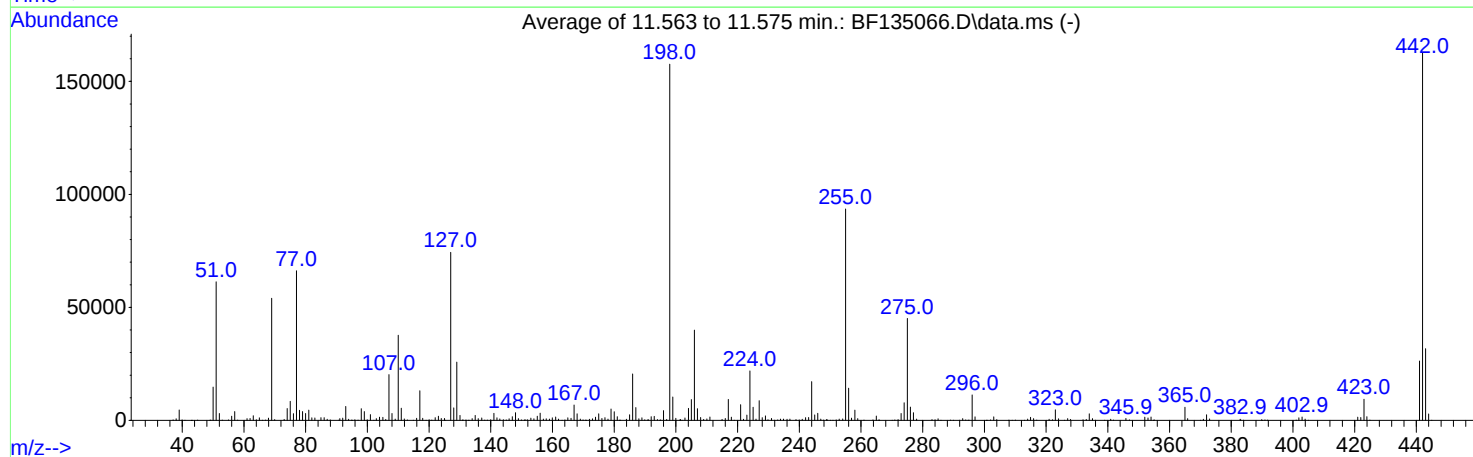


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090123\
 Data File : BF135066.D
 Acq On : 01 Sep 2023 09:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 31 03:48:08 2023

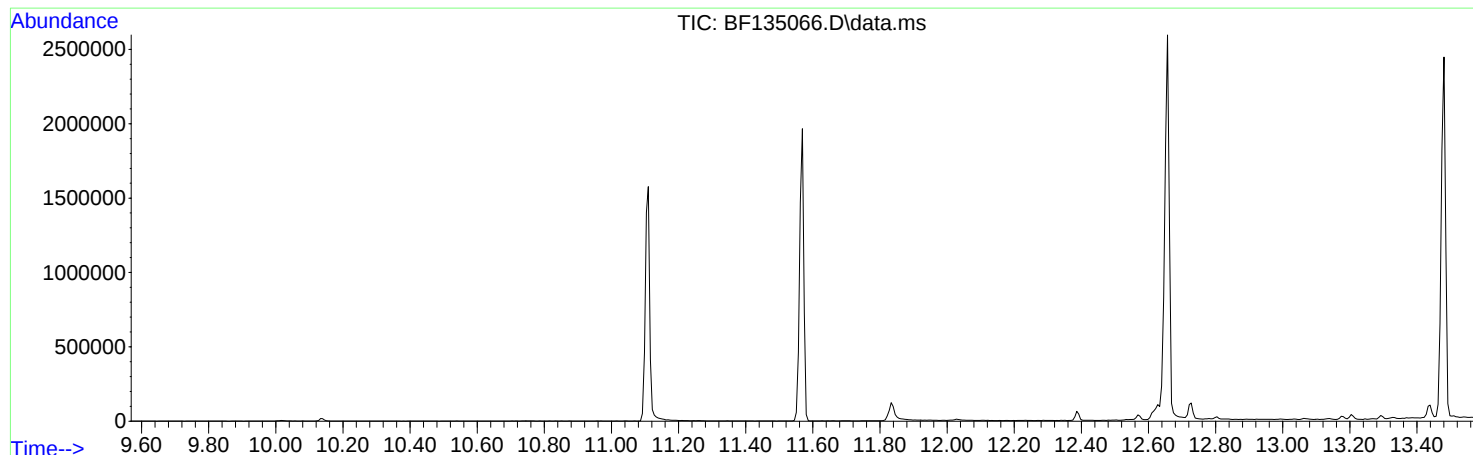




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	61309	PASS
68	69	0.00	2	1.9	1009	PASS
69	198	0.00	100	34.3	54047	PASS
70	69	0.00	2	0.6	346	PASS
127	198	10	80	47.2	74368	PASS
197	198	0.00	2	0.3	452	PASS
198	198	100	100	100.0	157595	PASS
199	198	5	9	6.6	10362	PASS
275	198	10	60	28.6	45096	PASS
365	198	1	100	3.7	5838	PASS
441	198	0.01	100	16.7	26293	PASS
442	442	50	100	100.0	162781	PASS
443	442	15	24	19.5	31688	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090123\
Data File : BF135066.D
Acq On : 01 Sep 2023 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 01 11:11:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

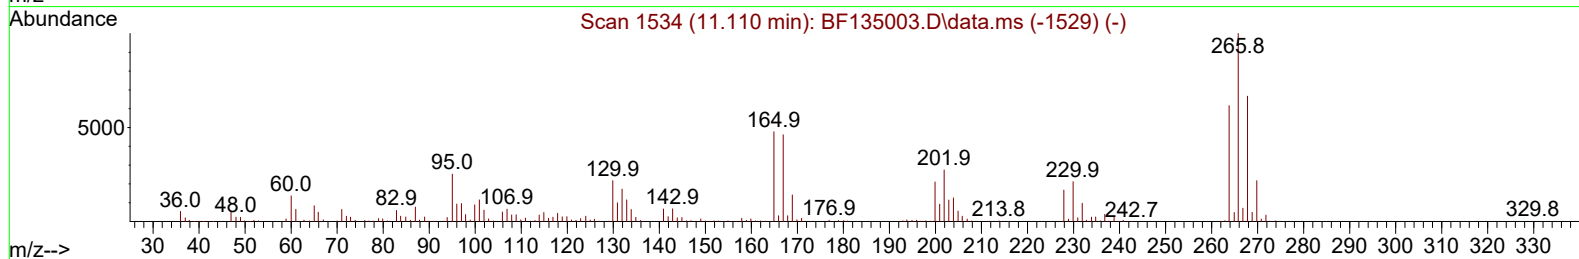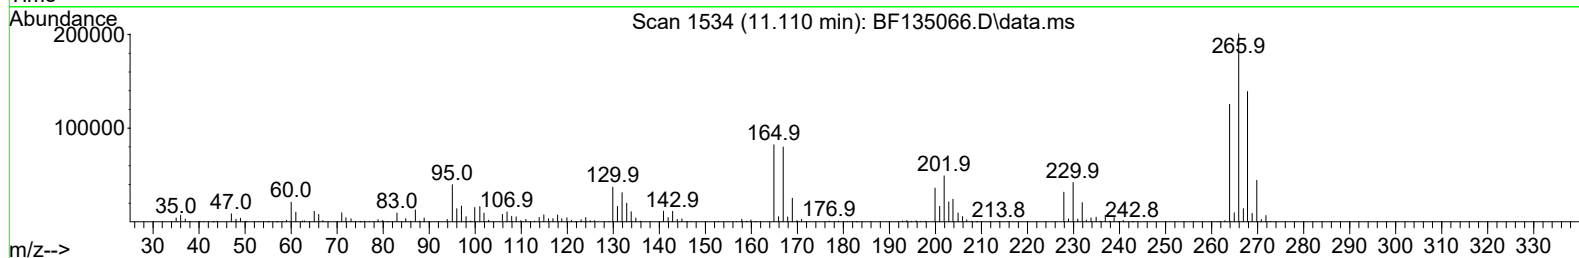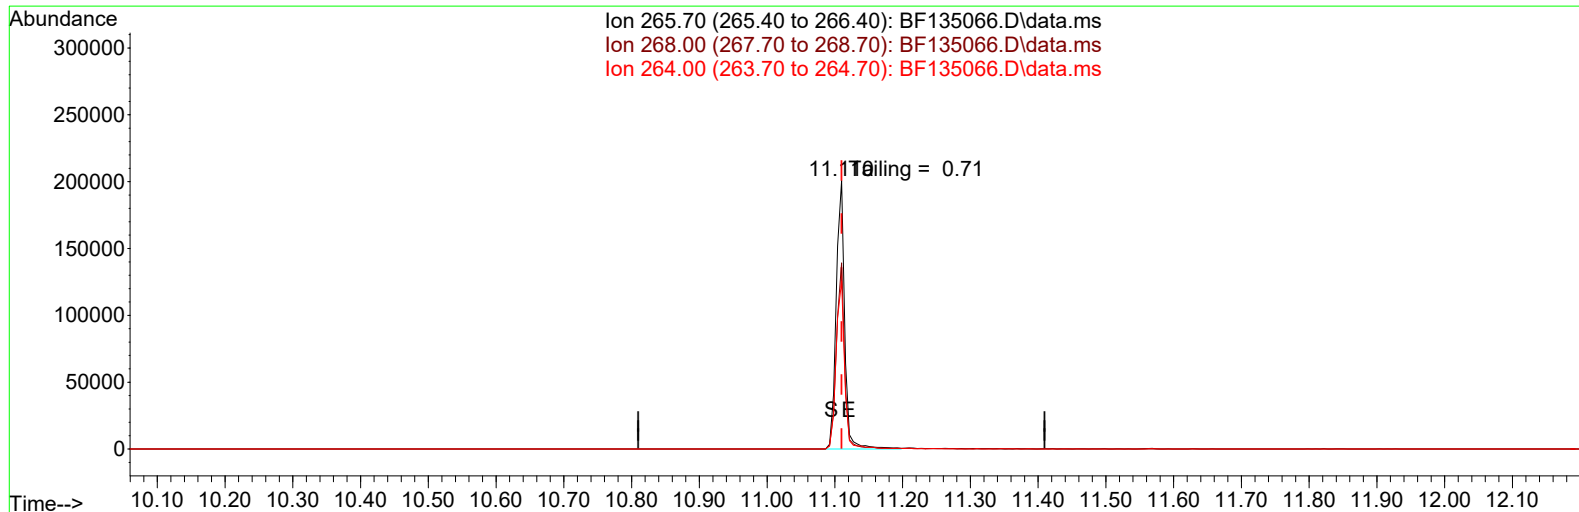

TIC: BF135066.D\data.ms

(70) Pentachlorophenol (C)

11.110min (+ 0.000) 32069.02 ng




response 174907

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.60	69.33
264.00	61.60	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090123\
Data File : BF135066.D
Acq On : 01 Sep 2023 09:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 01 11:11:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 31 03:48:08 2023
Response via : Initial Calibration

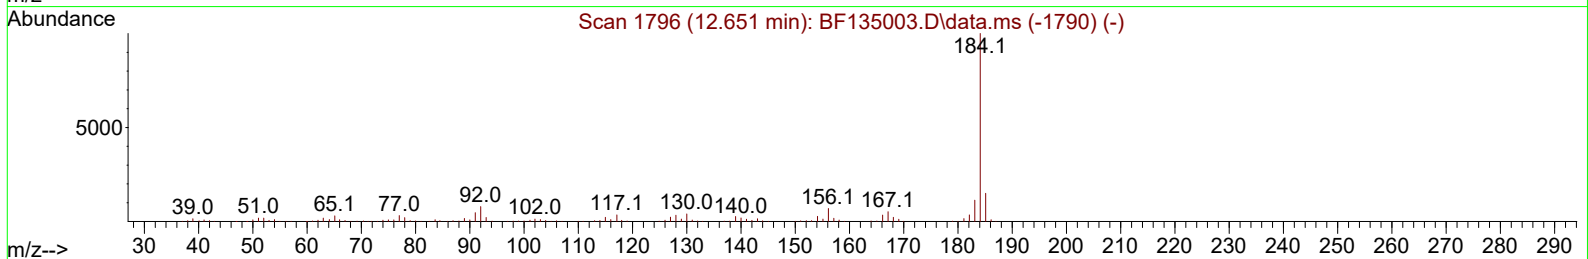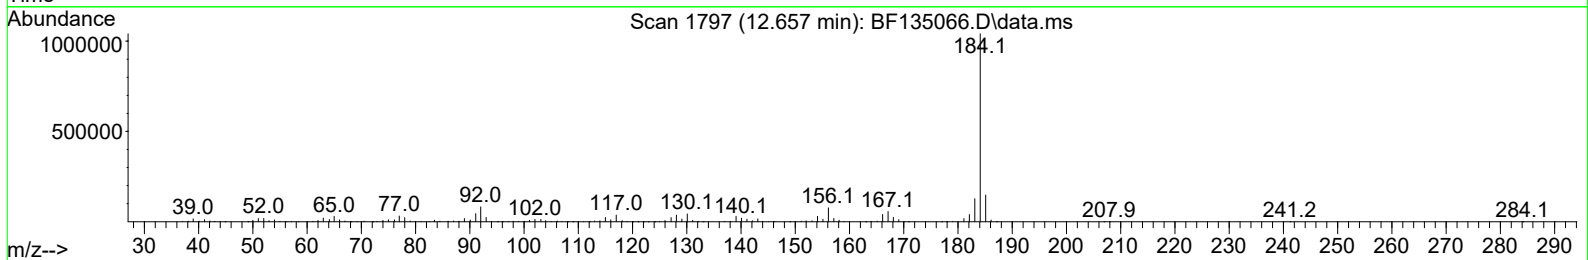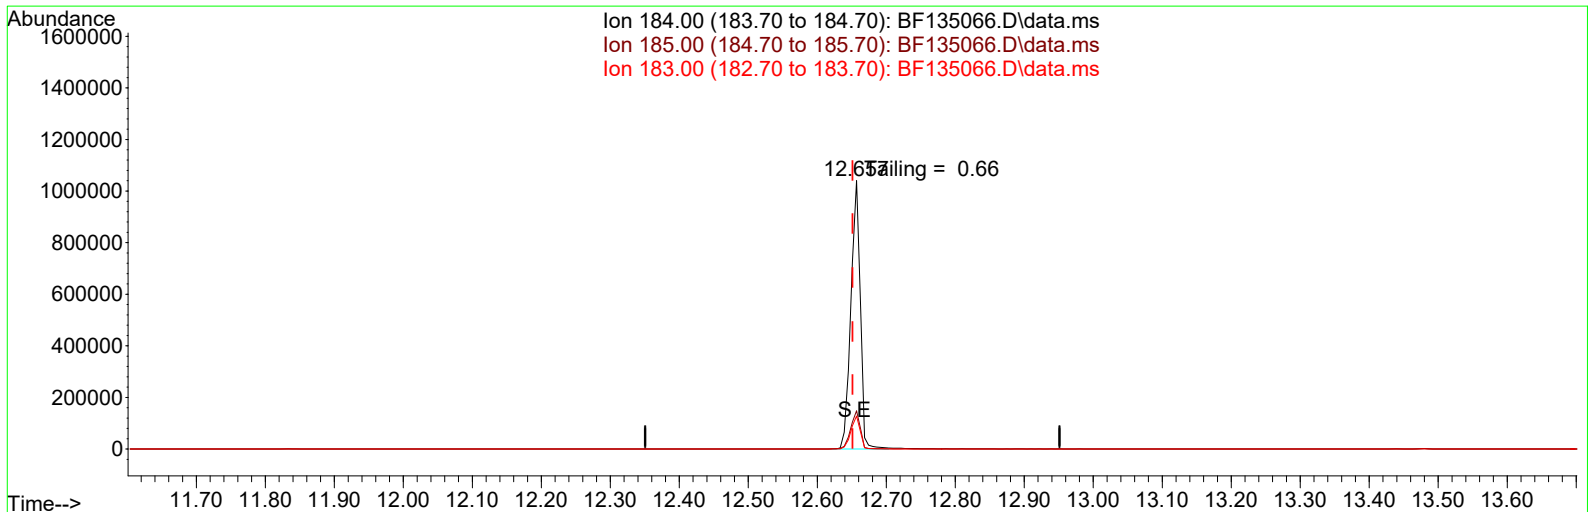

TIC: BF135066.D\data.ms

(77) Benzidine

12.657min (+ 0.006) 699419.11 ng m

response 983428

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.26
183.00	11.30	12.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/1/2023	BNA_F	<u>BF135066.D</u>
Compound Name	Response	Retention Time
DDT	433091	13.48
DDD	9436	13.204
DDE	3628	11.569
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13064	446155	2.93

Instrument :
BNA_F
ClientSampleId :
DFTPP