
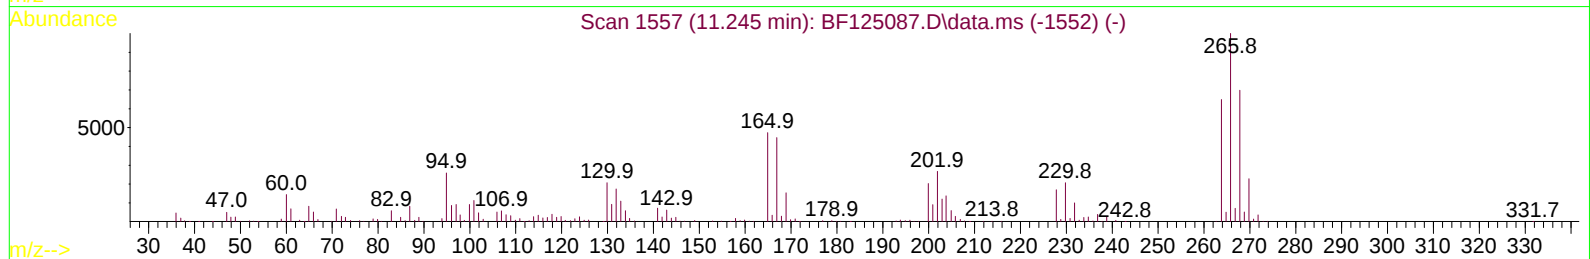
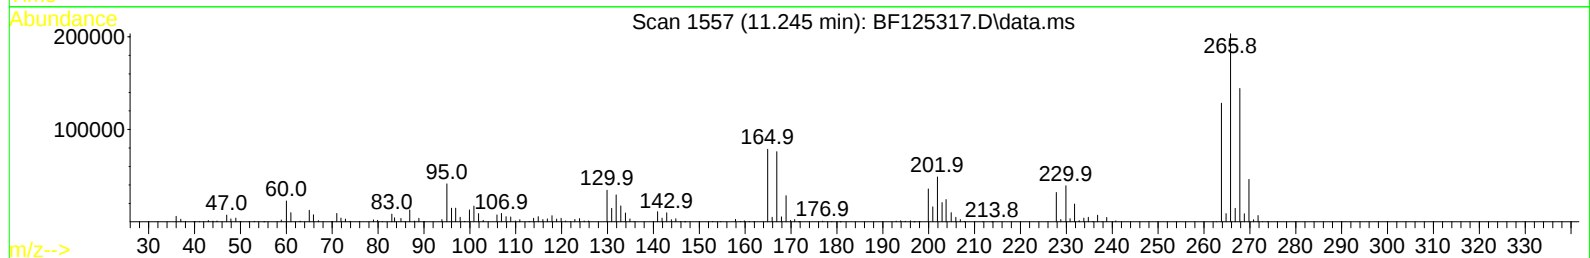


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090221\
Data File : BF125317.D
Acq On : 2 Sep 2021 13:08
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 13:46:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

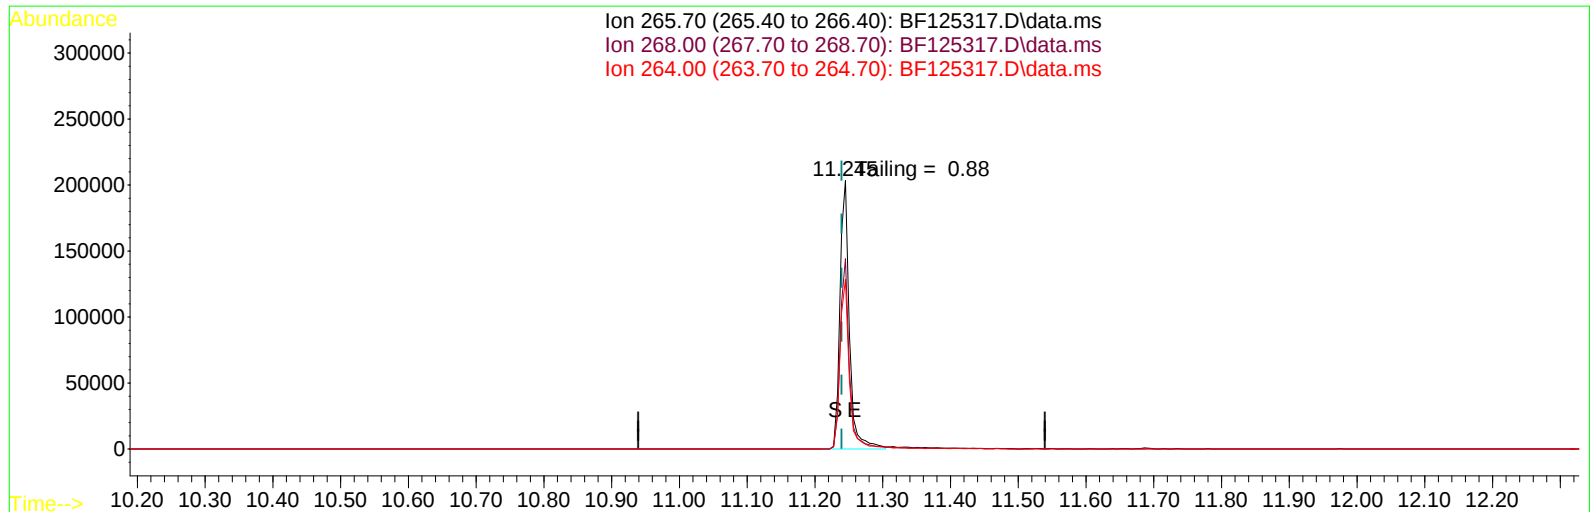

TIC: BF125317.D\data.ms

(70) Pentachlorophenol (C)




11.245min (+ 0.006) 29912.43 ng

response 200225

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	70.92
264.00	69.90	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090221\
Data File : BF125317.D
Acq On : 2 Sep 2021 13:08
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 02 13:46:24 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

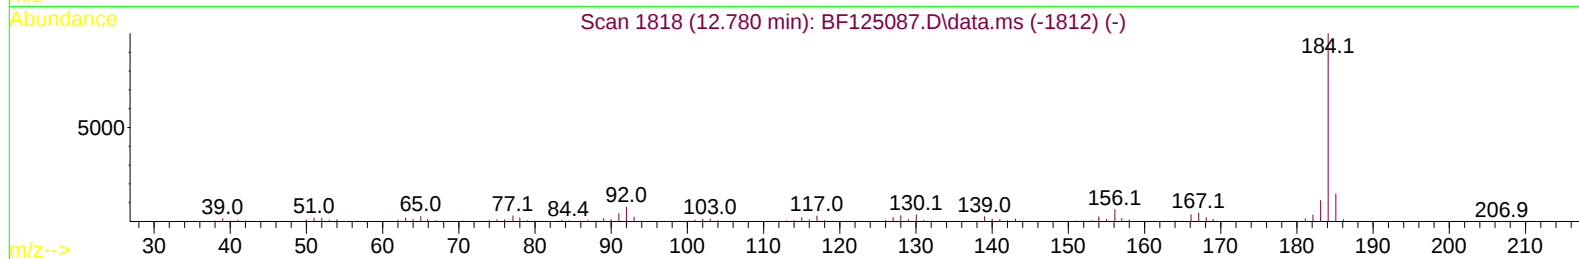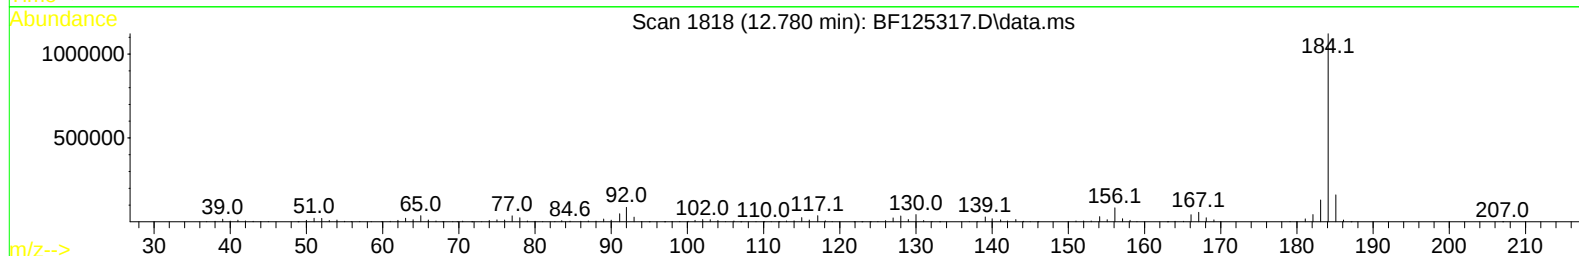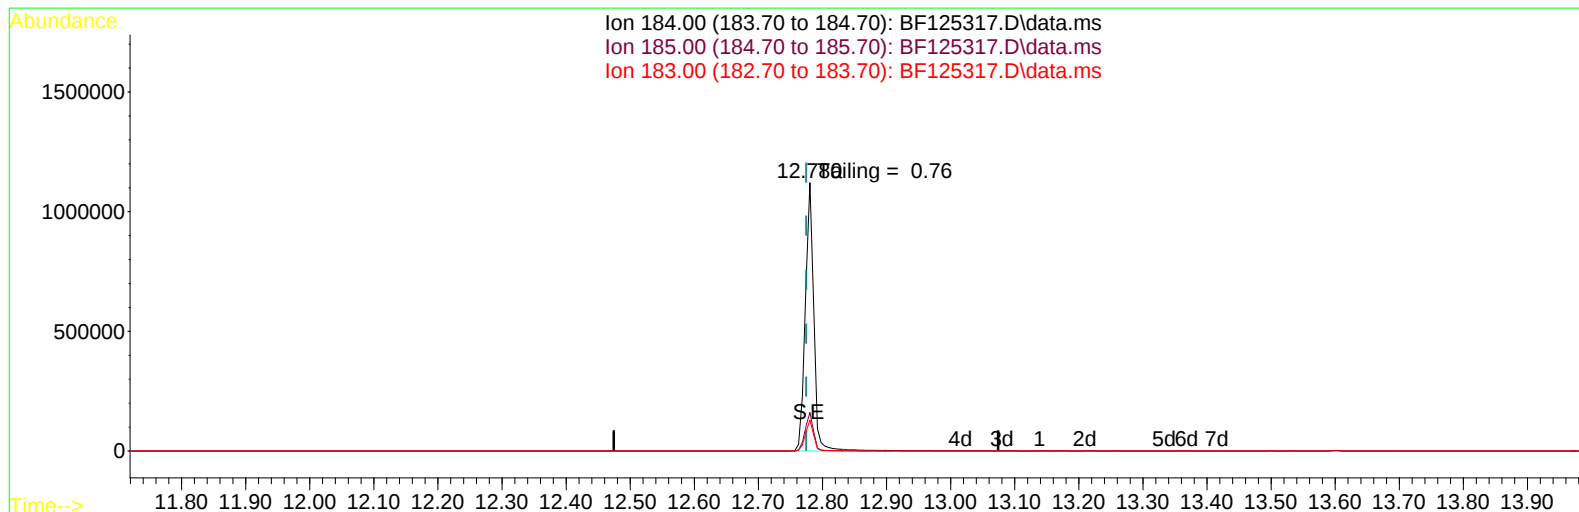

TIC: BF125317.D\data.ms

(77) Benzidine

12.780min (+ 0.006) 269392.90 ng m

response 1016117

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.36
183.00	10.10	11.60
0.00	0.00	0.00