

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090221\
 Data File : BF125320.D
 Acq On : 2 Sep 2021 14:42
 Operator : JU/CG
 Sample : PB138866BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138866BL

Quant Time: Sep 02 15:49:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.910	152	185094	20.000	ng	0.00
21) Naphthalene-d8	8.192	136	732076	20.000	ng	# 0.00
39) Acenaphthene-d10	9.951	164	386418	20.000	ng	0.00
64) Phenanthrene-d10	11.439	188	696478	20.000	ng	0.00
76) Chrysene-d12	14.080	240	411766	20.000	ng	# 0.00
86) Perylene-d12	15.586	264	368961	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.540	112	1334075	109.093	ng	0.01
7) Phenol-d6	6.545	99	1681214	106.301	ng	0.00
23) Nitrobenzene-d5	7.475	82	1120230	77.037	ng	0.00
42) 2,4,6-Tribromophenol	10.745	330	504528	130.798	ng	0.00
45) 2-Fluorobiphenyl	9.269	172	1960881	70.725	ng	0.00
79) Terphenyl-d14	13.027	244	2101327	81.299	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090221\
Data File : BF125320.D
Acq On : 2 Sep 2021 14:42
Operator : JU/CG
Sample : PB138866BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138866BL

Quant Time: Sep 02 15:49:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration




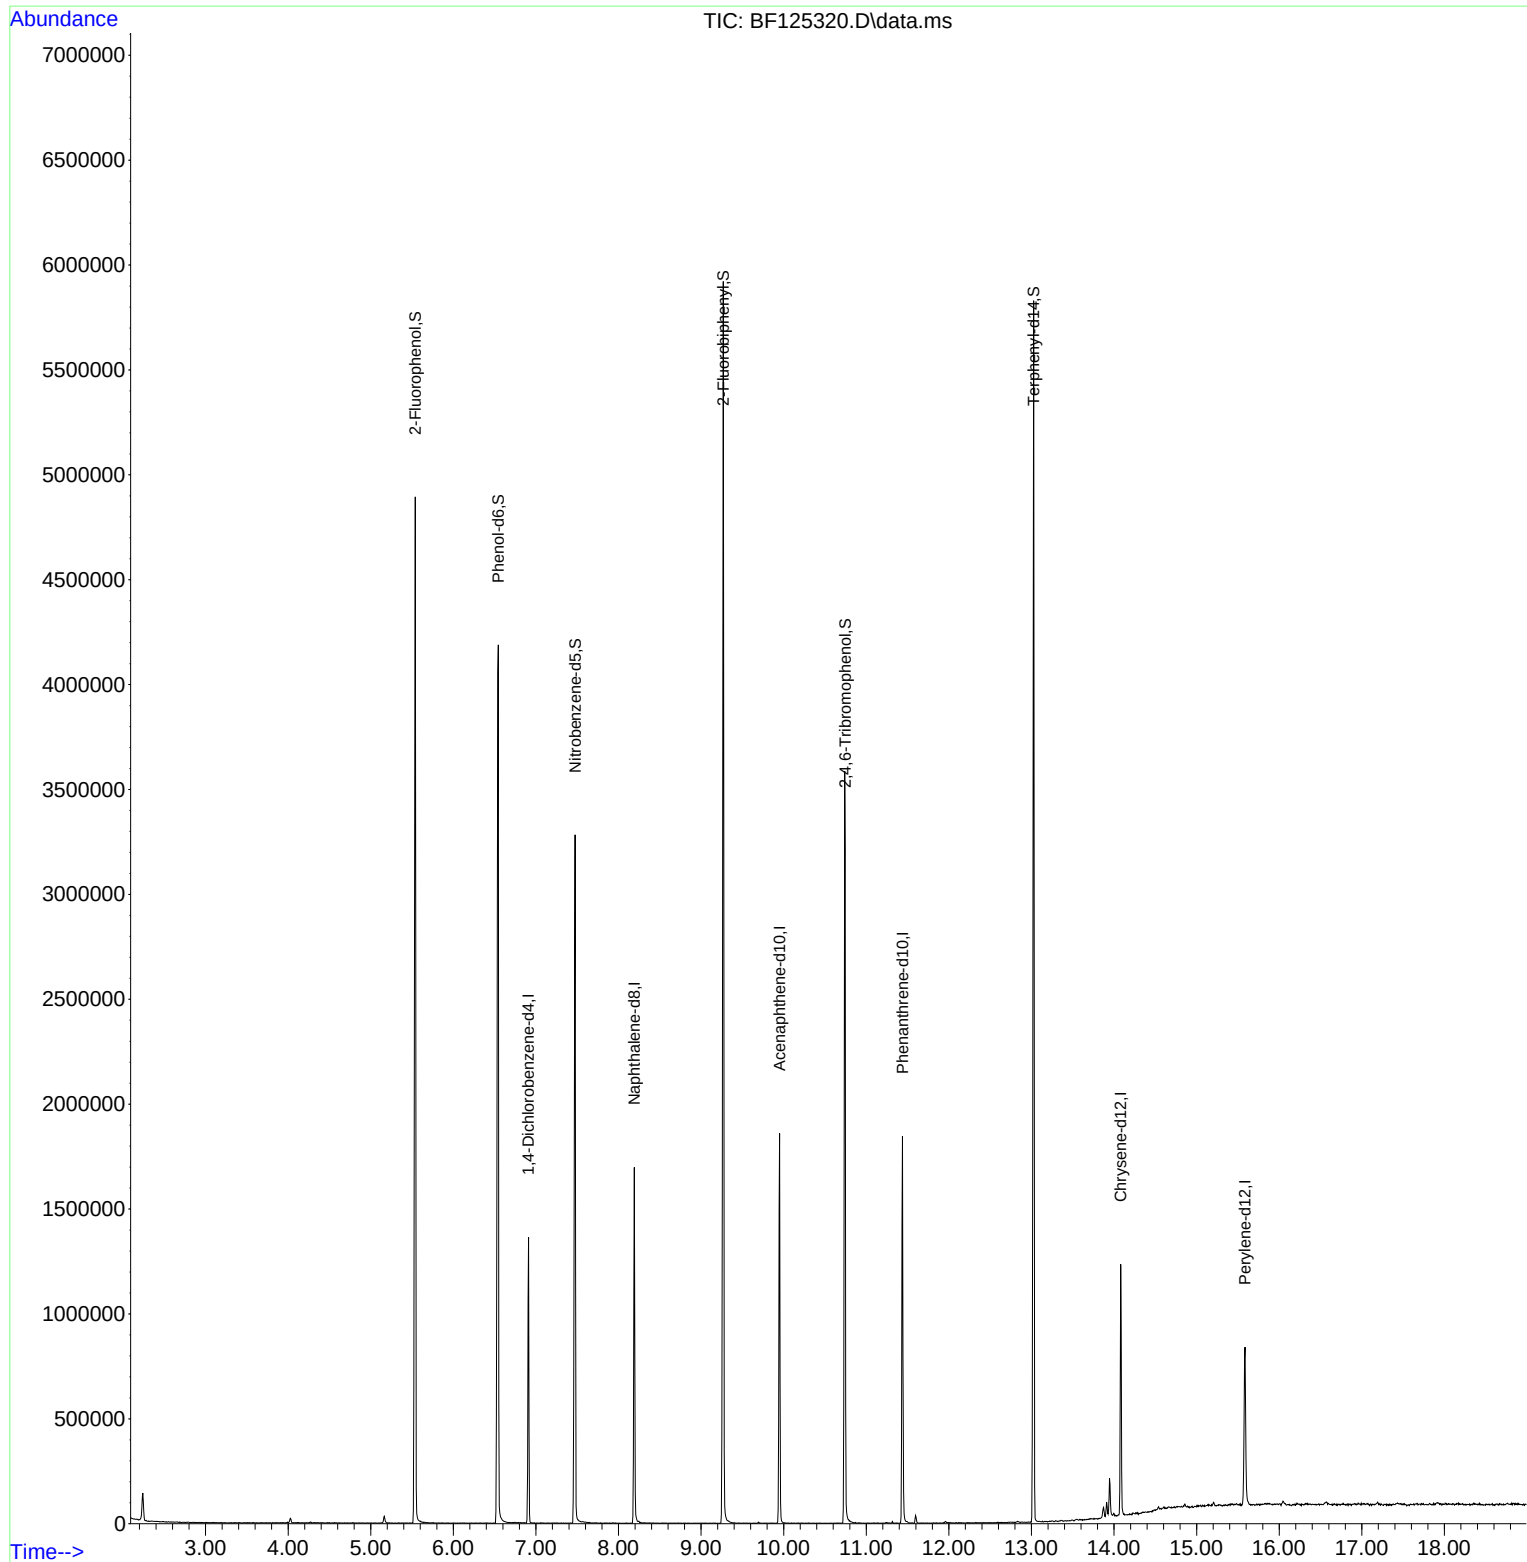




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.910 min Scan# 820
Delta R.T. -0.006 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42




Instrument :
BNA_F
ClientSampled :
PB138866BL


Tgt Ion:152 Resp: 185094
Ion Ratio Lower Upper
152 100
150 158.9 117.6 176.4
115 60.7 47.1 70.7

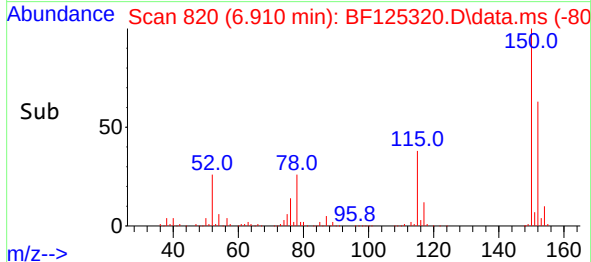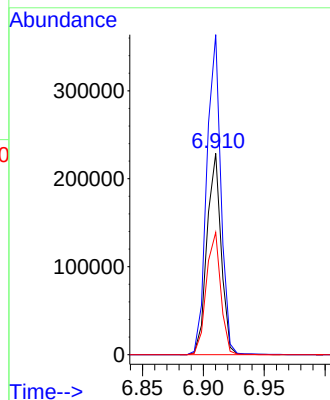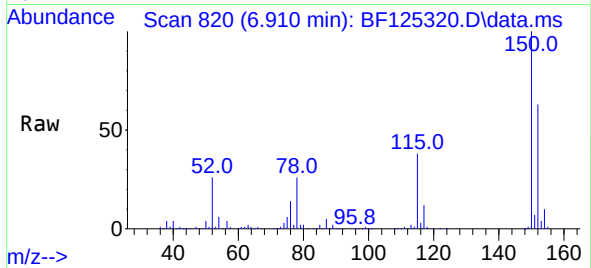

#5
2-Fluorophenol
Concen: 109.093 ng
RT: 5.540 min Scan# 587
Delta R.T. 0.012 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42

Tgt Ion:112 Resp: 1334075
Ion Ratio Lower Upper
112 100
64 73.1 44.2 66.2#
63 38.6 26.2 39.2


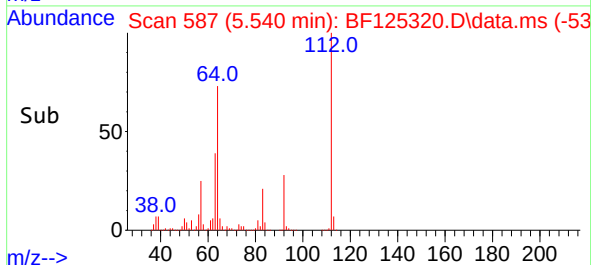
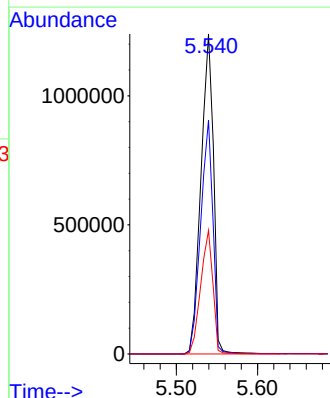
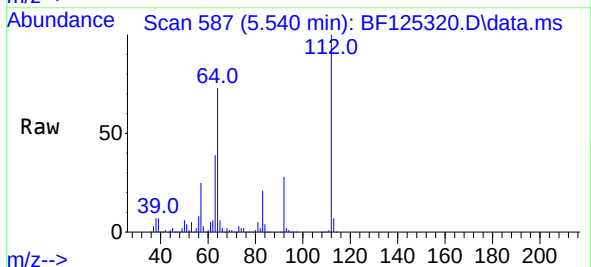


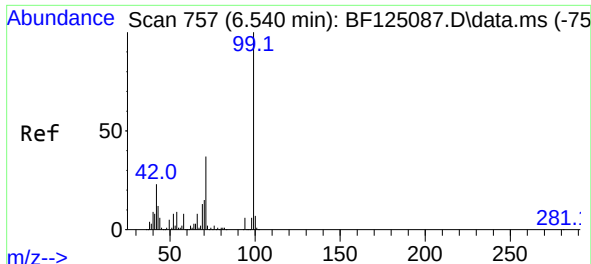

#7
Phenol-d6
Concen: 106.301 ng
RT: 6.545 min Scan# 758
Delta R.T. 0.006 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42




Instrument :
BNA_F
ClientSampleId :
PB138866BL


Tgt Ion: 99 Resp: 1681214
Ion Ratio Lower Upper
99 100
42 20.0 23.5 35.3#
71 36.5 25.6 38.4

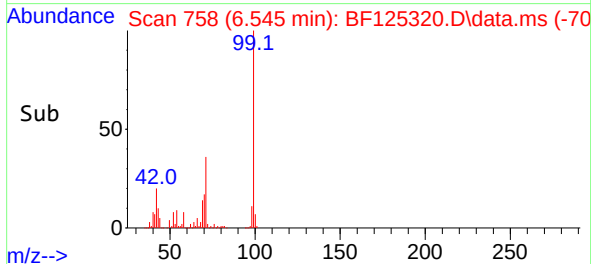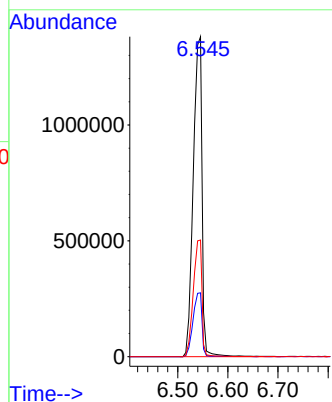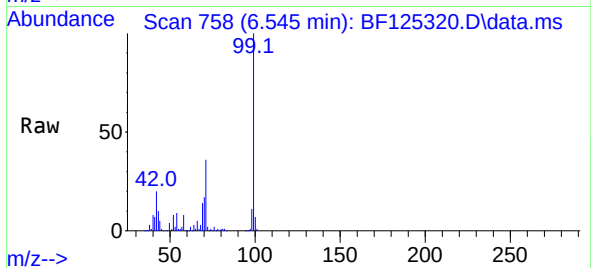

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.192 min Scan# 1038
Delta R.T. -0.006 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42

Tgt Ion: 136 Resp: 732076
Ion Ratio Lower Upper
136 100
137 11.0 9.8 14.6
54 10.4 6.4 9.6#
68 6.1 3.3 4.9#


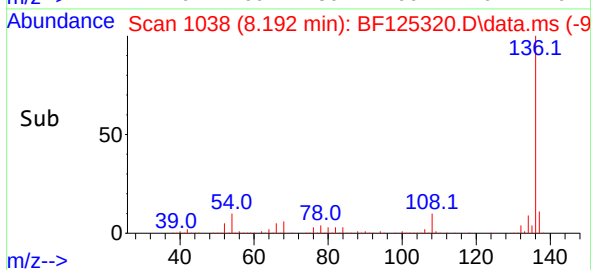
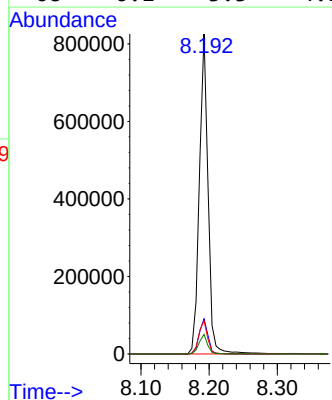
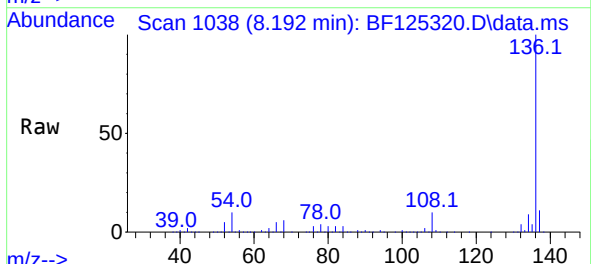


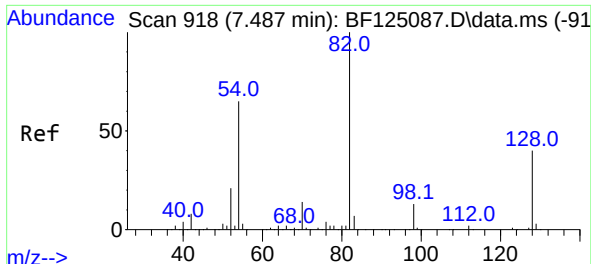

#23
Nitrobenzene-d5
Concen: 77.037 ng
RT: 7.475 min Scan# 916
Delta R.T. -0.006 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42




Instrument :
BNA_F
ClientSampleId :
PB138866BL


Tgt Ion: 82 Resp: 1120230
Ion Ratio Lower Upper
82 100
128 40.4 40.6 60.8#
54 61.7 49.6 74.4

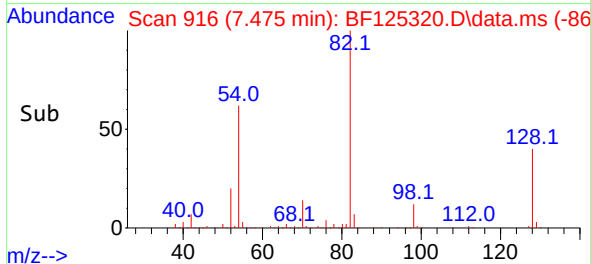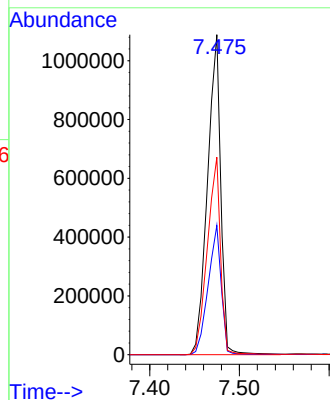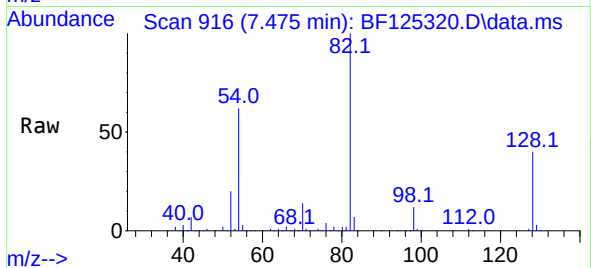

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.951 min Scan# 1337
Delta R.T. 0.000 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42

Tgt Ion:164 Resp: 386418
Ion Ratio Lower Upper
164 100
162 102.8 81.3 121.9
160 46.3 38.0 57.0


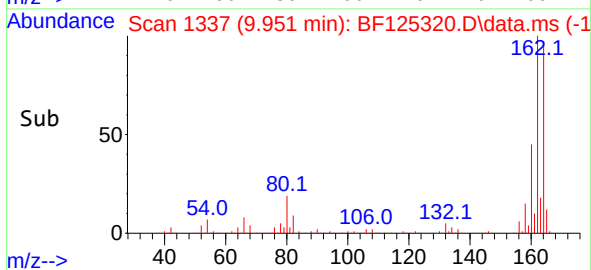
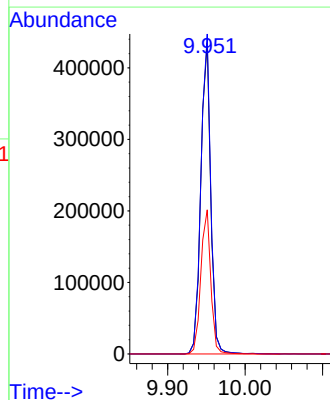
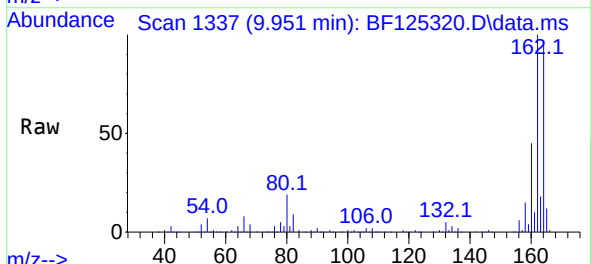




#42
2,4,6-Tribromophenol
Concen: 130.798 ng
RT: 10.745 min Scan# 1472
Delta R.T. 0.006 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42




Instrument :
BNA_F
ClientSampleId :
PB138866BL


Tgt Ion:330 Resp: 504528
Ion Ratio Lower Upper
330 100
332 96.2 76.2 114.4
141 28.7 44.6 66.8#

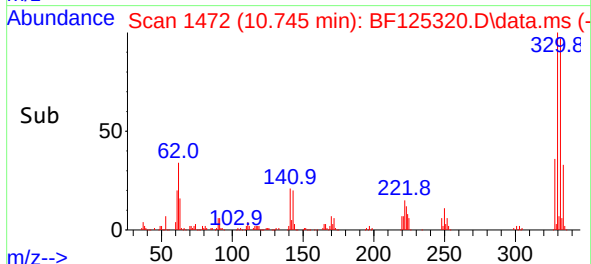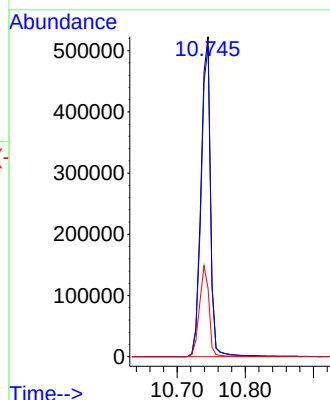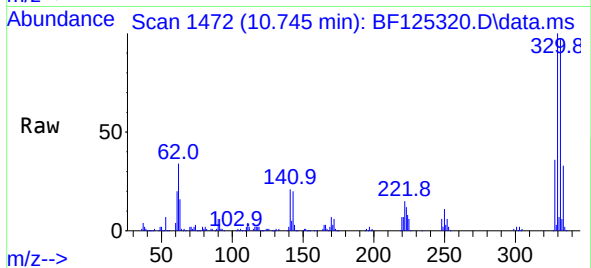

#45
2-Fluorobiphenyl
Concen: 70.725 ng
RT: 9.269 min Scan# 1221
Delta R.T. -0.006 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42

Tgt Ion:172 Resp: 1960881
Ion Ratio Lower Upper
172 100
171 35.5 26.5 39.7
170 24.0 18.8 28.2


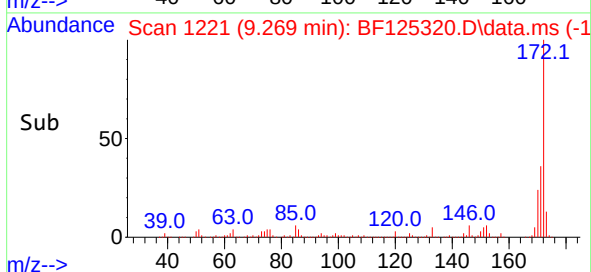
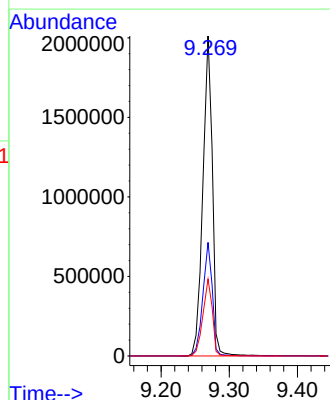
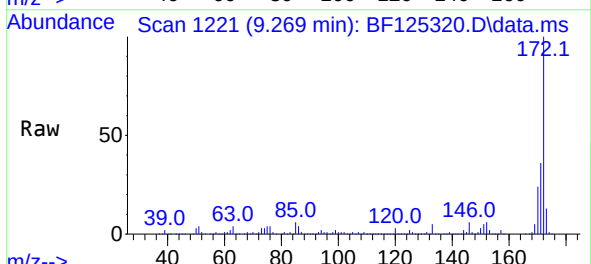




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.439 min Scan# 1590
Delta R.T. 0.000 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42




Instrument :
BNA_F
ClientSampleId :
PB138866BL


Tgt Ion:188 Resp: 696478
Ion Ratio Lower Upper
188 100
94 9.0 6.7 10.1
80 9.5 7.5 11.3

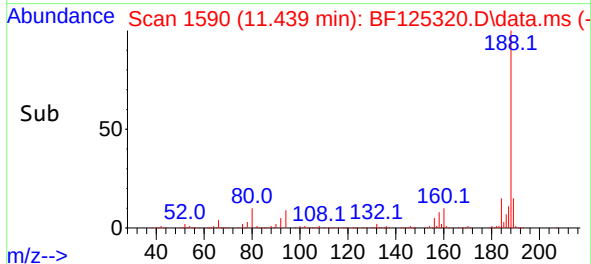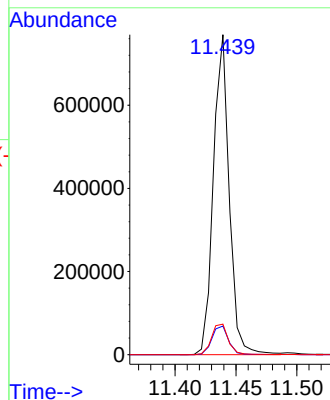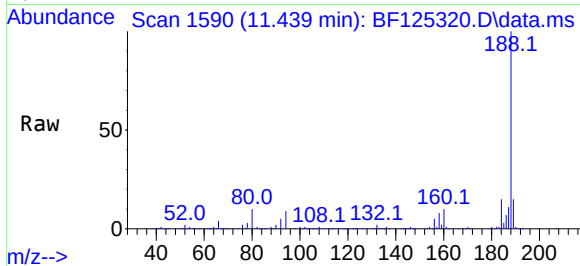

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.080 min Scan# 2039
Delta R.T. 0.000 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42


Tgt Ion:240 Resp: 411766
Ion Ratio Lower Upper
240 100
120 10.4 10.8 16.2#
236 25.0 21.6 32.4

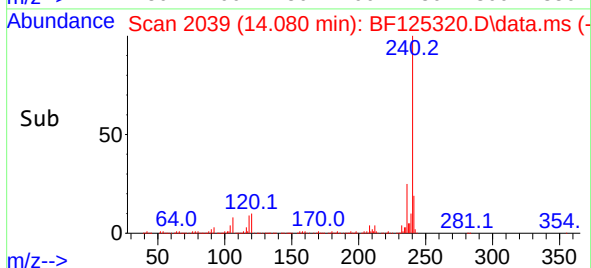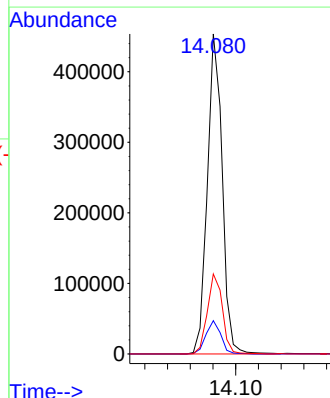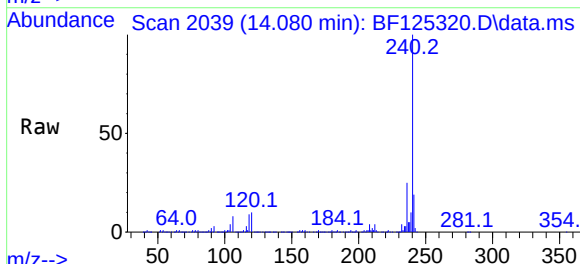






#79
Terphenyl-d14
Concen: 81.299 ng
RT: 13.027 min Scan# 1860
Delta R.T. 0.006 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42

Instrument :
BNA_F
ClientSampleId :
PB138866BL

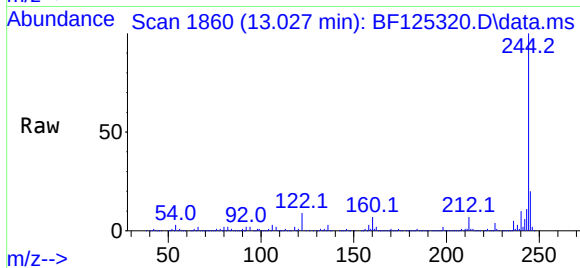

Tgt Ion:244 Resp: 2101327
Ion Ratio Lower Upper
244 100
212 6.9 5.9 8.9
122 9.0 9.0 13.4#

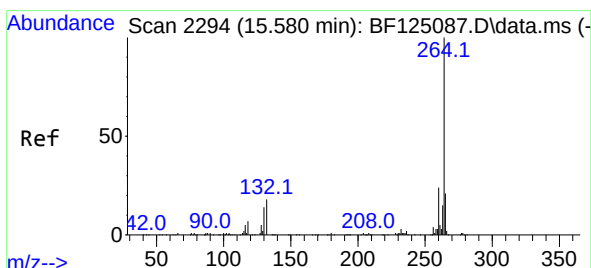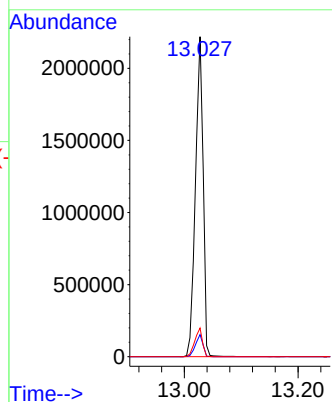

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.586 min Scan# 2295
Delta R.T. 0.012 min
Lab File: BF125320.D
Acq: 2 Sep 2021 14:42

Tgt Ion:264 Resp: 368961
Ion Ratio Lower Upper
264 100
260 24.4 19.6 29.4
265 21.6 17.2 25.8

