

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
 Data File : BF130113.D
 Acq On : 02 Sep 2022 16:13
 Operator : CG\JU
 Sample : N4446-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DUP-Y

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.887	438	442	456	rVB	230295	280308	4.32%	0.826%
2	5.298	508	512	515	rBV	2690609	2447637	37.68%	7.211%
3	6.322	682	686	689	rBV	1816321	1493595	23.00%	4.400%
4	6.704	747	751	754	rBV	1415320	1227502	18.90%	3.616%
5	7.269	841	847	850	rBV	3491557	3557325	54.77%	10.480%
6	7.980	964	968	972	rBV	1960908	1658863	25.54%	4.887%
7	9.063	1146	1152	1155	rBV	6576052	6495165	100.00%	19.135%
8	9.733	1261	1266	1269	rBV	2195349	1887905	29.07%	5.562%
9	10.521	1395	1400	1403	rBV	4524381	4212656	64.86%	12.410%
10	11.210	1513	1517	1521	rBV	2069449	1792979	27.60%	5.282%
11	11.745	1602	1608	1612	rBV	91085	98220	1.51%	0.289%
12	12.804	1783	1788	1791	rBV	6059986	6066000	93.39%	17.870%
13	13.839	1960	1964	1968	rBV	1441160	1258674	19.38%	3.708%
14	13.945	1977	1982	1987	rBV	122035	135988	2.09%	0.401%
15	15.245	2197	2203	2207	rBV	837642	1025321	15.79%	3.021%
16	15.292	2207	2211	2216	rVB	61845	82983	1.28%	0.244%
17	15.692	2275	2279	2285	rBV	58388	78788	1.21%	0.232%
18	16.156	2354	2358	2365	rVB2	49568	78841	1.21%	0.232%
19	16.703	2446	2451	2459	rVB3	34172	65851	1.01%	0.194%




Sum of corrected areas: 33944601

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130113.D
Acq On : 02 Sep 2022 16:13
Operator : CG\JU
Sample : N4446-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP-Y

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

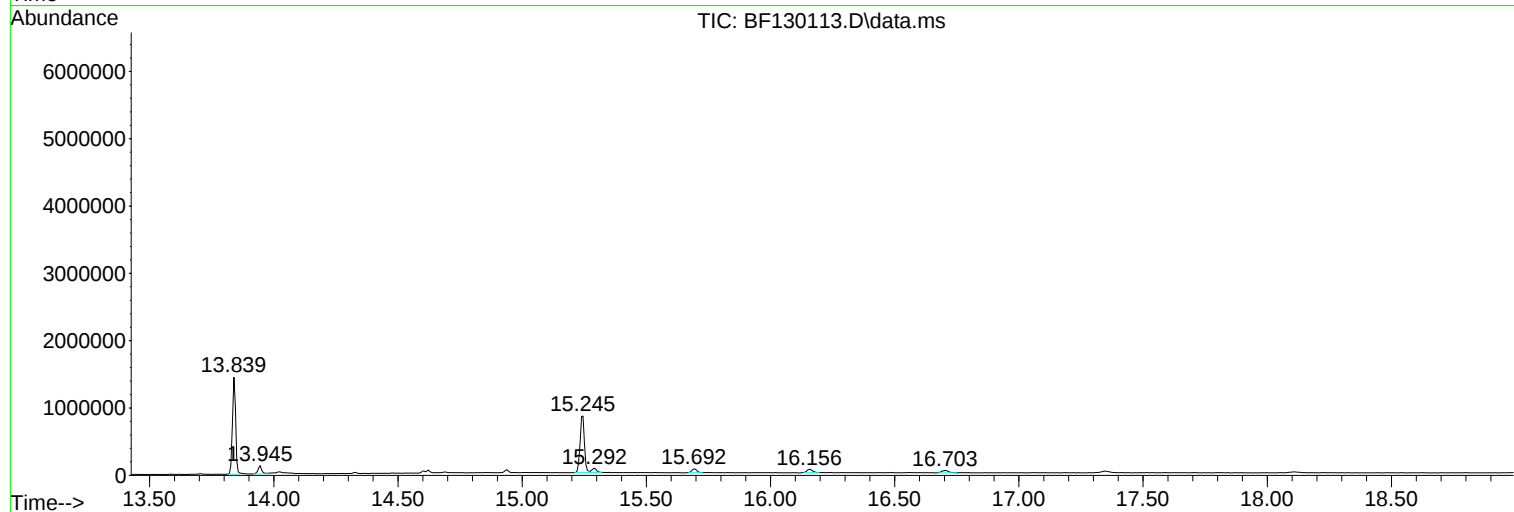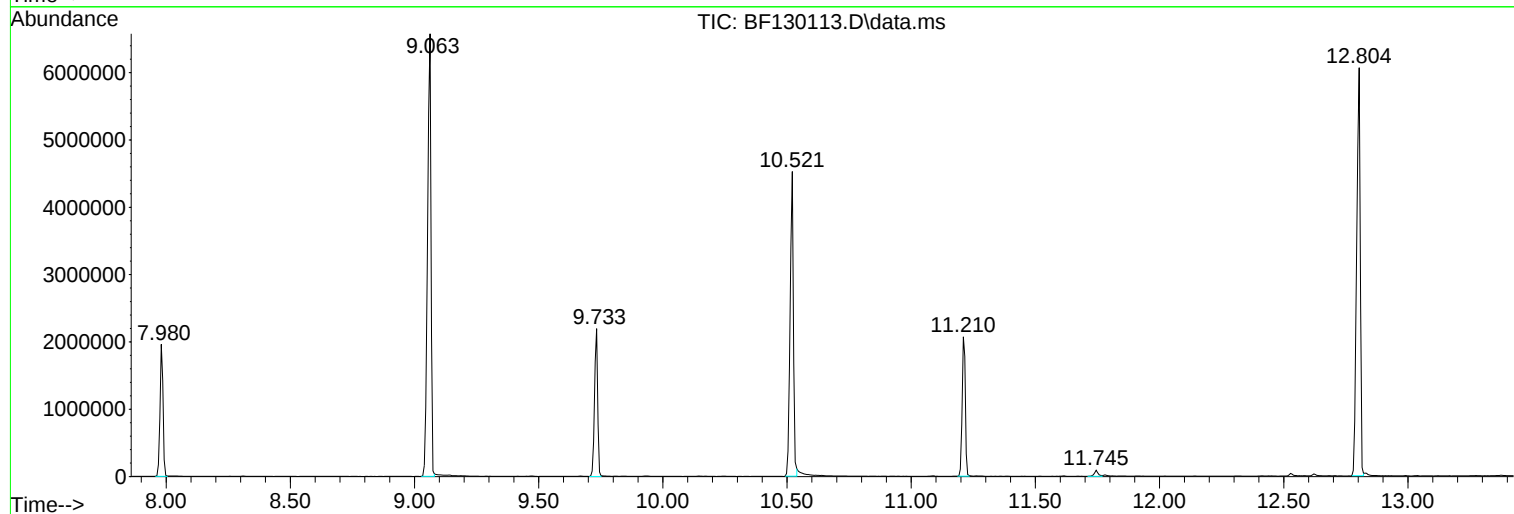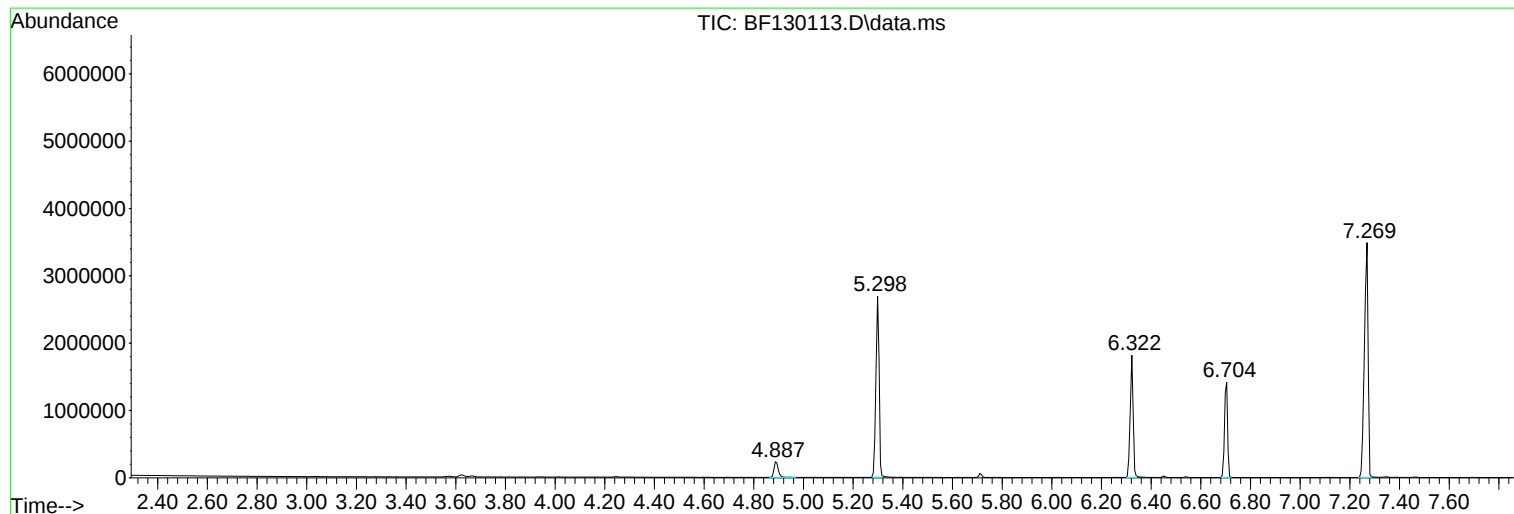

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130113.D
Acq On : 02 Sep 2022 16:13
Operator : CG\JU
Sample : N4446-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP-Y










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.887	4.57 ng	280308	1,4-Dichlorobenzene-d4	6.704

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	12		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

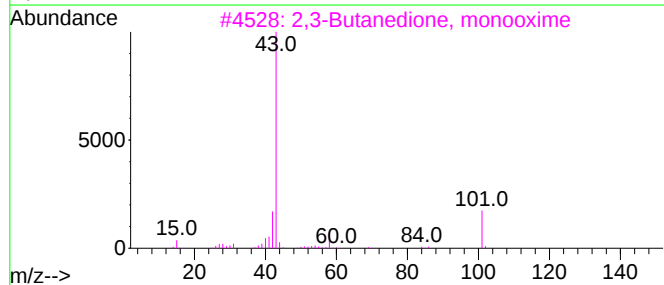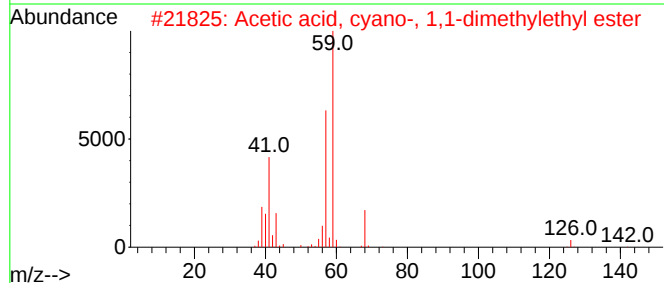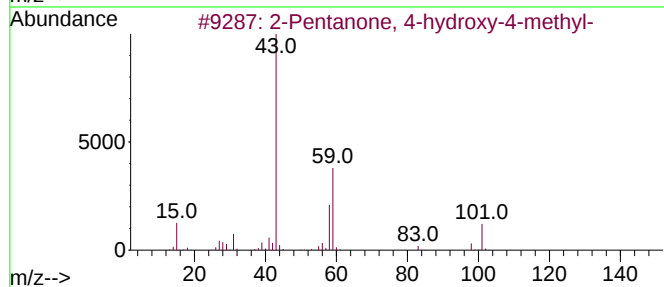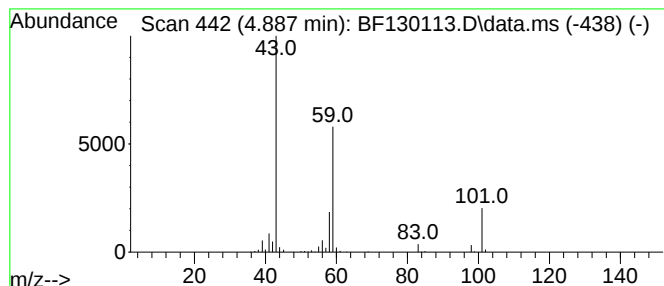

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130113.D
Acq On : 02 Sep 2022 16:13
Operator : CG\JU
Sample : N4446-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP-Y










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.945	2.16 ng	135988	Chrysene-d12	13.839

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	76
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
4			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	40
5			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	38

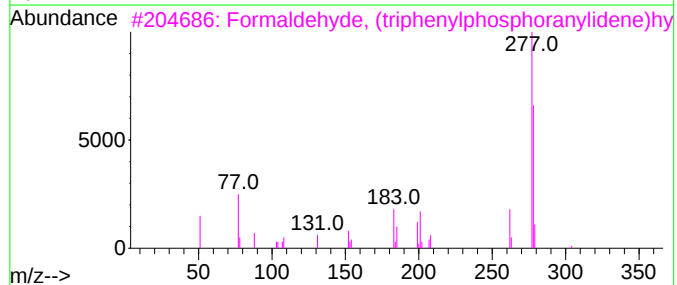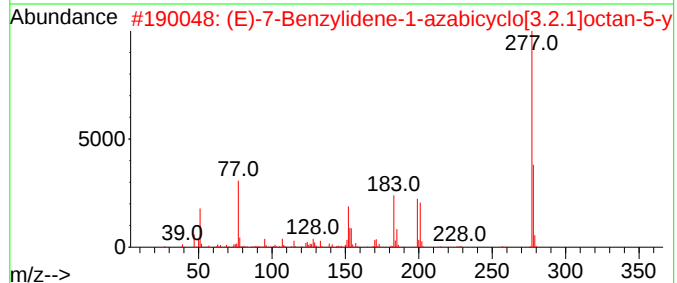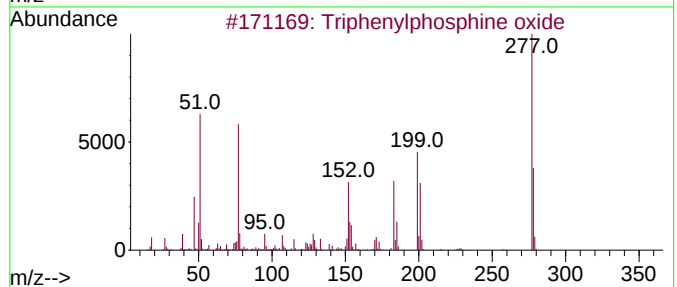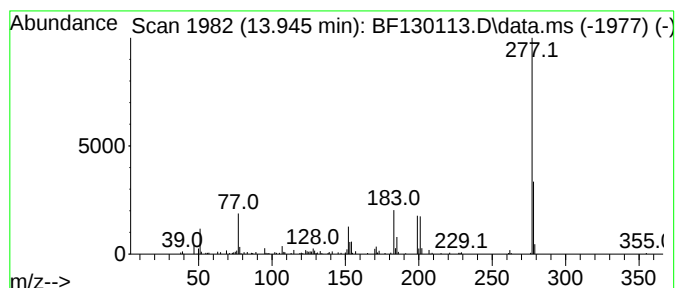

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130113.D
Acq On : 02 Sep 2022 16:13
Operator : CG\JU
Sample : N4446-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP-Y

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.887	4.6	ng	280308	1	6.704	1227500	20.0
Triphenylphosph...	13.945	2.2	ng	135988	5	13.839	1258670	20.0