

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
 Data File : BF130128.D
 Acq On : 03 Sep 2022 00:11
 Operator : CG\JU
 Sample : N4446-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-05

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.893	439	443	451	rVB	274540	299043	4.42%	0.844%
2	5.304	508	513	516	rBV	2886274	2661493	39.30%	7.514%
3	6.328	682	687	690	rBV	1698492	1613264	23.82%	4.555%
4	6.704	747	751	754	rBV	1417234	1245950	18.40%	3.518%
5	7.269	841	847	850	rBV	3739524	3808305	56.24%	10.752%
6	7.981	964	968	972	rBV	1969965	1695802	25.04%	4.788%
7	9.063	1146	1152	1155	rBV	6877678	6771621	100.00%	19.118%
8	9.734	1261	1266	1269	rBV	2382023	1983791	29.30%	5.601%
9	10.522	1395	1400	1403	rBV	4756743	4407760	65.09%	12.444%
10	11.210	1513	1517	1521	rBV	2106398	1826658	26.98%	5.157%
11	11.745	1605	1608	1612	rBV	80739	75043	1.11%	0.212%
12	12.804	1783	1788	1791	rBV	6284089	6168060	91.09%	17.414%
13	13.774	1947	1953	1960	rBV5	39917	99002	1.46%	0.280%
14	13.839	1960	1964	1968	rBV	1388997	1203623	17.77%	3.398%
15	13.945	1977	1982	1993	rVB	202604	214278	3.16%	0.605%
16	15.239	2197	2202	2207	rBV	911738	1051906	15.53%	2.970%
17	15.286	2207	2210	2216	rVB	60340	74884	1.11%	0.211%
18	15.692	2275	2279	2287	rVB	52282	75541	1.12%	0.213%
19	16.157	2353	2358	2365	rVB2	47317	76550	1.13%	0.216%
20	16.698	2445	2450	2458	rBV5	30768	67725	1.00%	0.191%




Sum of corrected areas: 35420299

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130128.D
Acq On : 03 Sep 2022 00:11
Operator : CG\JU
Sample : N4446-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

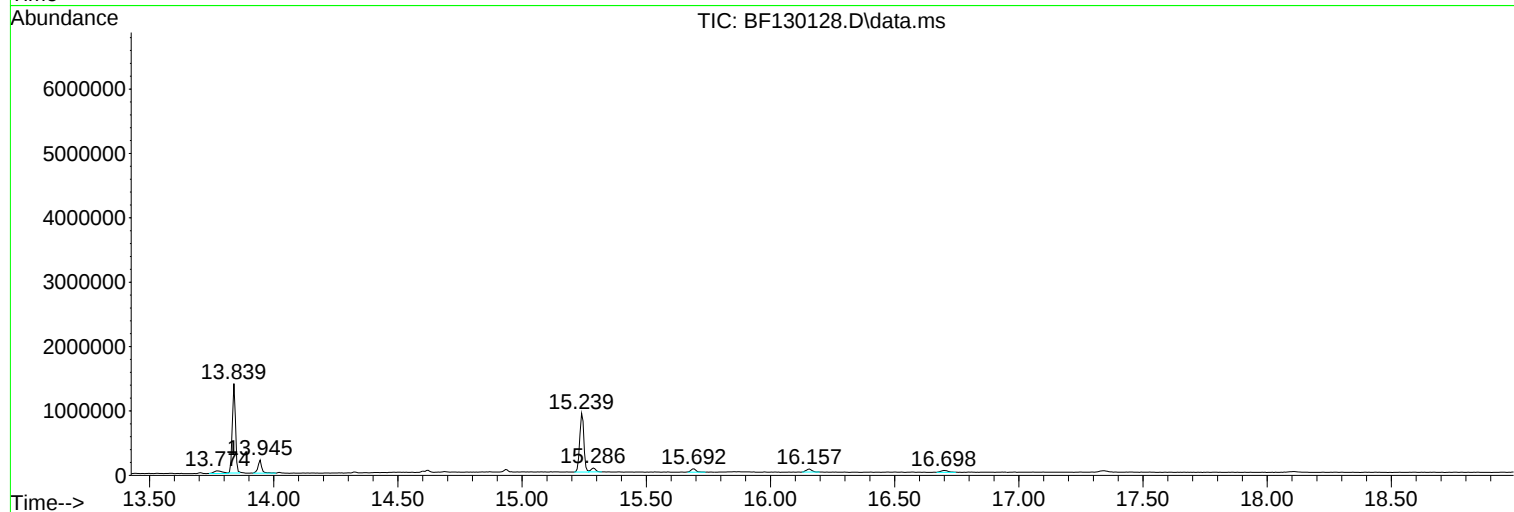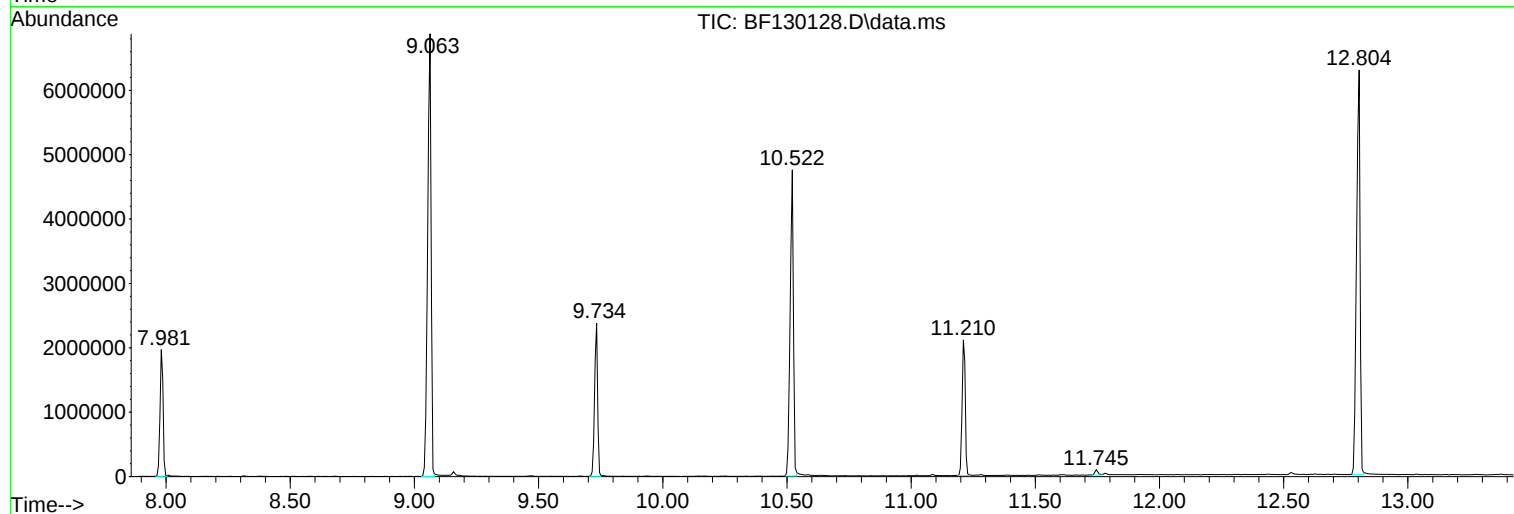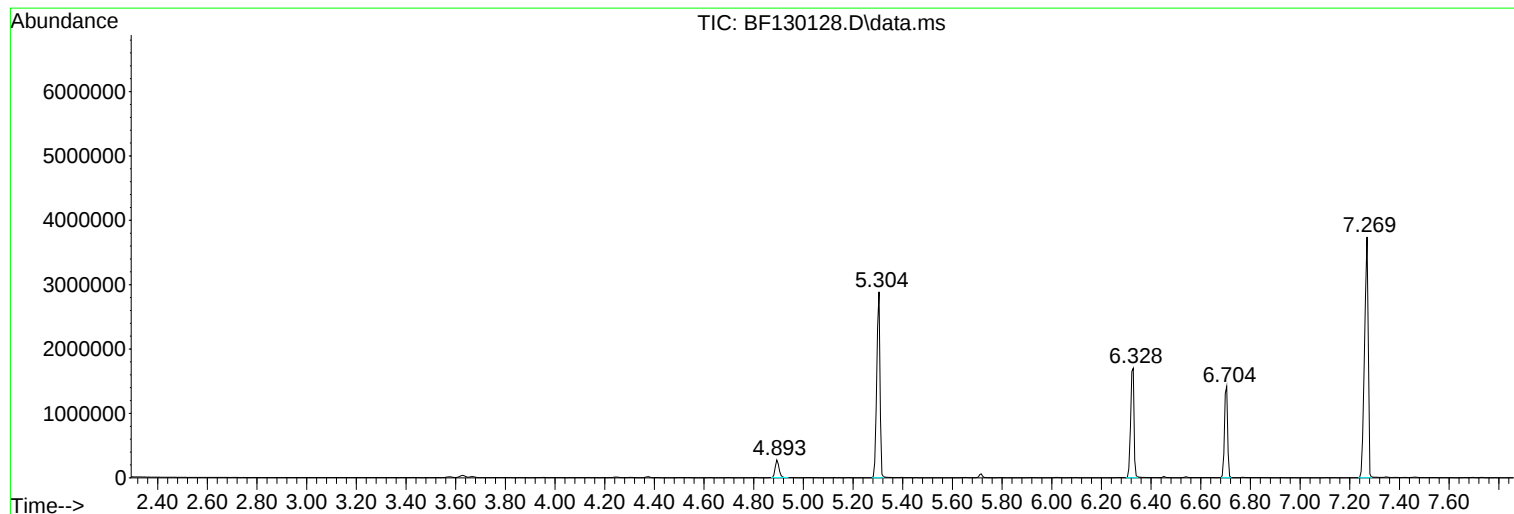

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130128.D
Acq On : 03 Sep 2022 00:11
Operator : CG\JU
Sample : N4446-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.893	4.80 ng	299043	1,4-Dichlorobenzene-d4	6.704

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	28		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

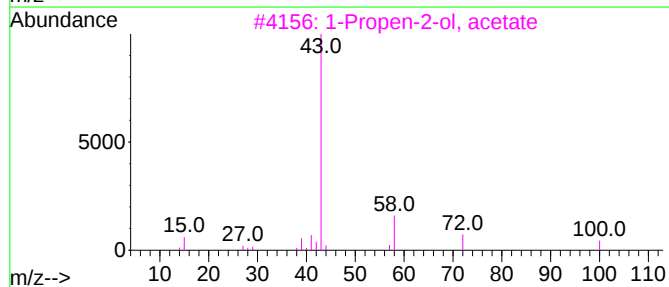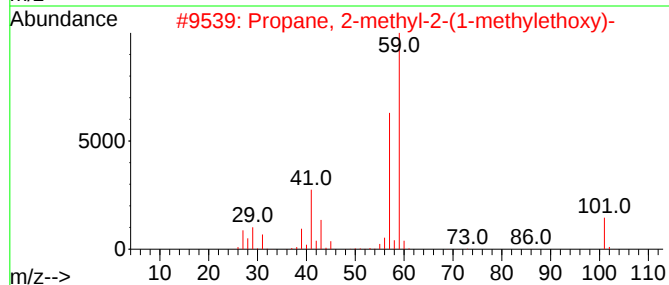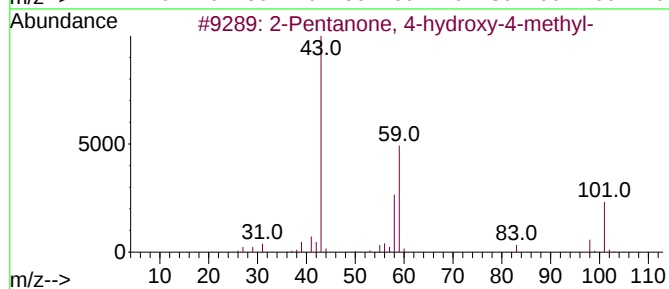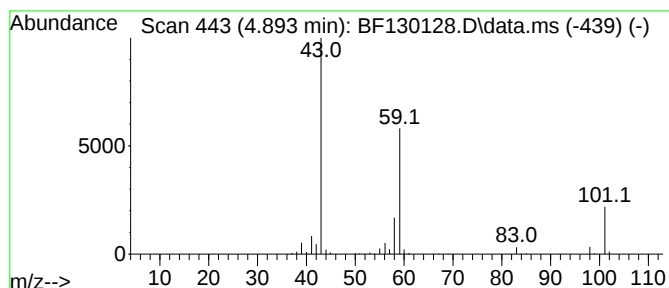

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130128.D
Acq On : 03 Sep 2022 00:11
Operator : CG\JU
Sample : N4446-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.945	3.56 ng	214278	Chrysene-d12	13.839

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	92
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	42
4			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	38
5			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	37

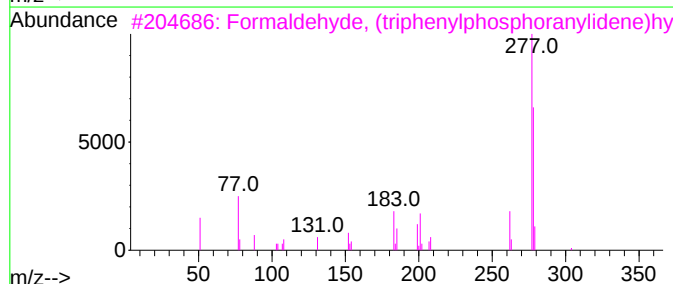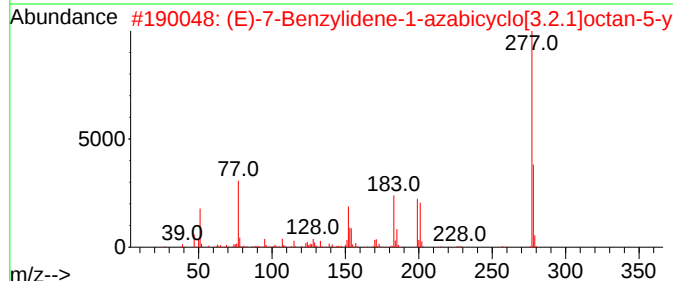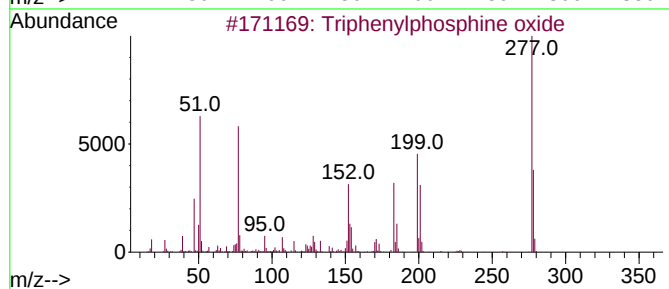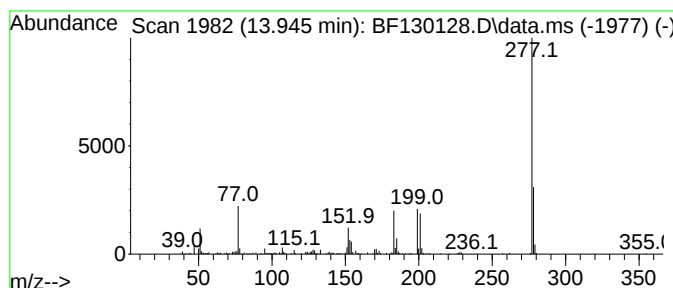

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090222\
Data File : BF130128.D
Acq On : 03 Sep 2022 00:11
Operator : CG\JU
Sample : N4446-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.893	4.8	ng	299043	1	6.704	1245950	20.0
Triphenylphosph...	13.945	3.6	ng	214278	5	13.839	1203620	20.0